
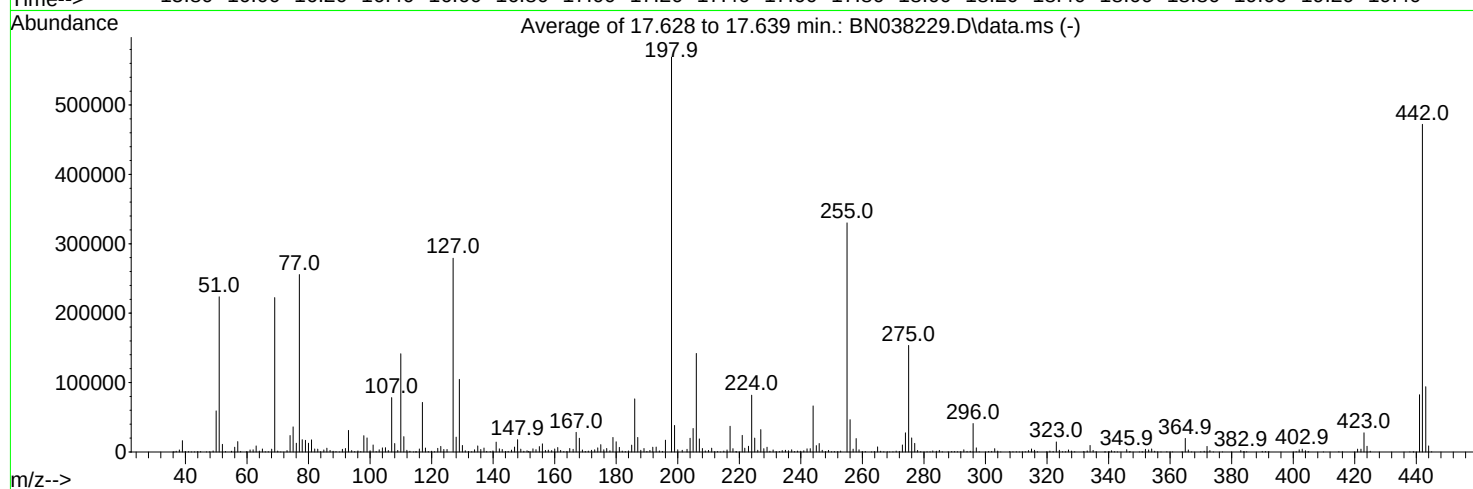


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038229.D
Acq On : 01 Dec 2025 17:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 28 21:04:10 2025

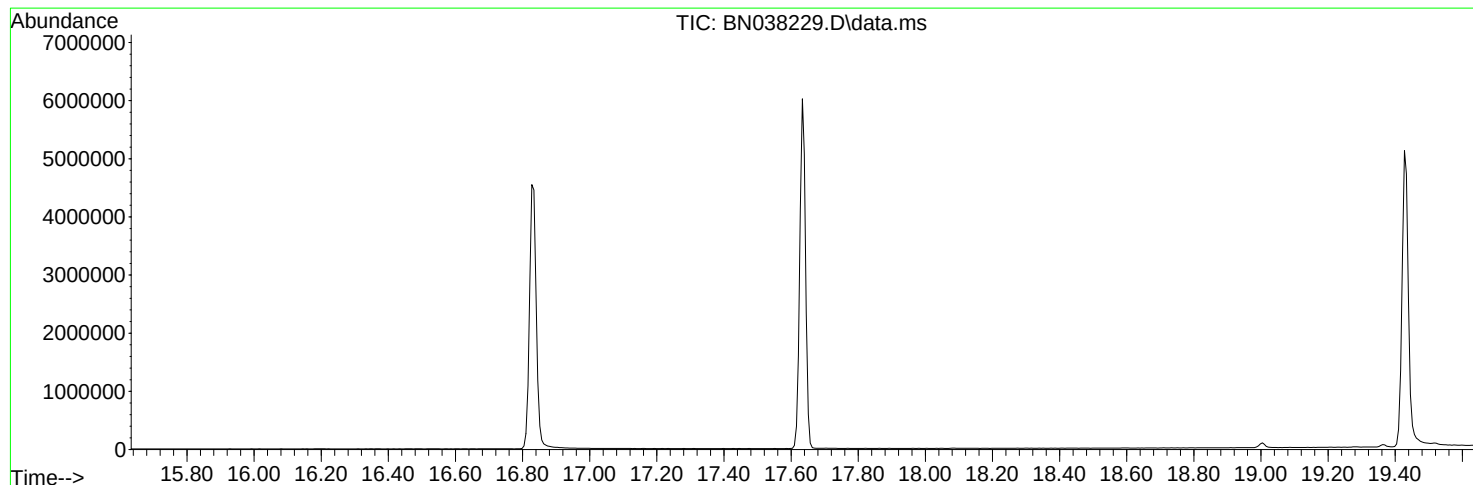




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3958	PASS
69	69	100	100	100.0	222464	PASS
70	69	0.00	2	0.5	1221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	569067	PASS
199	198	5	9	6.7	38248	PASS
365	198	1	100	3.4	19427	PASS
441	443	0.01	150	87.9	82573	PASS
442	442	100	100	100.0	472256	PASS
443	442	15	24	19.9	93936	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038229.D
Acq On : 01 Dec 2025 17:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 17:45:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 17:45:43 2025
Response via : Initial Calibration

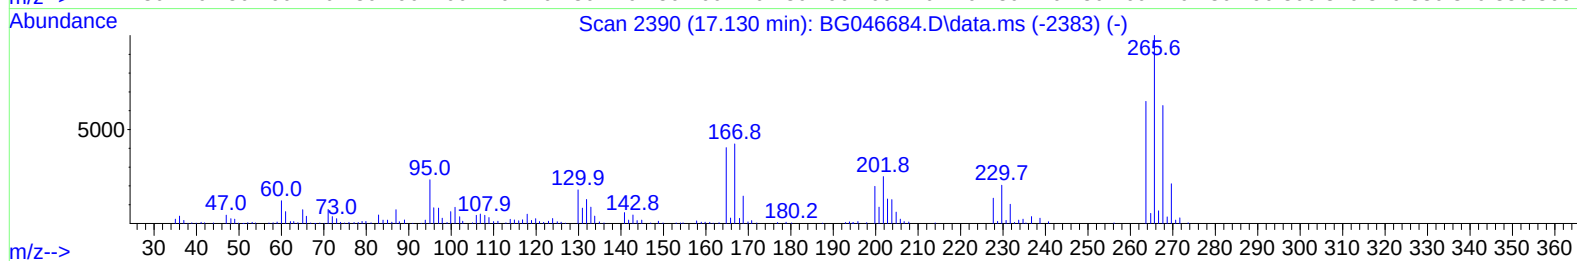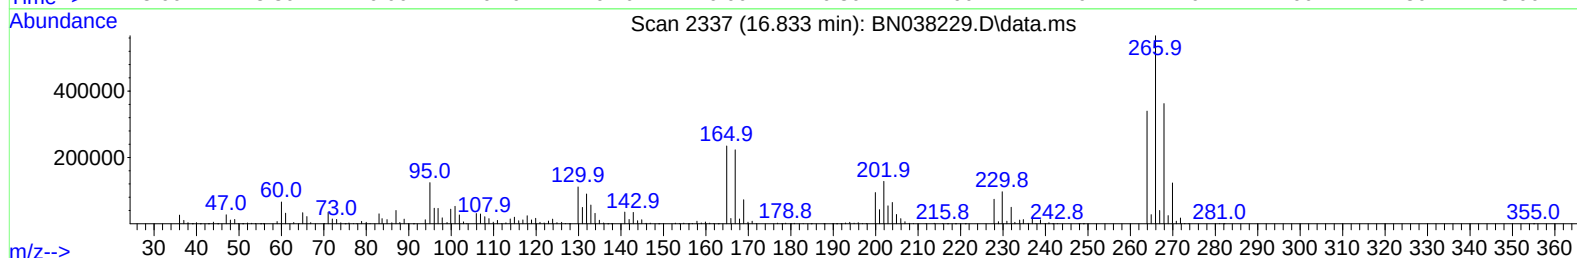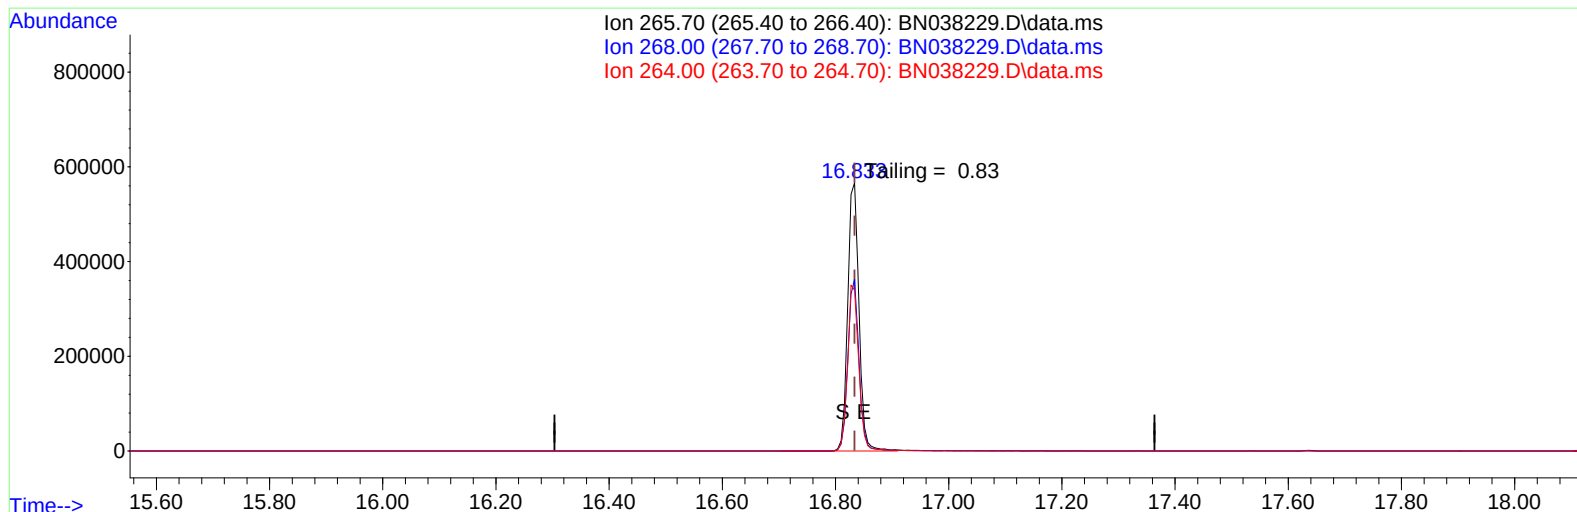

TIC: BN038229.D\data.ms

(70) Pentachlorophenol (C)

16.833min (0.000) 277.76 ng




response 785850

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	59.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120125\
Data File : BN038229.D
Acq On : 01 Dec 2025 17:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 17:45:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 17:45:43 2025
Response via : Initial Calibration

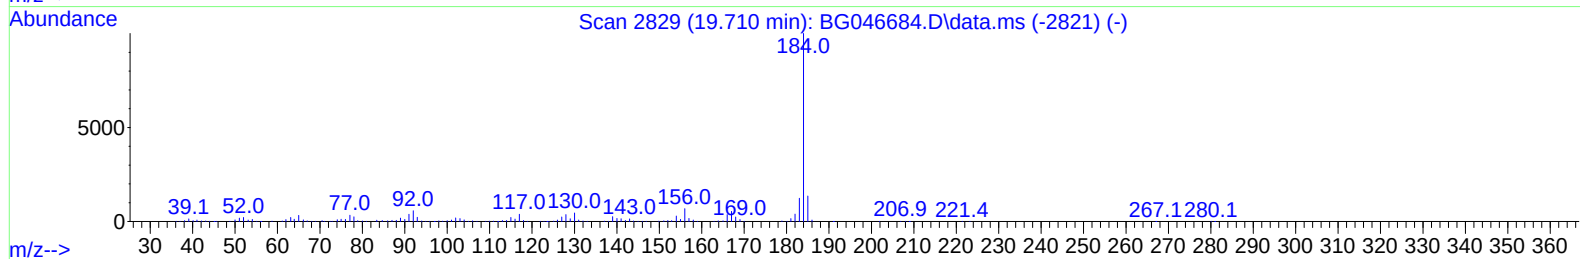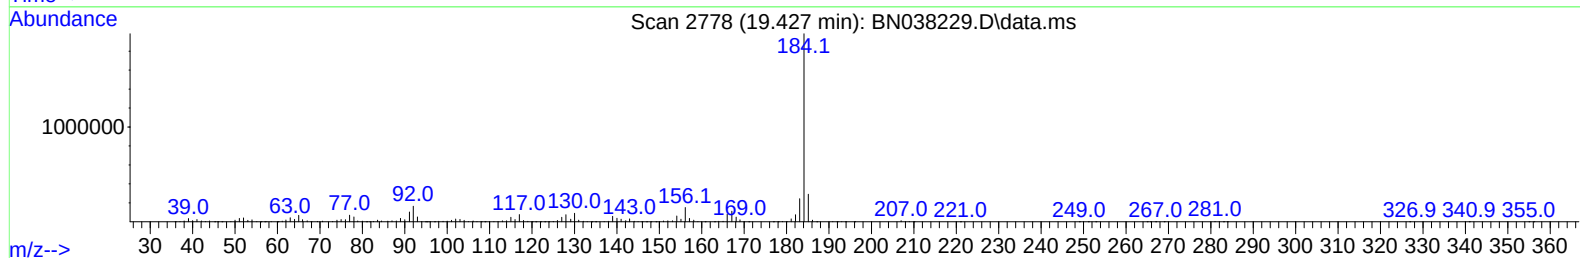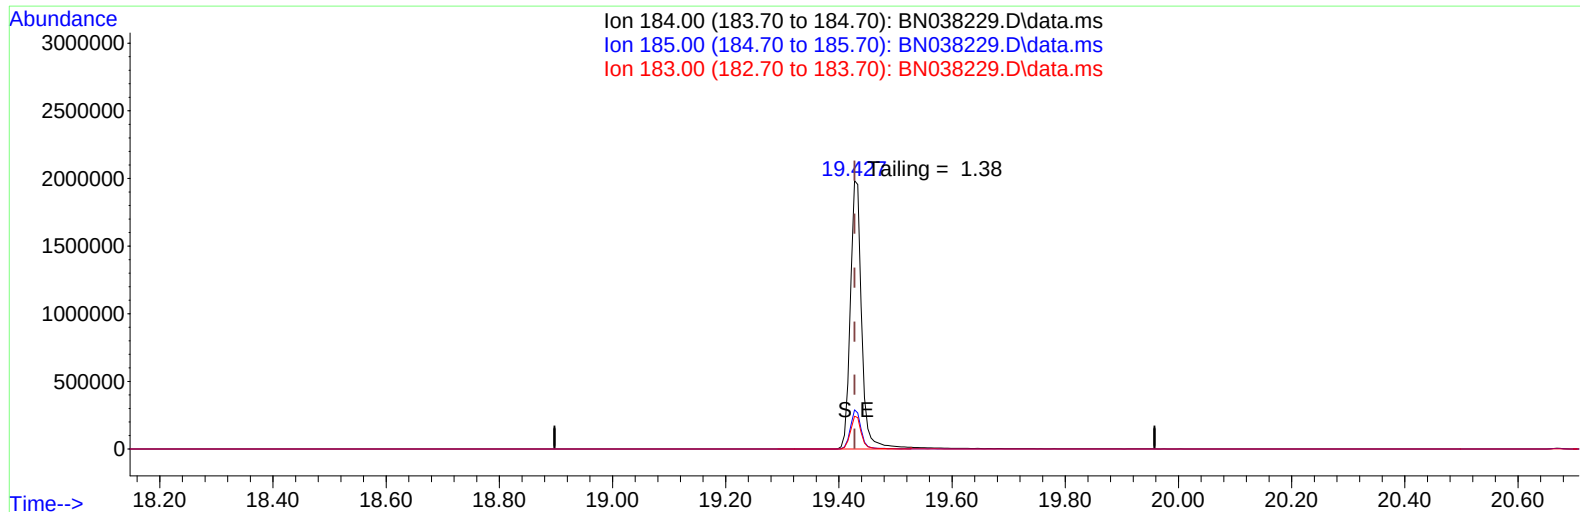

TIC: BN038229.D\data.ms

(77) Benzidine

19.427min (0.000) 0.00 ng

response 2797498

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.63
183.00	13.20	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2025	BNA_N	<u>BN038229.D</u>
Compound Name	Response	Retention Time
DDT	1521305	20.679
DDD	52158	20.227
DDE	1105	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53263	1574568	3.38

Instrument :
BNA_N
ClientSampleId :
DFTPP