


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112425\
 Data File : VL043277.D
 Acq On : 24 Nov 2025 08:53
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Nov 19 01:11:25 2025

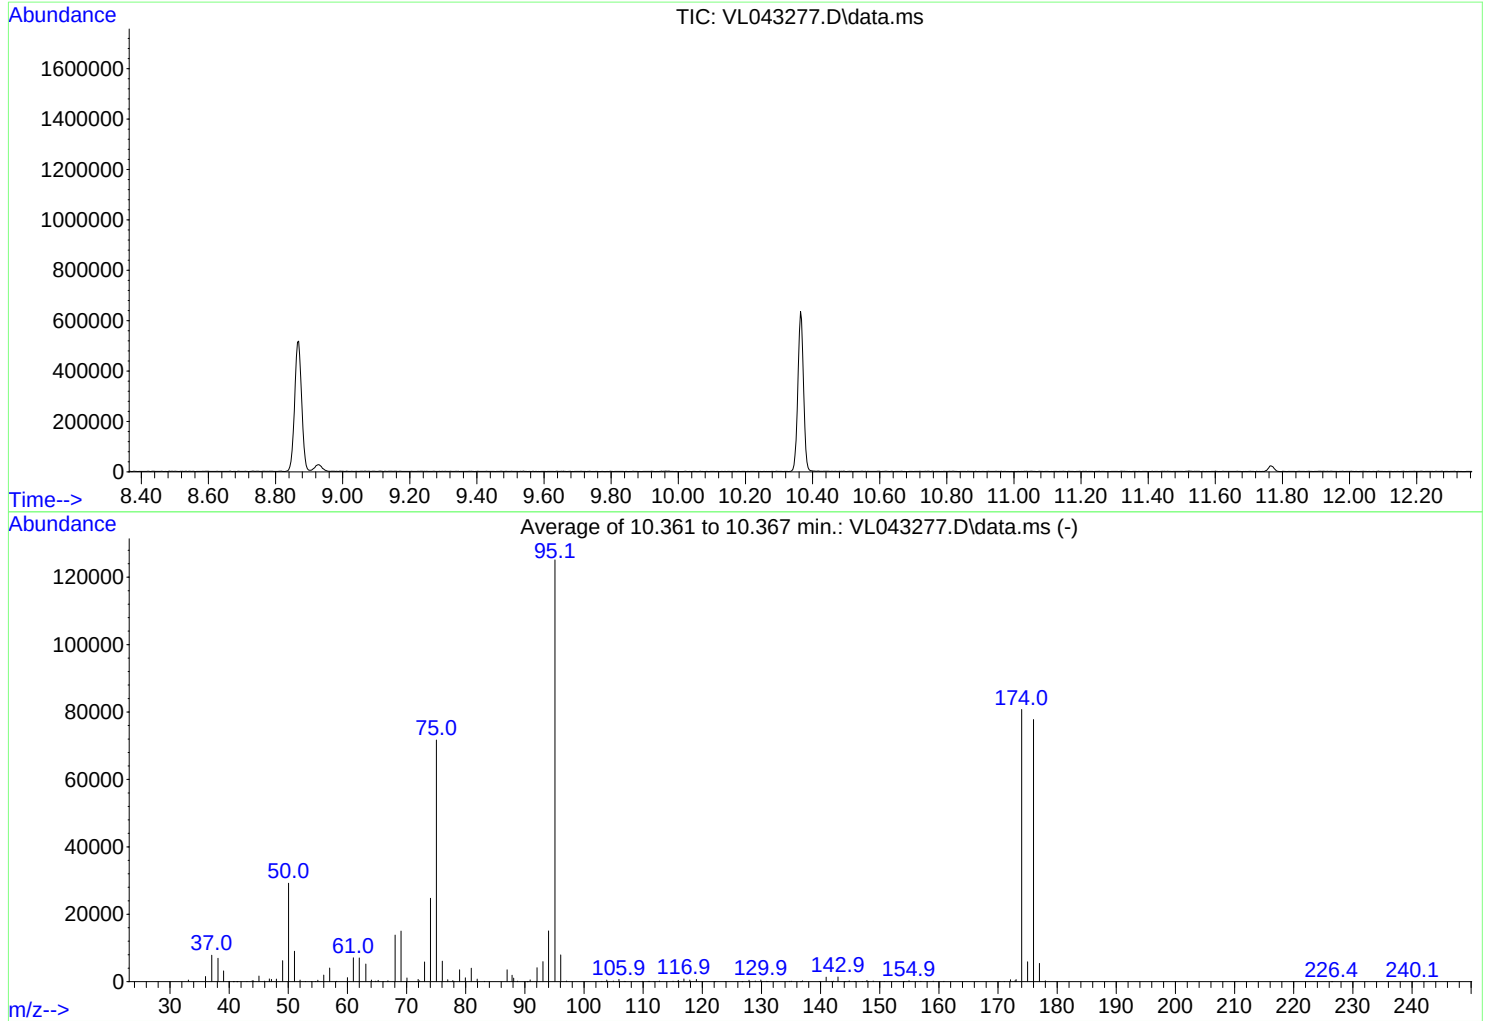

AutoFind: Scans 3174, 3175, 3176; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	29189	PASS
75	95	30	66	57.3	71715	PASS
95	95	100	100	100.0	125165	PASS
96	95	5	9	6.3	7928	PASS
173	174	0.00	2	0.8	642	PASS
174	95	50	120	64.5	80763	PASS
175	174	4	9	7.3	5908	PASS
176	174	93	101	96.3	77795	PASS
177	176	5	9	7.0	5416	PASS

Average of 10.361 to 10.367 min.: VL043277.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	478	45.05	1687	54.60	53	65.20	391
36.00	1507	45.95	136	55.00	422	66.05	51
37.05	7822	46.80	795	56.00	1965	66.85	28
38.10	6940	47.15	681	57.00	4054	68.05	1384
39.05	3202	48.00	783	58.15	117	69.05	14985
40.00	114	49.05	6220	60.00	1197	70.05	1092
40.70	19	50.05	29189	61.00	7095	71.95	679
41.30	25	51.05	9009	62.00	7024	72.20	235
43.00	59	52.00	501	63.10	5229	73.05	5870
43.90	284	52.90	47	64.05	495	74.05	24755
44.10	256	53.90	57	64.80	140	75.05	71715

Average of 10.361 to 10.367 min.: VL043277.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	6065	88.10	1041	103.85	501	115.80	83
76.95	589	88.75	144	104.95	191	115.95	362
77.80	287	90.40	26	105.90	660	116.90	815
78.00	158	90.90	546	106.80	120	117.90	469
78.95	3509	92.05	4129	107.00	77	119.00	667
79.95	1144	93.05	5957	109.85	82	122.00	22
80.95	3978	94.00	15063	110.85	96	123.90	67
81.95	783	95.10	125165	111.10	94	126.70	25
83.15	125	96.05	7928	111.80	72	127.90	444
87.00	3497	97.05	187	112.75	196	128.95	207
87.85	1920	103.00	101	115.05	163	129.90	485

Average of 10.361 to 10.367 min.: VL043277.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.90	113	142.95	1385	154.00	18	174.00	80763
131.10	39	144.00	19	154.95	310	175.00	5908
134.75	104	144.85	217	156.95	120	176.00	77795
135.05	136	145.70	62	158.05	59	177.00	5416
136.60	23	145.90	96	159.05	153	178.00	233
136.95	221	147.05	61	160.85	107	226.40	19
139.80	67	147.85	386	170.30	46	240.10	42
140.00	73	148.10	41	171.05	61		
140.95	1333	148.90	182	172.10	555		
141.85	103	150.05	72	172.90	300		
142.20	139	150.75	68	173.05	642		