


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL112025\
Data File : VL043256.D
Acq On : 20 Nov 2025 08:41
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Nov 19 01:11:25 2025

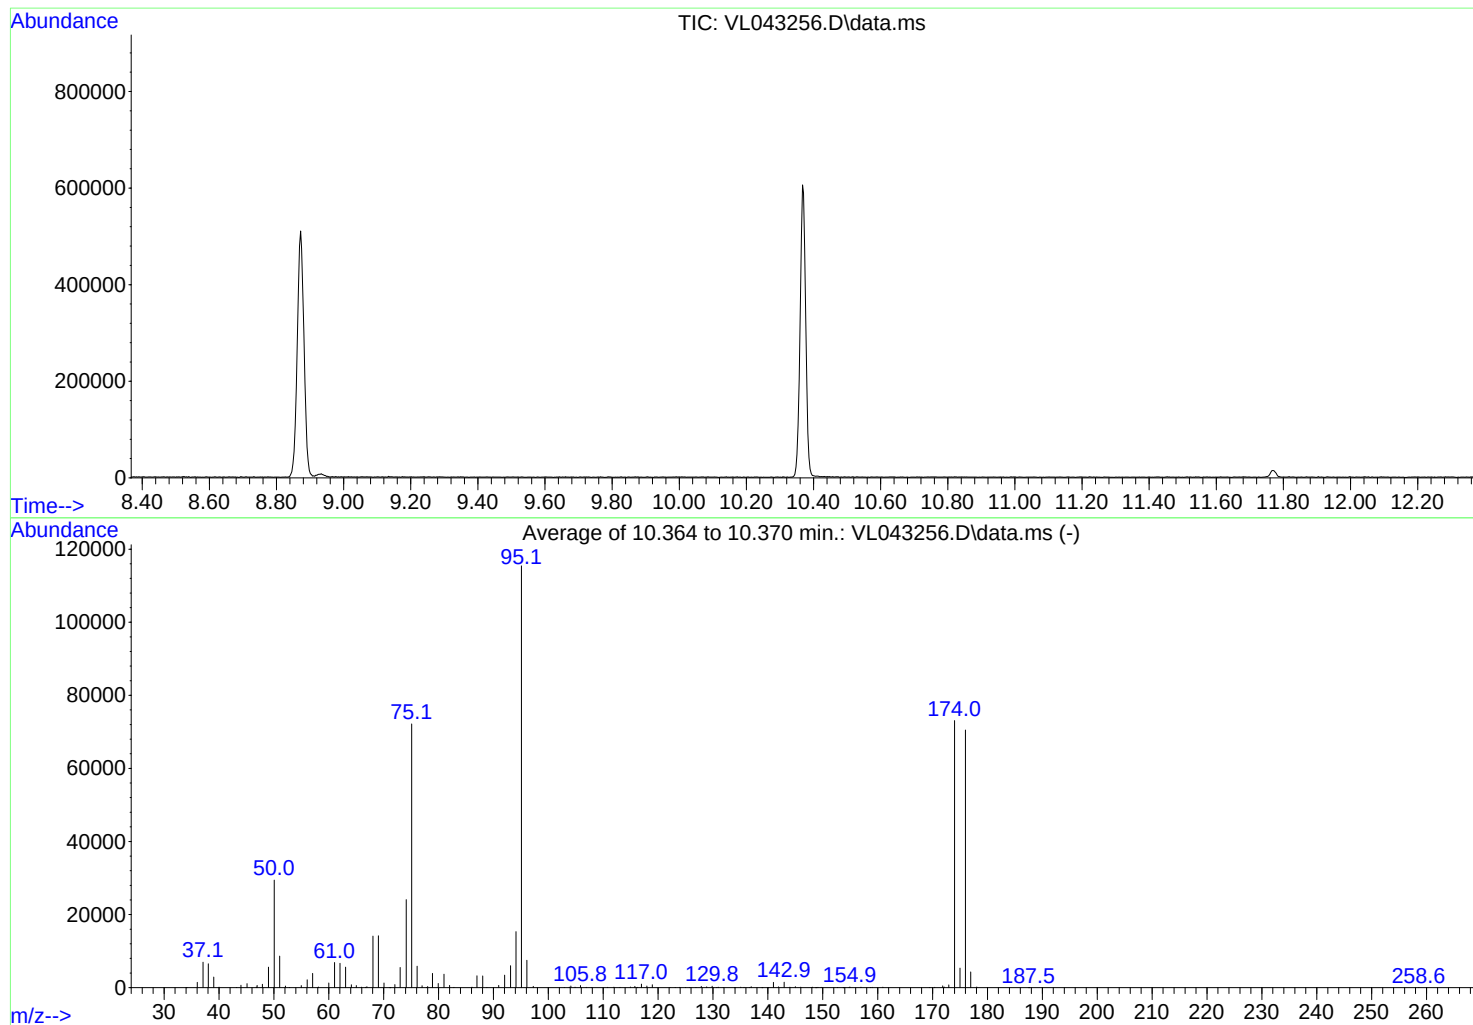

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.5	29432	PASS
75	95	30	66	62.5	72149	PASS
95	95	100	100	100.0	115432	PASS
96	95	5	9	6.5	7511	PASS
173	174	0.00	2	1.0	742	PASS
174	95	50	120	63.3	73064	PASS
175	174	4	9	7.3	5336	PASS
176	174	93	101	96.5	70507	PASS
177	176	5	9	6.1	4312	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
34.00	20	47.90	904	61.05	6896	71.10	1
36.05	1455	49.00	5622	62.05	6671	72.05	83
37.10	6956	50.05	29432	63.05	5612	73.00	550
38.05	6536	51.05	8642	64.10	779	74.10	2409
39.05	2877	52.10	434	65.00	576	75.10	72149
40.00	140	52.85	60	65.95	127	76.10	5882
43.20	31	55.00	567	66.70	81	77.00	535
44.00	643	56.05	2149	66.95	251	77.80	53
45.10	1087	57.05	3886	68.05	14086	78.00	328
46.80	184	58.10	194	69.05	14206	78.90	3882
46.95	633	60.00	1256	70.05	1290	79.95	1138

Average of 10.364 to 10.370 min.: VL043256.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.00	3680	95.10	115432	111.95	122	125.00	44
82.00	630	96.10	7511	113.05	70	125.80	24
82.80	85	97.25	341	114.95	171	126.90	41
86.10	116	102.90	56	115.75	361	127.85	344
87.00	3248	103.80	126	116.20	106	128.85	210
88.05	3213	104.10	445	116.95	947	129.85	378
88.80	64	104.85	112	117.95	441	130.70	55
90.95	600	105.85	595	118.95	769	130.95	123
92.05	3431	106.90	107	122.15	52	131.85	51
93.10	6011	107.80	38	123.10	31	133.90	19
94.10	15340	110.80	70	123.95	107	135.05	146

Average of 10.364 to 10.370 min.: VL043256.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
135.65	73	147.90	53	158.70	55	176.95	4312
136.70	46	148.10	113	159.00	94	178.05	185
136.95	261	148.70	20	160.95	142	187.50	19
138.90	18	149.10	87	169.50	44	258.60	30
140.00	18	149.70	85	170.40	76		
141.00	1471	152.70	26	171.85	502		
141.95	230	153.70	19	172.10	181		
142.95	1510	154.00	44	172.95	742		
144.00	120	154.80	101	174.00	73064		
145.00	268	154.95	163	175.00	5336		
146.00	131	156.95	144	176.00	70507		