
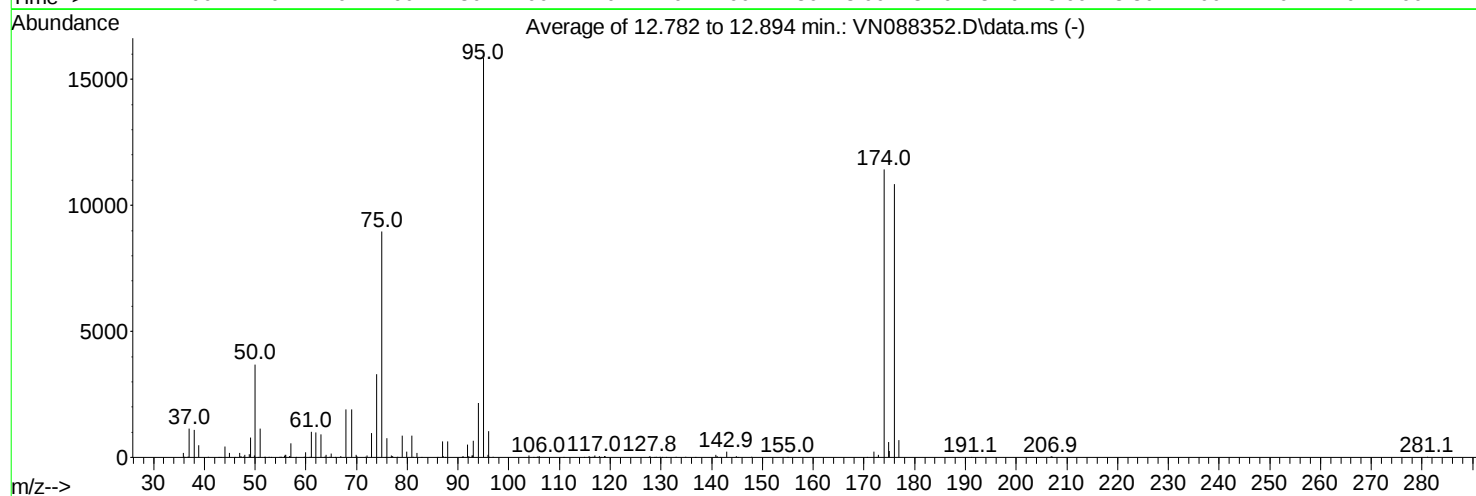


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN112525\  
Data File : VN088352.D  
Acq On : 25 Nov 2025 10:29  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N111325W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Fri Nov 14 00:49:21 2025

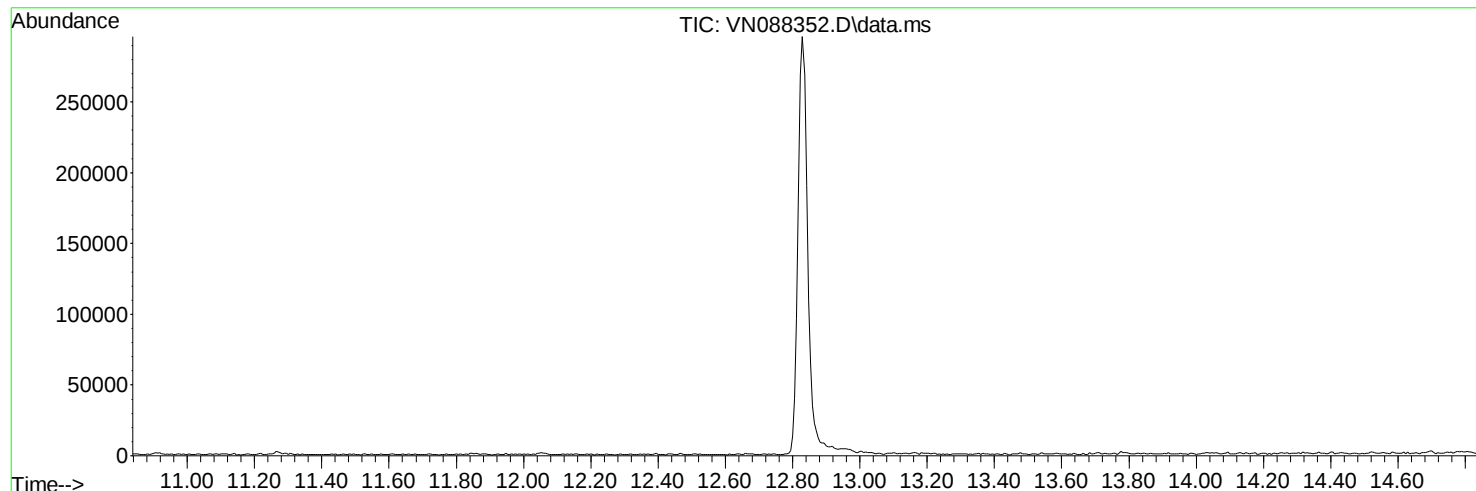

AutoFind: Averaged scan 1841 to 1860; Bkg corrected with scan 1840

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 23.3  | 3688  | PASS      |
| 75     | 95      | 30     | 60     | 56.5  | 8958  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 15841 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 1049  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.0   | 114   | PASS      |
| 174    | 95      | 50     | 100    | 72.1  | 11424 | PASS      |
| 175    | 174     | 5      | 9      | 5.4   | 616   | PASS      |
| 176    | 174     | 95     | 101    | 95.0  | 10852 | FAIL*     |
| 177    | 176     | 5      | 9      | 6.4   | 697   | PASS      |