

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112525\
 Data File : PQ071521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 16:16
 Operator : YP\AJ
 Sample : Q3717-07 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 7A7B7C

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/26/2025
 Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 05:10:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 19 04:02:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	2.854	18505091	20780740	2.126	2.226
2) SA Decachlor...	8.536	7.651	17992392	18842195	2.873m	2.062m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ112525\
Data File : PQ071521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 16:16
Operator : YP\AJ
Sample : Q3717-07 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
7A7B7C


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 05:10:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ111825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 19 04:02:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

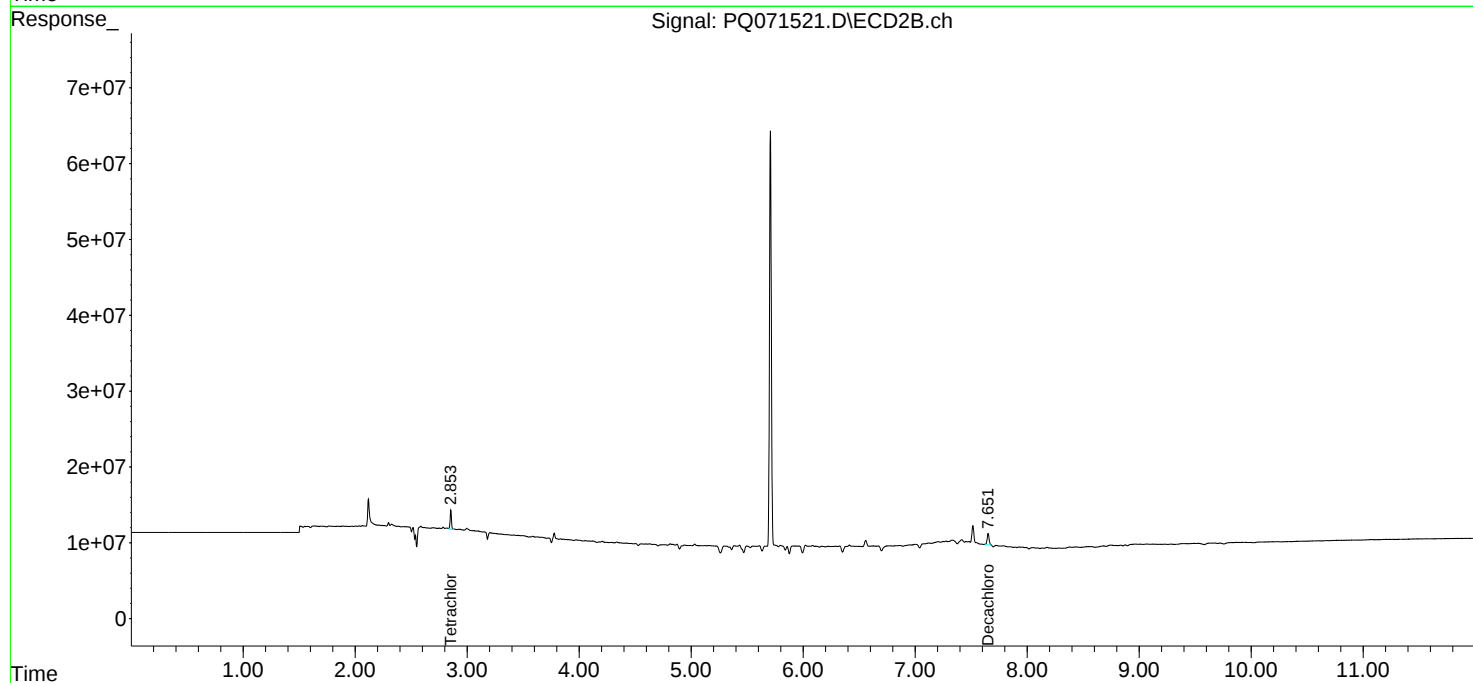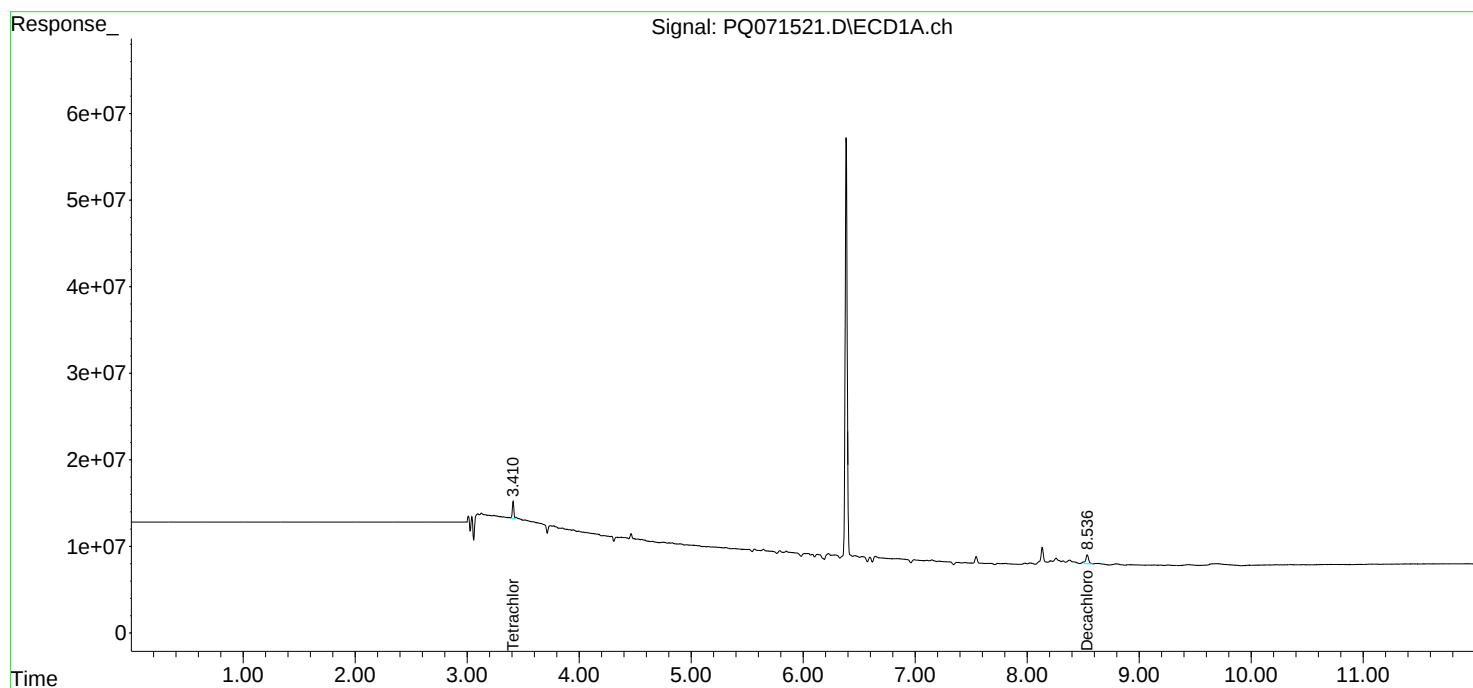

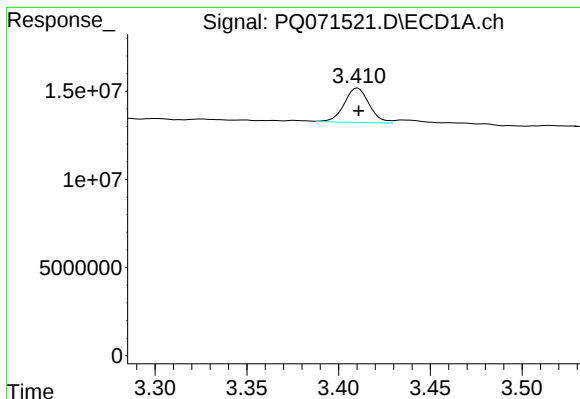


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 18505091
Conc: 2.13 ng/ml

Instrument :
ECD_Q
ClientSampleId :
7A7B7C


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/27/2025

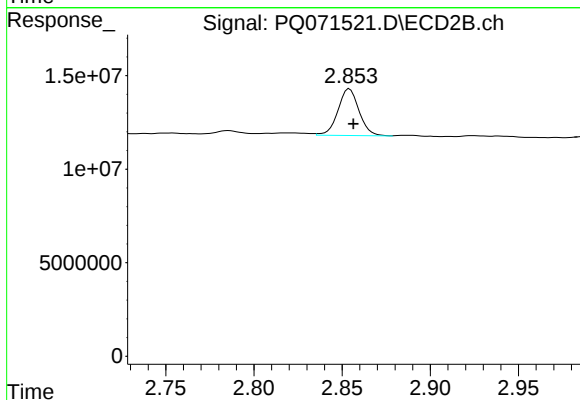


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: -0.002 min
Response: 20780740
Conc: 2.23 ng/ml

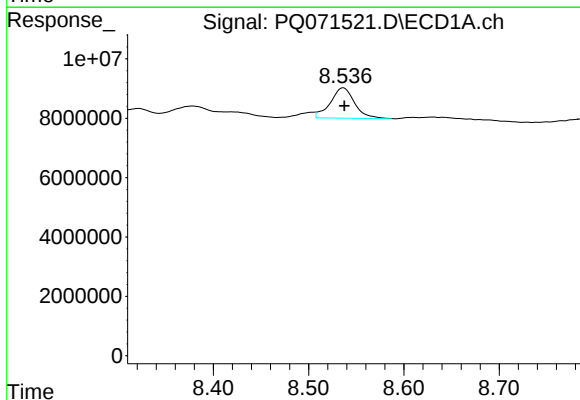

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: -0.002 min
Response: 17992392
Conc: 2.87 ng/ml m

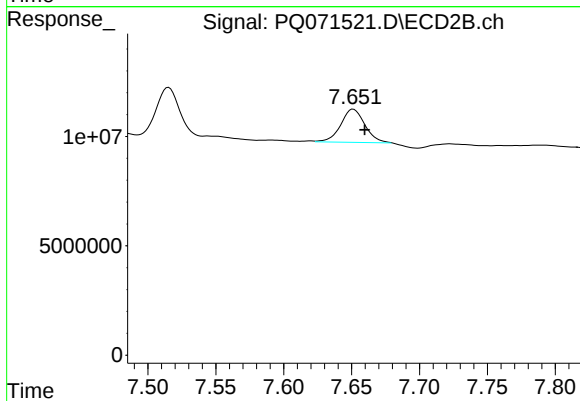

#2 Decachlorobiphenyl

R.T.: 7.651 min
Delta R.T.: -0.009 min
Response: 18842195
Conc: 2.06 ng/ml m