

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112525\
 Data File : VW032530.D
 Acq On : 25 Nov 2025 09:57
 Operator : SY/MD
 Sample : VW1125SBL01
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW1125SBL01

Quant Time: Nov 26 01:37:48 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 11 03:48:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	312940	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	616508	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	570663	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	260746	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	240172	59.529	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	119.060%
35) Dibromofluoromethane	7.898	113	201862	54.688	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	109.380%
50) Toluene-d8	10.325	98	732098	51.700	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	103.400%
62) 4-Bromofluorobenzene	12.617	95	270484	50.564	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	101.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112525\
Data File : VW032530.D
Acq On : 25 Nov 2025 09:57
Operator : SY/MD
Sample : VW1125SBL01
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW1125SBL01

Quant Time: Nov 26 01:37:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 11 03:48:21 2025
Response via : Initial Calibration




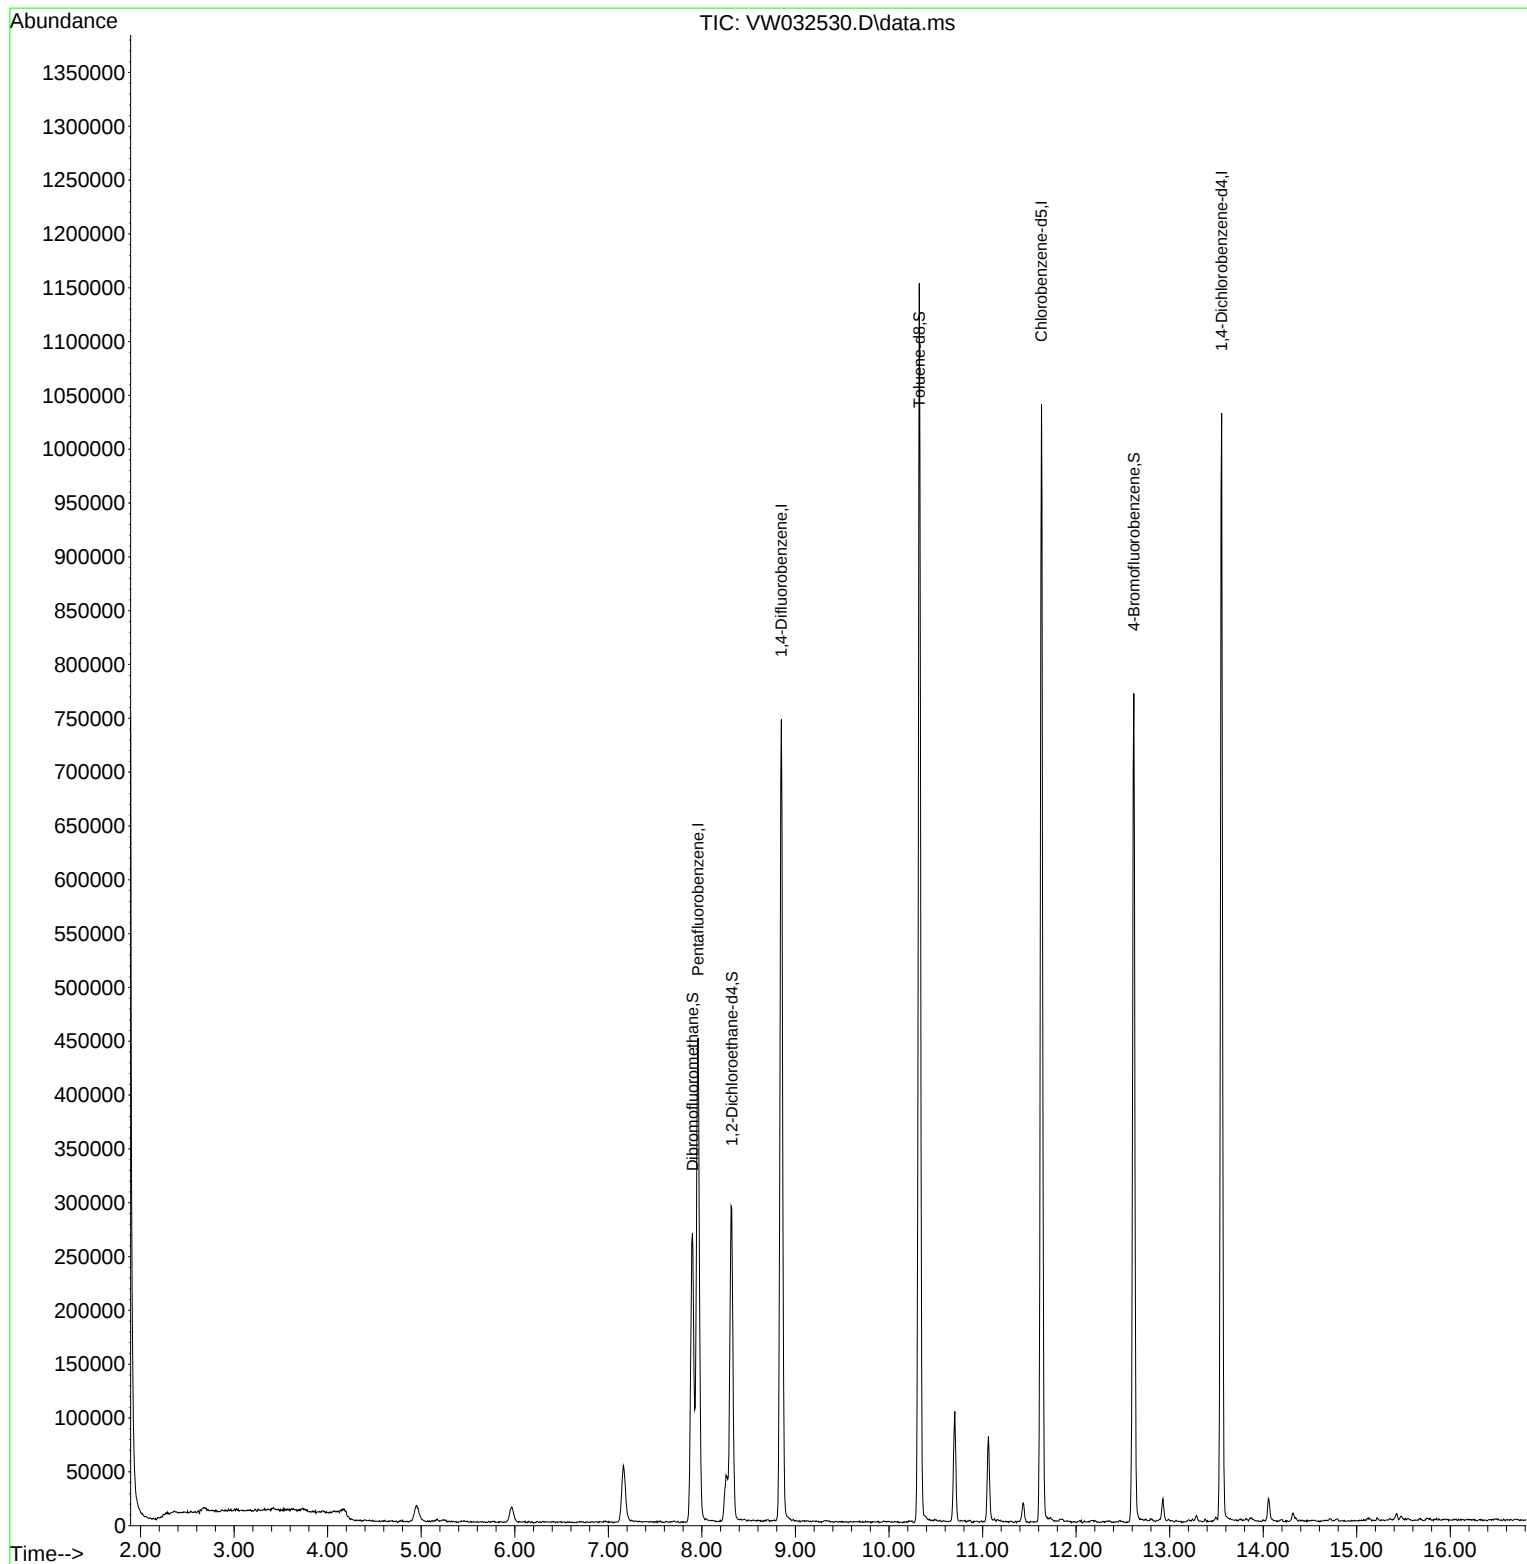


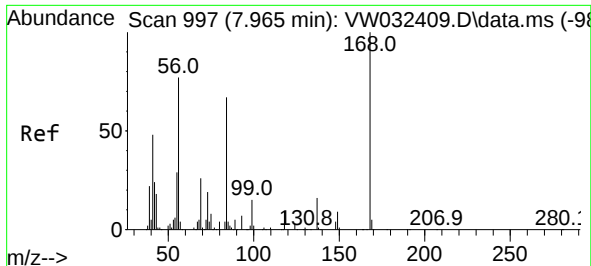

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 99
Delta R.T. -0.006 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57




Instrument :
MSVOA_W
ClientSampleId :
VW1125SBL01


Tgt Ion:168 Resp: 312940
Ion Ratio Lower Upper
168 100
99 65.5 45.4 68.2

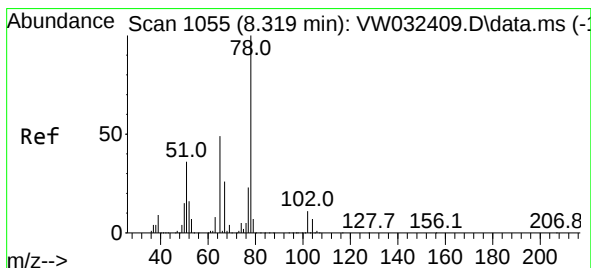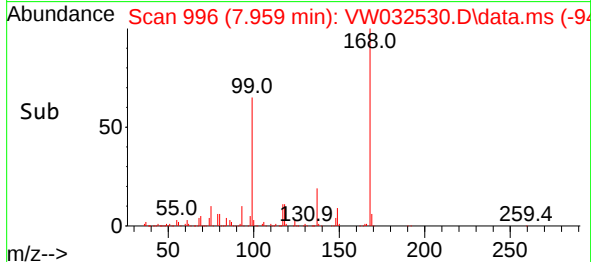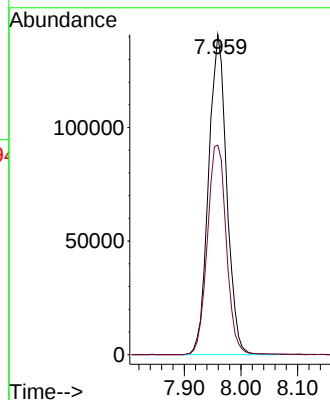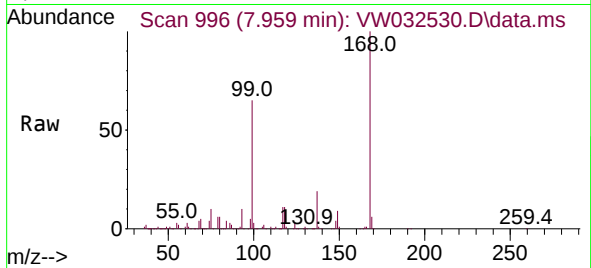

#33
1,2-Dichloroethane-d4
Concen: 59.529 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57

Tgt Ion: 65 Resp: 240172
Ion Ratio Lower Upper
65 100
67 53.4 0.0 106.8

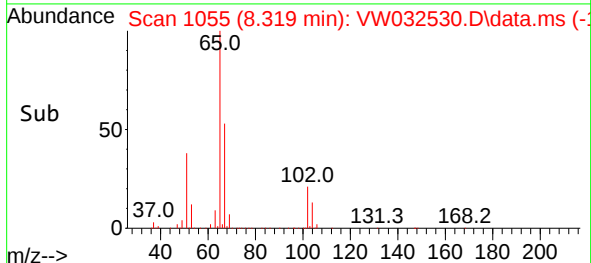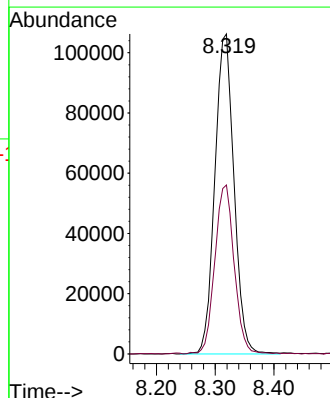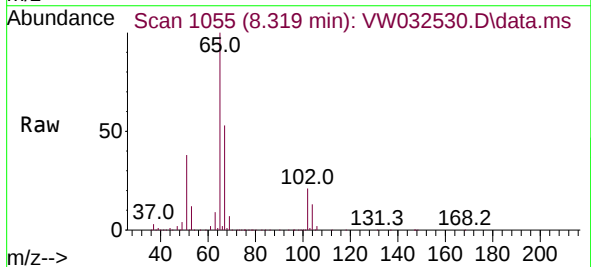

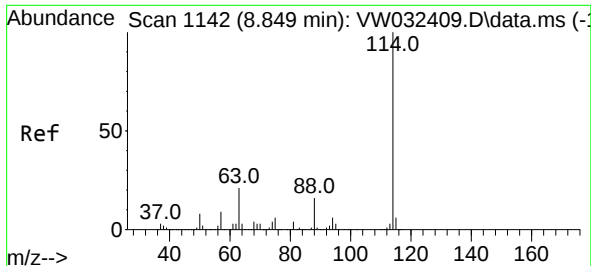

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.849 min Scan# 1142

Delta R.T. 0.000 min

Lab File: VW032530.D

Acq: 25 Nov 2025 09:57

Instrument :

MSVOA_W

ClientSampleId :

VW1125SBL01





Tgt Ion:114 Resp: 616508

Ion Ratio Lower Upper

114 100

63 21.4 0.0 41.8

88 16.2 0.0 32.6

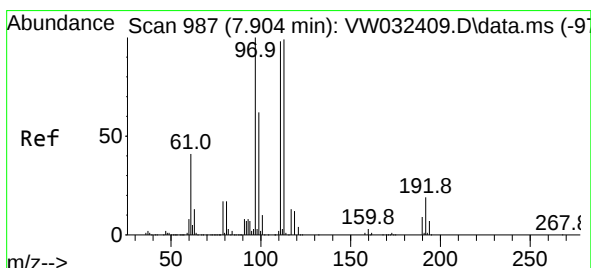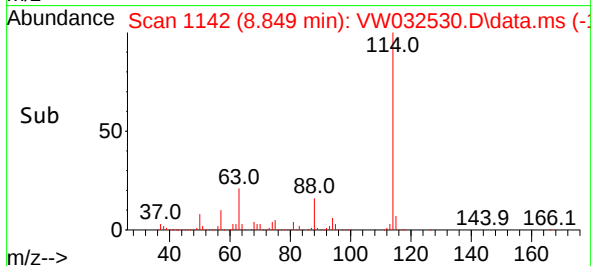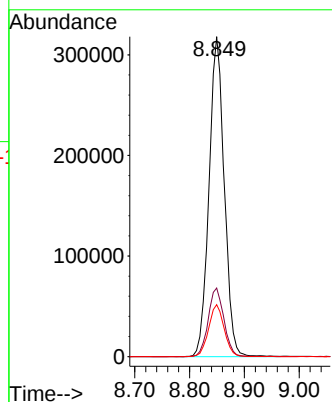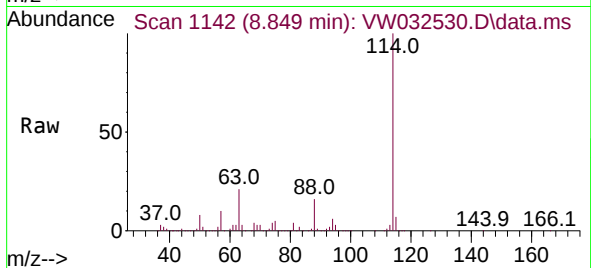

#35

Dibromofluoromethane

Concen: 54.688 ug/l

RT: 7.898 min Scan# 986

Delta R.T. -0.006 min

Lab File: VW032530.D

Acq: 25 Nov 2025 09:57




Tgt Ion:113 Resp: 201862


Ion Ratio Lower Upper

113 100

111 104.4 83.1 124.7

192 16.5 13.4 20.2


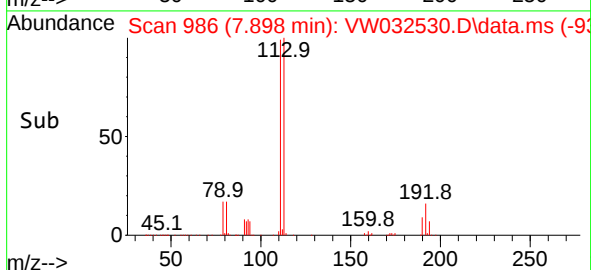
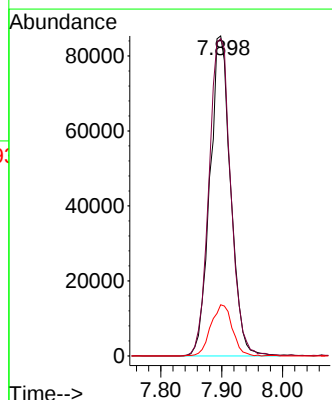
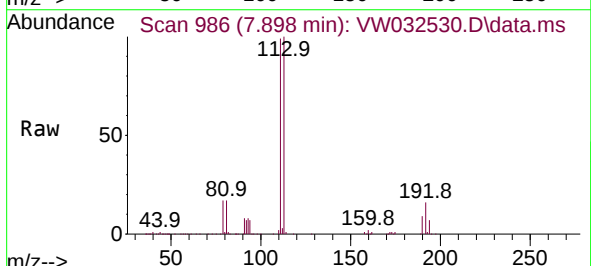


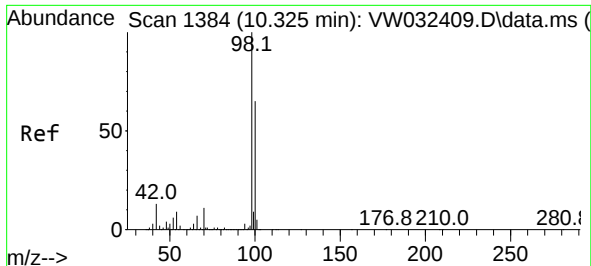

#50
Toluene-d8
Concen: 51.700 ug/l
RT: 10.325 min Scan# 1384
Delta R.T. 0.000 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57




Instrument :
MSVOA_W
ClientSampleId :
VW1125SBL01


Tgt Ion: 98 Resp: 732098
Ion Ratio Lower Upper
98 100
100 67.9 53.3 79.9

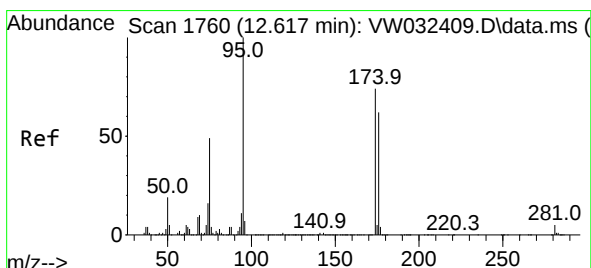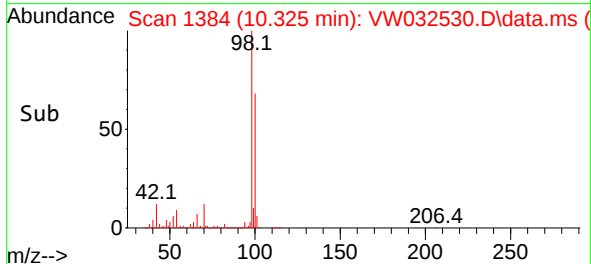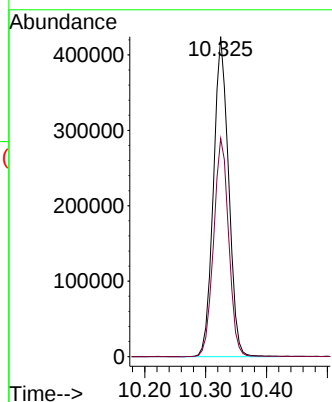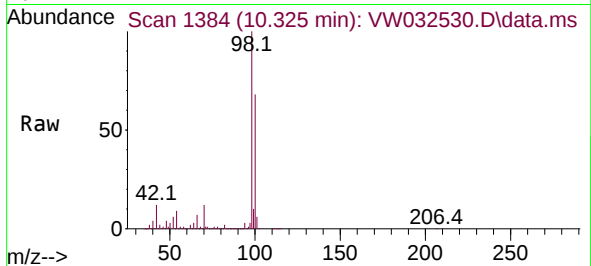

#62
4-Bromofluorobenzene
Concen: 50.564 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57

Tgt Ion: 95 Resp: 270484
Ion Ratio Lower Upper
95 100
174 67.3 0.0 135.4
176 62.9 0.0 131.8


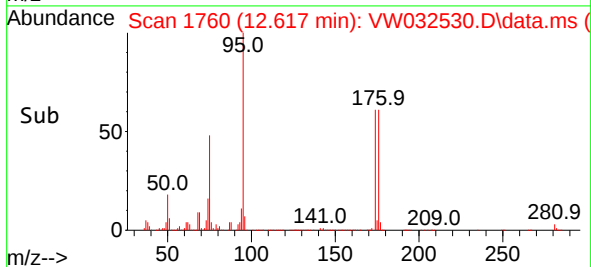
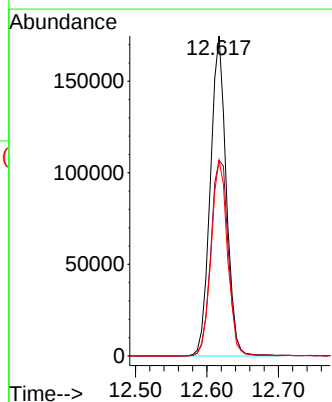
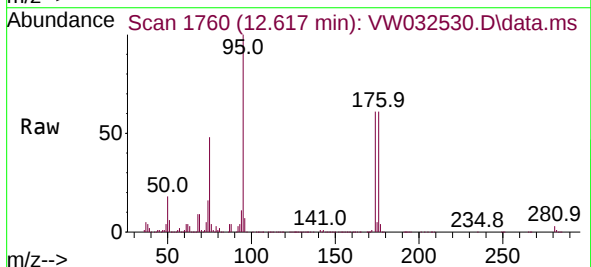


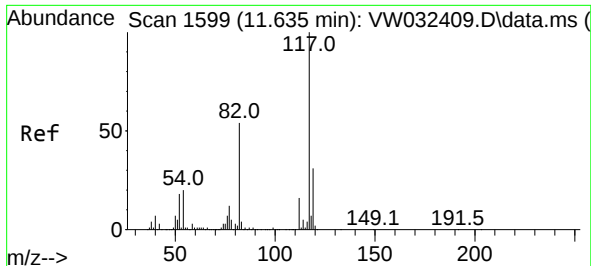

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 11
Delta R.T. -0.006 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57

Instrument :
MSVOA_W
ClientSampleId :
VW1125SBL01

Tgt Ion:117 Resp: 570663
Ion Ratio Lower Upper
117 100
82 62.6 43.0 64.4
119 34.4 25.0 37.6

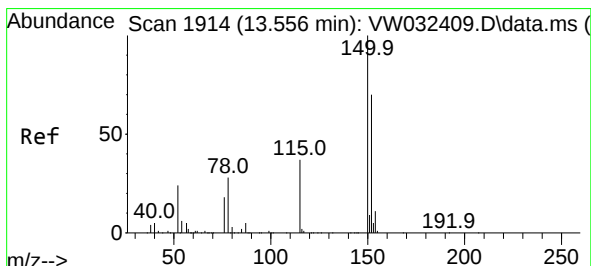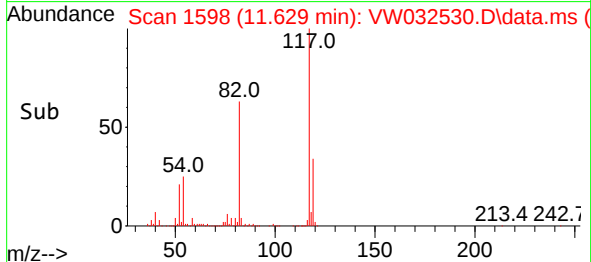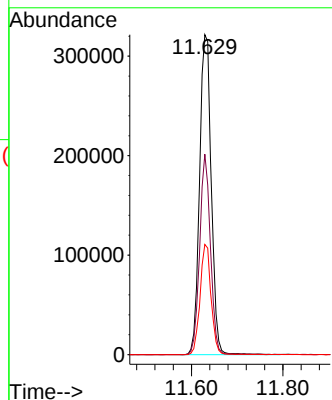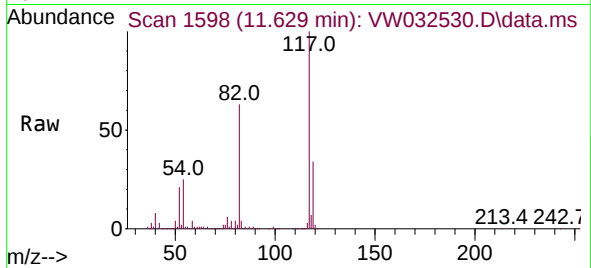

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. 0.000 min
Lab File: VW032530.D
Acq: 25 Nov 2025 09:57

Tgt Ion:152 Resp: 260746
Ion Ratio Lower Upper
152 100
115 62.9 32.8 98.3
150 157.3 0.0 356.6

