


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120125\
Data File : BF144381.D
Acq On : 01 Dec 2025 12:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

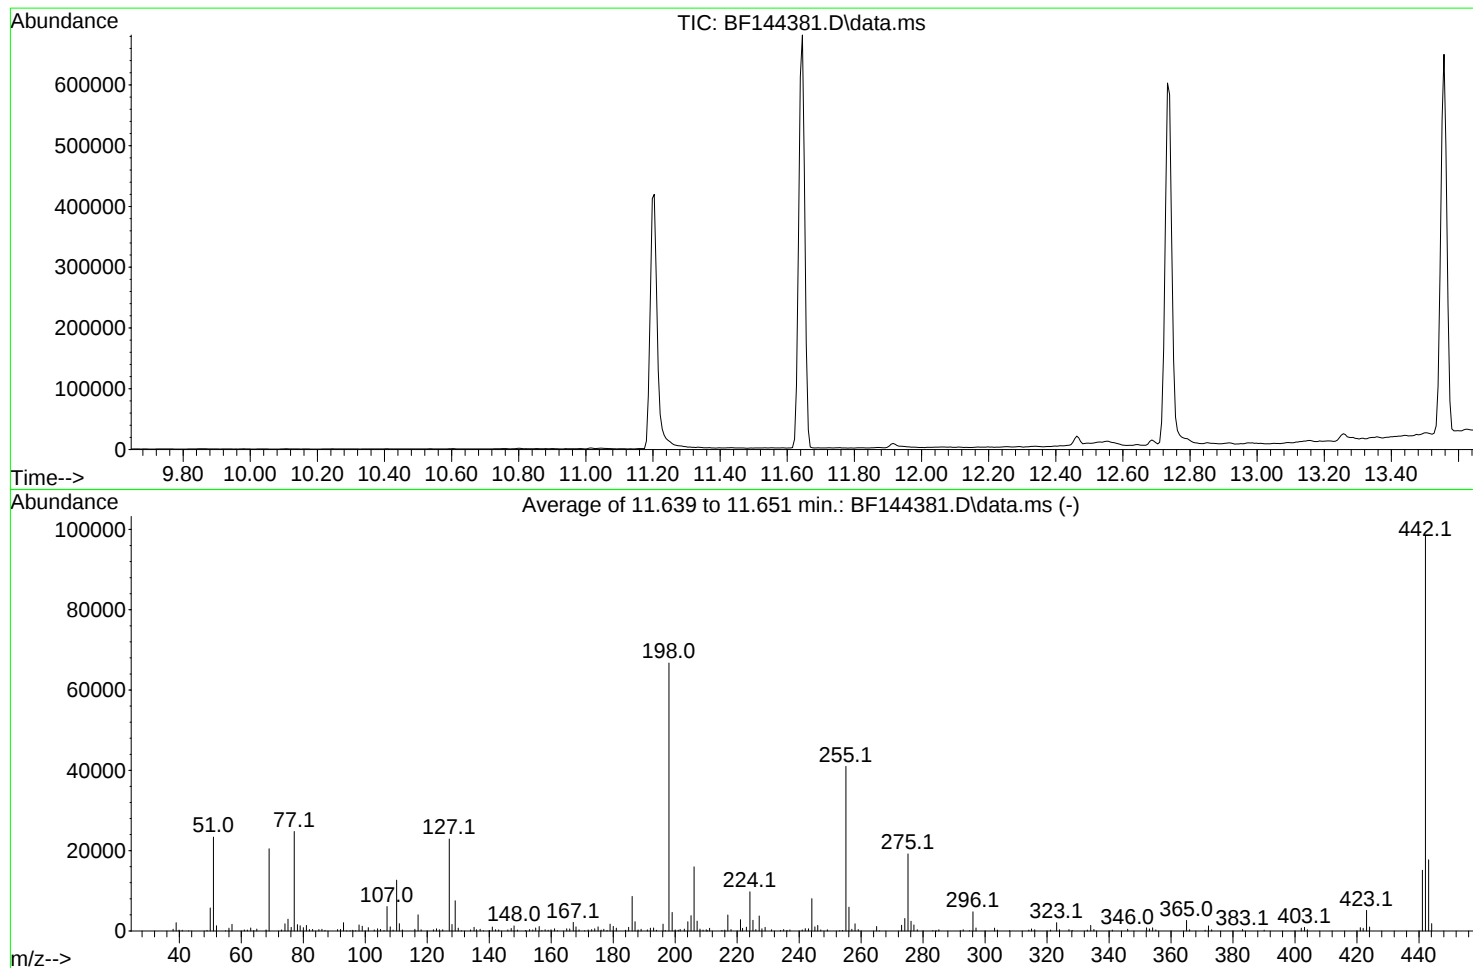




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	251	PASS
69	69	100	100	100.0	20457	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	141	PASS
198	198	100	100	100.0	66749	PASS
199	198	5	9	6.9	4598	PASS
365	198	1	100	3.9	2605	PASS
441	443	0.01	150	85.4	15120	PASS
442	442	100	100	100.0	98347	PASS
443	442	15	24	18.0	17705	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120125\
Data File : BF144381.D
Acq On : 01 Dec 2025 12:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 01 13:16:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

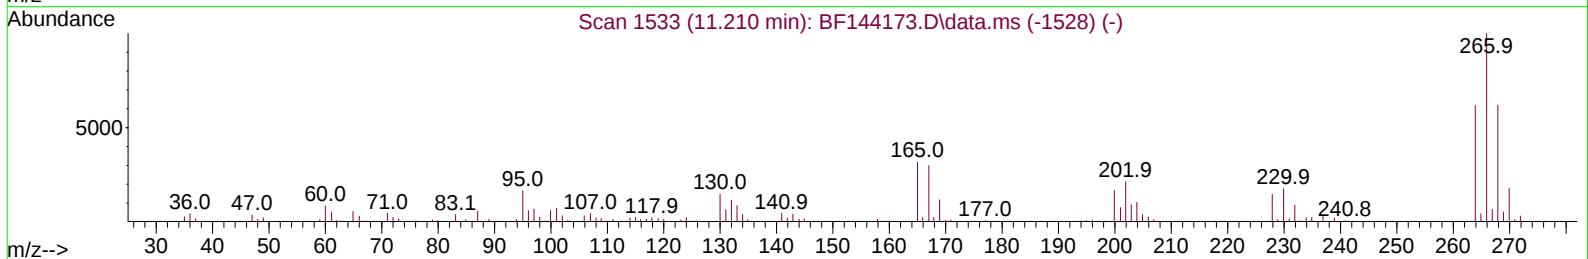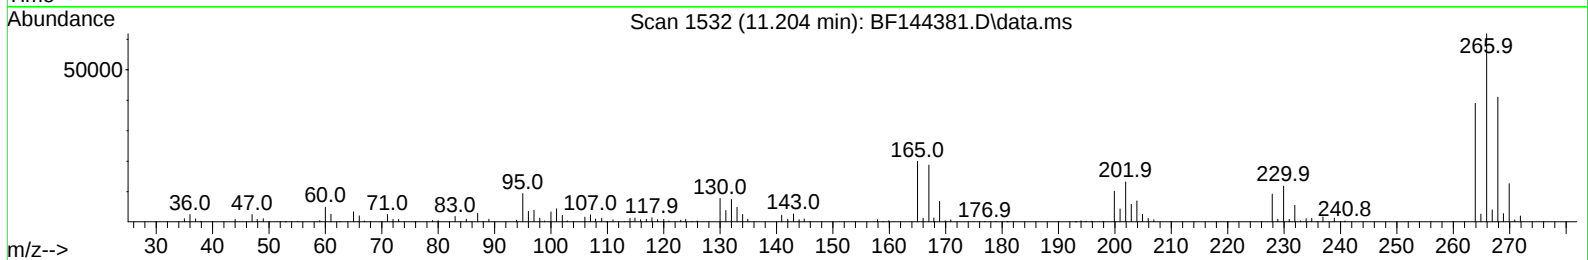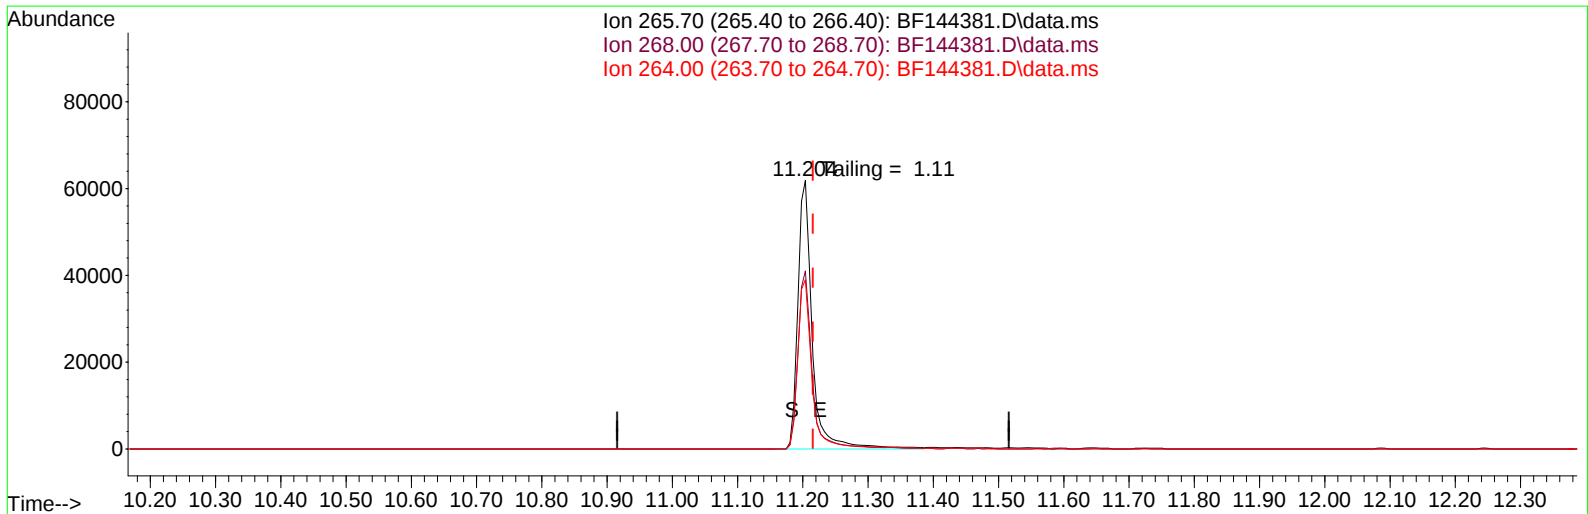

TIC: BF144381.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 40255.49 ng




response 94933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	66.35
264.00	61.80	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120125\
Data File : BF144381.D
Acq On : 01 Dec 2025 12:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 01 13:16:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

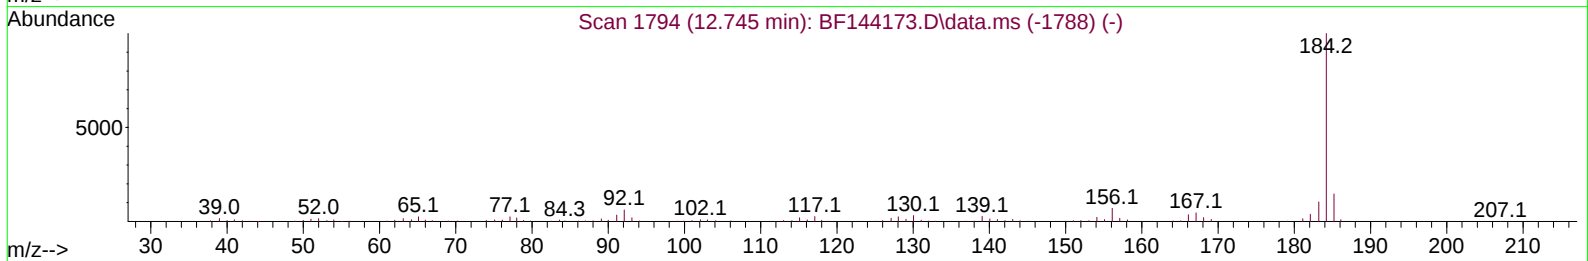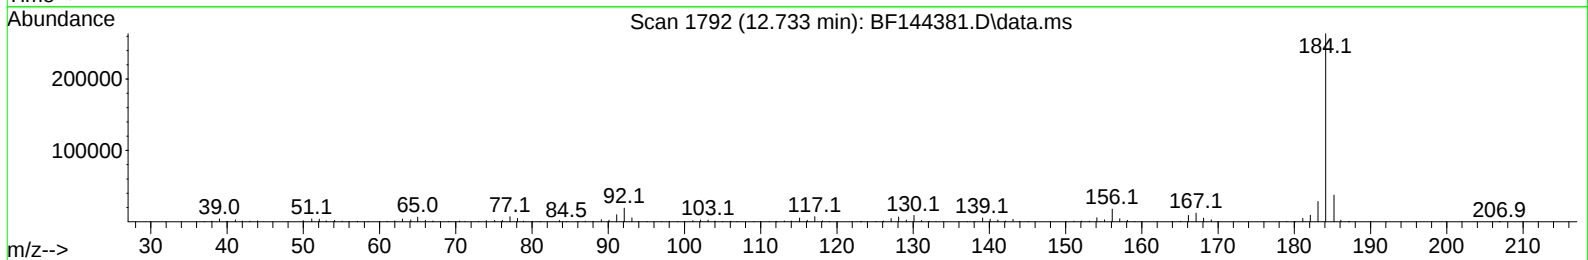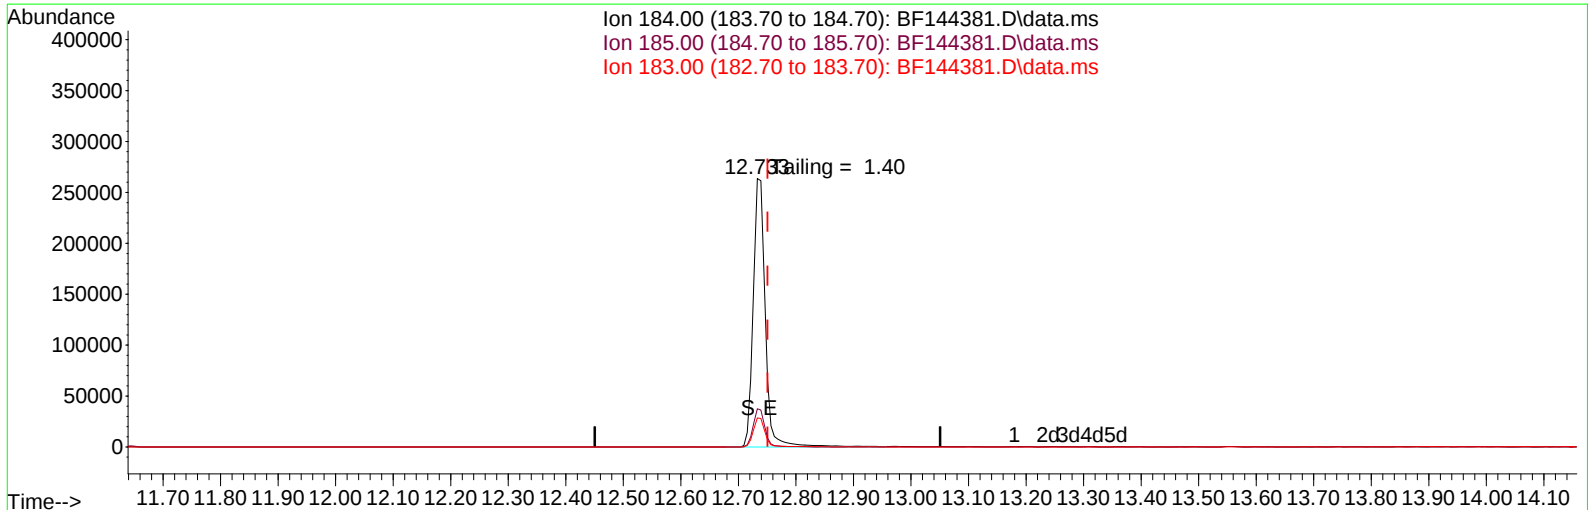

TIC: BF144381.D\data.ms

(77) Benzidine

12.733min (-0.018) 33019.21 ng m

response 387744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	10.40	10.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2025	BNA_F	<u>BF144381.D</u>
Compound Name	Response	Retention Time
DDT	172723	13.557
DDD	4880	13.257
DDE	463	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5343	178066	3.00

Instrument :
BNA_F
ClientSampleId :
DFTPP