
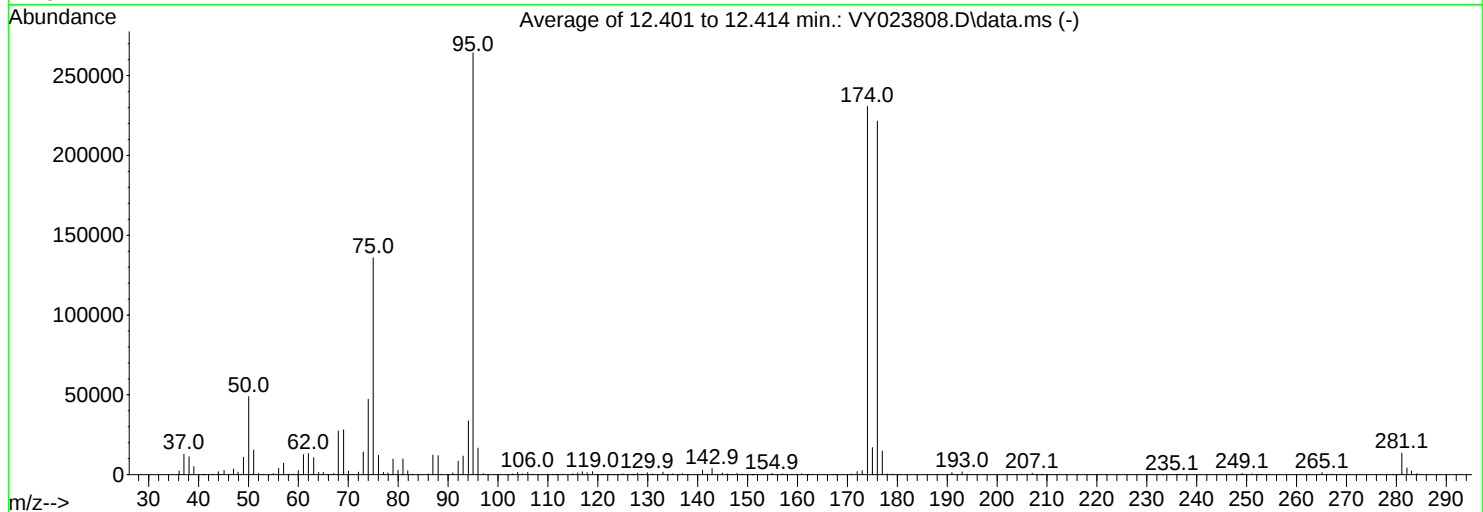


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112625\
Data File : VY023808.D
Acq On : 26 Nov 2025 07:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y112625S.M
Title : SW846 8260
Last Update : Thu Nov 27 01:14:36 2025

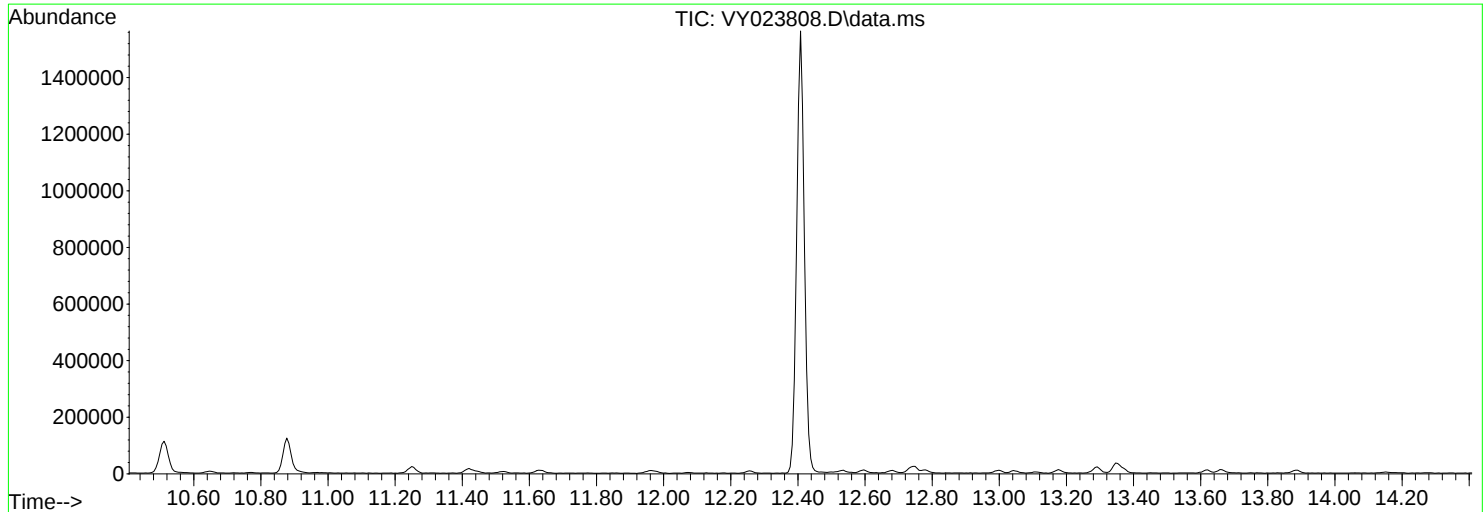

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	48904	PASS
75	95	30	60	51.4	135885	PASS
95	95	100	100	100.0	264277	PASS
96	95	5	9	6.3	16621	PASS
173	174	0.00	2	1.1	2509	PASS
174	95	50	100	87.3	230763	PASS
175	174	5	9	7.4	16984	PASS
176	174	95	101	96.0	221461	PASS
177	176	5	9	6.6	14721	PASS