


Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial v	Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 15:58	10	RM/IZ
STD2	0.417	0.655	0.659	2.182	0.549	0.953	3.345	IC1-110325	11/3/2025 16:22	10	RM/IZ
STD3	0.813	1.228	1.228	4.086	1.024	2.097	6.147	IC1-110325	11/3/2025 17:04	10	RM/IZ
STD4	1.014	1.491	1.496	4.984	1.245	2.506	7.444	IC1-110325	11/3/2025 17:47	10	RM/IZ
STD5	1.966	2.918	2.907	9.724	2.426	5.166	14.580	IC1-110325	11/3/2025 18:08	10	RM/IZ
STD6	3.912	5.914	5.907	19.694	4.918	9.286	29.234	IC1-110325	11/3/2025 18:30	10	RM/IZ
STD7	5.078	7.595	7.603	25.330	6.339	12.992	37.751	IC1-110325	11/3/2025 18:51	10	RM/IZ
ICV	1.960	2.885	2.908	9.698	2.364	5.176	14.547	IC1-110325	11/3/2025 19:13	10	RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 19:34	10	RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/26/2025 9:35	10	RM/IZ
LB138070BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/26/2025 9:57	10	RM/IZ
LB138070BSW	2.086	3.100	3.107	10.443	2.548	5.018	15.425	IC1-110325	11/26/2025 10:18	10	RM/IZ
Q3728-01	0.000	7.993	0.000	0.000	0.100	0.000	2.505	IC1-110325	11/26/2025 13:10	10	RM/IZ
Q3728-01MS	2.057	10.811	2.933	9.817	2.421	4.713	16.545	IC1-110325	11/26/2025 13:31	10	RM/IZ
Q3728-01MSD	1.831	10.613	2.817	9.397	2.324	4.377	16.097	IC1-110325	11/26/2025 13:53	10	RM/IZ
Q3734-01	0.516	157.927	0.098	0.000	0.204	0.000	32.040	IC1-110325	11/26/2025 14:58	10	RM/IZ
Q3734-02	0.200	17.273	0.107	0.000	0.202	0.000	28.222	IC1-110325	11/26/2025 15:19	10	RM/IZ
CCV	2.075	3.092	3.118	10.412	2.539	5.108	15.376	IC1-110325	11/26/2025 15:41	10	RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/26/2025 16:02	10	RM/IZ

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-110325	11/3/2025 15:58	10	RM/IZ
STD2	0.4170	0.6550	0.6590	2.1820	0.5490	0.9530	3.3450	IC1-110325	11/3/2025 16:22	10	RM/IZ
STD3	0.8130	1.2280	1.2280	4.0860	1.0240	2.0970	6.1470	IC1-110325	11/3/2025 17:04	10	RM/IZ
STD4	1.0140	1.4910	1.4960	4.9840	1.2450	2.5060	7.4440	IC1-110325	11/3/2025 17:47	10	RM/IZ
STD5	1.9660	2.9180	2.9070	9.7240	2.4260	5.1660	14.5800	IC1-110325	11/3/2025 18:08	10	RM/IZ
STD6	3.9120	5.9140	5.9070	19.6940	4.9180	9.2860	29.2340	IC1-110325	11/3/2025 18:30	10	RM/IZ
STD7	5.0780	7.5950	7.6030	25.3300	6.3390	12.9920	37.7510	IC1-110325	11/3/2025 18:51	10	RM/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1	4.2500	9.1667	9.8333	9.1000	9.8000	-4.7000	11.5000				
STD2	1.6250	2.3333	2.3333	2.1500	2.4000	4.8500	2.4500				
STD3	1.4000	-0.6000	-0.2667	-0.3200	-0.4000	0.2400	-0.7467				
STD4	-1.7000	-2.7333	-3.1000	-2.7600	-2.9600	3.3200	-2.8000				
STD5	-2.2000	-1.4333	-1.5500	-1.5300	-1.6400	-7.1400	-2.5533				
STD6	1.5600	1.2667	1.3733	1.3200	1.4240	3.9360	2.0297				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

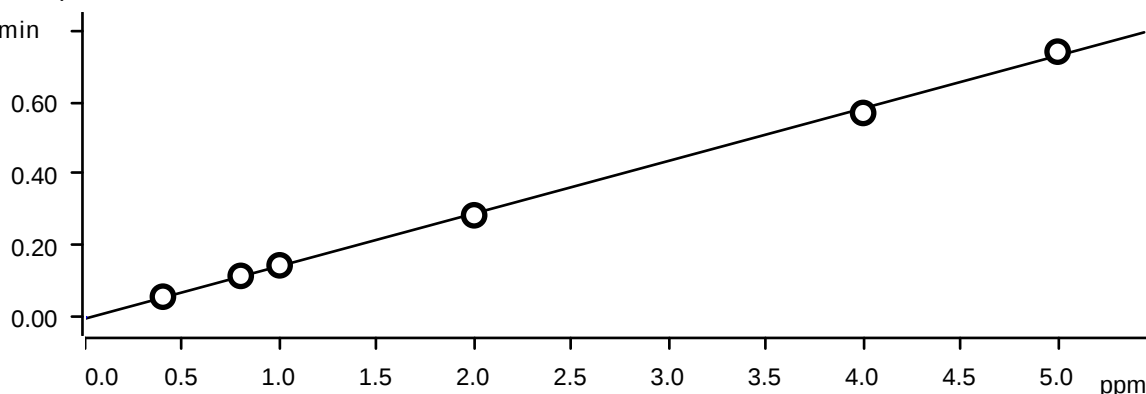

Function: $A = -3.63197E-3 + 0.0146595 \times Q$


Relative standard deviation 2.880512 %

Correlation coefficient 0.999558

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.116	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.145	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.285	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.570	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.741	STD7	2025-11-03 18:51:52 UTC-5	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

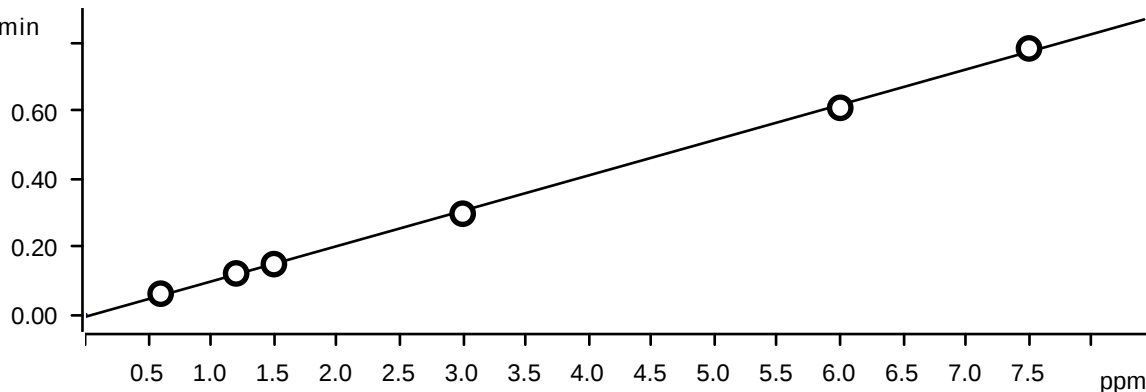


Function: $A = -7.14286E-3 + 0.0104011 \times Q$

Relative standard deviation 2.544562 %

Correlation coefficient 0.999662

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.061	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.148	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.296	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.608	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.783	STD7	2025-11-03 18:51:52 UTC-5	used

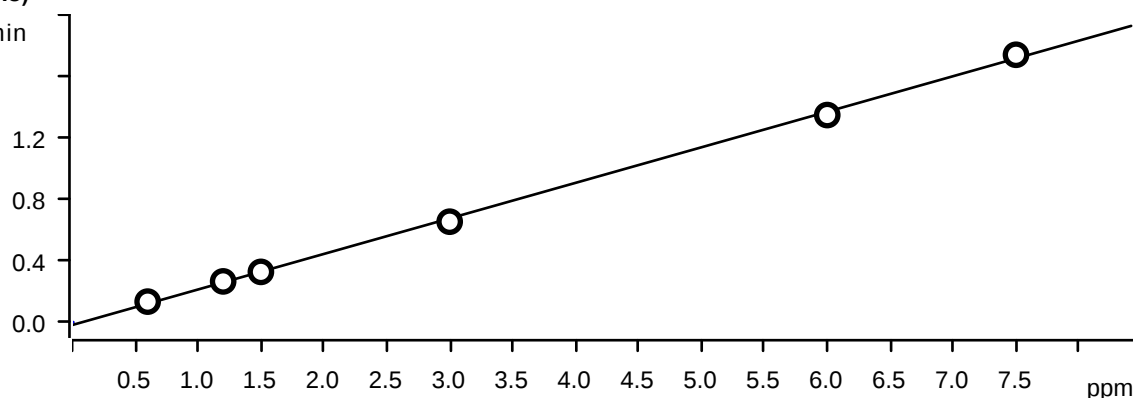Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0188106 + 0.0231263 \times Q$


Relative standard deviation 2.785229 %

Correlation coefficient 0.999598

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.134	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.265	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.654	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.347	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.740	STD7	2025-11-03 18:51:52 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

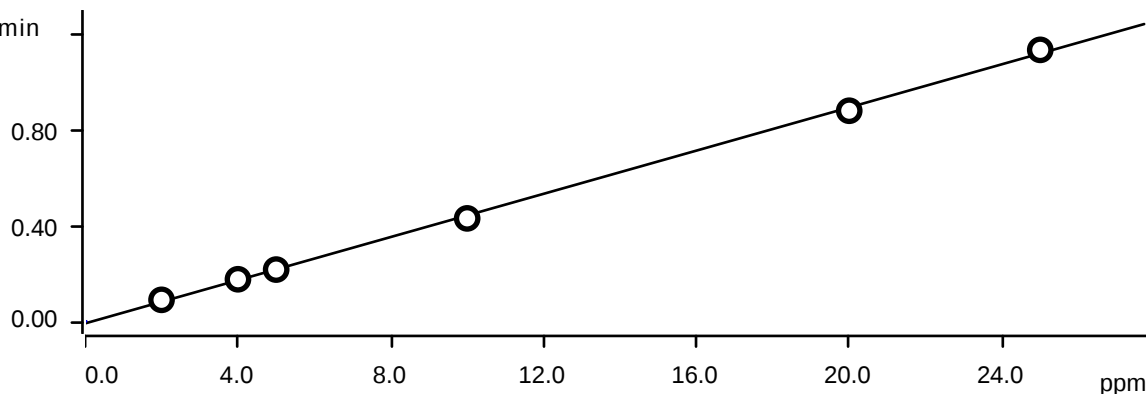

Function: $A = -8.73633E-3 + 4.51609E-3 \times Q$


Relative standard deviation: 2.618377 %

Correlation coefficient: 0.999640

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.090	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.176	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.216	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.430	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.881	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.135	STD7	2025-11-03 18:51:52 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

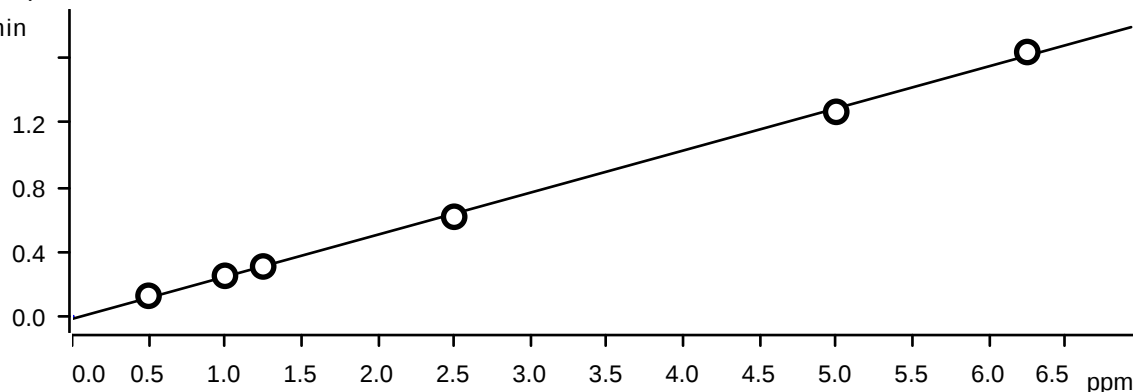


Function: $A = -0.0164240 + 0.0260850 \times Q$

Relative standard deviation: 2.824357 %

Correlation coefficient 0.999585

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.127	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.251	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.308	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.616	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.266	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.637	STD7	2025-11-03 18:51:52 UTC-5	used

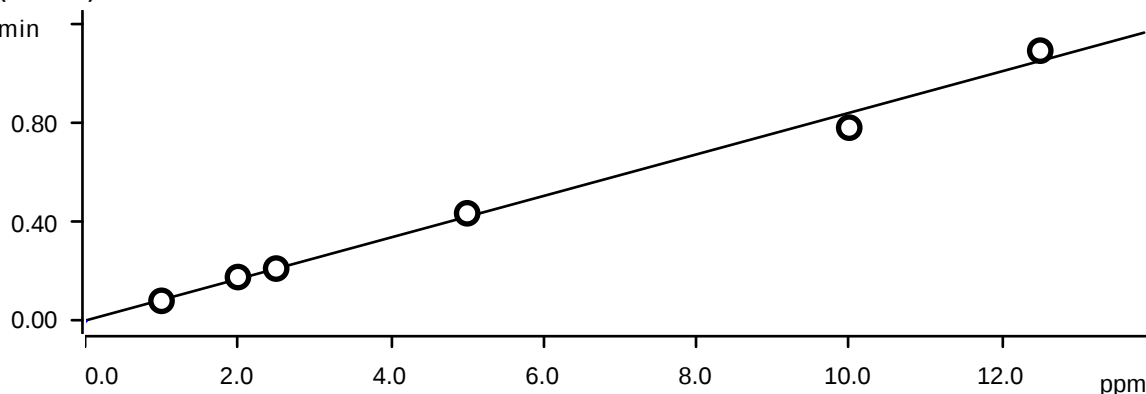
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = 1.95294E-3 + 8.36815E-3 \times Q$

Relative standard deviation 8.053642 %

Correlation coefficient 0.996454

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.212	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.434	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.779	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.089	STD7	2025-11-03 18:51:52 UTC-5	used

Sulfate (Anions)

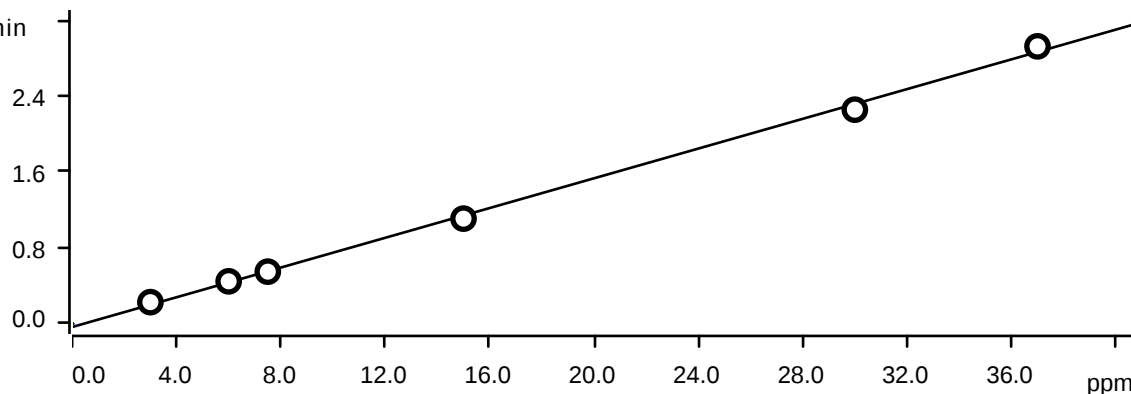 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0341972 + 7.83080E-3 \times Q$

Relative standard deviation 3.795793 %

Correlation coefficient 0.999249


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.228	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.447	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.549	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.108	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.255	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.922	STD7	2025-11-03 18:51:52 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-11-03 15:58:57 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

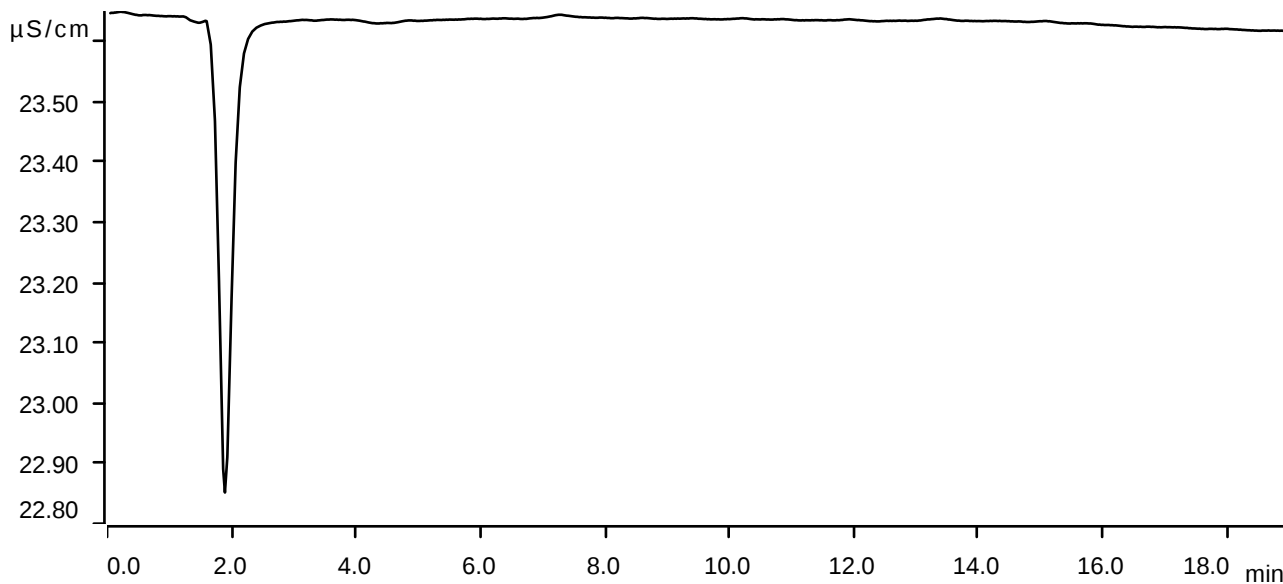Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-11-03 16:22:03 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

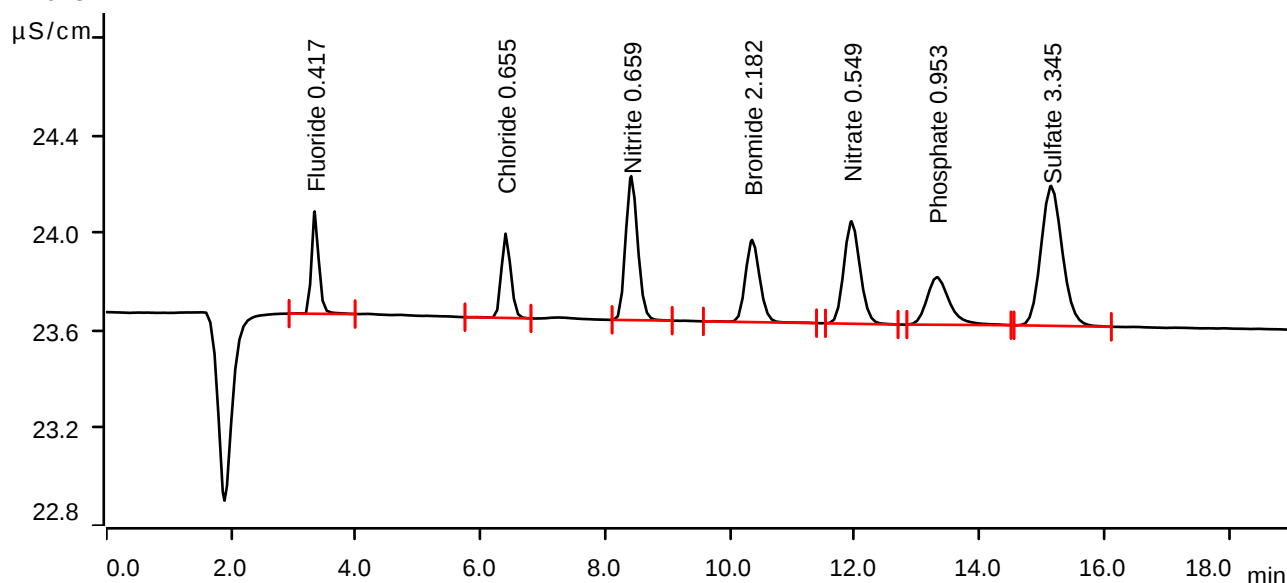

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.0576	0.420	0.417	Fluoride
2	6.402	0.0609	0.345	0.655	Chloride
3	8.415	0.1336	0.590	0.659	Nitrite
4	10.353	0.0898	0.337	2.182	Bromide
5	11.947	0.1268	0.420	0.549	Nitrate
6	13.317	0.0817	0.195	0.953	Phosphate
7	15.147	0.2277	0.574	3.345	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-11-03 17:04:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

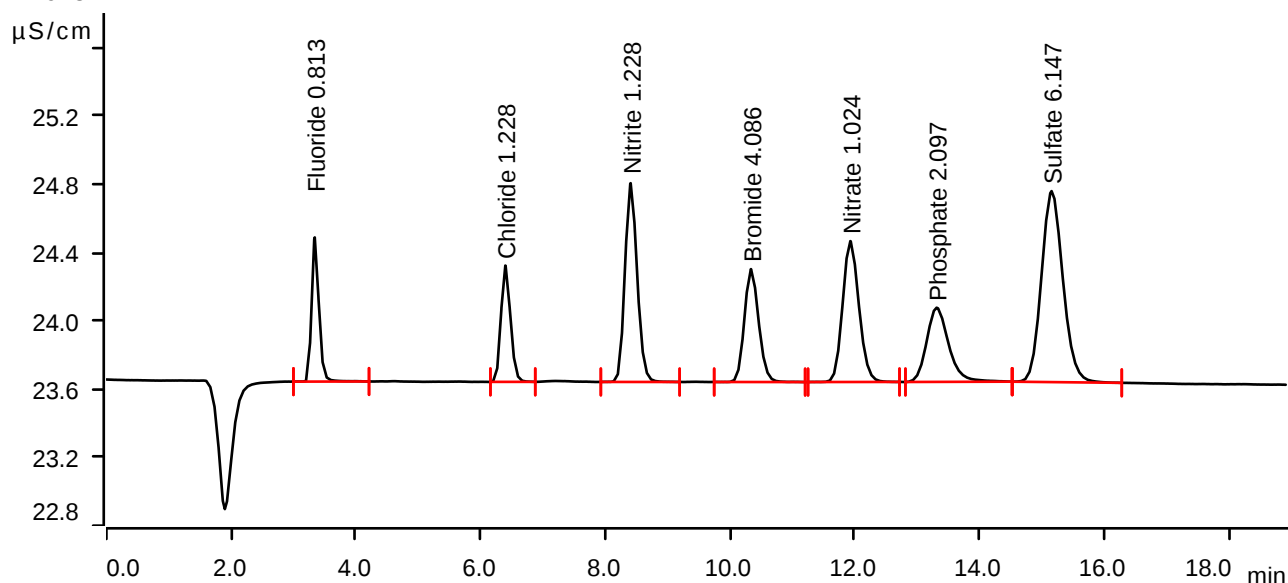

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.1156	0.844	0.813	Fluoride
2	6.397	0.1206	0.681	1.228	Chloride
3	8.407	0.2651	1.164	1.228	Nitrite
4	10.337	0.1758	0.661	4.086	Bromide
5	11.928	0.2506	0.825	1.024	Nitrate
6	13.312	0.1774	0.435	2.097	Phosphate
7	15.155	0.4471	1.119	6.147	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-11-03 17:47:32 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

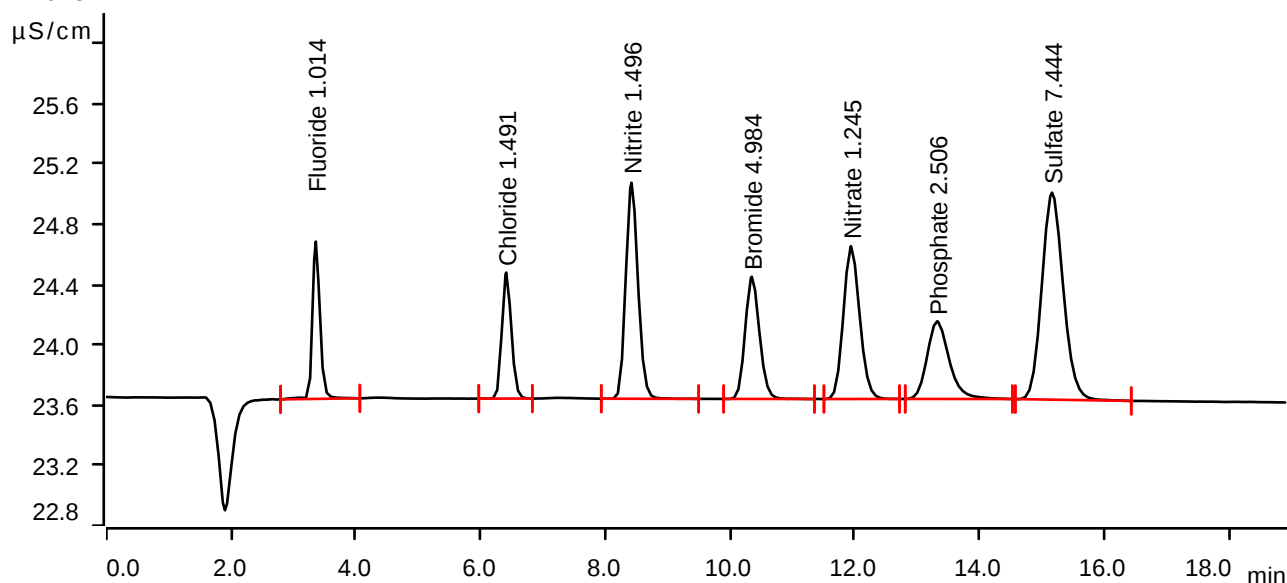

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.1450	1.044	1.014	Fluoride
2	6.412	0.1479	0.837	1.491	Chloride
3	8.420	0.3271	1.434	1.496	Nitrite
4	10.348	0.2164	0.811	4.984	Bromide
5	11.940	0.3084	1.014	1.245	Nitrate
6	13.320	0.2117	0.516	2.506	Phosphate
7	15.162	0.5487	1.374	7.444	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-11-03 18:08:59 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

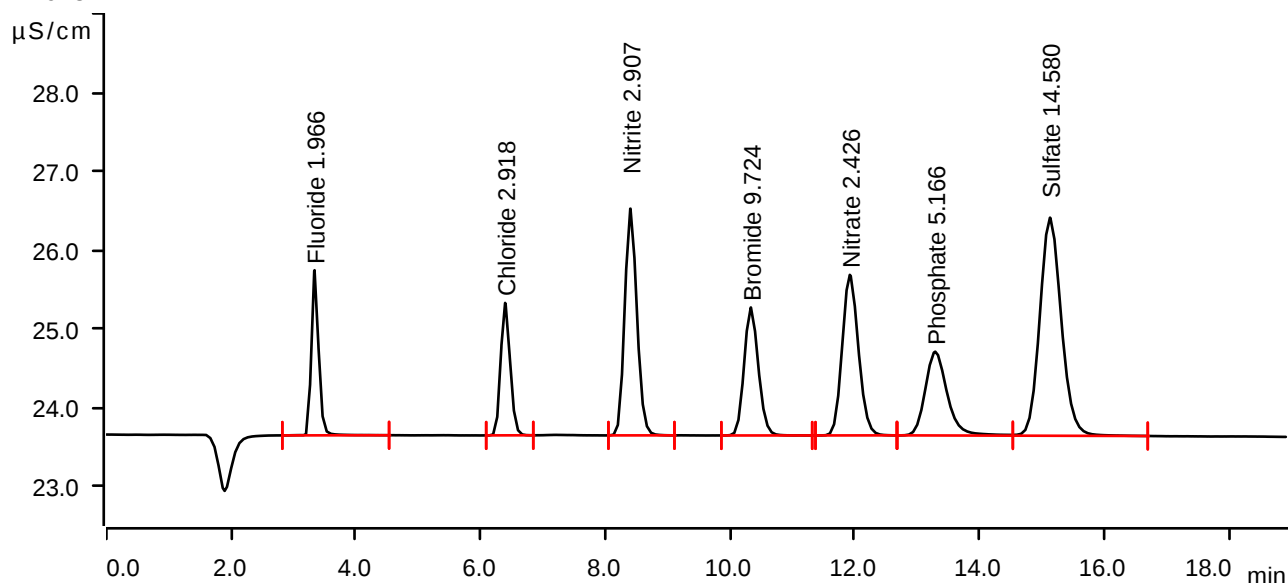

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2845	2.095	1.966	Fluoride
2	6.393	0.2963	1.681	2.918	Chloride
3	8.403	0.6535	2.878	2.907	Nitrite
4	10.332	0.4304	1.624	9.724	Bromide
5	11.920	0.6163	2.038	2.426	Nitrate
6	13.290	0.4342	1.063	5.166	Phosphate
7	15.128	1.1075	2.767	14.580	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-11-03 18:30:25 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

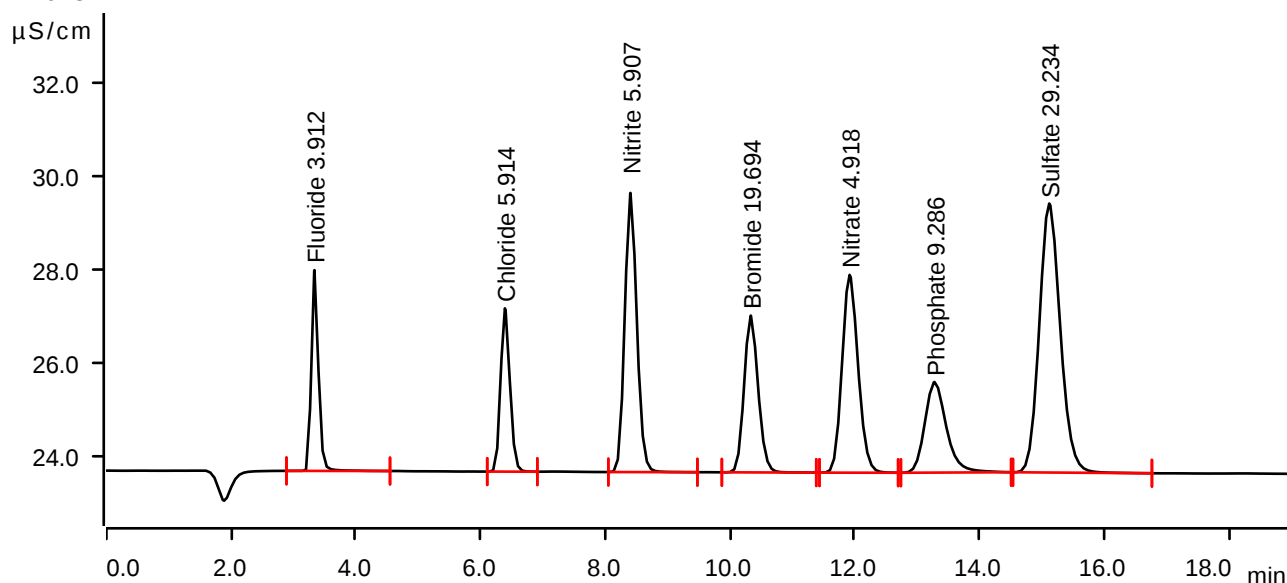

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.5698	4.312	3.912	Fluoride
2	6.390	0.6080	3.506	5.914	Chloride
3	8.403	1.3473	5.995	5.907	Nitrite
4	10.330	0.8806	3.367	19.694	Bromide
5	11.917	1.2665	4.248	4.918	Nitrate
6	13.278	0.7790	1.945	9.286	Phosphate
7	15.117	2.2550	5.777	29.234	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-11-03 18:51:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

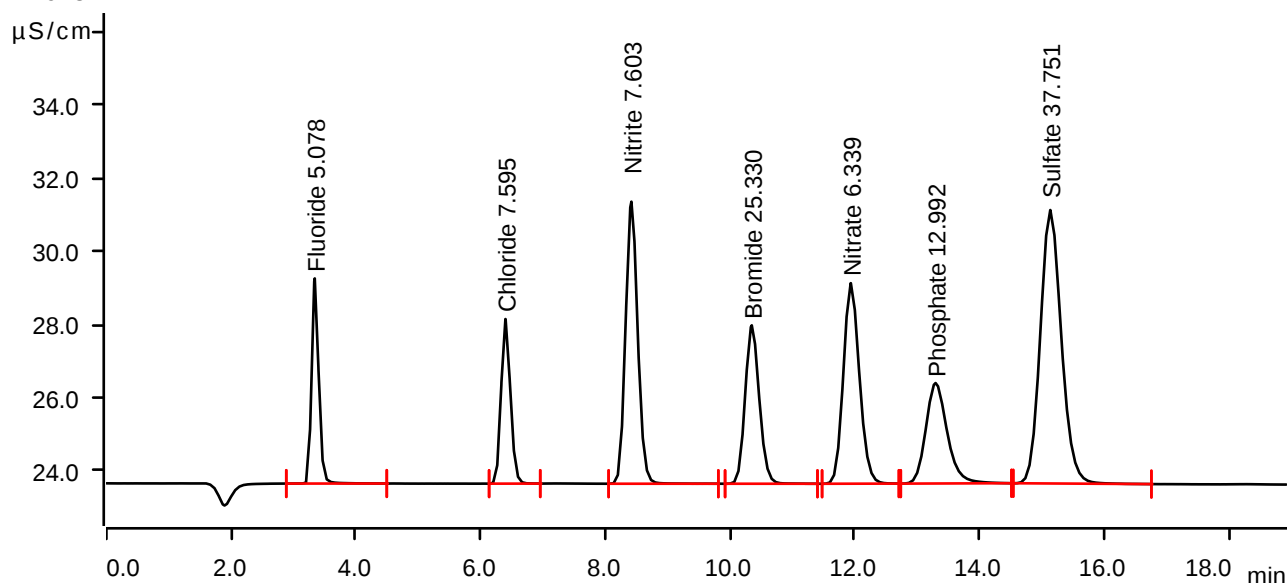

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.7408	5.606	5.078	Fluoride
2	6.398	0.7828	4.499	7.595	Chloride
3	8.418	1.7395	7.709	7.603	Nitrite
4	10.348	1.1352	4.330	25.330	Bromide
5	11.937	1.6370	5.482	6.339	Nitrate
6	13.295	1.0891	2.746	12.992	Phosphate
7	15.133	2.9220	7.473	37.751	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-11-03 19:13:20 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

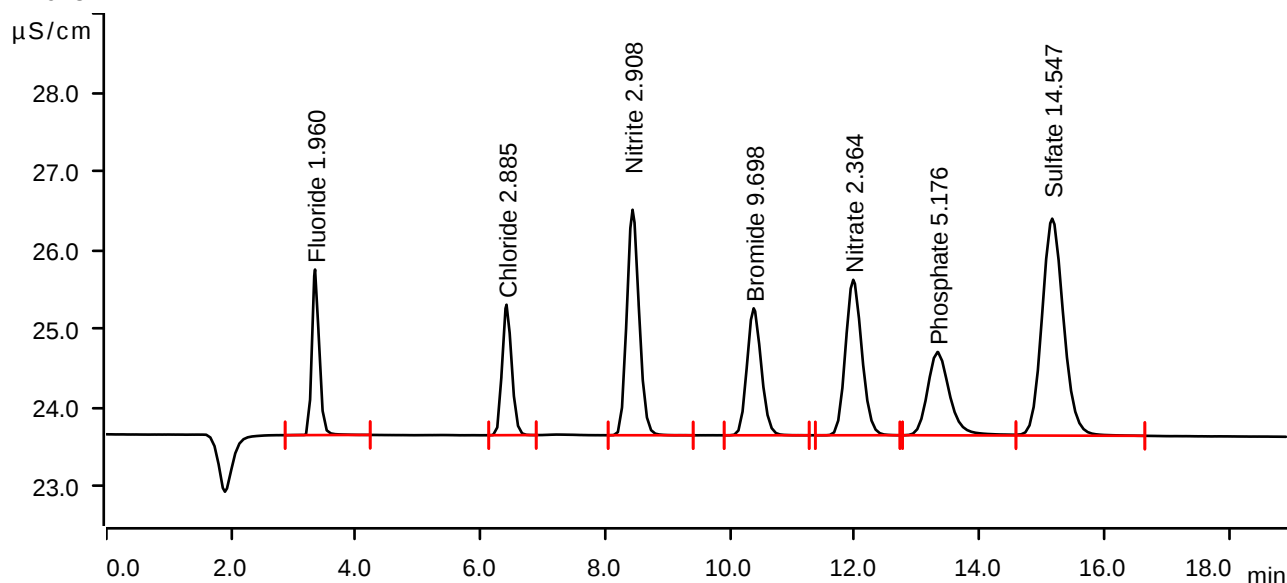


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.2837	2.100	1.960	Fluoride
2	6.417	0.2929	1.656	2.885	Chloride
3	8.437	0.6536	2.862	2.908	Nitrite
4	10.378	0.4292	1.611	9.698	Bromide
5	11.975	0.6003	1.973	2.364	Nitrate
6	13.327	0.4351	1.058	5.176	Phosphate
7	15.165	1.1050	2.753	14.547	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-11-03 19:34:48 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

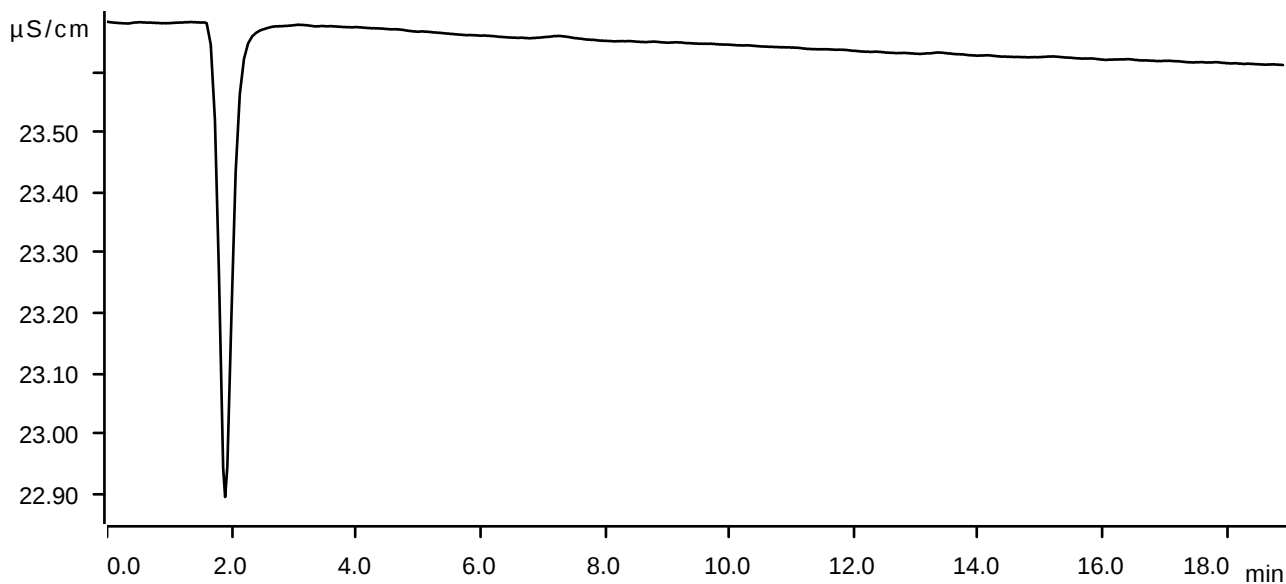Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-26 09:14:26 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

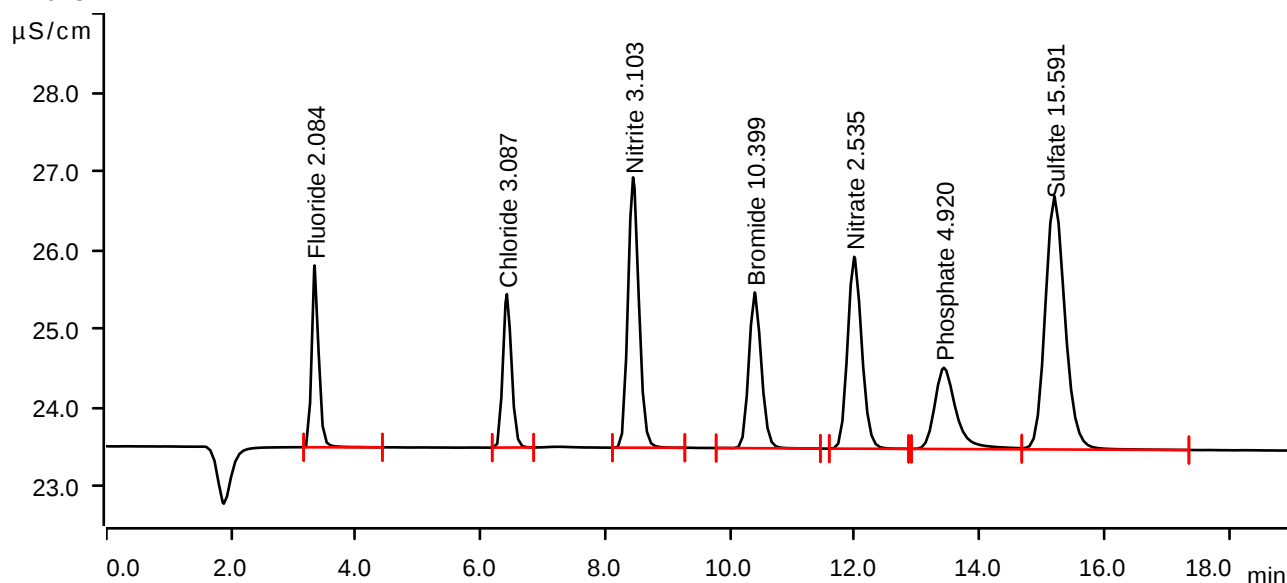


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.3019	2.306	2.084	Fluoride
2	6.422	0.3140	1.947	3.087	Chloride
3	8.445	0.6987	3.430	3.103	Nitrite
4	10.395	0.4609	1.977	10.399	Bromide
5	11.990	0.6449	2.435	2.535	Nitrate
6	13.428	0.4137	1.031	4.920	Phosphate
7	15.200	1.1867	3.214	15.591	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-26 09:35:57 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

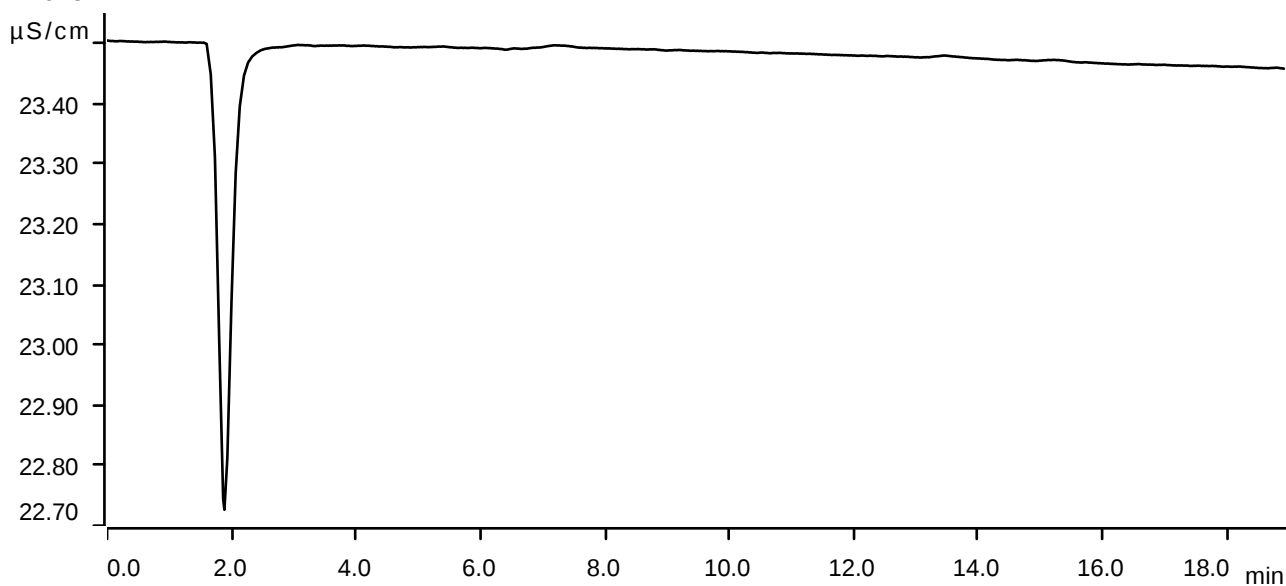
Anions

Sample data

Ident LB138070BLW
Sample type Sample
Determination start 2025-11-26 09:57:27 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

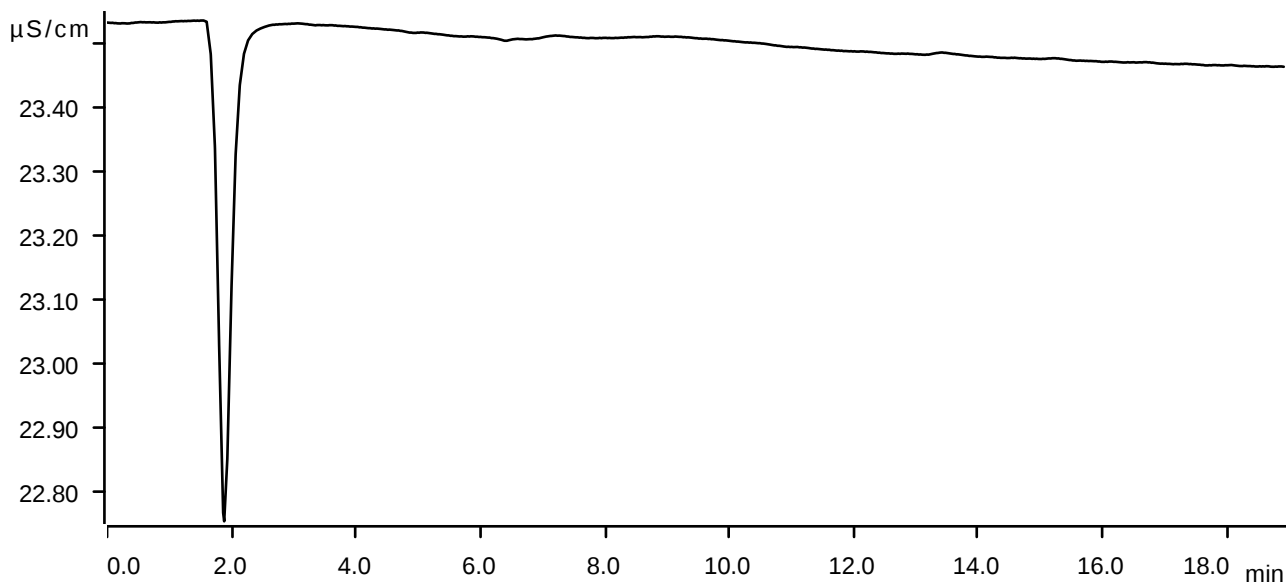Anions


Sample data

Ident LB138070BSW
Sample type Check standard 1
Determination start 2025-11-26 10:18:58 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

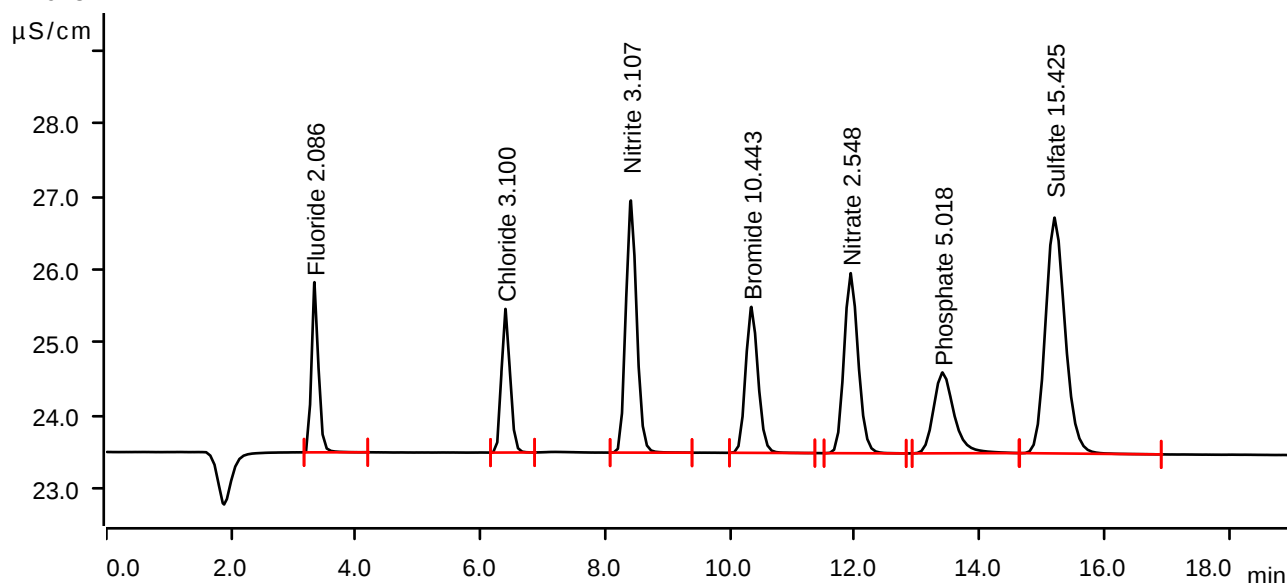

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.3022	2.325	2.086	Fluoride
2	6.398	0.3153	1.963	3.100	Chloride
3	8.410	0.6997	3.446	3.107	Nitrite
4	10.342	0.4629	1.995	10.443	Bromide
5	11.933	0.6482	2.461	2.548	Nitrate
6	13.407	0.4219	1.105	5.018	Phosphate
7	15.203	1.1737	3.222	15.425	Sulfate


Sample data

Ident Q3728-01
Sample type Sample
Determination start 2025-11-26 13:10:26 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

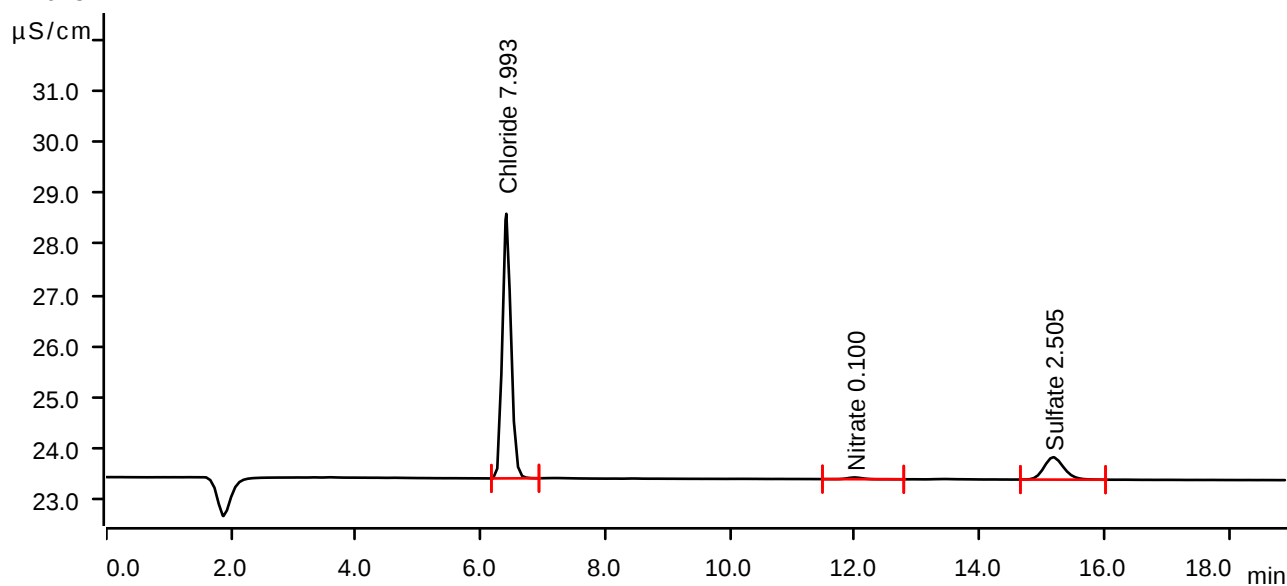

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.413	0.8242	5.165	7.993	Chloride
2	11.998	0.0096	0.034	0.100	Nitrate
3	15.182	0.1619	0.437	2.505	Sulfate


Sample data

Ident Q3728-01MS
Sample type Sample
Determination start 2025-11-26 13:31:58 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

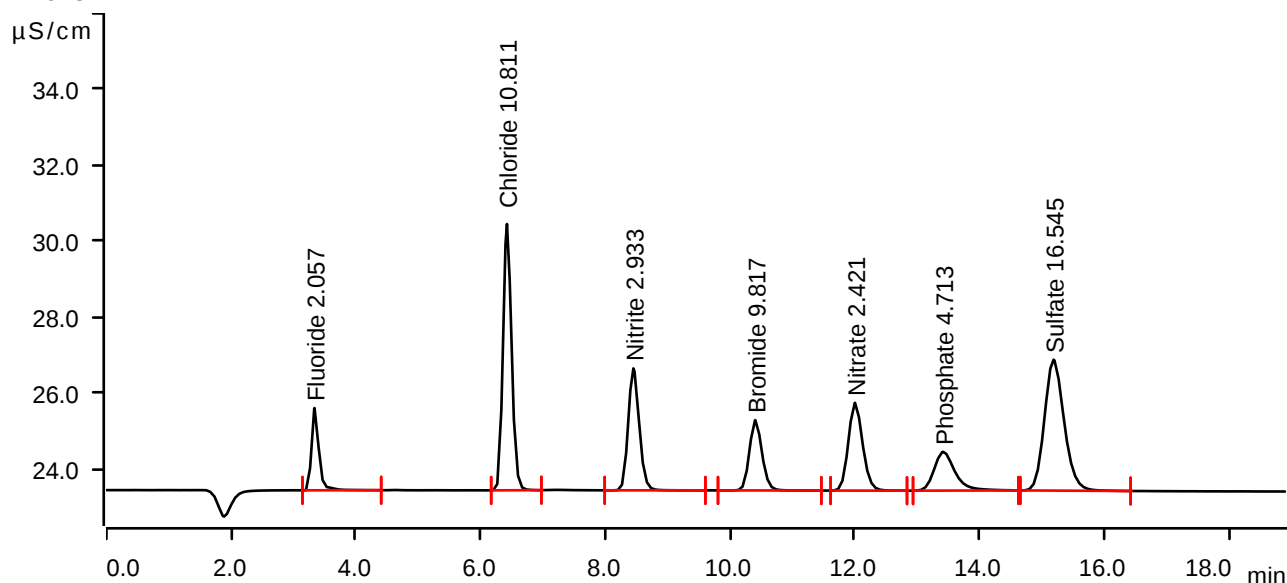

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2980	2.168	2.057	Fluoride
2	6.423	1.1173	7.019	10.811	Chloride
3	8.450	0.6596	3.214	2.933	Nitrite
4	10.405	0.4346	1.853	9.817	Bromide
5	12.003	0.6152	2.313	2.421	Nitrate
6	13.417	0.3964	1.023	4.713	Phosphate
7	15.187	1.2614	3.450	16.545	Sulfate


Sample data

Ident Q3728-01MSD
Sample type Sample
Determination start 2025-11-26 13:53:32 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

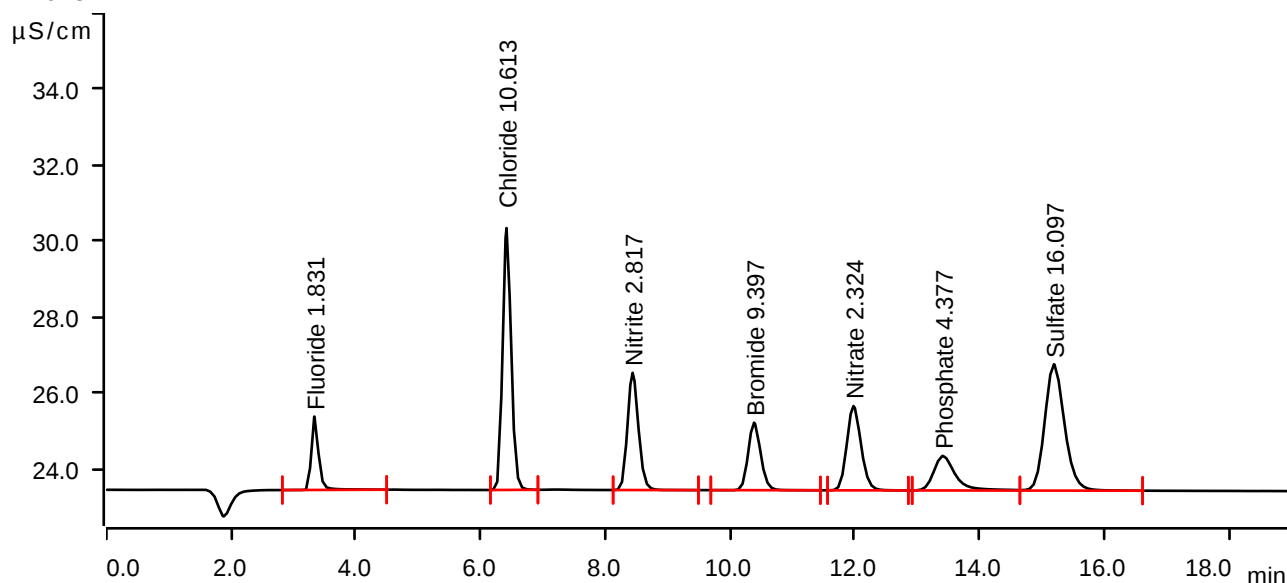

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.2648	1.935	1.831	Fluoride
2	6.417	1.0967	6.902	10.613	Chloride
3	8.438	0.6327	3.090	2.817	Nitrite
4	10.385	0.4157	1.779	9.397	Bromide
5	11.978	0.5897	2.222	2.324	Nitrate
6	13.413	0.3682	0.911	4.377	Phosphate
7	15.192	1.2263	3.330	16.097	Sulfate


Sample data

Ident Q3734-01
Sample type Sample
Determination start 2025-11-26 14:58:07 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

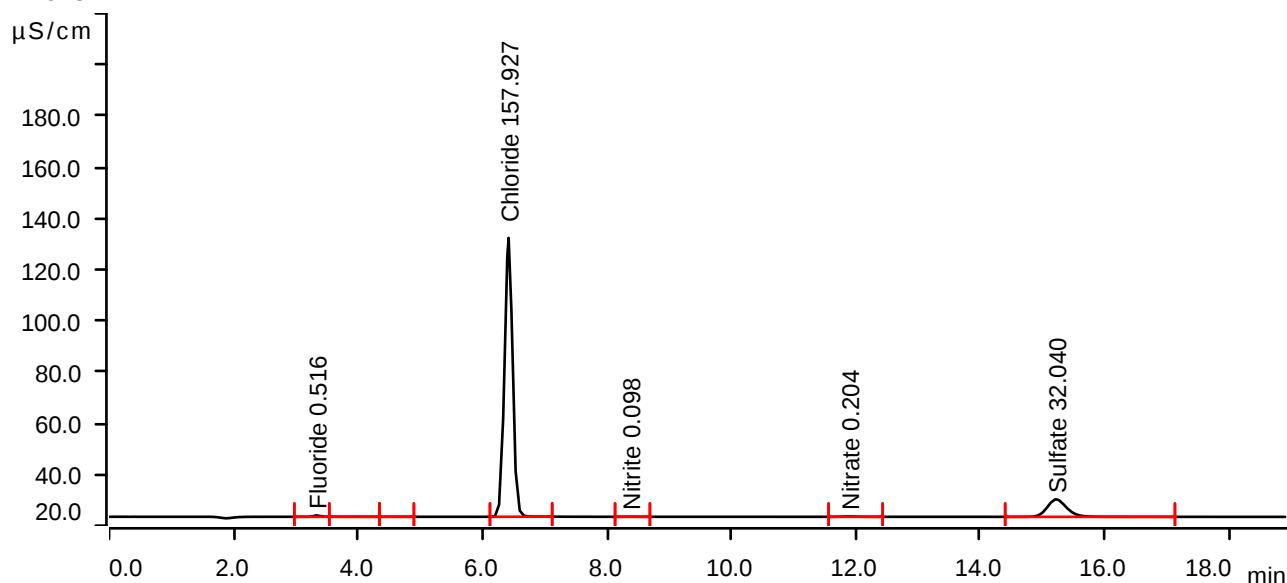

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.333	0.0720	0.540	0.516	Fluoride
2	3.600	0.0068	0.028	invalid	
3	4.615	0.0029	0.016	invalid	
4	6.422	16.4189	108.883	157.927	Chloride
5	8.377	0.0039	0.019	0.098	Nitrite
6	11.895	0.0368	0.140	0.204	Nitrate
7	15.220	2.4748	6.844	32.040	Sulfate


Sample data

Ident Q3734-02
Sample type Sample
Determination start 2025-11-26 15:19:31 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

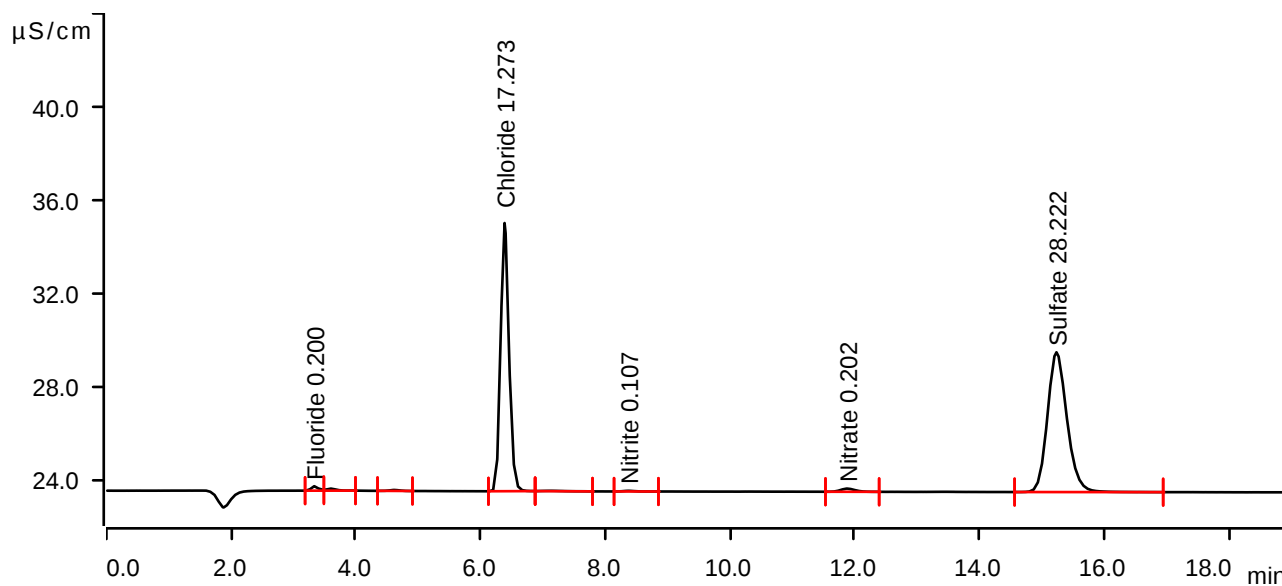

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.332	0.0257	0.190	0.200	Fluoride
2	3.602	0.0155	0.087	invalid	
3	4.615	0.0075	0.041	invalid	
4	6.385	1.7894	11.517	17.273	Chloride
5	7.105	0.0061	0.015	invalid	
6	8.368	0.0059	0.028	0.107	Nitrite
7	11.878	0.0364	0.137	0.202	Nitrate
8	15.233	2.1758	6.004	28.222	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-26 15:41:06 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

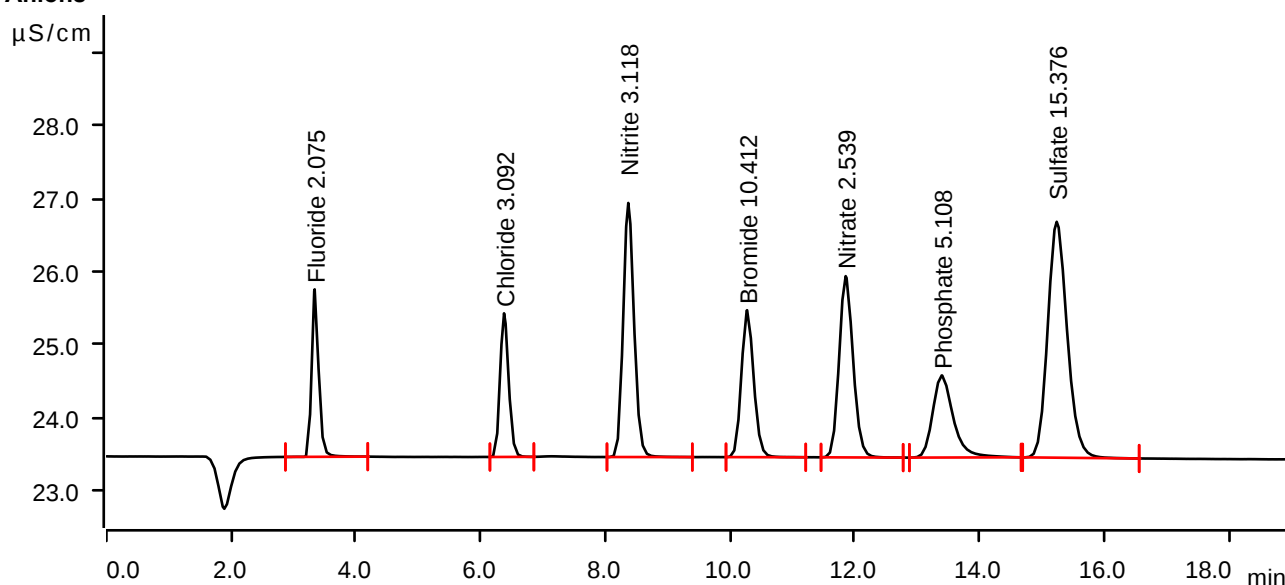

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.3006	2.288	2.075	Fluoride
2	6.377	0.3145	1.963	3.092	Chloride
3	8.368	0.7024	3.472	3.118	Nitrite
4	10.273	0.4615	2.008	10.412	Bromide
5	11.853	0.6459	2.477	2.539	Nitrate
6	13.393	0.4294	1.122	5.108	Phosphate
7	15.237	1.1698	3.224	15.376	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-26 16:02:36 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions