


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120225\
Data File : VN088395.D
Acq On : 02 Dec 2025 08:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

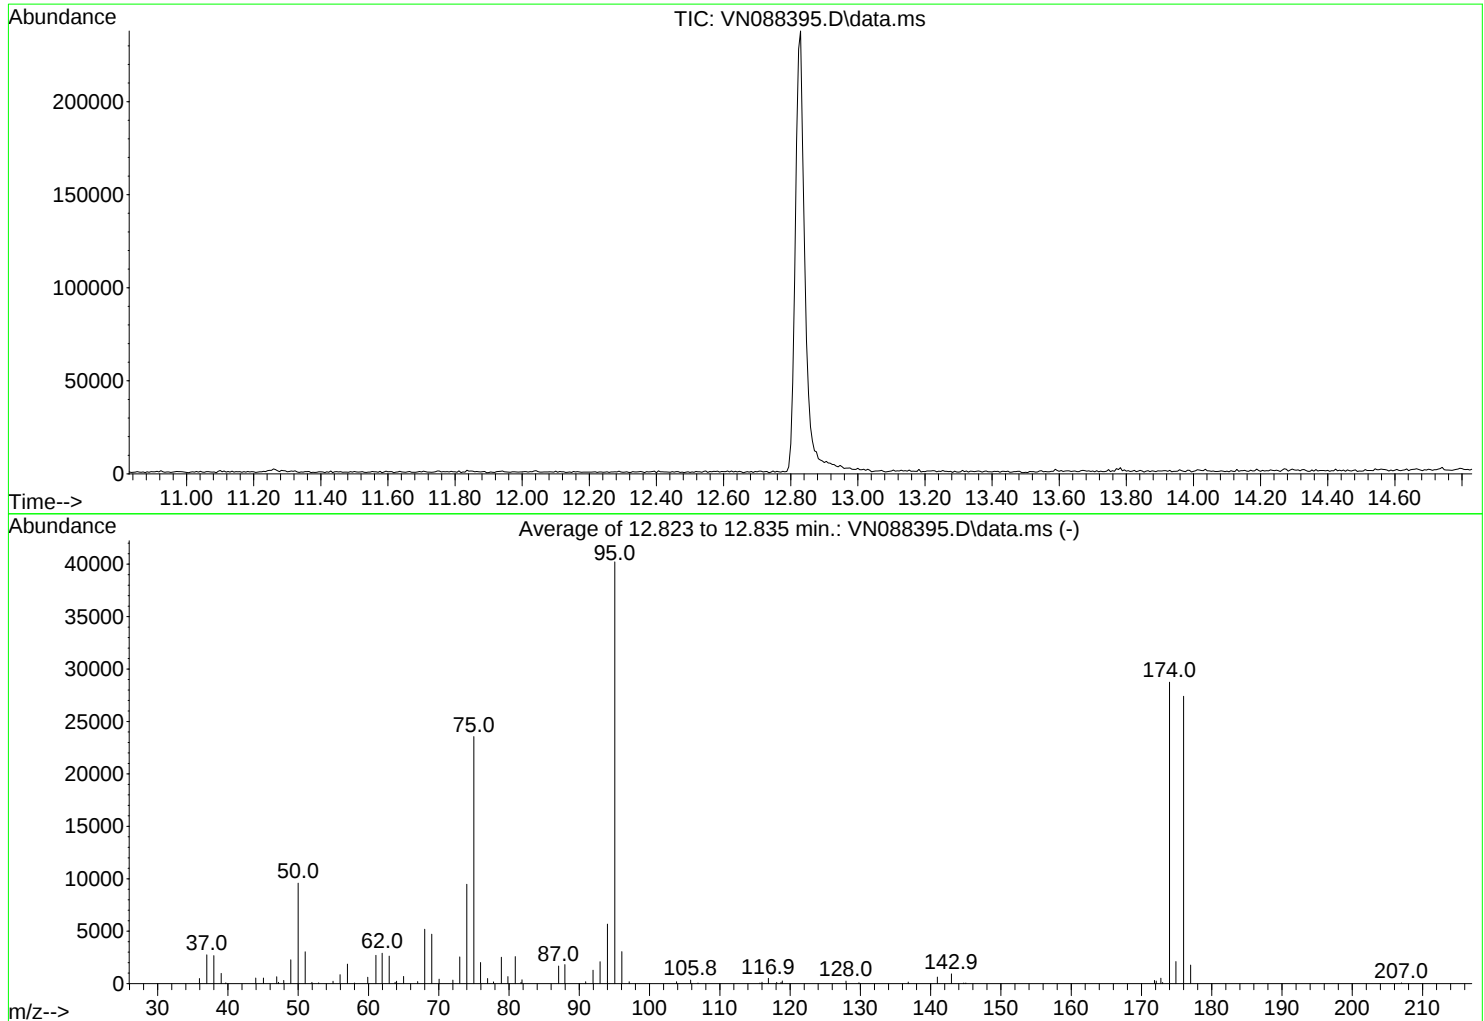

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	9585	PASS
75	95	30	60	58.6	23563	PASS
95	95	100	100	100.0	40224	PASS
96	95	5	9	7.6	3049	PASS
173	174	0.00	2	1.8	524	PASS
174	95	50	100	71.5	28741	PASS
175	174	5	9	7.3	2106	PASS
176	174	95	101	95.3	27400	PASS
177	176	5	9	6.5	1775	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	494	50.00	9585	62.95	2621	75.00	2356
37.00	2753	51.00	3035	63.80	123	75.95	200
38.00	2674	51.95	119	64.00	223	76.95	48
39.05	970	52.90	77	65.00	682	77.80	16
39.70	78	54.95	230	67.00	205	78.90	2513
43.95	536	55.95	848	68.00	5185	79.85	678
45.05	540	57.00	1862	69.00	4721	80.90	2577
46.95	655	58.00	54	70.05	424	81.70	125
47.20	120	59.90	607	72.00	337	81.85	367
47.95	302	61.05	2698	73.00	2556	87.05	1677
48.95	2279	61.95	2900	74.00	9481	87.95	1814

Average of 12.823 to 12.835 min.: VN088395.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	177	116.00	142	145.00	55		
91.95	1284	116.90	503	171.85	304		
92.95	2091	118.10	124	172.10	253		
94.00	5676	118.70	118	172.75	524		
95.05	40224	118.90	258	173.00	107		
96.05	3049	127.95	244	174.00	28741		
97.10	178	129.80	98	174.90	2106		
103.85	183	136.80	150	176.00	27400		
105.85	336	140.95	625	177.00	1775		
106.90	56	142.95	937	207.00	79		
115.70	65	144.70	66				

Instrument :

MSVOA_N

ClientSampleId :

BFB