

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q3741	OrderDate:	11/26/2025 4:57:55 PM
Client:	Core Environmental Consultants and Services, Inc.	Project:	Building 50 Probe Investigation
Contact:	Roland Scardino	Location:	--Select--,VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q3741-01	B50-SP3-111925	SOIL			11/19/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/04/25	
			Gasoline Range Organics	8015D			12/08/25	
Q3741-02	B50-SP13-112025	SOIL			11/20/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/04/25	
			Gasoline Range Organics	8015D			12/08/25	
Q3741-03	B50-SP14-112025	SOIL			11/20/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/05/25	
			Gasoline Range Organics	8015D			12/08/25	
Q3741-04	B50-SP9-112425	SOIL			11/24/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/04/25	
			Gasoline Range Organics	8015D			12/08/25	
Q3741-05	B50-SP11-112525	SOIL			11/25/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/04/25	
			Gasoline Range Organics	8015D			12/09/25	
			PCB	8082A		12/03/25	12/03/25	
Q3741-06	B50-SP4-112525	SOIL			11/25/25			11/26/25
			Diesel Range Organics	8015D		12/03/25	12/05/25	
			Gasoline Range Organics	8015D			12/08/25	
			PCB	8082A		12/03/25	12/03/25	



QC SUMMARY

SOIL GASOLINE RANGE ORGANICS SURROGATE RECOVERY

Lab Name: Alliance

Client: Core Environmental Consultants and Service

Lab Code: ACE

SDG No.: Q3741

CLIENT ID	S1 AAA-TFT	S2	S3	S4	TOT OUT
VBF1208S1	104				0
BSF1208S1	98				0
B50-SP4-112525	96				0
B50-SP9-112425	89				0
BSF1208S2	101				0
B50-SP3-111925	87				0
B50-SP13-112025	91				0
B50-SP14-112025	86				0
VBF1209S2	112				0
BSF1209S1	107				0
B50-SP11-112525	125				0

QC LIMITS

AAA-TFT

For Water : 50-150

For Soil : 50-150

Column to be used to flag recovery values

* Values outside of contract required QC limits

D Surrogate Diluted Out



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

SOIL GASOLINE RANGE ORGANICS LABORATORY CONTROL SPIKE/LABORATORY CONTROL SPIKE DUPLICATION

Lab Name: Alliance

Client: Core Environmental Consultants and

Lab Code: ACE

SDG No: Services, Inc.
Q3741

Client Sample ID : BSF1208S1

Datafile: FB032403.D

COMPOUND	SPIKE ADDED ug/kg	CONCENTRATION ug/kg	LCS/LCSD CONCENTRATION ug/kg	% REC	QC LIMITS (%)
GRO	180	0	170	94	50-150



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

SOIL GASOLINE RANGE ORGANICS LABORATORY CONTROL SPIKE/LABORATORY CONTROL SPIKE DUPLICATION

Lab Name: Alliance

Client: Core Environmental Consultants and

Lab Code: ACE

SDG No: Q3741

Client Sample ID : BSF1208S2

Datafile: FB032408.D

COMPOUND	SPIKE ADDED ug/kg	CONCENTRATION ug/kg	LCS/LCSD CONCENTRATION ug/kg	% REC	QC LIMITS (%)
GRO	180	0	174	97	50-150

LCS/LCSD % Recovery RPD : 2.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

SOIL GASOLINE RANGE ORGANICS LABORATORY CONTROL SPIKE/LABORATORY CONTROL SPIKE DUPLICATION

Lab Name: Alliance

Client: Core Environmental Consultants and

Lab Code: ACE

SDG No: Services, Inc.
Q3741

Client Sample ID : BSF1209S1

Datafile: FB032419.D

COMPOUND	SPIKE ADDED ug/kg	CONCENTRATION ug/kg	LCS/LCSD CONCENTRATION ug/kg	% REC	QC LIMITS (%)
GRO	180	0	183	102	50-150

METHOD BLANK SUMMARY

CLIENT SAMPLE NO.

VBF1208S1

Lab Name: Alliance

Contract: CORE02

Lab Code: ACE

SDG NO.: Q3741

Lab File ID: FB032401.D

Lab Sample ID: VBF1208S1

Date Analyzed: 12/08/25

Time Analyzed: 10:40

GC Column: RTX-502.2 ID: 0.53 (mm)

Heated Purge: (Y/N) Y

Instrument ID: FB

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

CLIENT SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
BSF1208S1	BSF1208S1	FB032403.D	12/08/25
B50-SP4-112525	Q3741-06	FB032405.D	12/08/25
B50-SP9-112425	Q3741-04	FB032407.D	12/08/25
BSF1208S2	BSF1208S2	FB032408.D	12/08/25
B50-SP3-111925	Q3741-01	FB032410.D	12/08/25
B50-SP13-112025	Q3741-02	FB032411.D	12/08/25
B50-SP14-112025	Q3741-03	FB032412.D	12/08/25

COMMENTS: _____

METHOD BLANK SUMMARY

CLIENT SAMPLE NO.

VBF1209S2

Lab Name: Alliance

Contract: CORE02

Lab Code: ACE

SDG NO.: Q3741

Lab File ID: FB032418.D

Lab Sample ID: VBF1209S2

Date Analyzed: 12/09/25

Time Analyzed: 11:06

GC Column: RTX-502.2 ID: 0.53 (mm)

Heated Purge: (Y/N) Y

Instrument ID: FB

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

CLIENT SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
BSF1209S1	BSF1209S1	FB032419.D	12/09/25
B50-SP11-112525	Q3741-05	FB032420.D	12/09/25

COMMENTS:



SAMPLE DATA

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/19/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP3-111925	SDG No.:	Q3741
Lab Sample ID:	Q3741-01	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	91.6
Sample Wt/Vol:	6.82 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	8.00	J	1	7.00	36.0	ug/kg	12/08/25 16:05	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	17.4			50 - 150	87%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032410.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 16:05
Operator : YP/AJ
Sample : Q3741-01
Misc : 6.82G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP3-111925

Integration File: Calibration.e
Quant Time: Dec 09 03:06:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	392483	17.421 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032410.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 16:05
Operator : YP/AJ
Sample : Q3741-01
Misc : 6.82G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP3-111925

Integration File: Calibration.e
Quant Time: Dec 09 03:06:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

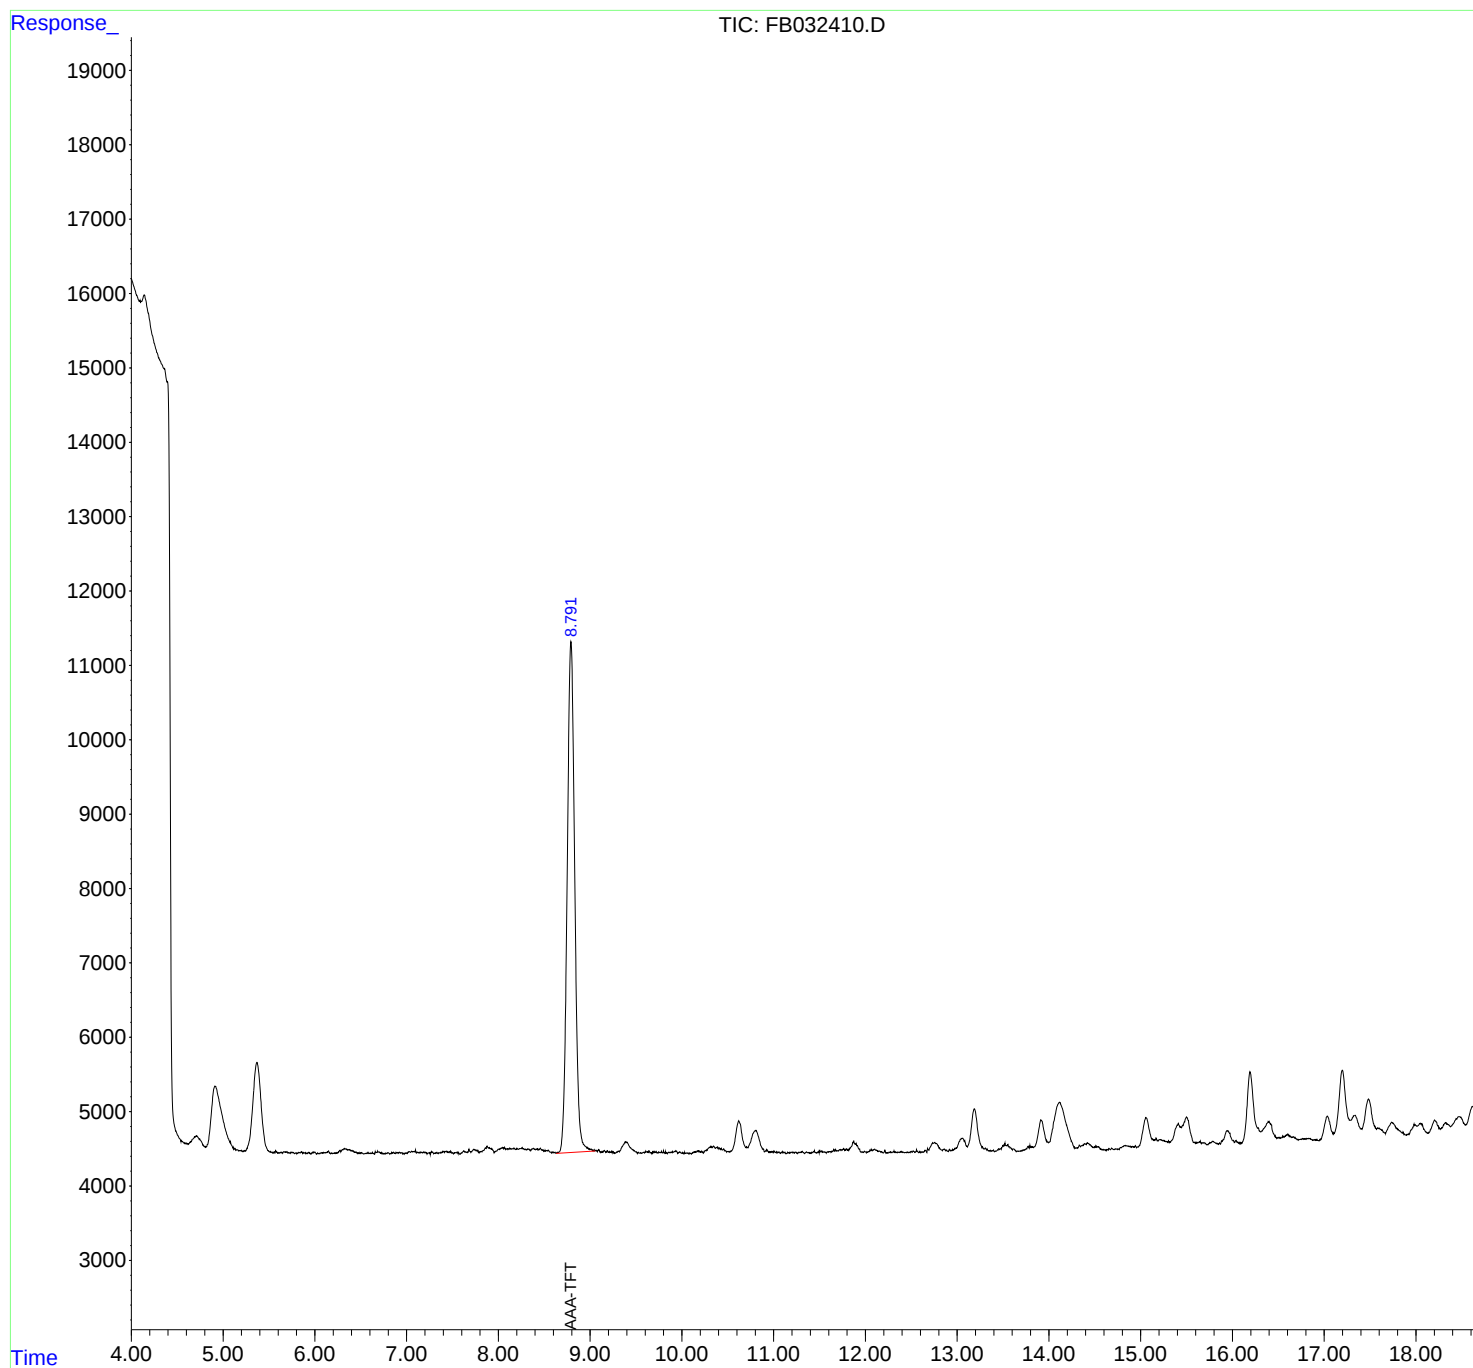

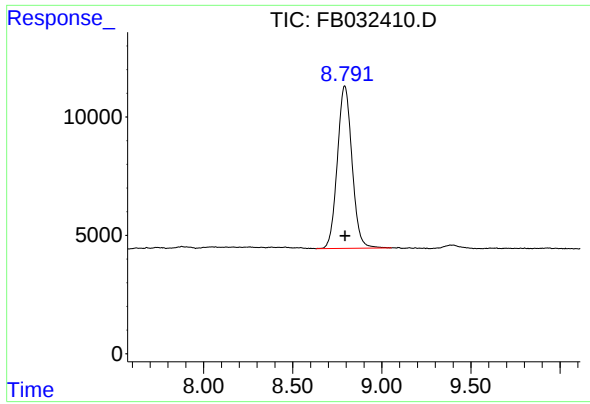

#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.003 min
Response: 392483
Conc: 17.42 ng/ml

Instrument :
FID_B
ClientSampleId :
B50-SP3-111925

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032410.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 16:05
 Sample : Q3741-01
 Misc : 6.82G/5.00 ML DI WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.597	4.554	4.622	BV	3	-118	-0.03%	-0.014%
2	4.711	4.622	4.813	PV	134	7494	1.87%	0.917%
3	5.577	5.548	5.611	PV	30	343	0.09%	0.042%
4	5.634	5.611	5.651	PV	15	176	0.04%	0.021%
5	5.665	5.651	5.731	VV	22	642	0.16%	0.079%
6	5.750	5.731	5.803	VV	17	373	0.09%	0.046%
7	5.856	5.803	5.905	PV	27	776	0.19%	0.095%
8	5.934	5.905	5.955	VV	21	307	0.08%	0.038%
9	5.999	5.955	6.023	PV	27	600	0.15%	0.073%
10	6.148	6.023	6.197	VV	37	1608	0.40%	0.197%
11	6.326	6.197	6.493	VV	76	6789	1.70%	0.831%
12	6.509	6.493	6.536	VV	24	351	0.09%	0.043%
13	6.580	6.536	6.619	VV	25	623	0.16%	0.076%
14	6.628	6.619	6.650	VV	25	247	0.06%	0.030%
15	6.687	6.650	6.761	PV	39	1367	0.34%	0.167%
16	6.799	6.761	6.819	VV	21	474	0.12%	0.058%
17	6.902	6.878	6.963	VV	25	973	0.24%	0.119%
18	7.029	6.963	7.045	VV	37	987	0.25%	0.121%
19	7.095	7.045	7.110	VV	45	1377	0.34%	0.168%
20	7.119	7.110	7.154	VV	28	617	0.15%	0.075%
21	7.191	7.154	7.226	VV	30	977	0.24%	0.120%
22	7.246	7.226	7.259	VV	18	309	0.08%	0.038%
23	7.277	7.259	7.299	VV	26	514	0.13%	0.063%
24	7.405	7.299	7.465	VV	39	2515	0.63%	0.308%
25	7.477	7.465	7.512	VV	34	706	0.18%	0.086%
26	7.552	7.512	7.585	VV	31	768	0.19%	0.094%
27	7.623	7.585	7.661	VV	48	1219	0.30%	0.149%
28	7.682	7.661	7.702	VV	64	957	0.24%	0.117%
29	7.735	7.702	7.791	VV	62	2622	0.66%	0.321%
30	7.879	7.791	7.957	VV	106	6251	1.56%	0.765%
31	8.067	7.957	8.097	VV	92	5590	1.40%	0.684%
32	8.127	8.097	8.144	VV	82	2070	0.52%	0.253%
33	8.166	8.144	8.189	VV	82	1973	0.49%	0.241%
34	8.203	8.189	8.218	VV	81	1226	0.31%	0.150%
35	8.260	8.218	8.309	VV	89	3910	0.98%	0.478%
36	8.325	8.309	8.350	VV	71	1539	0.38%	0.188%

					rteres			
37	8.382	8.350	8.409	VV	78	2352	0.59%	0.288%
38	8.458	8.409	8.517	VV	81	3876	0.97%	0.474%
39	8.545	8.517	8.630	VV	55	2137	0.53%	0.261%
40	8.792	8.630	9.082	VV	6889	400127	100.00%	48.947%
41	9.094	9.082	9.117	VV	58	879	0.22%	0.108%
42	9.156	9.117	9.180	VV	50	1278	0.32%	0.156%
43	9.189	9.180	9.270	VV	49	1570	0.39%	0.192%
44	9.388	9.270	9.564	VV	164	11881	2.97%	1.453%
45	9.644	9.564	9.675	VV	44	1637	0.41%	0.200%
46	9.698	9.675	9.739	VV	33	860	0.21%	0.105%
47	9.779	9.739	9.844	VV	37	1350	0.34%	0.165%
48	9.930	9.844	9.959	VV	43	1784	0.45%	0.218%
49	9.977	9.959	10.026	VV	29	711	0.18%	0.087%
50	10.032	10.026	10.104	VV	23	490	0.12%	0.060%
51	10.178	10.104	10.236	PV	49	2143	0.54%	0.262%
52	10.316	10.236	10.332	VV	98	3732	0.93%	0.457%
53	10.345	10.332	10.367	VV	105	1965	0.49%	0.240%
54	10.387	10.367	10.523	VV	94	5413	1.35%	0.662%
55	10.621	10.523	10.722	VV	443	23718	5.93%	2.901%
56	10.805	10.722	10.905	VV	315	20174	5.04%	2.468%
57	10.927	10.905	10.978	VV	59	1450	0.36%	0.177%
58	11.006	10.978	11.038	VV	31	816	0.20%	0.100%
59	11.060	11.038	11.075	VV	23	361	0.09%	0.044%
60	11.094	11.075	11.142	VV	30	496	0.12%	0.061%
61	11.197	11.142	11.260	PV	22	964	0.24%	0.118%
62	11.313	11.260	11.339	VV	28	719	0.18%	0.088%
63	11.358	11.339	11.412	VV	24	488	0.12%	0.060%
64	11.443	11.412	11.470	VV	29	610	0.15%	0.075%
65	11.506	11.470	11.576	VV	35	1267	0.32%	0.155%
66	11.655	11.576	11.693	VV	49	1990	0.50%	0.243%
67	11.764	11.693	11.785	VV	61	2547	0.64%	0.312%
68	11.797	11.785	11.816	VV	58	881	0.22%	0.108%
69	11.873	11.816	11.980	VV	167	7708	1.93%	0.943%
70	11.992	11.980	12.019	VV	25	388	0.10%	0.047%
71	12.100	12.019	12.195	VV	54	3116	0.78%	0.381%
72	12.214	12.195	12.246	VV	41	344	0.09%	0.042%
73	12.315	12.246	12.339	PV	23	619	0.15%	0.076%
74	12.384	12.339	12.429	VV	15	521	0.13%	0.064%
75	12.524	12.429	12.545	VV	23	633	0.16%	0.077%
76	12.560	12.545	12.582	VV	39	357	0.09%	0.044%
77	12.756	12.582	12.843	PV	138	9045	2.26%	1.106%
78	12.858	12.843	12.904	VV	43	1098	0.27%	0.134%
79	13.055	12.904	13.115	VV	188	11469	2.87%	1.403%
80	13.189	13.115	13.380	VV	582	30350	7.59%	3.713%
81	13.393	13.380	13.410	VV	17	214	0.05%	0.026%
82	13.523	13.410	13.680	VV	110	6788	1.70%	0.830%
83	13.794	13.680	13.832	VV	78	3260	0.81%	0.399%
84	13.916	13.832	13.996	VV	417	21785	5.44%	2.665%
85	14.117	13.996	14.296	VV	655	61941	15.48%	7.577%
86	14.422	14.296	14.490	VV	102	8122	2.03%	0.994%
87	14.514	14.490	14.627	VV	58	2378	0.59%	0.291%
88	14.687	14.627	14.709	PV	21	644	0.16%	0.079%
89	14.832	14.709	14.927	VV	52	3864	0.97%	0.473%

					rteres				
90	14.943	14.927	14.959	VV	41	539	0.13%	0.066%	
91	15.060	14.959	15.147	VV	409	22378	5.59%	2.737%	
92	15.169	15.147	15.189	VV	131	2735	0.68%	0.335%	
93	15.213	15.189	15.318	VV	108	6862	1.71%	0.839%	
94	15.412	15.318	15.446	VV	306	15471	3.87%	1.893%	
95	15.501	15.446	15.623	VV	391	21646	5.41%	2.648%	
96	15.647	15.623	15.726	VV	49	2006	0.50%	0.245%	
97	15.786	15.726	15.849	VV	46	1851	0.46%	0.226%	
98	15.944	15.849	16.085	VV	180	9515	2.38%	1.164%	
					Sum of corrected areas:		817475		

FB120525.M Tue Dec 09 04:24:33 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/20/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP13-112025	SDG No.:	Q3741
Lab Sample ID:	Q3741-02	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	86.4
Sample Wt/Vol:	4.84 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	10.0	U	1	10.0	54.0	ug/kg	12/08/25 16:34	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	18.3			50 - 150	91%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032411.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 16:34
Operator : YP/AJ
Sample : Q3741-02
Misc : 4.84G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP13-112025

Integration File: Calibration.e
Quant Time: Dec 09 03:06:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	411278	18.255 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032411.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 16:34
Operator : YP/AJ
Sample : Q3741-02
Misc : 4.84G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP13-112025

Integration File: Calibration.e
Quant Time: Dec 09 03:06:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

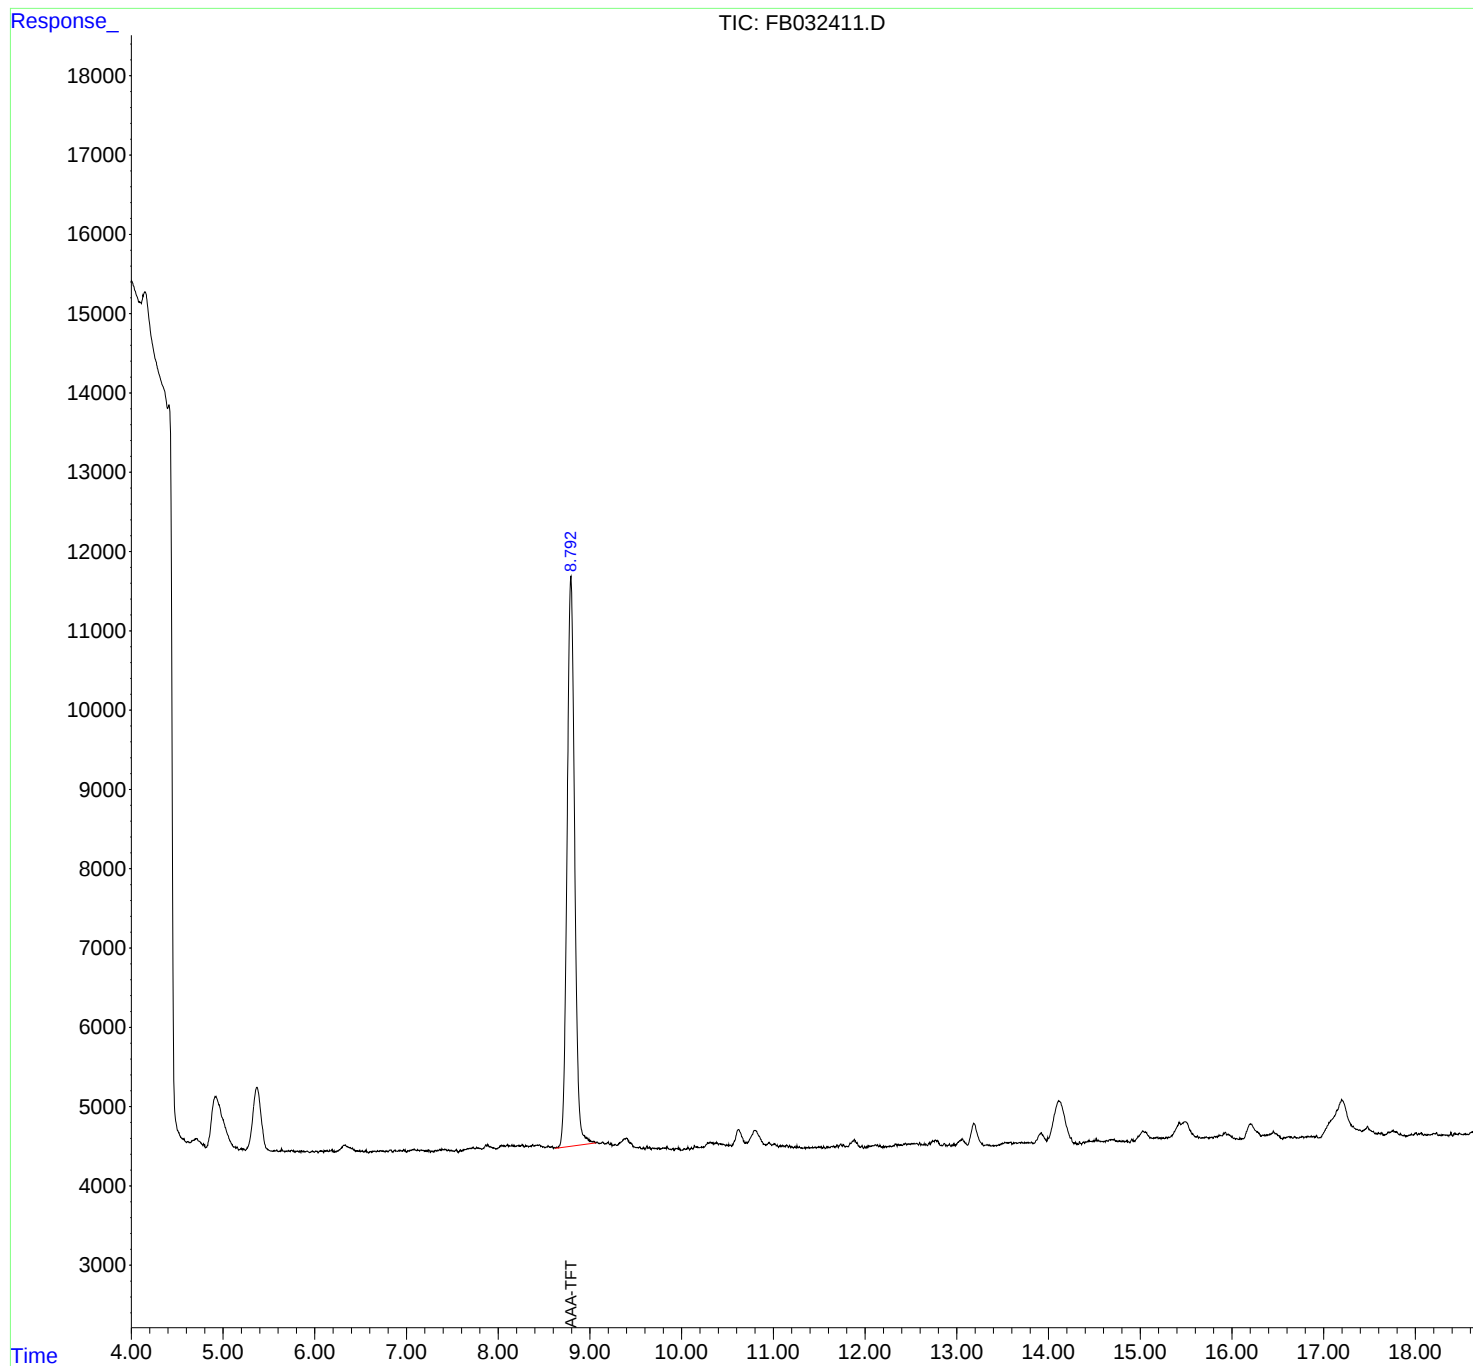

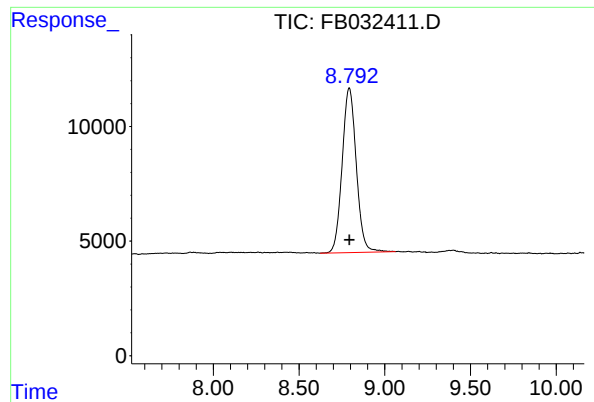

#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 411278
Conc: 18.26 ng/ml

Instrument :

FID_B

ClientSampleId :

B50-SP13-112025

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032411.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 16:34
 Sample : Q3741-02
 Misc : 4.84G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.411	4.353	4.604	BV	1970	-180457	-41.60%	29.630%
2	4.616	4.604	4.646	PV	16	257	0.06%	0.042%
3	4.710	4.646	4.811	VV	84	4730	1.09%	0.777%
4	5.155	5.144	5.181	VV	38	383	0.09%	0.063%
5	5.197	5.181	5.219	VV	23	303	0.07%	0.050%
6	5.227	5.219	5.244	VV	21	177	0.04%	0.029%
7	5.587	5.541	5.603	VV	21	307	0.07%	0.050%
8	5.639	5.603	5.684	PV	39	476	0.11%	0.078%
9	5.714	5.684	5.722	VV	19	235	0.05%	0.039%
10	5.748	5.722	5.765	VV	23	371	0.09%	0.061%
11	5.771	5.765	5.804	VV	24	266	0.06%	0.044%
12	5.813	5.804	5.841	VV	16	237	0.05%	0.039%
13	5.854	5.841	5.863	VV	24	202	0.05%	0.033%
14	5.883	5.863	5.895	VV	19	241	0.06%	0.040%
15	5.919	5.895	5.944	VV	18	324	0.07%	0.053%
16	5.974	5.944	5.996	PV	22	332	0.08%	0.055%
17	6.012	5.996	6.039	VV	22	341	0.08%	0.056%
18	6.069	6.039	6.077	PV	27	372	0.09%	0.061%
19	6.082	6.077	6.096	VV	23	184	0.04%	0.030%
20	6.112	6.096	6.124	VV	23	315	0.07%	0.052%
21	6.135	6.124	6.149	VV	29	315	0.07%	0.052%
22	6.161	6.149	6.171	VV	30	289	0.07%	0.047%
23	6.187	6.171	6.218	VV	39	624	0.14%	0.102%
24	6.334	6.218	6.378	VV	99	5581	1.29%	0.916%
25	6.388	6.378	6.445	VV	70	1962	0.45%	0.322%
26	6.456	6.445	6.461	VV	28	239	0.06%	0.039%
27	6.466	6.461	6.502	VV	29	584	0.13%	0.096%
28	6.517	6.502	6.536	VV	26	430	0.10%	0.071%
29	6.556	6.536	6.586	VV	37	564	0.13%	0.093%
30	6.605	6.586	6.622	PV	19	258	0.06%	0.042%
31	6.645	6.622	6.673	VV	24	621	0.14%	0.102%
32	6.686	6.673	6.705	VV	29	428	0.10%	0.070%
33	6.721	6.705	6.800	VV	30	1275	0.29%	0.209%
34	6.928	6.904	6.954	VV	32	786	0.18%	0.129%
35	6.973	6.954	7.000	VV	45	734	0.17%	0.121%
36	7.081	7.000	7.144	VV	43	2697	0.62%	0.443%

					rteres			
37	7.161	7.144	7.208	VV	36	1101	0.25%	0.181%
38	7.246	7.208	7.293	VV	37	1135	0.26%	0.186%
39	7.391	7.293	7.521	VV	46	4045	0.93%	0.664%
40	7.543	7.521	7.565	VV	36	564	0.13%	0.093%
41	7.589	7.565	7.610	PV	26	521	0.12%	0.086%
42	7.729	7.610	7.755	VV	62	4004	0.92%	0.657%
43	7.765	7.755	7.823	VV	62	2126	0.49%	0.349%
44	7.866	7.823	7.974	VV	97	5921	1.36%	0.972%
45	8.041	7.974	8.079	VV	89	4329	1.00%	0.711%
46	8.103	8.079	8.139	VV	95	2929	0.68%	0.481%
47	8.161	8.139	8.190	VV	89	2398	0.55%	0.394%
48	8.217	8.190	8.241	VV	85	2394	0.55%	0.393%
49	8.262	8.241	8.287	VV	99	2206	0.51%	0.362%
50	8.301	8.287	8.348	VV	79	2629	0.61%	0.432%
51	8.376	8.348	8.390	VV	94	2000	0.46%	0.328%
52	8.449	8.390	8.512	VV	88	5487	1.26%	0.901%
53	8.546	8.512	8.622	VV	75	3892	0.90%	0.639%
54	8.793	8.622	9.107	VV	7257	433838	100.00%	71.235%
55	9.139	9.107	9.165	VV	118	3552	0.82%	0.583%
56	9.199	9.165	9.249	VV	109	4729	1.09%	0.776%
57	9.274	9.249	9.292	VV	87	2023	0.47%	0.332%
58	9.400	9.292	9.530	VV	165	14042	3.24%	2.306%
59	9.544	9.530	9.567	VV	47	829	0.19%	0.136%
60	9.588	9.567	9.602	VV	35	642	0.15%	0.105%
61	9.622	9.602	9.672	VV	58	1541	0.36%	0.253%
62	9.686	9.672	9.734	VV	36	1056	0.24%	0.173%
63	9.750	9.734	9.773	VV	33	599	0.14%	0.098%
64	9.842	9.773	9.889	VV	49	1900	0.44%	0.312%
65	9.904	9.889	9.926	VV	22	315	0.07%	0.052%
66	9.965	9.926	10.004	VV	34	785	0.18%	0.129%
67	10.070	10.004	10.089	VV	32	849	0.20%	0.139%
68	10.109	10.089	10.122	VV	35	439	0.10%	0.072%
69	10.141	10.122	10.194	VV	62	1672	0.39%	0.275%
70	10.313	10.194	10.354	VV	100	6394	1.47%	1.050%
71	10.379	10.354	10.403	VV	95	2525	0.58%	0.415%
72	10.415	10.403	10.483	VV	80	3454	0.80%	0.567%
73	10.495	10.483	10.546	VV	69	2181	0.50%	0.358%
74	10.622	10.546	10.715	VV	258	15085	3.48%	2.477%
75	10.798	10.715	10.916	VV	242	18538	4.27%	3.044%
76	10.953	10.916	10.985	VV	83	2931	0.68%	0.481%
77	11.015	10.985	11.058	VV	74	2494	0.57%	0.410%
78	11.078	11.058	11.121	VV	51	1621	0.37%	0.266%
79	11.148	11.121	11.223	VV	53	2285	0.53%	0.375%
80	11.259	11.223	11.329	VV	40	1397	0.32%	0.229%
81	11.386	11.329	11.474	VV	29	1599	0.37%	0.263%
82	11.521	11.474	11.535	VV	38	871	0.20%	0.143%
83	11.550	11.535	11.570	VV	26	388	0.09%	0.064%
84	11.595	11.570	11.618	VV	35	616	0.14%	0.101%
85	11.653	11.618	11.671	VV	40	897	0.21%	0.147%
86	11.696	11.671	11.710	VV	45	809	0.19%	0.133%
87	11.735	11.710	11.757	VV	58	1276	0.29%	0.210%
88	11.765	11.757	11.786	VV	47	686	0.16%	0.113%
89	11.798	11.786	11.818	VV	33	586	0.14%	0.096%

					rteres			
90	11.883	11.818	11.949	VV	117	5342	1.23%	0.877%
91	11.967	11.949	11.985	VV	36	466	0.11%	0.077%
92	11.997	11.985	12.016	PV	25	313	0.07%	0.051%
93	12.114	12.016	12.151	VV	44	2663	0.61%	0.437%
94	12.163	12.151	12.194	VV	37	588	0.14%	0.097%
95	12.336	12.194	12.408	VV	50	3709	0.85%	0.609%
96	12.441	12.408	12.583	VV	60	5010	1.15%	0.823%
97	12.597	12.583	12.630	VV	63	1144	0.26%	0.188%
98	12.649	12.630	12.680	VV	40	1062	0.24%	0.174%
99	12.768	12.680	12.847	VV	92	5649	1.30%	0.928%
100	12.865	12.847	12.898	VV	47	894	0.21%	0.147%
101	12.921	12.898	12.937	VV	37	557	0.13%	0.091%
102	13.060	12.937	13.117	VV	100	5249	1.21%	0.862%
103	13.188	13.117	13.297	VV	291	14258	3.29%	2.341%
104	13.332	13.297	13.376	VV	24	596	0.14%	0.098%
105	13.527	13.376	13.548	VV	45	1933	0.45%	0.317%
106	13.587	13.548	13.606	VV	45	1324	0.31%	0.217%
107	13.639	13.606	13.664	VV	38	1152	0.27%	0.189%
108	13.709	13.664	13.760	VV	41	1978	0.46%	0.325%
109	13.769	13.760	13.801	VV	40	834	0.19%	0.137%
110	13.815	13.801	13.843	VV	42	785	0.18%	0.129%
111	13.921	13.843	13.982	VV	159	7906	1.82%	1.298%
112	14.115	13.982	14.324	VV	552	49903	11.50%	8.194%
113	14.340	14.324	14.361	PV	34	308	0.07%	0.051%
114	14.442	14.361	14.474	VV	41	1877	0.43%	0.308%
115	14.522	14.474	14.601	VV	67	2797	0.64%	0.459%
116	14.689	14.601	14.712	VV	50	2578	0.59%	0.423%
117	14.715	14.712	14.757	VV	52	909	0.21%	0.149%
118	14.777	14.757	14.831	VV	27	1016	0.23%	0.167%
119	14.851	14.831	14.888	VV	25	596	0.14%	0.098%
120	14.910	14.888	14.935	PV	47	698	0.16%	0.115%
121	15.030	14.935	15.137	VV	146	10507	2.42%	1.725%
122	15.186	15.137	15.233	VV	57	2962	0.68%	0.486%
123	15.251	15.233	15.268	VV	49	982	0.23%	0.161%
124	15.427	15.268	15.445	VV	237	12288	2.83%	2.018%
125	15.490	15.445	15.663	VV	244	17537	4.04%	2.880%
126	15.720	15.663	15.747	VV	48	1872	0.43%	0.307%
127	15.783	15.747	15.796	VV	40	1015	0.23%	0.167%
128	15.870	15.796	15.892	VV	61	2744	0.63%	0.450%
129	15.929	15.892	16.074	VV	95	4917	1.13%	0.807%
				Sum of corrected areas:		609024		

FB120525.M Tue Dec 09 04:25:04 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/20/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP14-112025	SDG No.:	Q3741
Lab Sample ID:	Q3741-03	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	87.3
Sample Wt/Vol:	4.55 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	10.0	U	1	10.0	57.0	ug/kg	12/08/25 17:03	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	17.2			50 - 150	86%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032412.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 17:03
Operator : YP/AJ
Sample : Q3741-03
Misc : 4.55G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP14-112025

Integration File: Calibration.e
Quant Time: Dec 09 03:06:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	387927	17.219 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032412.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 17:03
Operator : YP/AJ
Sample : Q3741-03
Misc : 4.55G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP14-112025

Integration File: Calibration.e
Quant Time: Dec 09 03:06:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

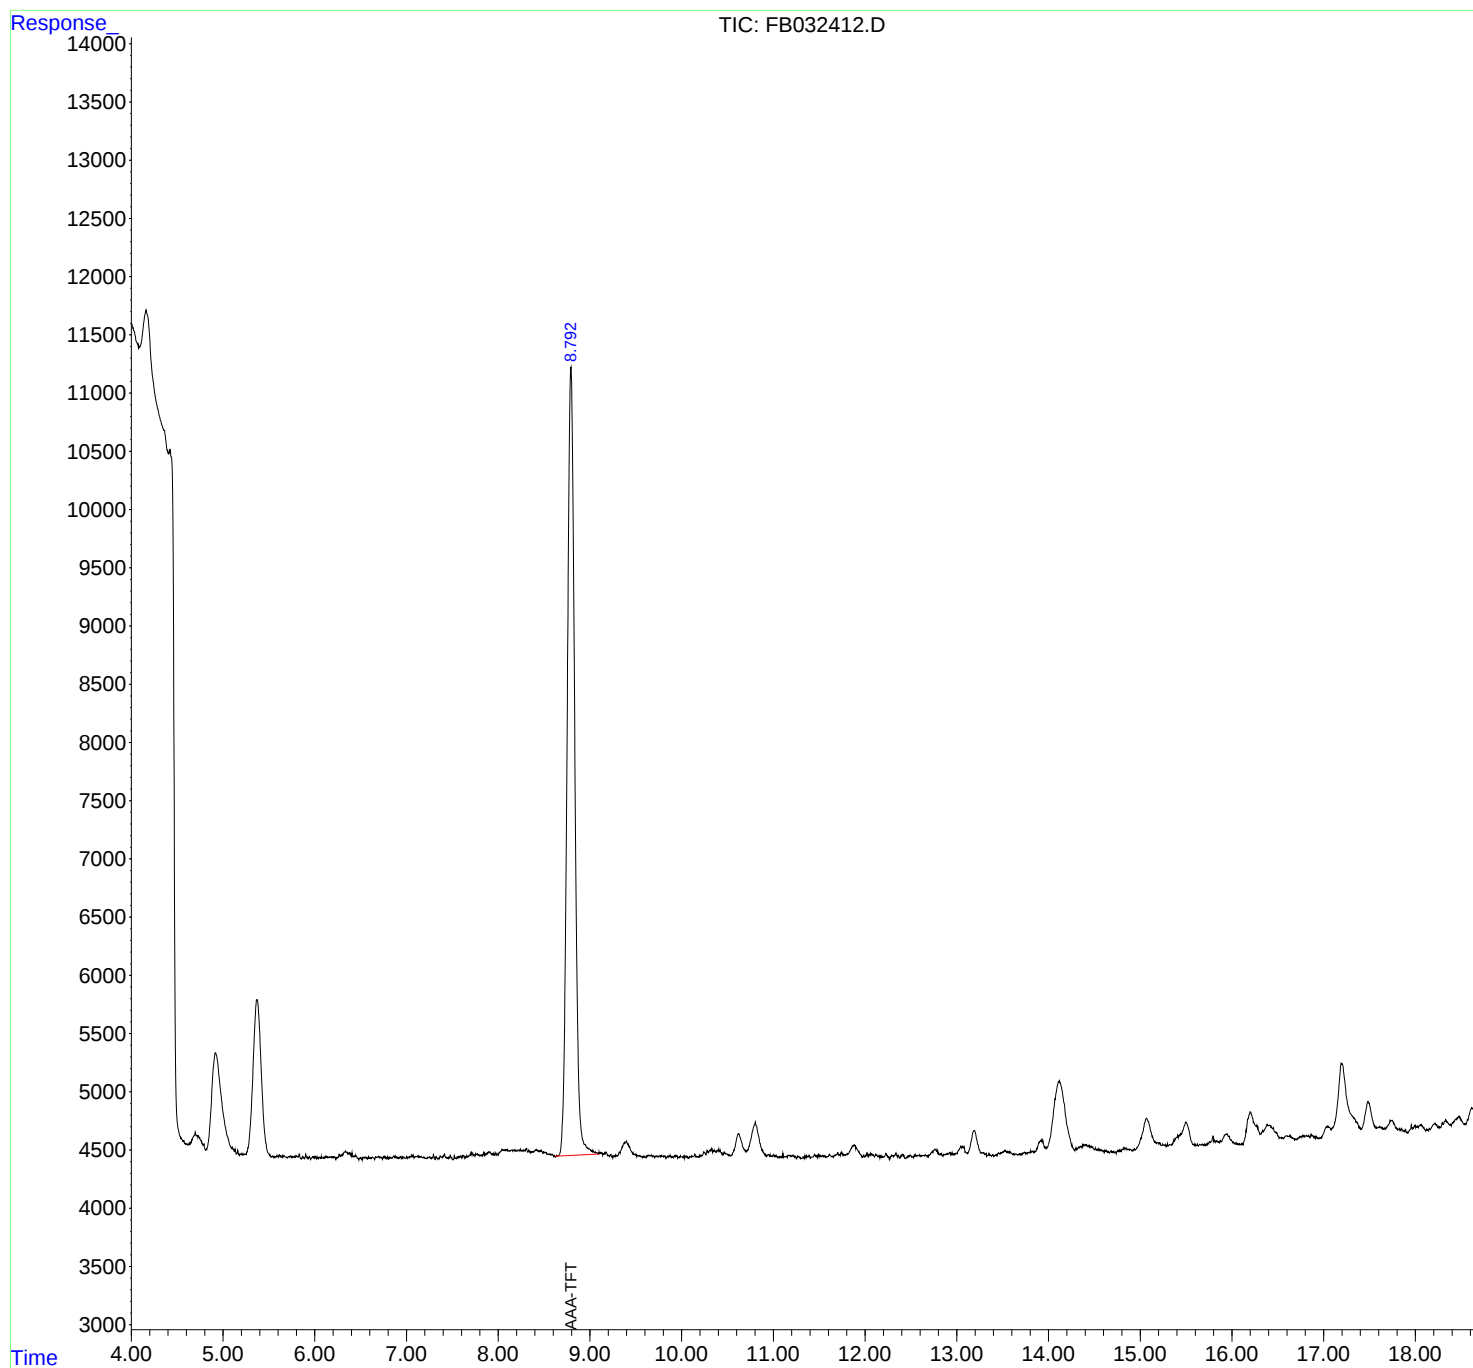

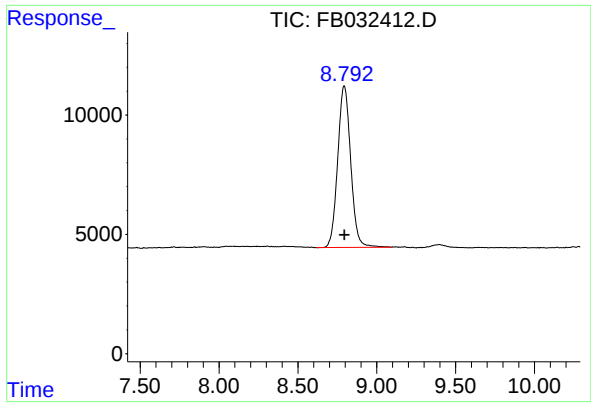

#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 387927
Conc: 17.22 ng/ml

Instrument :
FID_B
ClientSampleId :
B50-SP14-112025

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032412.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 17:03
 Sample : Q3741-03
 Misc : 4.55G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.423	4.370	4.598	BV	1292	-58187	-14.62%	-8.700%
2	4.603	4.598	4.636	PV	4	74	0.02%	0.011%
3	4.699	4.636	4.713	VV	125	3219	0.81%	0.481%
4	4.721	4.713	4.813	VV	106	3867	0.97%	0.578%
5	5.102	5.094	5.147	VV	52	1115	0.28%	0.167%
6	5.161	5.147	5.181	VV	36	251	0.06%	0.037%
7	5.590	5.531	5.600	VV	14	210	0.05%	0.031%
8	5.615	5.600	5.640	VV	23	299	0.08%	0.045%
9	5.666	5.640	5.701	VV	19	362	0.09%	0.054%
10	5.736	5.701	5.751	VV	21	358	0.09%	0.054%
11	5.765	5.751	5.774	VV	15	168	0.04%	0.025%
12	5.783	5.774	5.823	VV	22	502	0.13%	0.075%
13	5.832	5.823	5.859	VV	42	353	0.09%	0.053%
14	5.872	5.859	5.886	PV	21	164	0.04%	0.025%
15	5.903	5.886	5.935	VV	41	524	0.13%	0.078%
16	5.944	5.935	5.957	VV	23	174	0.04%	0.026%
17	5.977	5.957	5.987	PV	25	261	0.07%	0.039%
18	5.993	5.987	6.023	VV	28	415	0.10%	0.062%
19	6.032	6.023	6.040	VV	20	134	0.03%	0.020%
20	6.049	6.040	6.099	VV	20	522	0.13%	0.078%
21	6.124	6.099	6.154	VV	26	634	0.16%	0.095%
22	6.163	6.154	6.171	VV	24	205	0.05%	0.031%
23	6.184	6.171	6.229	VV	24	690	0.17%	0.103%
24	6.268	6.229	6.284	VV	47	800	0.20%	0.120%
25	6.338	6.284	6.397	VV	71	3536	0.89%	0.529%
26	6.407	6.397	6.435	VV	58	783	0.20%	0.117%
27	6.449	6.435	6.482	VV	37	564	0.14%	0.084%
28	6.498	6.482	6.524	VV	16	260	0.07%	0.039%
29	6.532	6.524	6.579	VV	20	504	0.13%	0.075%
30	6.588	6.579	6.614	VV	24	291	0.07%	0.044%
31	6.630	6.614	6.654	VV	21	366	0.09%	0.055%
32	6.664	6.654	6.670	VV	24	156	0.04%	0.023%
33	6.695	6.670	6.737	VV	27	782	0.20%	0.117%
34	6.757	6.737	6.782	VV	27	483	0.12%	0.072%
35	6.796	6.782	6.806	VV	18	212	0.05%	0.032%
36	6.940	6.928	6.949	VV	28	275	0.07%	0.041%

					rteres				
37	6.973	6.949	6.989	VV	21	423	0.11%	0.063%	
38	7.001	6.989	7.019	VV	24	305	0.08%	0.046%	
39	7.062	7.019	7.085	VV	38	1044	0.26%	0.156%	
40	7.102	7.085	7.110	VV	27	378	0.09%	0.057%	
41	7.121	7.110	7.152	VV	30	635	0.16%	0.095%	
42	7.162	7.152	7.181	VV	29	380	0.10%	0.057%	
43	7.191	7.181	7.225	VV	20	399	0.10%	0.060%	
44	7.235	7.225	7.242	VV	20	166	0.04%	0.025%	
45	7.254	7.242	7.270	VV	24	311	0.08%	0.046%	
46	7.295	7.270	7.313	VV	42	535	0.13%	0.080%	
47	7.324	7.313	7.345	VV	27	300	0.08%	0.045%	
48	7.369	7.345	7.396	VV	31	607	0.15%	0.091%	
49	7.415	7.396	7.443	VV	49	815	0.20%	0.122%	
50	7.479	7.443	7.512	VV	39	684	0.17%	0.102%	
51	7.524	7.512	7.546	PV	24	297	0.07%	0.044%	
52	7.572	7.546	7.579	VV	26	413	0.10%	0.062%	
53	7.592	7.579	7.607	VV	31	431	0.11%	0.064%	
54	7.623	7.607	7.651	VV	35	680	0.17%	0.102%	
55	7.714	7.651	7.746	VV	64	2196	0.55%	0.328%	
56	7.769	7.746	7.802	VV	49	1394	0.35%	0.208%	
57	7.811	7.802	7.819	VV	41	362	0.09%	0.054%	
58	7.846	7.819	7.855	VV	66	938	0.24%	0.140%	
59	7.898	7.855	7.947	VV	67	2955	0.74%	0.442%	
60	7.952	7.947	7.963	VV	53	430	0.11%	0.064%	
61	7.970	7.963	7.999	VV	57	975	0.25%	0.146%	
62	8.053	7.999	8.063	VV	83	2663	0.67%	0.398%	
63	8.071	8.063	8.082	VV	85	945	0.24%	0.141%	
64	8.100	8.082	8.131	VV	85	2311	0.58%	0.345%	
65	8.151	8.131	8.159	VV	84	1335	0.34%	0.200%	
66	8.177	8.159	8.206	VV	82	2186	0.55%	0.327%	
67	8.221	8.206	8.264	VV	83	2691	0.68%	0.402%	
68	8.287	8.264	8.297	VV	82	1548	0.39%	0.232%	
69	8.310	8.297	8.325	VV	94	1364	0.34%	0.204%	
70	8.335	8.325	8.379	VV	79	2175	0.55%	0.325%	
71	8.417	8.379	8.437	VV	87	2652	0.67%	0.397%	
72	8.445	8.437	8.453	VV	78	718	0.18%	0.107%	
73	8.470	8.453	8.492	VV	78	1609	0.40%	0.241%	
74	8.502	8.492	8.556	VV	65	2069	0.52%	0.309%	
75	8.568	8.556	8.577	VV	48	553	0.14%	0.083%	
76	8.589	8.577	8.626	VV	48	1024	0.26%	0.153%	
77	8.641	8.626	8.648	VV	35	391	0.10%	0.058%	
78	8.794	8.648	9.094	VV	6804	397984	100.00%	59.506%	
79	9.102	9.094	9.149	VV	62	1729	0.43%	0.259%	
80	9.178	9.149	9.215	VV	63	1798	0.45%	0.269%	
81	9.229	9.215	9.251	VV	44	621	0.16%	0.093%	
82	9.280	9.251	9.302	VV	38	891	0.22%	0.133%	
83	9.400	9.302	9.526	VV	156	11252	2.83%	1.682%	
84	9.536	9.526	9.585	VV	31	872	0.22%	0.130%	
85	9.592	9.585	9.605	VV	27	243	0.06%	0.036%	
86	9.637	9.605	9.645	VV	37	660	0.17%	0.099%	
87	9.653	9.645	9.684	VV	35	720	0.18%	0.108%	
88	9.697	9.684	9.708	VV	30	372	0.09%	0.056%	
89	9.731	9.708	9.749	VV	30	584	0.15%	0.087%	

					rteres				
90	9.759	9.749	9.776	VV	30	411	0.10%	0.061%	
91	9.784	9.776	9.805	VV	30	464	0.12%	0.069%	
92	9.814	9.805	9.836	VV	30	407	0.10%	0.061%	
93	9.852	9.836	9.866	VV	29	414	0.10%	0.062%	
94	9.875	9.866	9.894	VV	34	405	0.10%	0.061%	
95	9.903	9.894	9.912	VV	24	208	0.05%	0.031%	
96	9.933	9.912	9.959	VV	34	707	0.18%	0.106%	
97	9.989	9.959	10.034	VV	27	909	0.23%	0.136%	
98	10.042	10.034	10.054	VV	26	263	0.07%	0.039%	
99	10.059	10.054	10.078	VV	27	248	0.06%	0.037%	
100	10.093	10.078	10.107	VV	24	301	0.08%	0.045%	
101	10.146	10.107	10.177	VV	44	1058	0.27%	0.158%	
102	10.202	10.177	10.224	VV	38	769	0.19%	0.115%	
103	10.243	10.224	10.268	VV	61	1280	0.32%	0.191%	
104	10.279	10.268	10.295	VV	77	1013	0.25%	0.152%	
105	10.329	10.295	10.341	VV	90	2056	0.52%	0.307%	
106	10.354	10.341	10.375	VV	79	1393	0.35%	0.208%	
107	10.401	10.375	10.449	VV	81	2897	0.73%	0.433%	
108	10.467	10.449	10.540	VV	55	2280	0.57%	0.341%	
109	10.623	10.540	10.708	VV	219	12183	3.06%	1.822%	
110	10.804	10.708	10.935	VV	312	20447	5.14%	3.057%	
111	10.947	10.935	10.976	VV	39	775	0.19%	0.116%	
112	10.997	10.976	11.016	VV	34	645	0.16%	0.096%	
113	11.032	11.016	11.053	VV	32	502	0.13%	0.075%	
114	11.090	11.053	11.100	VV	26	471	0.12%	0.070%	
115	11.106	11.100	11.129	VV	45	417	0.10%	0.062%	
116	11.144	11.129	11.152	VV	22	277	0.07%	0.041%	
117	11.163	11.152	11.171	VV	33	295	0.07%	0.044%	
118	11.177	11.171	11.199	VV	32	442	0.11%	0.066%	
119	11.210	11.199	11.253	VV	33	725	0.18%	0.108%	
120	11.272	11.253	11.309	PV	25	444	0.11%	0.066%	
121	11.325	11.309	11.345	VV	20	256	0.06%	0.038%	
122	11.365	11.345	11.383	VV	29	474	0.12%	0.071%	
123	11.392	11.383	11.409	VV	32	293	0.07%	0.044%	
124	11.450	11.409	11.479	VV	35	966	0.24%	0.144%	
125	11.496	11.479	11.523	VV	42	699	0.18%	0.104%	
126	11.536	11.523	11.573	VV	29	714	0.18%	0.107%	
127	11.612	11.573	11.640	VV	40	986	0.25%	0.147%	
128	11.652	11.640	11.659	VV	25	259	0.07%	0.039%	
129	11.703	11.659	11.731	VV	55	1526	0.38%	0.228%	
130	11.741	11.731	11.786	VV	58	1254	0.32%	0.188%	
131	11.884	11.786	11.975	VV	120	7741	1.94%	1.157%	
132	11.987	11.975	11.996	VV	32	283	0.07%	0.042%	
133	12.023	11.996	12.035	VV	54	717	0.18%	0.107%	
134	12.048	12.035	12.055	VV	36	369	0.09%	0.055%	
135	12.063	12.055	12.084	VV	46	665	0.17%	0.099%	
136	12.091	12.084	12.104	VV	36	341	0.09%	0.051%	
137	12.118	12.104	12.144	VV	38	658	0.17%	0.098%	
138	12.158	12.144	12.192	VV	29	555	0.14%	0.083%	
139	12.229	12.192	12.264	VV	47	999	0.25%	0.149%	
140	12.290	12.264	12.311	PV	31	540	0.14%	0.081%	
141	12.337	12.311	12.358	VV	49	848	0.21%	0.127%	

					rt	eres		
142	12.363	12.358	12.379	VV	25	214	0.05%	0.032%
143	12.406	12.379	12.442	VV	34	690	0.17%	0.103%
144	12.496	12.442	12.515	PV	30	735	0.18%	0.110%
145	12.595	12.515	12.616	VV	28	1263	0.32%	0.189%
146	12.632	12.616	12.648	VV	23	406	0.10%	0.061%
147	12.660	12.648	12.684	VV	26	461	0.12%	0.069%
148	12.764	12.684	12.851	VV	75	4163	1.05%	0.622%
149	12.923	12.851	12.979	VV	36	2242	0.56%	0.335%
150	13.045	12.979	13.115	VV	90	4833	1.21%	0.723%
151	13.191	13.115	13.333	VV	228	12050	3.03%	1.802%
152	13.352	13.333	13.407	VV	28	470	0.12%	0.070%
153	13.527	13.407	13.629	VV	52	3414	0.86%	0.511%
154	13.647	13.629	13.669	VV	16	289	0.07%	0.043%
155	13.684	13.669	13.700	VV	18	224	0.06%	0.034%
156	13.740	13.700	13.761	VV	29	695	0.17%	0.104%
157	13.830	13.761	13.847	VV	36	1412	0.35%	0.211%
158	13.935	13.847	13.981	VV	129	6652	1.67%	0.995%
159	14.119	13.981	14.312	VV	626	58474	14.69%	8.743%
160	14.380	14.312	14.532	VV	84	8014	2.01%	1.198%
161	14.552	14.532	14.608	VV	40	1345	0.34%	0.201%
162	14.628	14.608	14.665	VV	24	603	0.15%	0.090%
163	14.684	14.665	14.741	VV	18	517	0.13%	0.077%
164	14.829	14.741	14.911	PV	42	2499	0.63%	0.374%
165	15.070	14.911	15.176	VV	283	20128	5.06%	3.010%
166	15.188	15.176	15.236	VV	68	2083	0.52%	0.311%
167	15.248	15.236	15.311	VV	46	1757	0.44%	0.263%
168	15.501	15.311	15.636	VV	225	18687	4.70%	2.794%
169	15.652	15.636	15.663	VV	26	346	0.09%	0.052%
170	15.678	15.663	15.704	VV	29	523	0.13%	0.078%
171	15.795	15.704	15.824	VV	91	2864	0.72%	0.428%
172	15.834	15.824	15.868	VV	48	1062	0.27%	0.159%
173	15.944	15.868	16.105	VV	98	6108	1.53%	0.913%
						Sum of corrected areas:	668813	

FB120525.M Tue Dec 09 04:25:57 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/24/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP9-112425	SDG No.:	Q3741
Lab Sample ID:	Q3741-04	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	85.2
Sample Wt/Vol:	5.07 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	10.0	U	1	10.0	52.0	ug/kg	12/08/25 14:17	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	17.7			50 - 150	89%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032407.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 14:17
Operator : YP/AJ
Sample : Q3741-04
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP9-112425

Integration File: Calibration.e
Quant Time: Dec 09 03:05:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	399708	17.742 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032407.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 14:17
Operator : YP/AJ
Sample : Q3741-04
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP9-112425

Integration File: Calibration.e
Quant Time: Dec 09 03:05:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

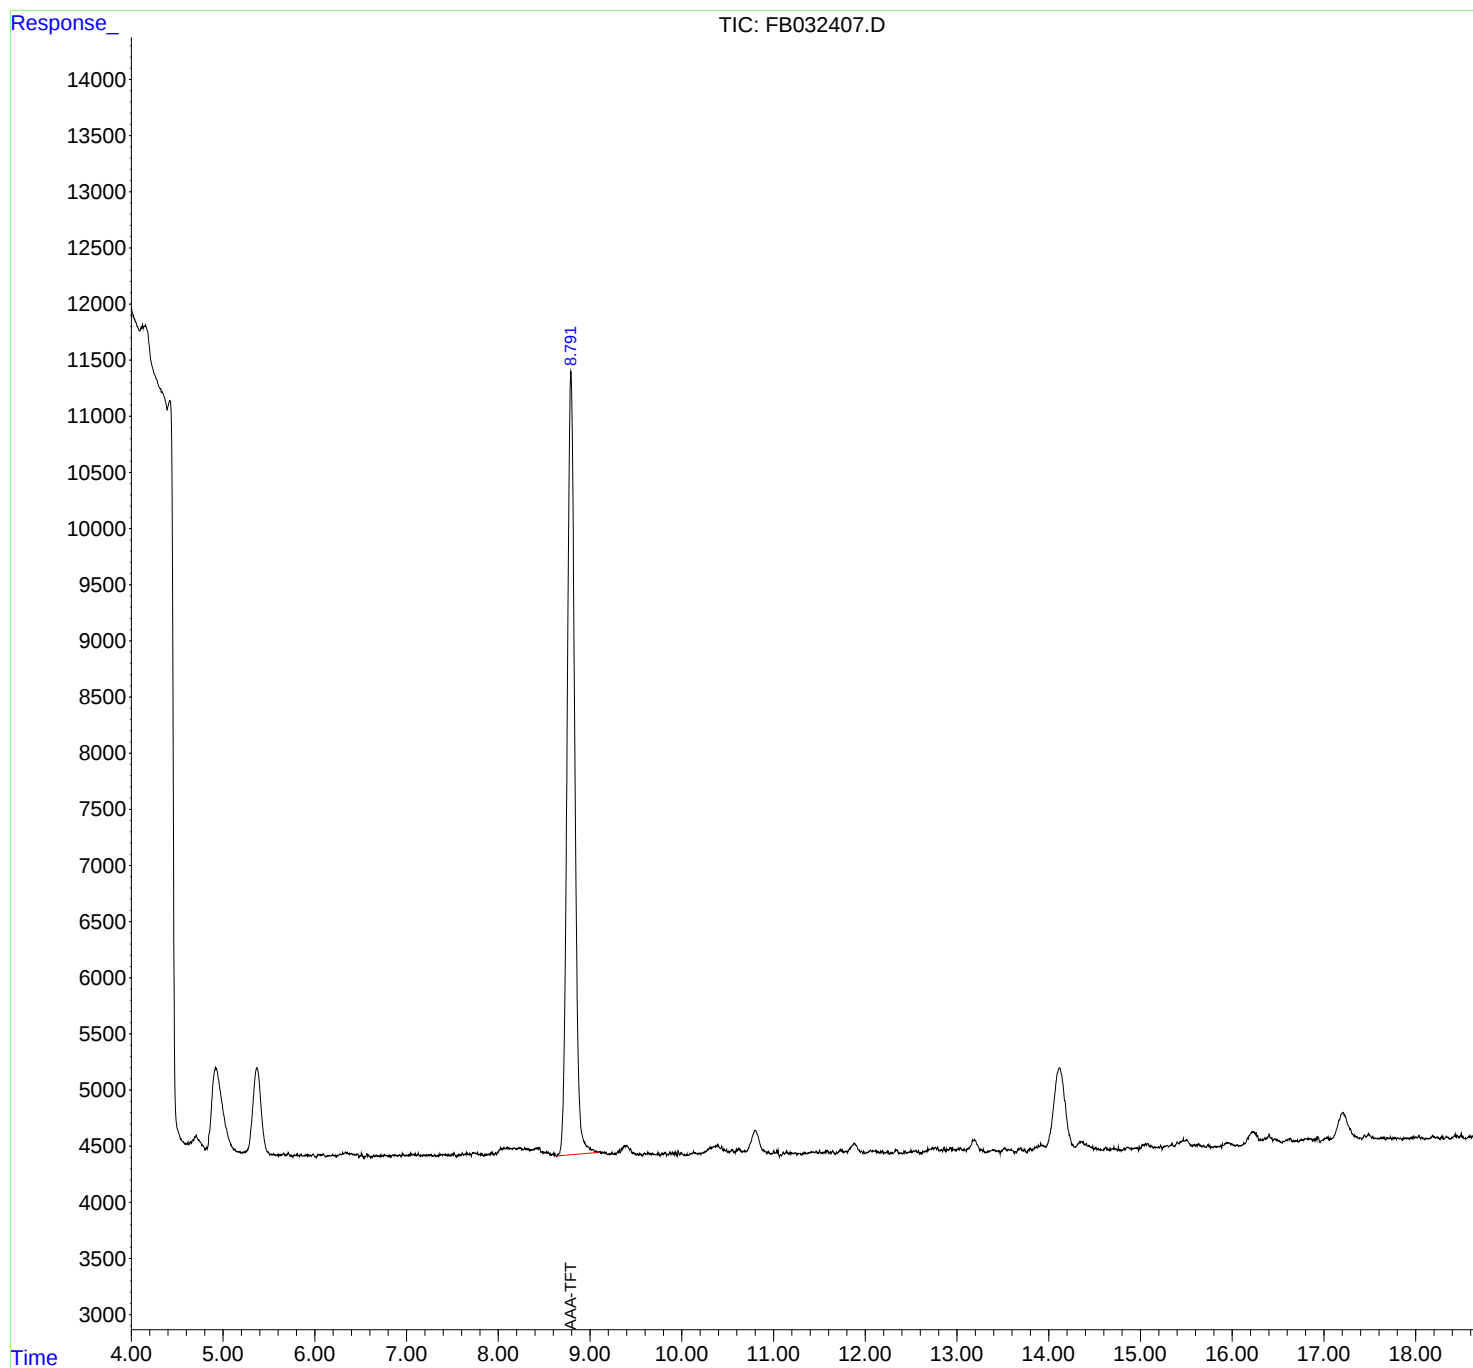

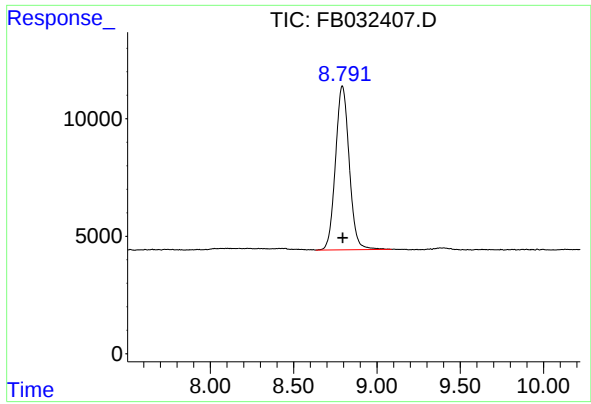

#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.002 min
Response: 399708
Conc: 17.74 ng/ml

Instrument :
FID_B
ClientSampleId :
B50-SP9-112425

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032407.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 14:17
 Sample : Q3741-04
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.421	4.353	4.591	BV	1851	-52794	-13.08%	-8.586%
2	4.598	4.591	4.606	PV	5	53	0.01%	0.009%
3	4.618	4.606	4.628	VV	25	156	0.04%	0.025%
4	4.645	4.628	4.660	VV	37	485	0.12%	0.079%
5	4.674	4.660	4.681	VV	63	683	0.17%	0.111%
6	4.709	4.681	4.808	VV	108	4314	1.07%	0.702%
7	5.175	5.166	5.220	VV	9	115	0.03%	0.019%
8	5.250	5.220	5.257	VV	19	228	0.06%	0.037%
9	5.527	5.510	5.537	VV	10	110	0.03%	0.018%
10	5.551	5.537	5.591	VV	14	209	0.05%	0.034%
11	5.601	5.591	5.609	VV	16	90	0.02%	0.015%
12	5.625	5.609	5.642	PV	13	202	0.05%	0.033%
13	5.662	5.642	5.694	VV	25	439	0.11%	0.071%
14	5.713	5.694	5.731	VV	38	408	0.10%	0.066%
15	5.741	5.731	5.759	VV	16	118	0.03%	0.019%
16	5.780	5.759	5.793	PV	15	204	0.05%	0.033%
17	5.812	5.793	5.833	VV	23	334	0.08%	0.054%
18	5.853	5.833	5.865	VV	24	301	0.07%	0.049%
19	5.884	5.865	5.892	VV	15	175	0.04%	0.028%
20	5.912	5.892	5.926	VV	22	329	0.08%	0.053%
21	5.952	5.926	5.961	VV	21	338	0.08%	0.055%
22	5.984	5.961	6.018	VV	32	537	0.13%	0.087%
23	6.094	6.018	6.124	PV	32	1110	0.27%	0.181%
24	6.194	6.124	6.253	VV	15	525	0.13%	0.085%
25	6.282	6.253	6.292	VV	17	264	0.07%	0.043%
26	6.305	6.292	6.319	VV	28	299	0.07%	0.049%
27	6.335	6.319	6.345	VV	32	374	0.09%	0.061%
28	6.354	6.345	6.427	VB	28	648	0.16%	0.105%
29	6.469	6.430	6.483	BV	24	334	0.08%	0.054%
30	6.511	6.483	6.554	PV	28	507	0.13%	0.082%
31	6.569	6.554	6.578	VV	34	347	0.09%	0.056%
32	6.585	6.578	6.611	VV	27	270	0.07%	0.044%
33	6.619	6.611	6.627	PV	14	66	0.02%	0.011%
34	6.645	6.627	6.667	PV	26	352	0.09%	0.057%
35	6.675	6.667	6.686	VV	22	189	0.05%	0.031%
36	6.690	6.686	6.711	VV	17	211	0.05%	0.034%

					rteres				
37	6.720	6.711	6.729	VV	27	162	0.04%	0.026%	
38	6.761	6.729	6.775	VV	26	518	0.13%	0.084%	
39	6.782	6.775	6.798	VV	21	216	0.05%	0.035%	
40	6.928	6.903	6.941	VV	25	393	0.10%	0.064%	
41	6.956	6.941	6.998	VV	33	678	0.17%	0.110%	
42	7.005	6.998	7.019	VV	22	215	0.05%	0.035%	
43	7.046	7.019	7.070	VV	37	765	0.19%	0.124%	
44	7.096	7.070	7.105	VV	35	504	0.12%	0.082%	
45	7.129	7.105	7.151	VV	36	578	0.14%	0.094%	
46	7.157	7.151	7.163	VV	22	125	0.03%	0.020%	
47	7.169	7.163	7.176	VV	20	127	0.03%	0.021%	
48	7.189	7.176	7.206	VV	24	325	0.08%	0.053%	
49	7.270	7.206	7.295	VV	24	952	0.24%	0.155%	
50	7.309	7.295	7.335	VV	25	360	0.09%	0.059%	
51	7.366	7.335	7.390	VV	27	625	0.15%	0.102%	
52	7.398	7.390	7.421	VV	27	430	0.11%	0.070%	
53	7.429	7.421	7.452	VV	28	365	0.09%	0.059%	
54	7.460	7.452	7.476	VV	28	252	0.06%	0.041%	
55	7.502	7.476	7.512	VV	31	437	0.11%	0.071%	
56	7.520	7.512	7.544	VV	38	415	0.10%	0.068%	
57	7.579	7.544	7.596	VV	26	536	0.13%	0.087%	
58	7.609	7.596	7.623	VV	38	427	0.11%	0.070%	
59	7.633	7.623	7.641	VV	27	241	0.06%	0.039%	
60	7.653	7.641	7.675	VV	43	650	0.16%	0.106%	
61	7.691	7.675	7.707	VV	31	499	0.12%	0.081%	
62	7.727	7.707	7.736	VV	42	569	0.14%	0.092%	
63	7.746	7.736	7.769	VV	41	652	0.16%	0.106%	
64	7.774	7.769	7.789	VV	43	365	0.09%	0.059%	
65	7.816	7.789	7.849	VV	31	724	0.18%	0.118%	
66	7.861	7.849	7.869	VV	22	221	0.05%	0.036%	
67	7.875	7.869	7.902	VV	24	440	0.11%	0.072%	
68	7.922	7.902	7.956	VV	40	905	0.22%	0.147%	
69	7.974	7.956	7.983	VV	41	469	0.12%	0.076%	
70	8.060	7.983	8.085	VV	83	3985	0.99%	0.648%	
71	8.106	8.085	8.130	VV	86	2129	0.53%	0.346%	
72	8.175	8.130	8.207	VV	81	3396	0.84%	0.552%	
73	8.224	8.207	8.276	VV	86	3045	0.75%	0.495%	
74	8.289	8.276	8.298	VV	83	972	0.24%	0.158%	
75	8.308	8.298	8.316	VV	76	754	0.19%	0.123%	
76	8.324	8.316	8.355	VV	75	1537	0.38%	0.250%	
77	8.414	8.355	8.425	VV	81	2870	0.71%	0.467%	
78	8.452	8.425	8.540	VV	83	3513	0.87%	0.571%	
79	8.548	8.540	8.578	VV	41	642	0.16%	0.104%	
80	8.590	8.578	8.598	VV	26	236	0.06%	0.038%	
81	8.605	8.598	8.643	VV	30	441	0.11%	0.072%	
82	8.792	8.643	9.016	VV	6996	403652	100.00%	65.649%	
83	9.032	9.016	9.088	VV	65	2202	0.55%	0.358%	
84	9.103	9.088	9.191	VV	44	2209	0.55%	0.359%	
85	9.402	9.191	9.503	VV	100	8812	2.18%	1.433%	
86	9.516	9.503	9.578	VV	27	704	0.17%	0.115%	
87	9.596	9.578	9.622	VV	29	604	0.15%	0.098%	
88	9.632	9.622	9.734	VV	26	1397	0.35%	0.227%	
89	9.747	9.734	9.764	VV	19	298	0.07%	0.048%	

					rteres			
90	9.813	9.764	9.859	VV	31	1060	0.26%	0.172%
91	9.873	9.859	9.926	VV	34	980	0.24%	0.159%
92	9.932	9.926	9.951	VV	33	270	0.07%	0.044%
93	9.963	9.951	9.978	VV	47	412	0.10%	0.067%
94	9.996	9.978	10.051	VV	31	714	0.18%	0.116%
95	10.130	10.051	10.174	VV	34	1518	0.38%	0.247%
96	10.315	10.174	10.329	VV	75	3899	0.97%	0.634%
97	10.393	10.329	10.521	VV	95	7810	1.93%	1.270%
98	10.549	10.521	10.580	VV	57	1515	0.38%	0.246%
99	10.634	10.580	10.666	VV	64	2504	0.62%	0.407%
100	10.801	10.666	10.927	VV	227	16358	4.05%	2.660%
101	10.947	10.927	10.983	VV	41	836	0.21%	0.136%
102	11.002	10.983	11.025	VV	45	696	0.17%	0.113%
103	11.036	11.025	11.088	VV	44	683	0.17%	0.111%
104	11.108	11.088	11.123	PV	32	371	0.09%	0.060%
105	11.141	11.123	11.169	VV	38	685	0.17%	0.111%
106	11.183	11.169	11.223	VV	27	647	0.16%	0.105%
107	11.241	11.223	11.257	VV	25	403	0.10%	0.066%
108	11.274	11.257	11.311	VV	19	473	0.12%	0.077%
109	11.337	11.311	11.379	VV	27	732	0.18%	0.119%
110	11.418	11.379	11.452	VV	34	1182	0.29%	0.192%
111	11.466	11.452	11.493	VV	39	640	0.16%	0.104%
112	11.504	11.493	11.534	VV	42	637	0.16%	0.104%
113	11.574	11.534	11.610	VV	38	1281	0.32%	0.208%
114	11.648	11.610	11.674	VV	41	870	0.22%	0.141%
115	11.729	11.674	11.763	VV	51	1547	0.38%	0.252%
116	11.790	11.763	11.807	VV	36	772	0.19%	0.126%
117	11.884	11.807	11.999	VV	98	6224	1.54%	1.012%
118	12.060	11.999	12.161	VV	41	2570	0.64%	0.418%
119	12.188	12.161	12.223	VV	36	752	0.19%	0.122%
120	12.243	12.223	12.264	VV	34	463	0.11%	0.075%
121	12.345	12.264	12.409	VV	39	1504	0.37%	0.245%
122	12.436	12.409	12.461	VV	28	491	0.12%	0.080%
123	12.553	12.461	12.614	VV	37	1839	0.46%	0.299%
124	12.764	12.614	12.826	VV	60	4701	1.16%	0.765%
125	12.860	12.826	12.882	VV	42	1150	0.28%	0.187%
126	12.930	12.882	12.990	VV	52	2448	0.61%	0.398%
127	13.039	12.990	13.079	VV	52	2021	0.50%	0.329%
128	13.192	13.079	13.316	VV	122	7987	1.98%	1.299%
129	13.399	13.316	13.474	VV	33	1868	0.46%	0.304%
130	13.524	13.474	13.580	VV	48	1862	0.46%	0.303%
131	13.594	13.580	13.650	VV	35	693	0.17%	0.113%
132	13.695	13.650	13.764	PV	43	1650	0.41%	0.268%
133	13.798	13.764	13.820	PV	40	823	0.20%	0.134%
134	13.916	13.820	13.975	VV	79	4737	1.17%	0.770%
135	14.118	13.975	14.284	VV	749	66430	16.46%	10.804%
136	14.357	14.284	14.496	VV	90	7454	1.85%	1.212%
137	14.513	14.496	14.589	VV	37	1105	0.27%	0.180%
138	14.622	14.589	14.652	VV	32	725	0.18%	0.118%
139	14.713	14.652	14.799	VV	26	1271	0.31%	0.207%
140	14.863	14.799	14.908	VV	33	1331	0.33%	0.216%
141	14.959	14.908	14.978	VV	24	817	0.20%	0.133%

					rteres				
142	15.077	14.978	15.175	PV	61	4322	1.07%	0.703%	
143	15.222	15.175	15.239	VV	44	964	0.24%	0.157%	
144	15.292	15.239	15.309	VV	40	1258	0.31%	0.205%	
145	15.347	15.309	15.375	VV	58	1506	0.37%	0.245%	
146	15.403	15.375	15.421	VV	68	1392	0.34%	0.226%	
147	15.468	15.421	15.484	VV	91	2654	0.66%	0.432%	
148	15.506	15.484	15.565	VV	86	2860	0.71%	0.465%	
149	15.636	15.565	15.673	VV	48	2091	0.52%	0.340%	
150	15.687	15.673	15.712	VV	30	484	0.12%	0.079%	
151	15.737	15.712	15.765	VV	30	627	0.16%	0.102%	
152	15.811	15.765	15.838	PV	18	505	0.13%	0.082%	
153	15.940	15.838	15.957	VV	41	1534	0.38%	0.250%	
154	15.968	15.957	16.037	VV	35	1023	0.25%	0.166%	
155	16.057	16.037	16.089	VV	13	156	0.04%	0.025%	

Sum of corrected areas: 614860

FB120525.M Tue Dec 09 04:24:07 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/25/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP11-112525	SDG No.:	Q3741
Lab Sample ID:	Q3741-05	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	84.6
Sample Wt/Vol:	5.43 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	3500		50	450	2450	ug/kg	12/09/25 12:25	FB120925
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	25.1			50 - 150	125%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032420.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 12:25
Operator : YP/AJ
Sample : Q3741-05 50X
Misc : 5.43G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP11-112525

Integration File: Calibration.e
Quant Time: Dec 10 00:39:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	564270	25.046 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032420.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 12:25
Operator : YP/AJ
Sample : Q3741-05 50X
Misc : 5.43G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP11-112525

Integration File: Calibration.e
Quant Time: Dec 10 00:39:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

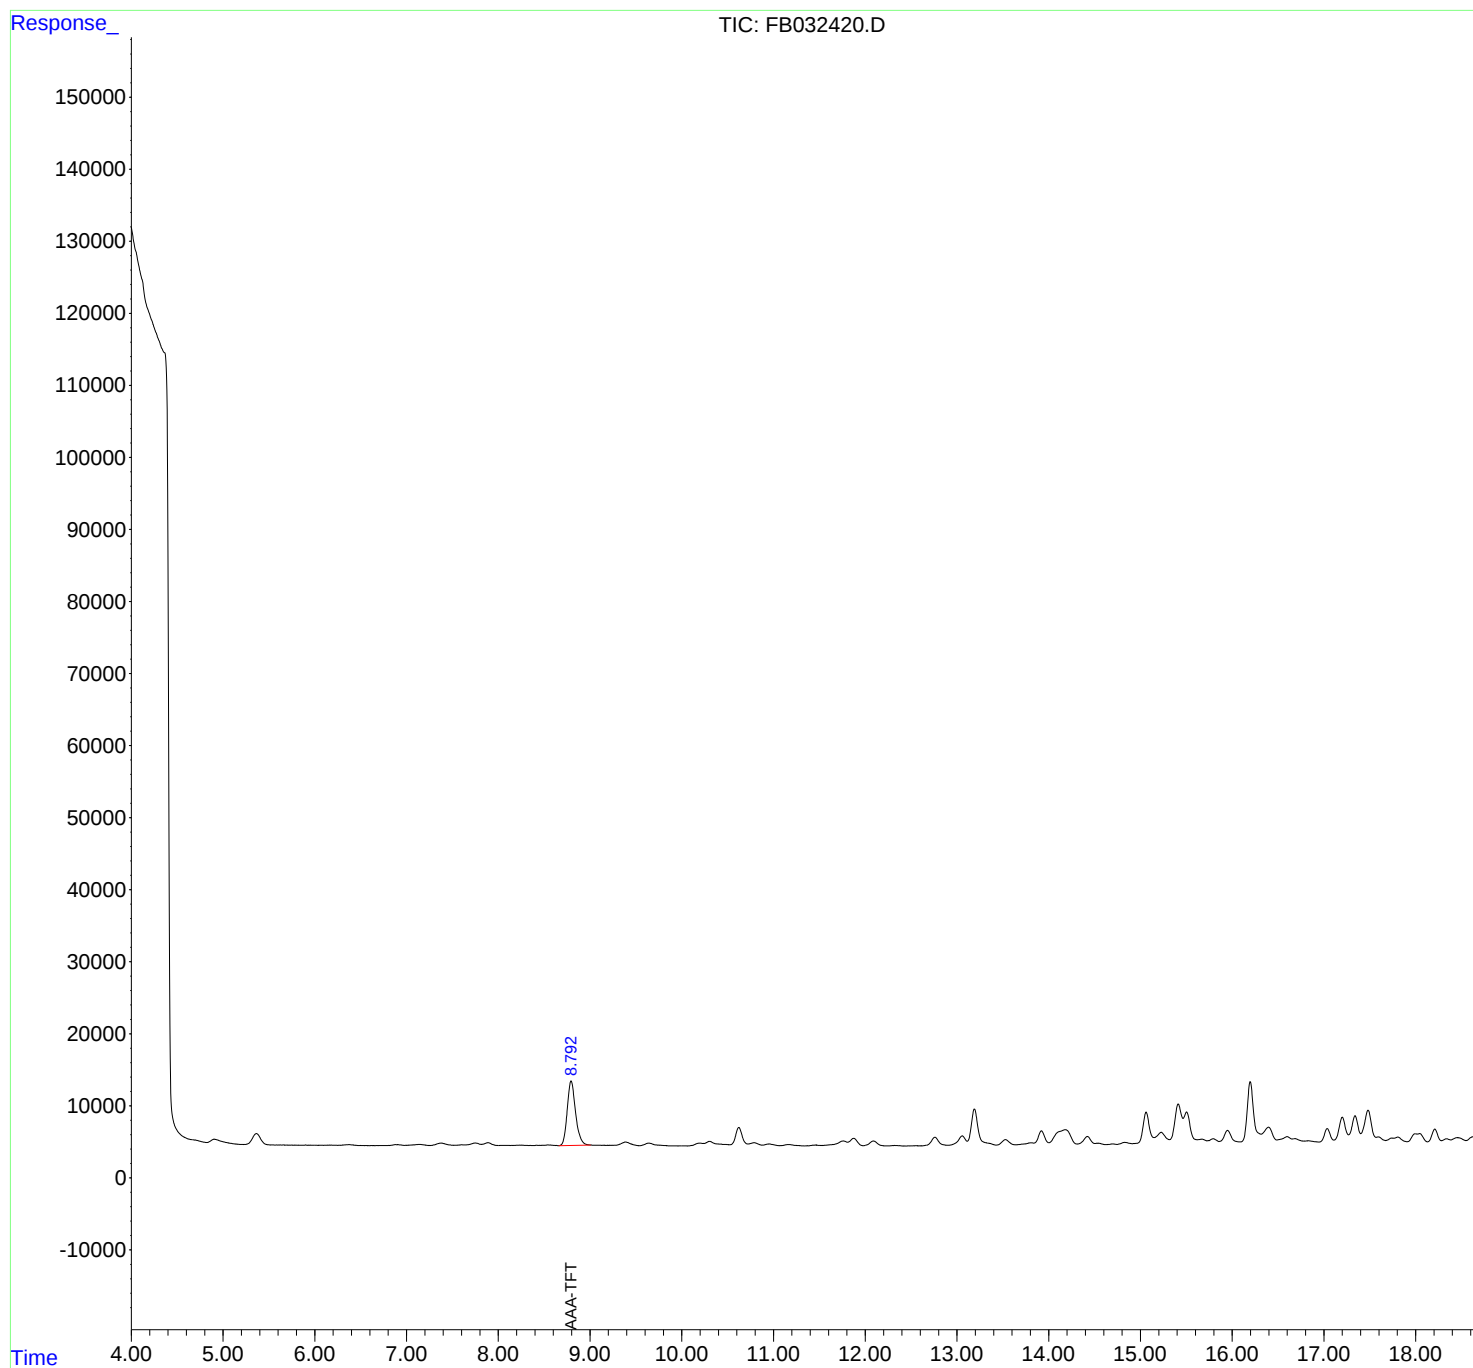

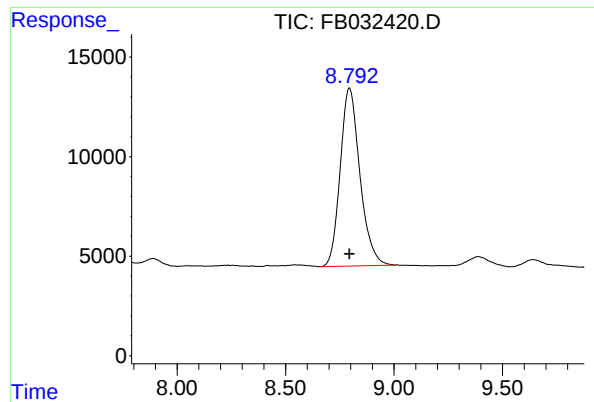

#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 564270
Conc: 25.05 ng/ml

Instrument :

FID_B

ClientSampleId :

B50-SP11-112525

rteres

Area Percent

Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032420.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 12:25
 Sample : Q3741-05 50X
 Misc : 5.43G/5.00 ML MEOH
 ALS Vial : 5 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	5.191	5.182	5.201	PV	11	70	0.01%	0.002%
2	5.215	5.201	5.225	PV	18	141	0.02%	0.004%
3	5.235	5.225	5.244	VV	17	130	0.02%	0.004%
4	5.550	5.545	5.564	VV	30	174	0.03%	0.006%
5	5.586	5.564	5.599	PV	17	198	0.03%	0.006%
6	5.623	5.599	5.644	VV	26	449	0.08%	0.014%
7	5.665	5.644	5.678	VV	33	417	0.07%	0.013%
8	5.687	5.678	5.734	VV	19	401	0.07%	0.013%
9	5.745	5.734	5.766	VV	24	283	0.05%	0.009%
10	5.796	5.766	5.808	VV	26	293	0.05%	0.009%
11	5.821	5.808	5.829	PV	19	112	0.02%	0.004%
12	5.877	5.829	5.884	VV	20	460	0.08%	0.015%
13	5.899	5.884	5.925	VV	51	614	0.11%	0.019%
14	5.953	5.925	5.999	VV	30	968	0.17%	0.031%
15	6.009	5.999	6.035	VV	26	412	0.07%	0.013%
16	6.060	6.035	6.074	VV	26	411	0.07%	0.013%
17	6.082	6.074	6.096	VV	21	241	0.04%	0.008%
18	6.137	6.096	6.152	VV	44	1082	0.19%	0.034%
19	6.166	6.152	6.173	VV	53	617	0.11%	0.020%
20	6.181	6.173	6.199	VV	52	704	0.12%	0.022%
21	6.217	6.199	6.251	VV	47	1133	0.20%	0.036%
22	6.268	6.251	6.281	VV	38	597	0.10%	0.019%
23	6.305	6.281	6.312	VV	77	911	0.16%	0.029%
24	6.378	6.312	6.493	VV	144	8378	1.44%	0.265%
25	6.502	6.493	6.516	VV	23	176	0.03%	0.006%
26	6.532	6.516	6.558	VV	19	189	0.03%	0.006%

rteres								
27	6.566	6.558	6.583	VV	7	60	0.01%	0.002%
28	6.591	6.583	6.601	PV	6	41	0.01%	0.001%
29	6.621	6.601	6.633	VV	20	232	0.04%	0.007%
30	6.641	6.633	6.657	VV	16	133	0.02%	0.004%
31	6.678	6.657	6.694	PV	23	314	0.05%	0.010%
32	6.705	6.694	6.714	VV	22	193	0.03%	0.006%
33	6.723	6.714	6.764	VV	22	596	0.10%	0.019%
34	6.809	6.764	6.817	VV	53	951	0.16%	0.030%
35	6.907	6.890	6.982	VV	155	5786	1.00%	0.183%
36	6.993	6.982	7.005	VV	69	819	0.14%	0.026%
37	7.132	7.005	7.272	VV	188	17817	3.07%	0.564%
38	7.380	7.272	7.499	VV	376	28775	4.95%	0.910%
39	7.506	7.499	7.517	VV	92	849	0.15%	0.027%
40	7.600	7.517	7.634	VV	142	7098	1.22%	0.225%
41	7.750	7.634	7.824	VV	391	28467	4.90%	0.901%
42	7.890	7.824	8.005	VV	431	25440	4.38%	0.805%
43	8.051	8.005	8.068	VV	67	2129	0.37%	0.067%
44	8.107	8.068	8.131	VV	60	2156	0.37%	0.068%
45	8.156	8.131	8.164	VV	58	1005	0.17%	0.032%
46	8.235	8.164	8.331	VV	109	7374	1.27%	0.233%
47	8.347	8.331	8.367	VV	67	1084	0.19%	0.034%
48	8.375	8.367	8.384	VV	42	415	0.07%	0.013%
49	8.415	8.384	8.431	VV	84	1704	0.29%	0.054%
50	8.454	8.431	8.464	VV	79	1358	0.23%	0.043%
51	8.488	8.464	8.499	VV	80	1531	0.26%	0.048%
52	8.545	8.499	8.561	VV	121	3823	0.66%	0.121%
53	8.568	8.561	8.653	VV	120	4153	0.72%	0.131%
54	8.794	8.653	9.034	VV	9011	580805	100.00%	18.376%
55	9.044	9.034	9.074	VV	103	2400	0.41%	0.076%
56	9.098	9.074	9.135	VV	99	3320	0.57%	0.105%
57	9.145	9.135	9.227	VV	91	4461	0.77%	0.141%
58	9.233	9.227	9.254	VV	86	1315	0.23%	0.042%
59	9.270	9.254	9.282	VV	99	1573	0.27%	0.050%
60	9.388	9.282	9.533	VV	542	41137	7.08%	1.302%
61	9.639	9.533	9.737	VV	397	26092	4.49%	0.826%
62	9.744	9.737	9.901	VV	125	5547	0.96%	0.175%
63	9.912	9.901	9.965	VV	16	289	0.05%	0.009%
64	9.989	9.965	10.026	PV	23	400	0.07%	0.013%
65	10.037	10.026	10.067	VV	23	266	0.05%	0.008%
66	10.195	10.067	10.247	VV	394	24401	4.20%	0.772%
67	10.301	10.247	10.418	VV	637	43839	7.55%	1.387%
68	10.425	10.418	10.466	VV	261	6733	1.16%	0.213%
69	10.471	10.466	10.529	VV	226	7409	1.28%	0.234%
70	10.624	10.529	10.727	VV	2577	133833	23.04%	4.234%

rteres

71	10.790	10.727	10.886	VV	449	29025	5.00%	0.918%
72	10.959	10.886	11.070	VV	273	18887	3.25%	0.598%
73	11.157	11.070	11.351	VV	201	15937	2.74%	0.504%
74	11.447	11.351	11.453	VV	128	3978	0.68%	0.126%
75	11.461	11.453	11.528	VV	136	4264	0.73%	0.135%
76	11.538	11.528	11.543	VV	79	623	0.11%	0.020%
77	11.762	11.543	11.808	VV	701	54831	9.44%	1.735%
78	11.876	11.808	11.983	VV	1058	61149	10.53%	1.935%
79	12.094	11.983	12.233	VV	694	41195	7.09%	1.303%
80	12.320	12.233	12.367	VV	83	3621	0.62%	0.115%
81	12.377	12.367	12.447	VV	52	881	0.15%	0.028%
82	12.474	12.447	12.486	PV	14	200	0.03%	0.006%
83	12.496	12.486	12.500	VV	20	118	0.02%	0.004%
84	12.559	12.500	12.592	VV	38	1292	0.22%	0.041%
85	12.760	12.592	12.901	VV	1190	68555	11.80%	2.169%
86	12.911	12.901	12.918	VV	77	768	0.13%	0.024%
87	13.059	12.918	13.114	VV	1356	77147	13.28%	2.441%
88	13.191	13.114	13.428	VV	5068	274713	47.30%	8.692%
89	13.531	13.428	13.647	VV	796	45802	7.89%	1.449%
90	13.715	13.647	13.721	VV	157	4871	0.84%	0.154%
91	13.806	13.721	13.842	VV	328	18394	3.17%	0.582%
92	13.922	13.842	14.003	VV	1983	99924	17.20%	3.162%
93	14.181	14.003	14.315	VV	2113	237151	40.83%	7.503%
94	14.422	14.315	14.505	VV	1153	64640	11.13%	2.045%
95	14.540	14.505	14.620	VV	203	8979	1.55%	0.284%
96	14.698	14.620	14.749	PV	76	2749	0.47%	0.087%
97	14.831	14.749	14.913	PV	265	14002	2.41%	0.443%
98	15.063	14.913	15.153	VV	4396	220531	37.97%	6.978%
99	15.228	15.153	15.316	VV	1558	104851	18.05%	3.317%
100	15.413	15.316	15.466	VV	5438	285618	49.18%	9.037%
101	15.504	15.466	15.623	VV	4299	213349	36.73%	6.750%
102	15.671	15.623	15.726	VV	489	25404	4.37%	0.804%
103	15.794	15.726	15.860	VV	524	27165	4.68%	0.860%
104	15.951	15.860	16.085	VV	1638	82298	14.17%	2.604%
Sum of corrected areas:						3160598		

FB120525.M Wed Dec 10 01:18:59 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	11/25/25
Project:	Building 50 Probe Investigation	Date Received:	11/26/25
Client Sample ID:	B50-SP4-112525	SDG No.:	Q3741
Lab Sample ID:	Q3741-06	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	85.9
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	103		1	10.0	52.0	ug/kg	12/08/25 13:19	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	19.2			50 - 150	96%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032405.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 13:19
Operator : YP/AJ
Sample : Q3741-06
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP4-112525

Integration File: Calibration.e
Quant Time: Dec 09 03:05:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	433184	19.228 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032405.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 13:19
Operator : YP/AJ
Sample : Q3741-06
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B50-SP4-112525

Integration File: Calibration.e
Quant Time: Dec 09 03:05:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

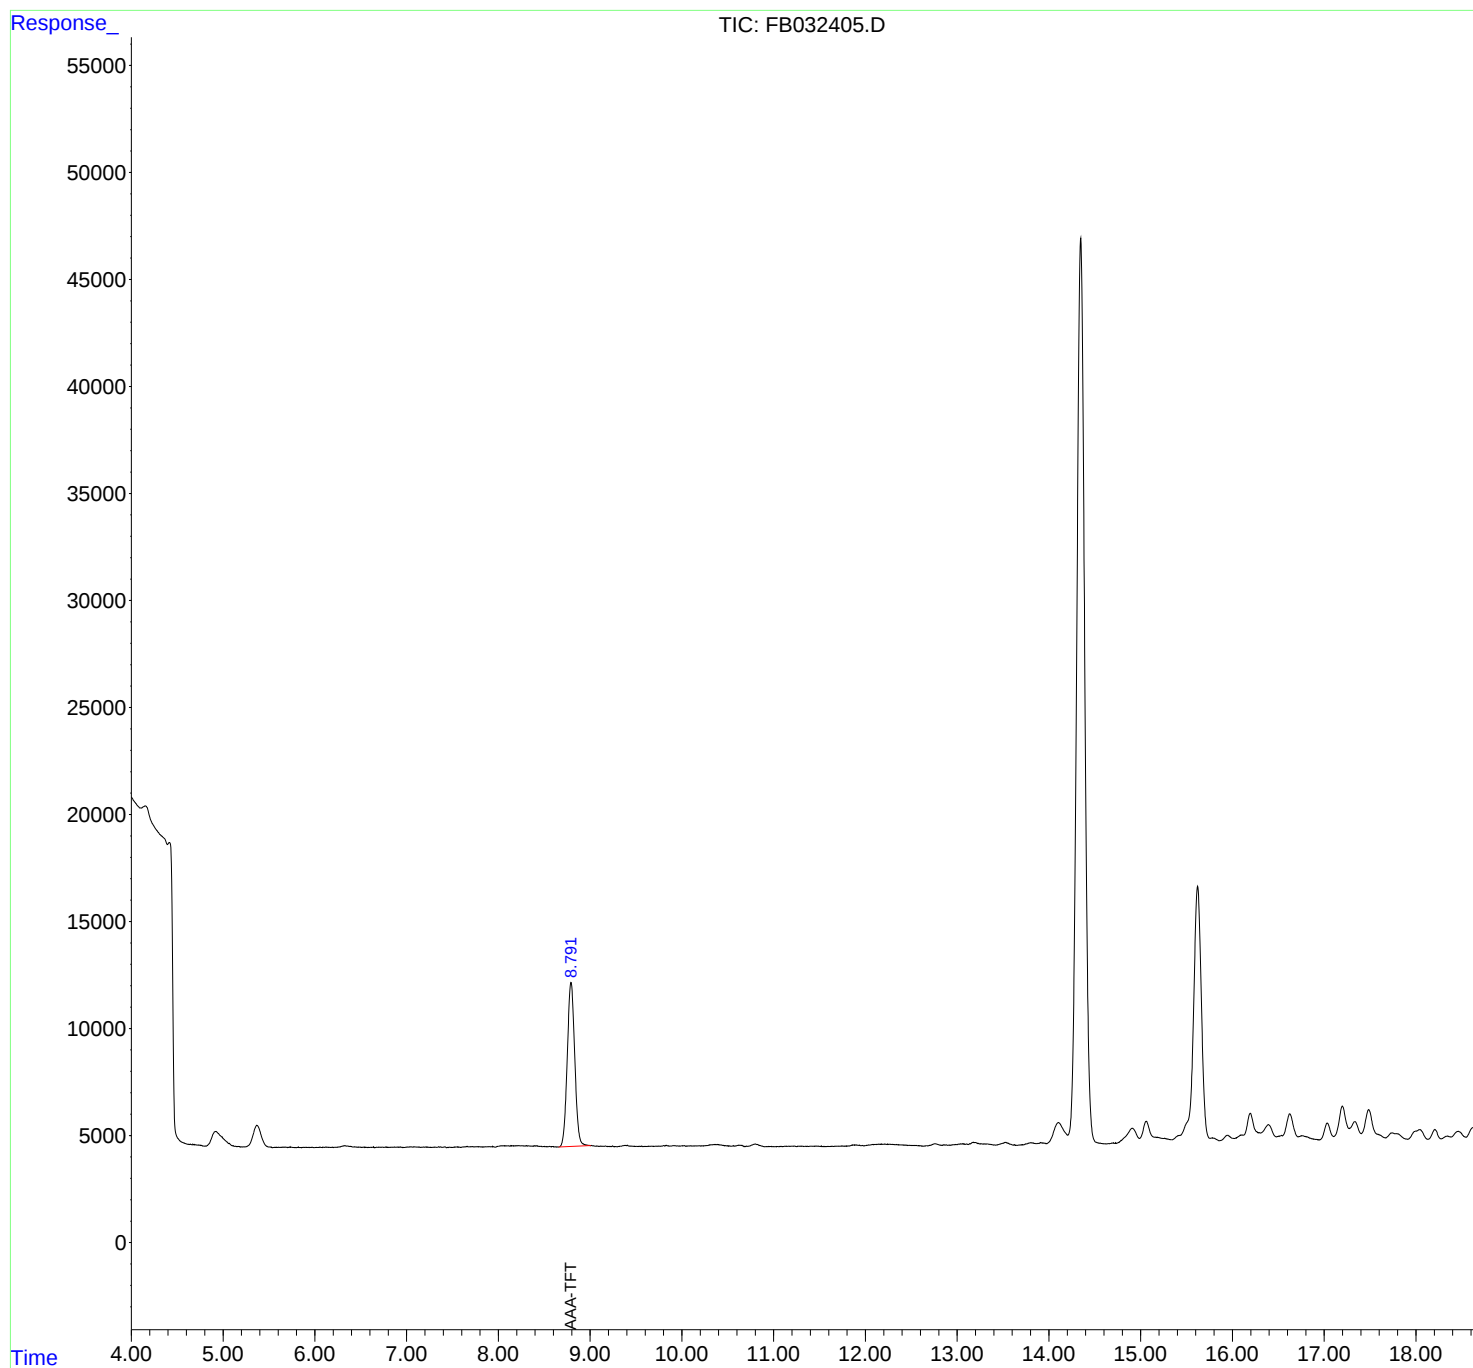

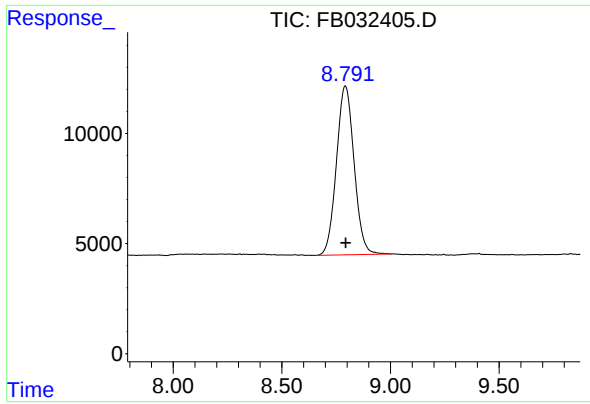

#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.002 min
Response: 433184
Conc: 19.23 ng/ml

Instrument :
FID_B
ClientSampleId :
B50-SP4-112525

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032405.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 13:19
 Sample : Q3741-06
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: SAMPLE.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	8.792	8.657	9.004	BV	7671	433184	17.63%	10.803%
2	10.800	10.688	10.900	PV	128	7155	0.29%	0.178%
3	12.755	12.681	12.832	PV	93	4202	0.17%	0.105%
4	13.176	13.121	13.252	PV	98	3681	0.15%	0.092%
5	13.532	13.391	13.616	BV	129	6568	0.27%	0.164%
6	13.803	13.647	13.859	BB	64	2758	0.11%	0.069%
7	14.105	13.934	14.209	BV	729	42382	1.73%	1.057%
8	14.347	14.232	14.630	BV	41769	2456768	100.00%	61.268%
9	14.910	14.630	14.988	PV	703	54930	2.24%	1.370%
10	15.062	14.988	15.328	VV	1007	75159	3.06%	1.874%
11	15.621	15.328	15.759	VV	11916	735024	29.92%	18.330%
12	15.783	15.759	15.857	VV	152	5543	0.23%	0.138%
13	15.947	15.857	16.024	PV	238	11689	0.48%	0.292%
14	16.195	16.024	16.308	VV	1213	75969	3.09%	1.895%
15	16.393	16.308	16.480	VV	643	39451	1.61%	0.984%
16	16.626	16.480	16.717	VV	1094	55410	2.26%	1.382%
Sum of corrected areas:						4009873		

FB120525.M Tue Dec 09 04:23:10 2025



CALIBRATION SUMMARY

GASOLINE RANGE ORGANICS INITIAL CALIBRATION SUMMARY

Lab Name: Alliance

Contract: CORE02

ProjectID: Building 50 Probe Investigation

Lab Code: ACE

SDG No.: Q3741

Calibration Sequence : FB120525		Test : Gasoline Range Organics	
Concentration (PPB)	Area Count	Reference Factor	File ID
45	1739642	38659	FB032390.D
90	3579845	39776	FB032391.D
180	7374551	40970	FB032392.D
450	18417070	40927	FB032393.D
900	37134788	41261	FB032394.D
AVG RF : 40319		% RSD : 2.697	AVG RT : 8.794

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane Contract: CORE02
ProjectID: Building 50 Probe Investigation
Lab Code: ACE SDG No.: Q3741
DataFile: FB032400.D Analyst Name: YP/AJ Analyst Date: 12-08-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	6013442	33408	40319	17.141

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032400.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 9:16
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Dec 08 13:01:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	433413	19.238 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	964930	27.812 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1131792	28.293 ng/ml
3) t n-Heptane	7.748	375196	9.496 ng/ml
4) t Benzene	7.887	213499	4.742 ng/ml
6) t Toluene	10.617	744126	16.287 ng/ml
7) t Ethylbenzene	13.053	375635	9.223 ng/ml
8) t m-Xylene	13.186	797698	18.524 ng/ml
9) t O-Xylene	13.913	764498	18.467 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	646068	18.355 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032400.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 9:16
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Dec 08 13:01:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

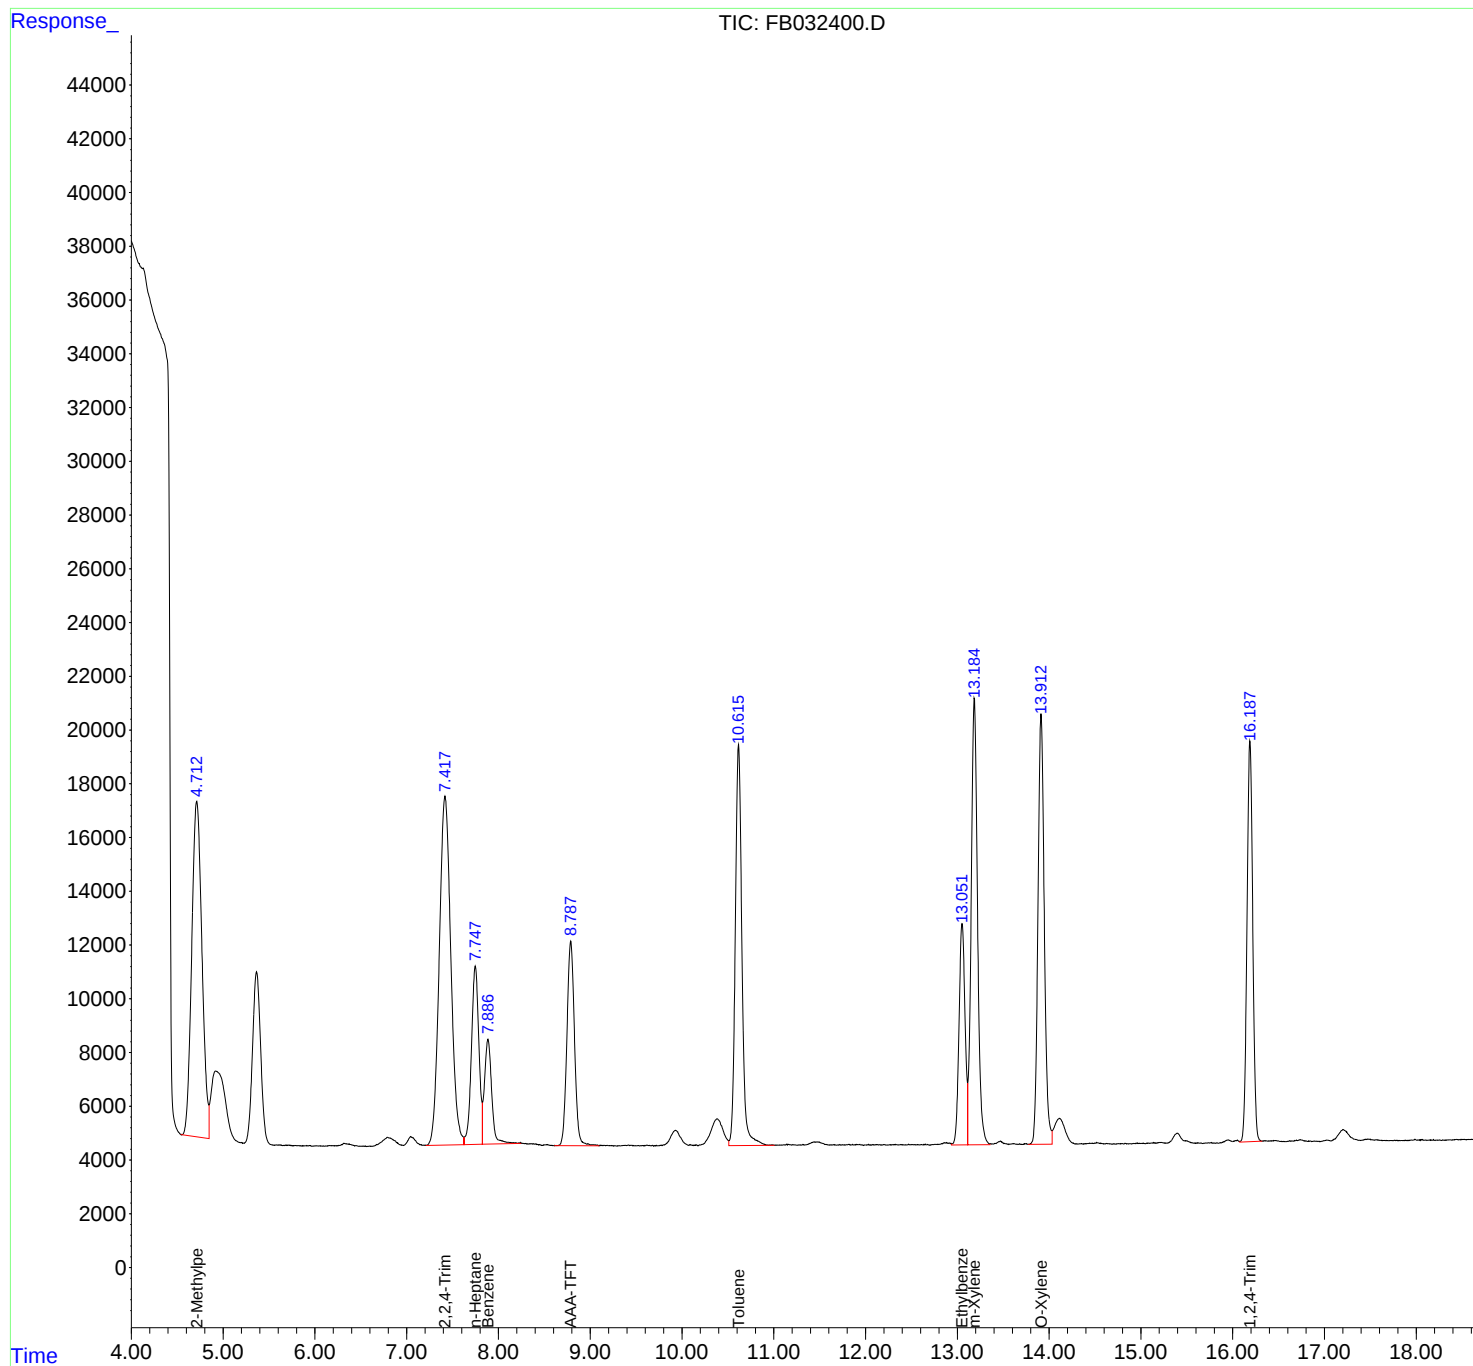

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032400.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 9:16
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.714	4.543	4.847	BV	12480	964930	85.26%	14.967%
2	7.418	7.209	7.624	PV	12978	1131792	100.00%	17.556%
3	7.748	7.624	7.826	VV	6630	375196	33.15%	5.820%
4	7.887	7.826	8.247	VB	3906	213499	18.86%	3.312%
5	8.788	8.612	9.099	BV	7612	433413	38.29%	6.723%
6	10.617	10.510	11.008	VB	14919	744126	65.75%	11.542%
7	13.053	12.937	13.113	VV	8238	375635	33.19%	5.827%
8	13.186	13.113	13.356	VV	16618	797698	70.48%	12.373%
9	13.913	13.775	14.033	BV	16021	764498	67.55%	11.858%
10	16.189	16.077	16.322	VV	14907	646068	57.08%	10.021%

Sum of corrected areas: 6446855

FB120525.M Mon Dec 08 13:07:27 2025

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane Contract: CORE02
ProjectID: Building 50 Probe Investigation
Lab Code: ACE SDG No.: Q3741
DataFile: FB032409.D Analyst Name: YP/AJ Analyst Date: 12-08-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	6789651	37720	40319	6.446

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032409.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 15:18
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/09/2025
 Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
 Quant Time: Dec 09 03:06:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	467307	20.742 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	898849	25.907 ng/mlm
2) t 2,2,4-Trimethylpentane	7.422	1135686	28.390 ng/ml
3) t n-Heptane	7.754	375044	9.492 ng/ml
4) t Benzene	7.893	445015	9.885 ng/ml
6) t Toluene	10.623	1287952	28.190 ng/ml
7) t Ethylbenzene	13.058	386736	9.496 ng/ml
8) t m-Xylene	13.192	813771	18.897 ng/ml
9) t O-Xylene	13.919	783055	18.915 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	663543	18.852 ng/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032409.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 15:18
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/09/2025
Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
Quant Time: Dec 09 03:06:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

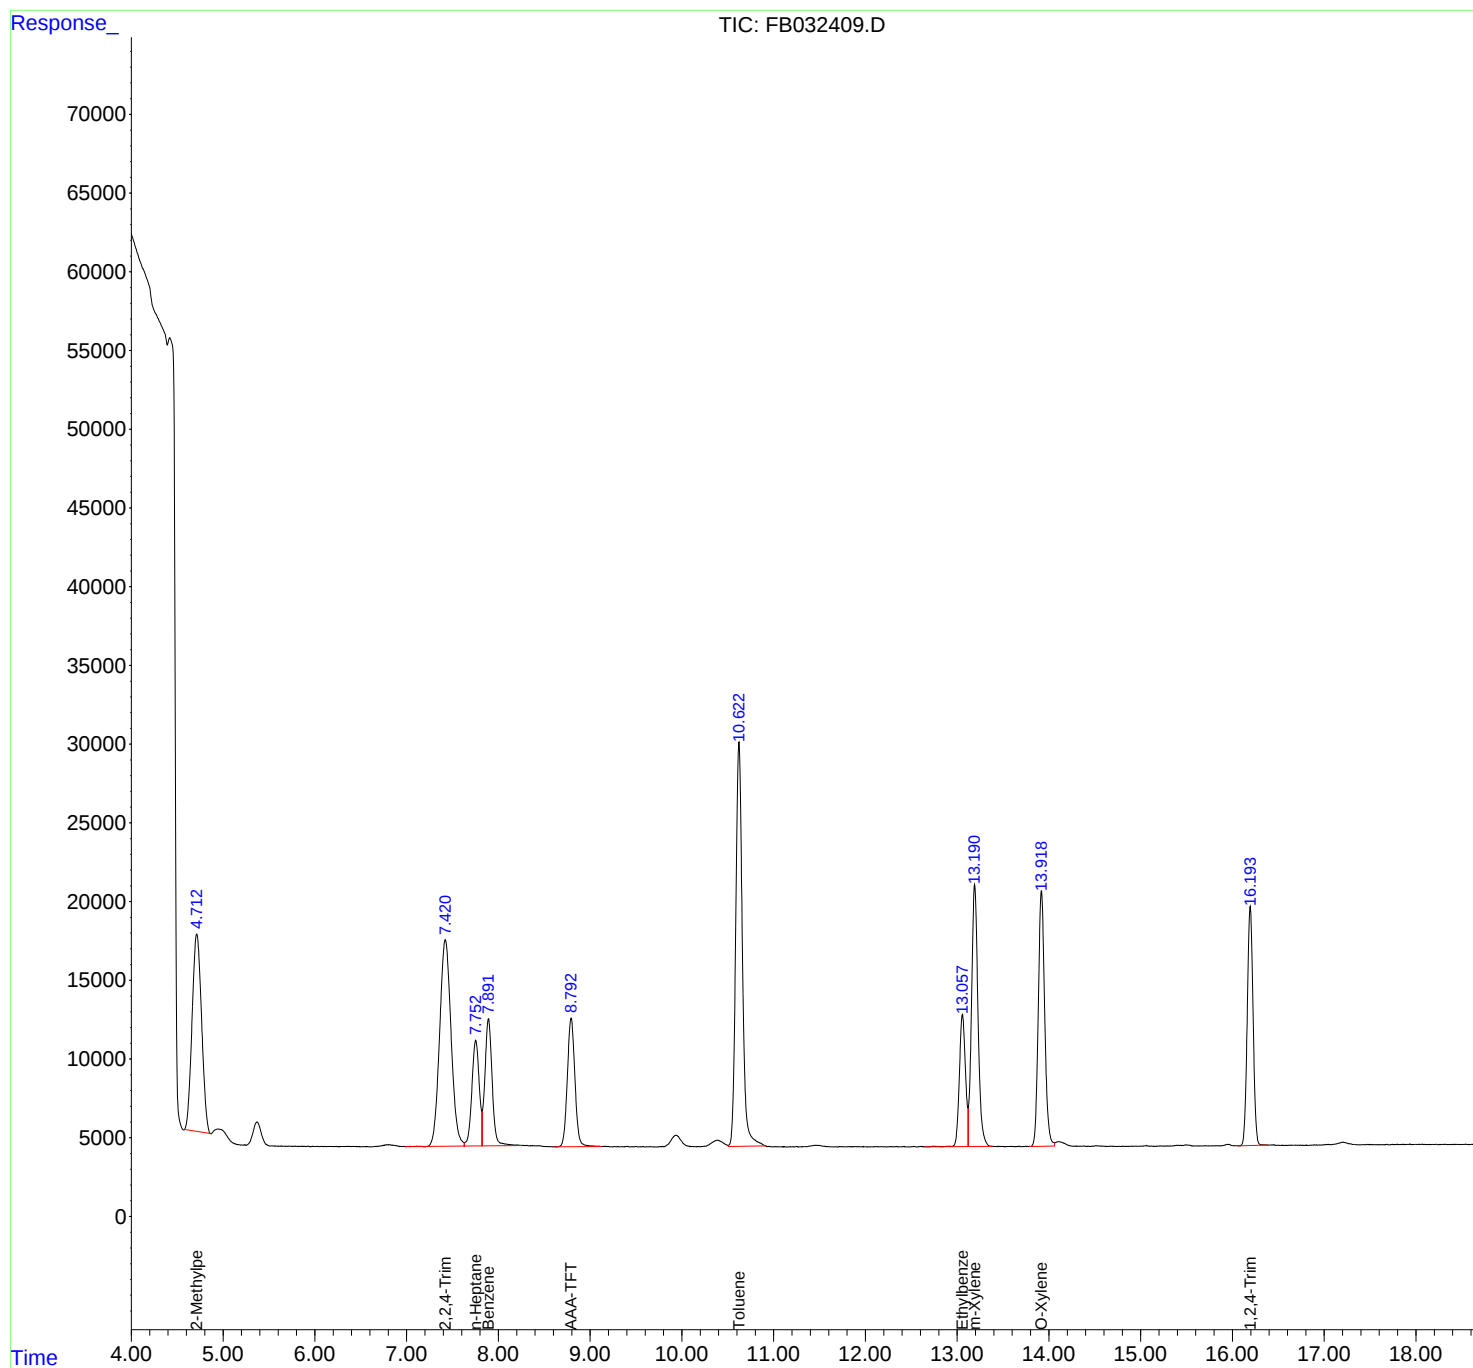

rteres

Instrument :

FID_B

LabSampleId :

20 PPB GRO STD

Area Percent Report

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 12/09/2025

Supervised By :Yogesh Patel 12/09/2025

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB12082
Data File : FB032409.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 15:18
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibrat.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.712	4.575	4.867	M	12559	902386	70.06%	12.429%
2	7.422	6.984	7.630	PV	13118	1135686	88.18%	15.642%
3	7.754	7.630	7.823	VV	6725	375044	29.12%	5.166%
4	7.893	7.823	8.253	VB	8080	445015	34.55%	6.129%
5	8.794	8.604	9.124	BV	8172	467307	36.28%	6.436%
6	10.623	10.506	10.911	VBA	25678	1287952	100.00%	17.739%
7	13.058	12.642	13.119	PV	8385	386736	30.03%	5.327%
8	13.192	13.119	13.391	VBA	16619	813771	63.18%	11.208%
9	13.919	13.783	14.062	BV	16230	783055	60.80%	10.785%
10	16.194	16.057	16.386	PV	15176	663543	51.52%	9.139%

Sum of corrected areas: 7260495

FB120525.M Tue Dec 09 03:37:33 2025

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane Contract: CORE02
ProjectID: Building 50 Probe Investigation
Lab Code: ACE SDG No.: Q3741
DataFile: FB032415.D Analyst Name: YP/AJ Analyst Date: 12-08-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	7473138	41517	40319	2.971

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032415.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 18:30
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/09/2025
 Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
 Quant Time: Dec 09 03:07:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	486319	21.586 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	998757	28.787 ng/mlm
2) t 2,2,4-Trimethylpentane	7.423	1257528	31.436 ng/ml
3) t n-Heptane	7.754	422101	10.683 ng/ml
4) t Benzene	7.894	479218	10.645 ng/ml
6) t Toluene	10.624	1405940	30.773 ng/ml
7) t Ethylbenzene	13.061	416772	10.233 ng/ml
8) t m-Xylene	13.194	892966	20.736 ng/ml
9) t O-Xylene	13.921	841292	20.322 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	758564	21.551 ng/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032415.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 18:30
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/09/2025
Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
Quant Time: Dec 09 03:07:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

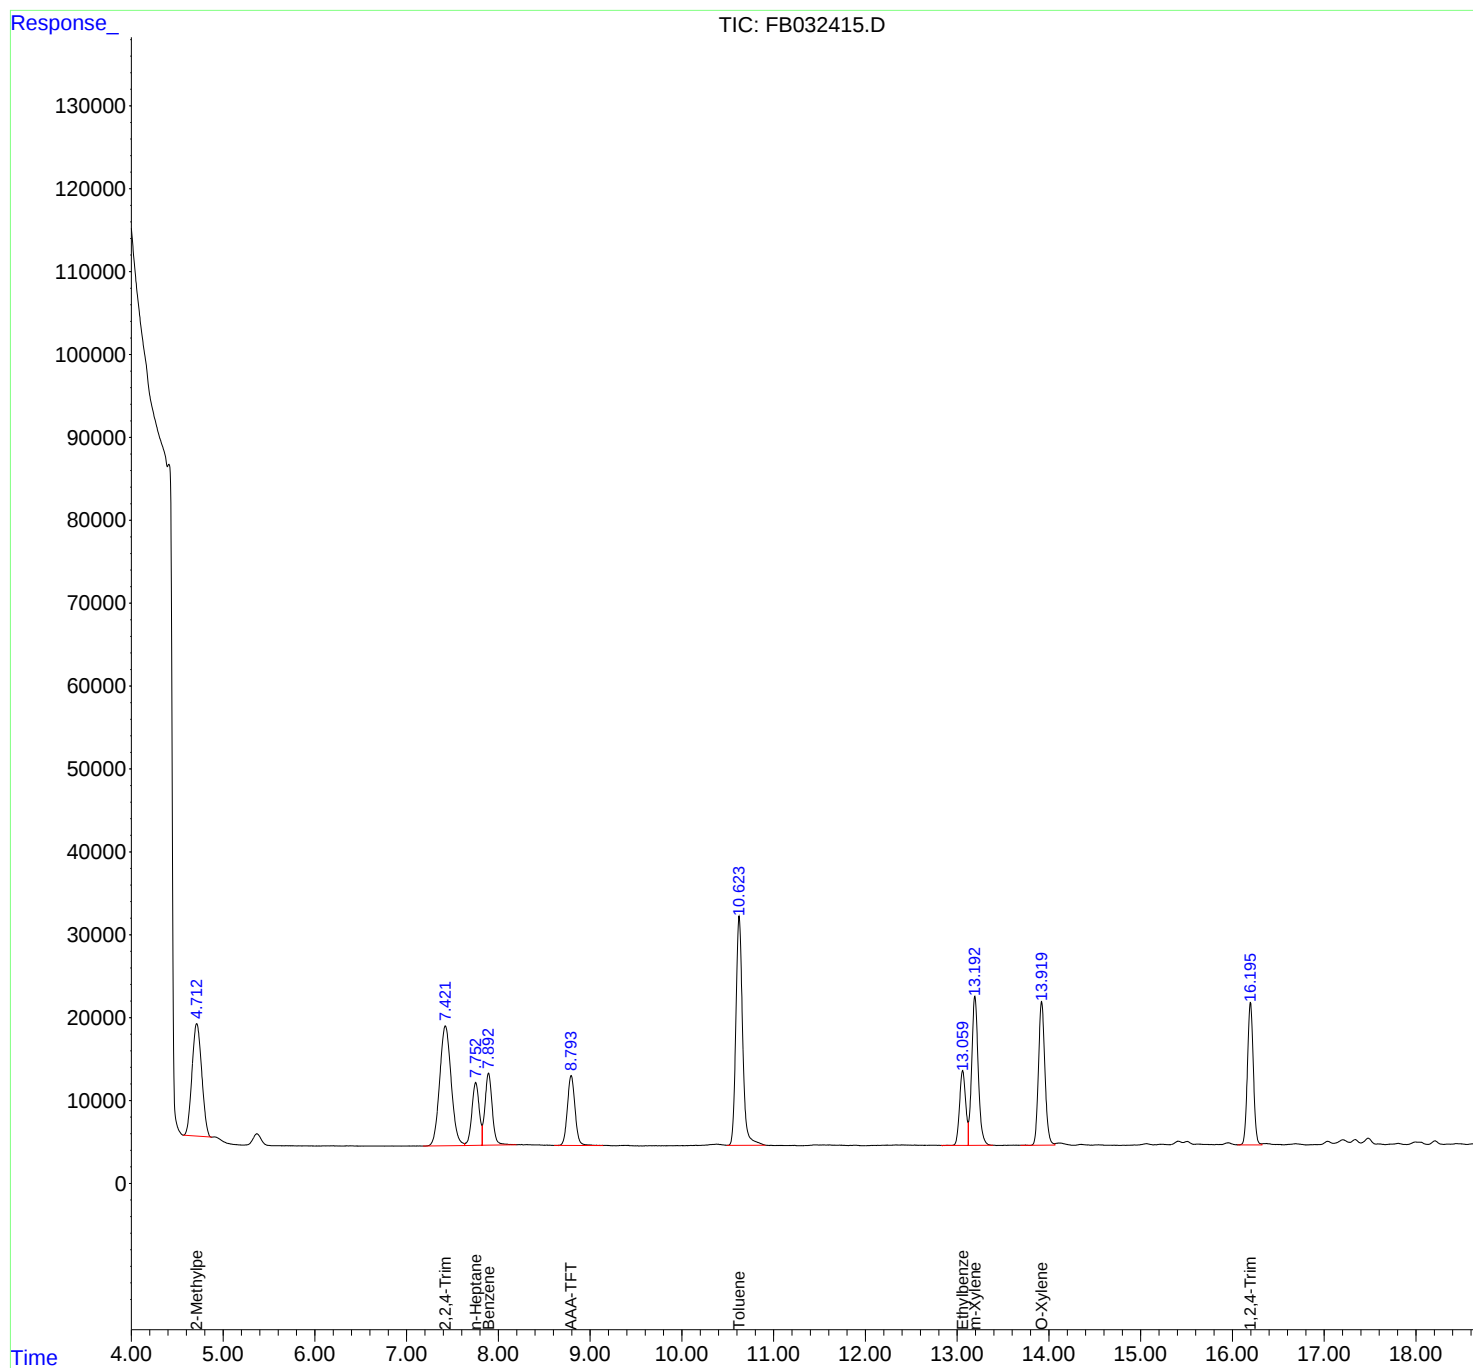

rteres

Instrument :

FID_B

LabSampleId :

20 PPB GRO STD

Area Percent Report

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 12/09/2025

Supervised By :Yogesh Patel 12/09/2025

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB12082
Data File : FB032415.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 18:30
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibrat.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.712	4.565	4.864	M	13611	1005789	71.54%	12.625%
2	7.423	7.179	7.633	BV	14464	1257528	89.44%	15.785%
3	7.754	7.633	7.824	VV	7596	422101	30.02%	5.298%
4	7.894	7.824	8.197	VV	8691	479218	34.09%	6.015%
5	8.794	8.606	9.144	BV	8430	486319	34.59%	6.105%
6	10.624	10.493	10.911	VBA	27656	1405940	100.00%	17.648%
7	13.061	12.823	13.121	BV	9016	416772	29.64%	5.232%
8	13.194	13.121	13.391	VBA	17990	892966	63.51%	11.209%
9	13.921	13.692	14.065	BV	17321	841292	59.84%	10.560%
10	16.197	16.057	16.322	PV	17190	758564	53.95%	9.522%

Sum of corrected areas: 7966488

FB120525.M Tue Dec 09 03:41:18 2025

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane Contract: CORE02
ProjectID: Building 50 Probe Investigation
Lab Code: ACE SDG No.: Q3741
DataFile: FB032416.D Analyst Name: YP/AJ Analyst Date: 12-09-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	7346952	40816	40319	1.233

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032416.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 9:26
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Dec 10 00:39:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	459394	20.391 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	1041536	30.020 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1230555	30.762 ng/ml
3) t n-Heptane	7.747	411572	10.417 ng/ml
4) t Benzene	7.887	475187	10.555 ng/ml
6) t Toluene	10.617	1377017	30.140 ng/ml
7) t Ethylbenzene	13.054	408671	10.034 ng/ml
8) t m-Xylene	13.187	860843	19.990 ng/ml
9) t O-Xylene	13.914	821779	19.851 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	719792	20.450 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032416.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 9:26
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Dec 10 00:39:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

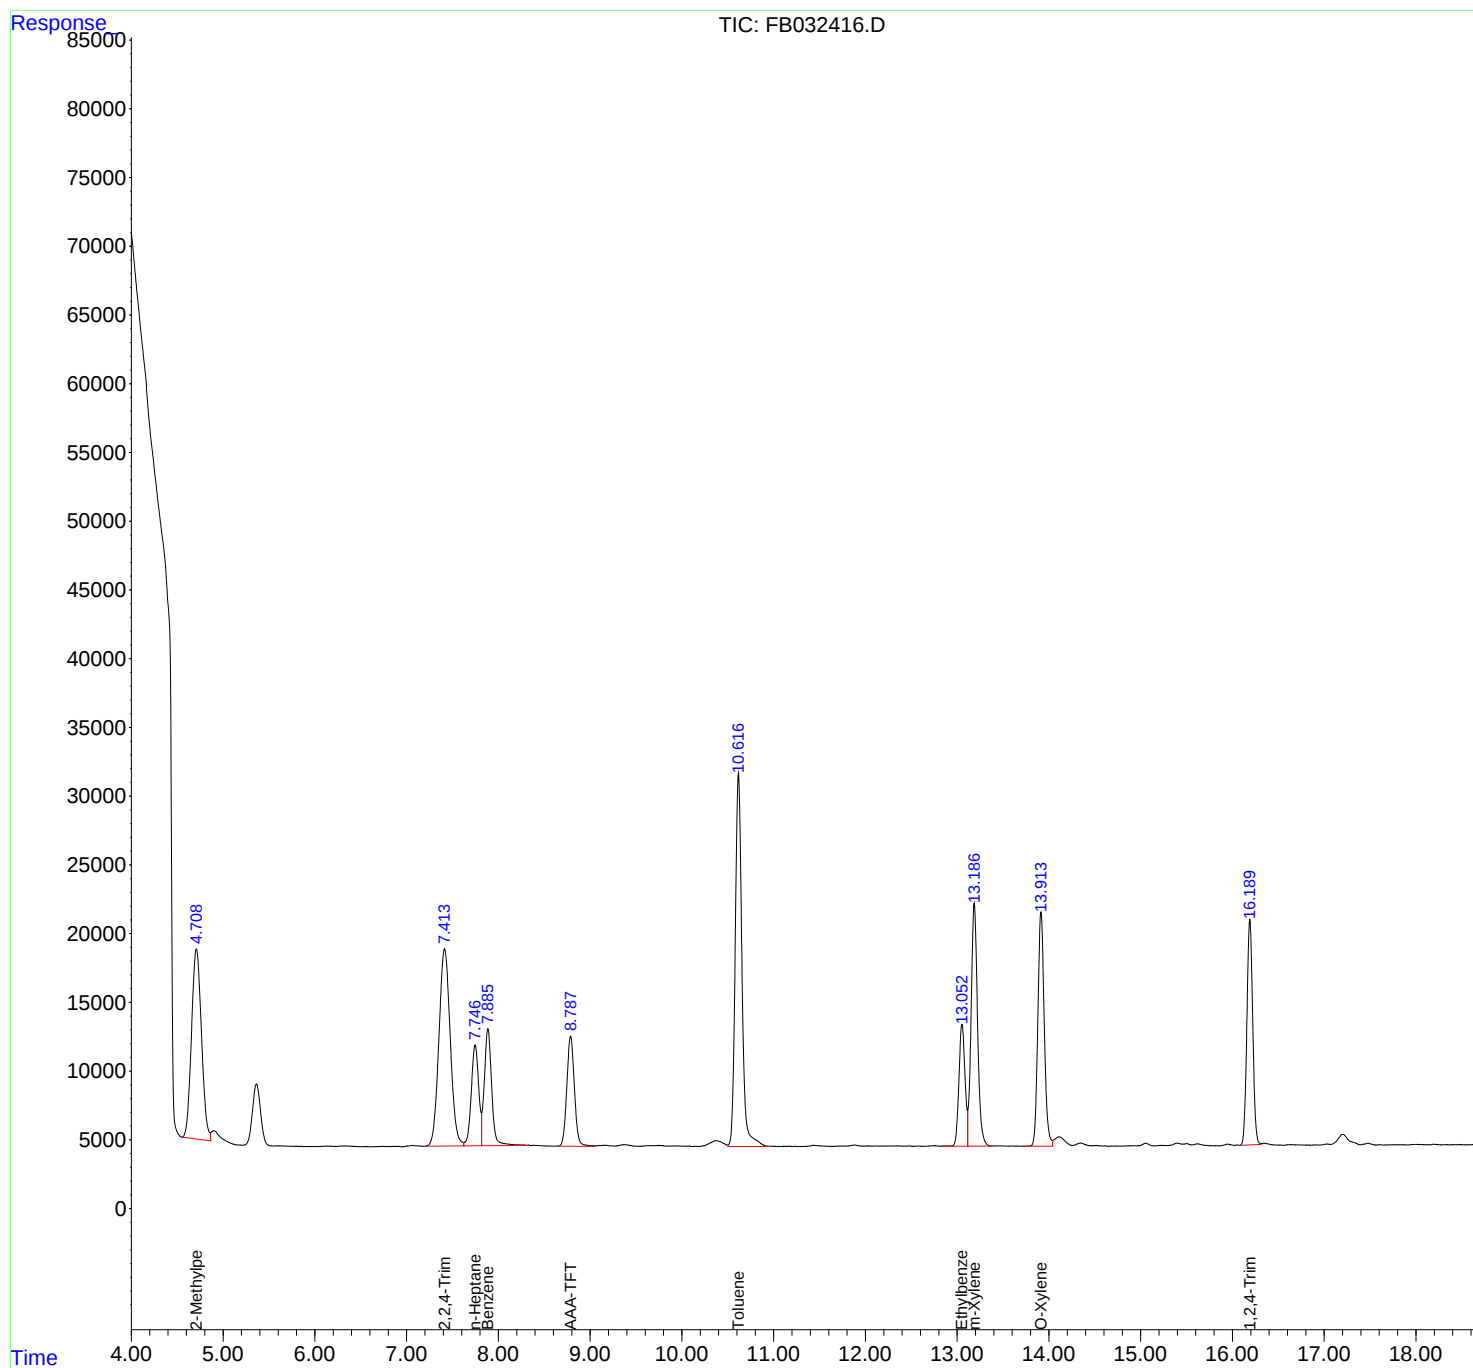

Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032416.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 9:26
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.710	4.543	4.863	BV	13826	1041536	75.64%	13.342%
2	7.414	7.211	7.622	PV	14364	1230555	89.36%	15.764%
3	7.747	7.622	7.817	VV	7345	411572	29.89%	5.272%
4	7.887	7.817	8.309	VV	8515	475187	34.51%	6.087%
5	8.788	8.648	9.055	PV	8010	459394	33.36%	5.885%
6	10.617	10.501	10.964	VV	27163	1377017	100.00%	17.640%
7	13.054	12.837	13.115	BV	8867	408671	29.68%	5.235%
8	13.187	13.115	13.387	VB	17692	860843	62.52%	11.027%
9	13.914	13.708	14.039	BV	17030	821779	59.68%	10.527%
10	16.190	16.076	16.313	PV	16409	719792	52.27%	9.221%

Sum of corrected areas: 7806345

FB120525.M Wed Dec 10 01:16:16 2025

GASOLINE RANGE ORGANICS CONTINUING CALIBRATION SUMMARY

20 PPB GRO STD

Lab Name: Alliane Contract: CORE02
ProjectID: Building 50 Probe Investigation
Lab Code: ACE SDG No.: Q3741
DataFile: FB032422.D Analyst Name: YP/AJ Analyst Date: 12-09-2025

Conc. (PPB)	Area Count	RF	Average RF	%D
180	7319969	40666	40319	0.861

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032422.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 13:45
 Operator : YP/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Dec 10 00:40:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	477409	21.191 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	1069122	30.815 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1213977	30.347 ng/ml
3) t n-Heptane	7.754	404842	10.246 ng/ml
4) t Benzene	7.894	466497	10.362 ng/ml
6) t Toluene	10.624	1382946	30.270 ng/ml
7) t Ethylbenzene	13.060	402588	9.885 ng/ml
8) t m-Xylene	13.193	855530	19.867 ng/ml
9) t O-Xylene	13.921	822641	19.871 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	701826	19.939 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032422.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 13:45
Operator : YP/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Dec 10 00:40:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

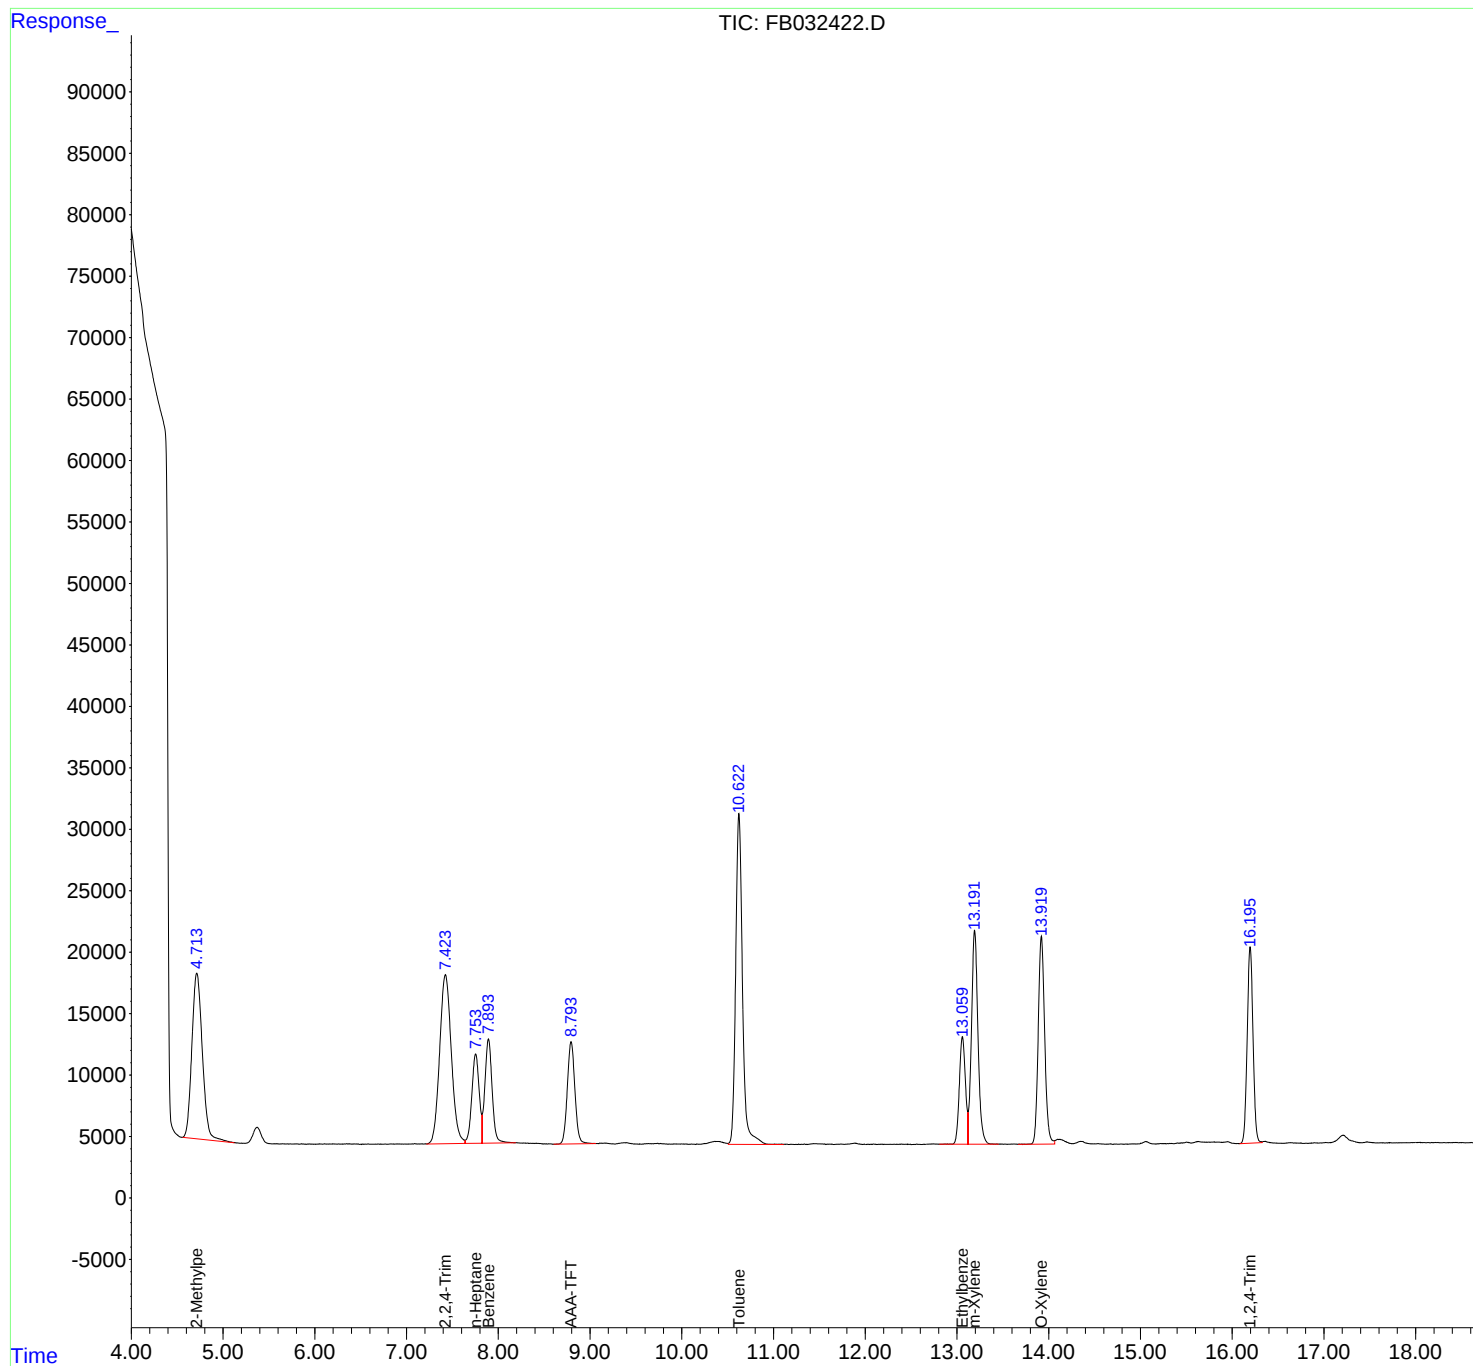

rteres

Area Percent

Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032422.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 13:45
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.714	4.558	5.122	PV	13474	1069122	77.31%	13.711%
2	7.424	7.214	7.639	PV	13755	1213977	87.78%	15.569%
3	7.754	7.639	7.823	VV	7265	404842	29.27%	5.192%
4	7.894	7.823	8.192	VV	8480	466497	33.73%	5.983%
5	8.794	8.604	9.066	BV	8316	477409	34.52%	6.123%
6	10.624	10.507	11.109	VB	26917	1382946	100.00%	17.736%
7	13.060	12.806	13.121	BV	8750	402588	29.11%	5.163%
8	13.193	13.121	13.455	VB	17373	855530	61.86%	10.972%
9	13.921	13.667	14.065	PV	16914	822641	59.48%	10.550%
10	16.196	16.080	16.327	BV	15971	701826	50.75%	9.001%

Sum of corrected areas: 7797377

FB120525.M Wed Dec 10 01:18:19 2025

Analytical Sequence

Client: Core Environmental Consultants and Services, Inc.

SDG No.: Q3741

Project: Building 50 Probe Investigation

Instrument ID: FID_B

GC Column: RTX-502.2 **ID:** 0.53 (mm)

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

MEAN SUROGATE RT FROM INITIAL CALIBRATION 8.794					
CLIENT SAMPLE NO.	LAB SAMPLE ID	DATE AND TIME ANALYZED	DATAFILE	RT	#
20 PPB GRO STD	20 PPB GRO STD	8 Dec 2025 9:16	FB032400.D	8.788	
VBF1208S1	VBF1208S1	8 Dec 2025 10:40	FB032401.D	8.793	
BSF1208S1	BSF1208S1	8 Dec 2025 11:38	FB032403.D	8.794	
B50-SP4-112525	Q3741-06	8 Dec 2025 13:19	FB032405.D	8.792	
B50-SP9-112425	Q3741-04	8 Dec 2025 14:17	FB032407.D	8.792	
BSF1208S2	BSF1208S2	8 Dec 2025 14:49	FB032408.D	8.792	
20 PPB GRO STD	20 PPB GRO STD	8 Dec 2025 15:18	FB032409.D	8.794	
B50-SP3-111925	Q3741-01	8 Dec 2025 16:05	FB032410.D	8.792	
B50-SP13-112025	Q3741-02	8 Dec 2025 16:34	FB032411.D	8.793	
B50-SP14-112025	Q3741-03	8 Dec 2025 17:03	FB032412.D	8.794	
20 PPB GRO STD	20 PPB GRO STD	8 Dec 2025 18:30	FB032415.D	8.794	
20 PPB GRO STD	20 PPB GRO STD	9 Dec 2025 9:26	FB032416.D	8.788	
VBF1209S2	VBF1209S2	9 Dec 2025 11:06	FB032418.D	8.793	
BSF1209S1	BSF1209S1	9 Dec 2025 11:34	FB032419.D	8.793	
B50-SP11-112525	Q3741-05	9 Dec 2025 12:25	FB032420.D	8.794	
20 PPB GRO STD	20 PPB GRO STD	9 Dec 2025 13:45	FB032422.D	8.794	



QC SAMPLE DATA

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	
Project:	Building 50 Probe Investigation	Date Received:	
Client Sample ID:	VBF1208S1	SDG No.:	Q3741
Lab Sample ID:	VBF1208S1	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	100
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	8.00	U	1	8.00	45.0	ug/kg	12/08/25 10:40	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	20.8			50 - 150	104%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032401.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 10:40
Operator : YP/AJ
Sample : VBF1208S2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1208S2

Integration File: Calibration.e
Quant Time: Dec 08 13:01:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	467898	20.768 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032401.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 10:40
Operator : YP/AJ
Sample : VBF1208S2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1208S2

Integration File: Calibration.e
Quant Time: Dec 08 13:01:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

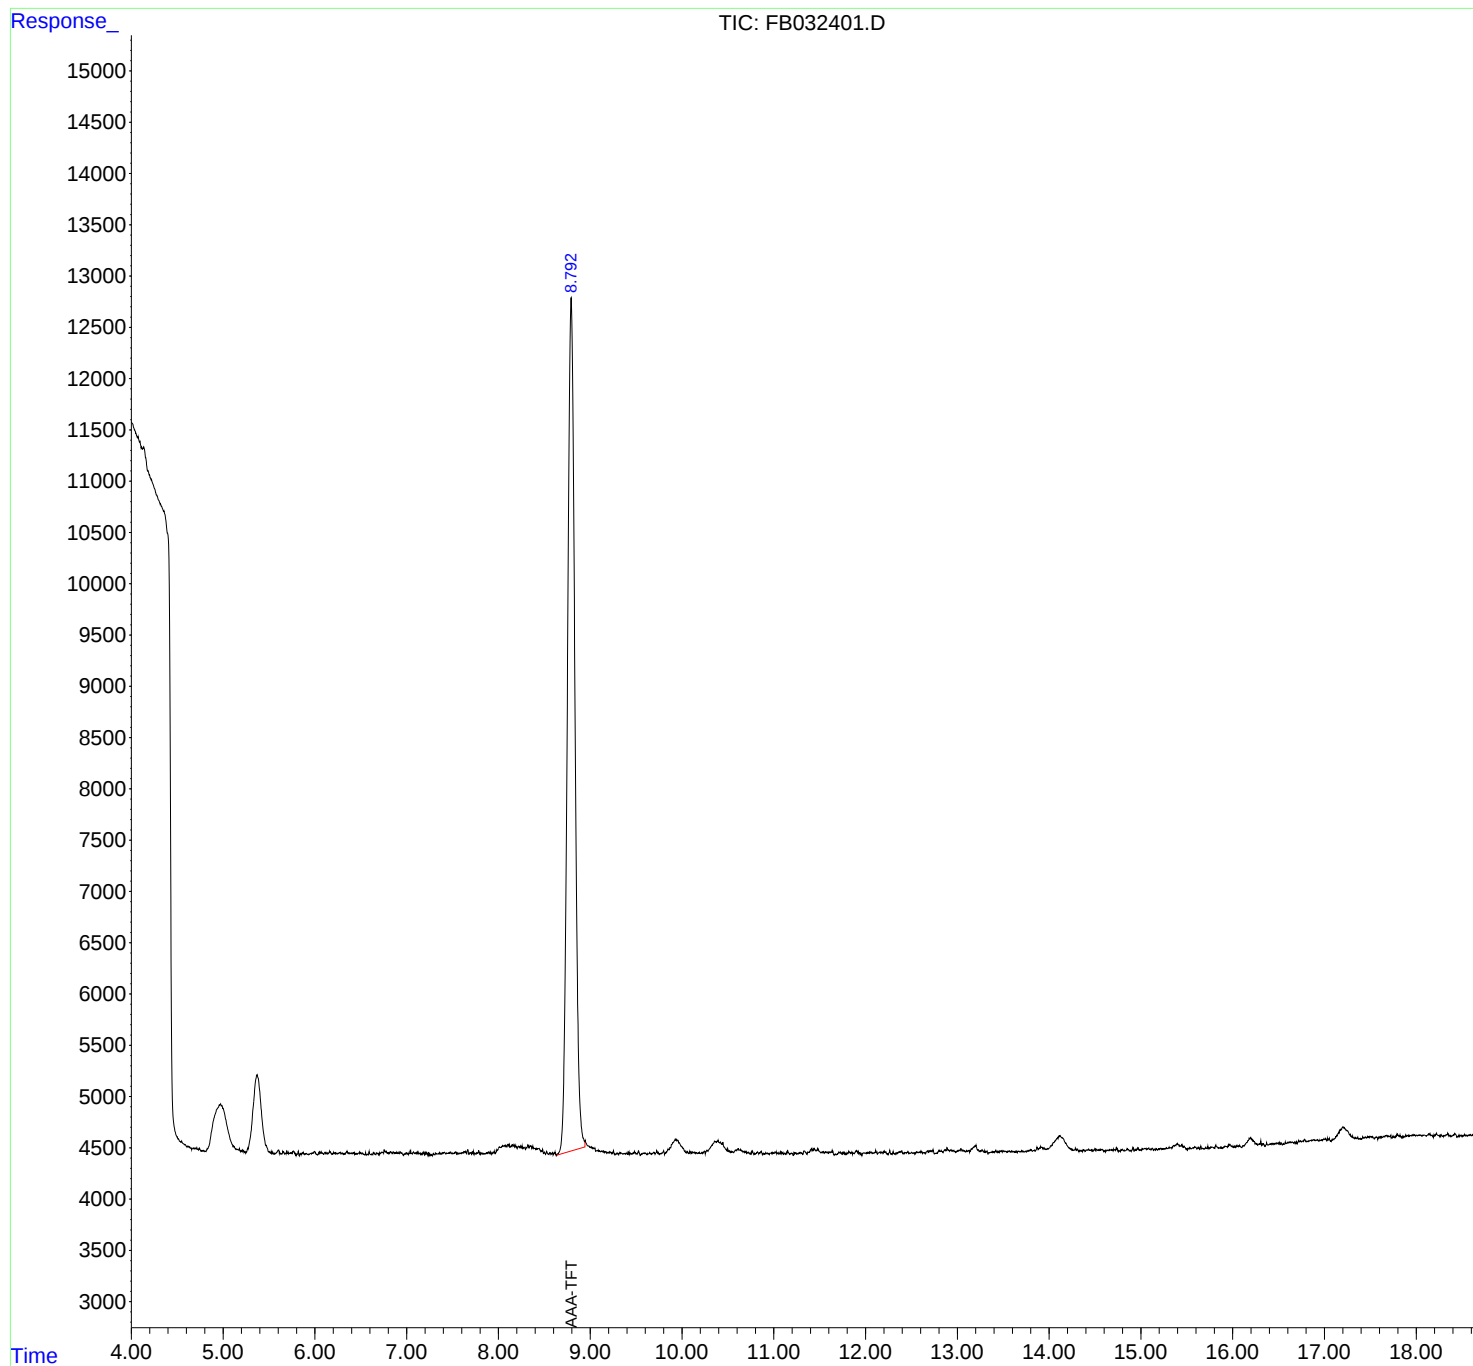

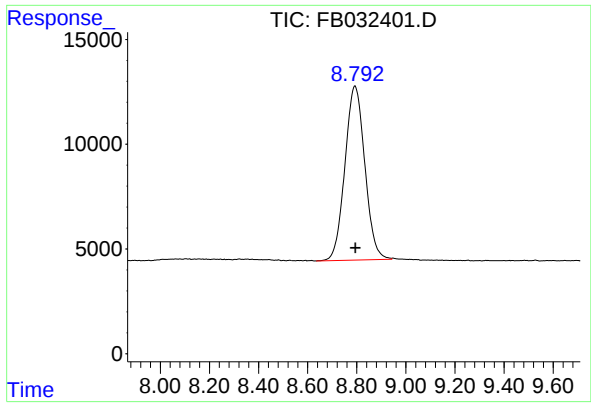

#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 467898
Conc: 20.77 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1208S2

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032401.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 10:40
Sample : VBF1208S2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	8.793	8.634	8.943	PV	8321	467898	100.00%	100.000%
Sum of corrected areas:						467898		

FB120525.M Mon Dec 08 13:07:51 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	
Project:	Building 50 Probe Investigation	Date Received:	
Client Sample ID:	VBF1209S2	SDG No.:	Q3741
Lab Sample ID:	VBF1209S2	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	100
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	413	U	50	413	2250	ug/kg	12/09/25 11:06	FB120925
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	22.3			50 - 150	112%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032418.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 11:06
Operator : YP/AJ
Sample : VBF1209S2 50X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1209S2

Integration File: Calibration.e
Quant Time: Dec 10 00:39:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	502622	22.310 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032418.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 11:06
Operator : YP/AJ
Sample : VBF1209S2 50X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1209S2

Integration File: Calibration.e
Quant Time: Dec 10 00:39:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

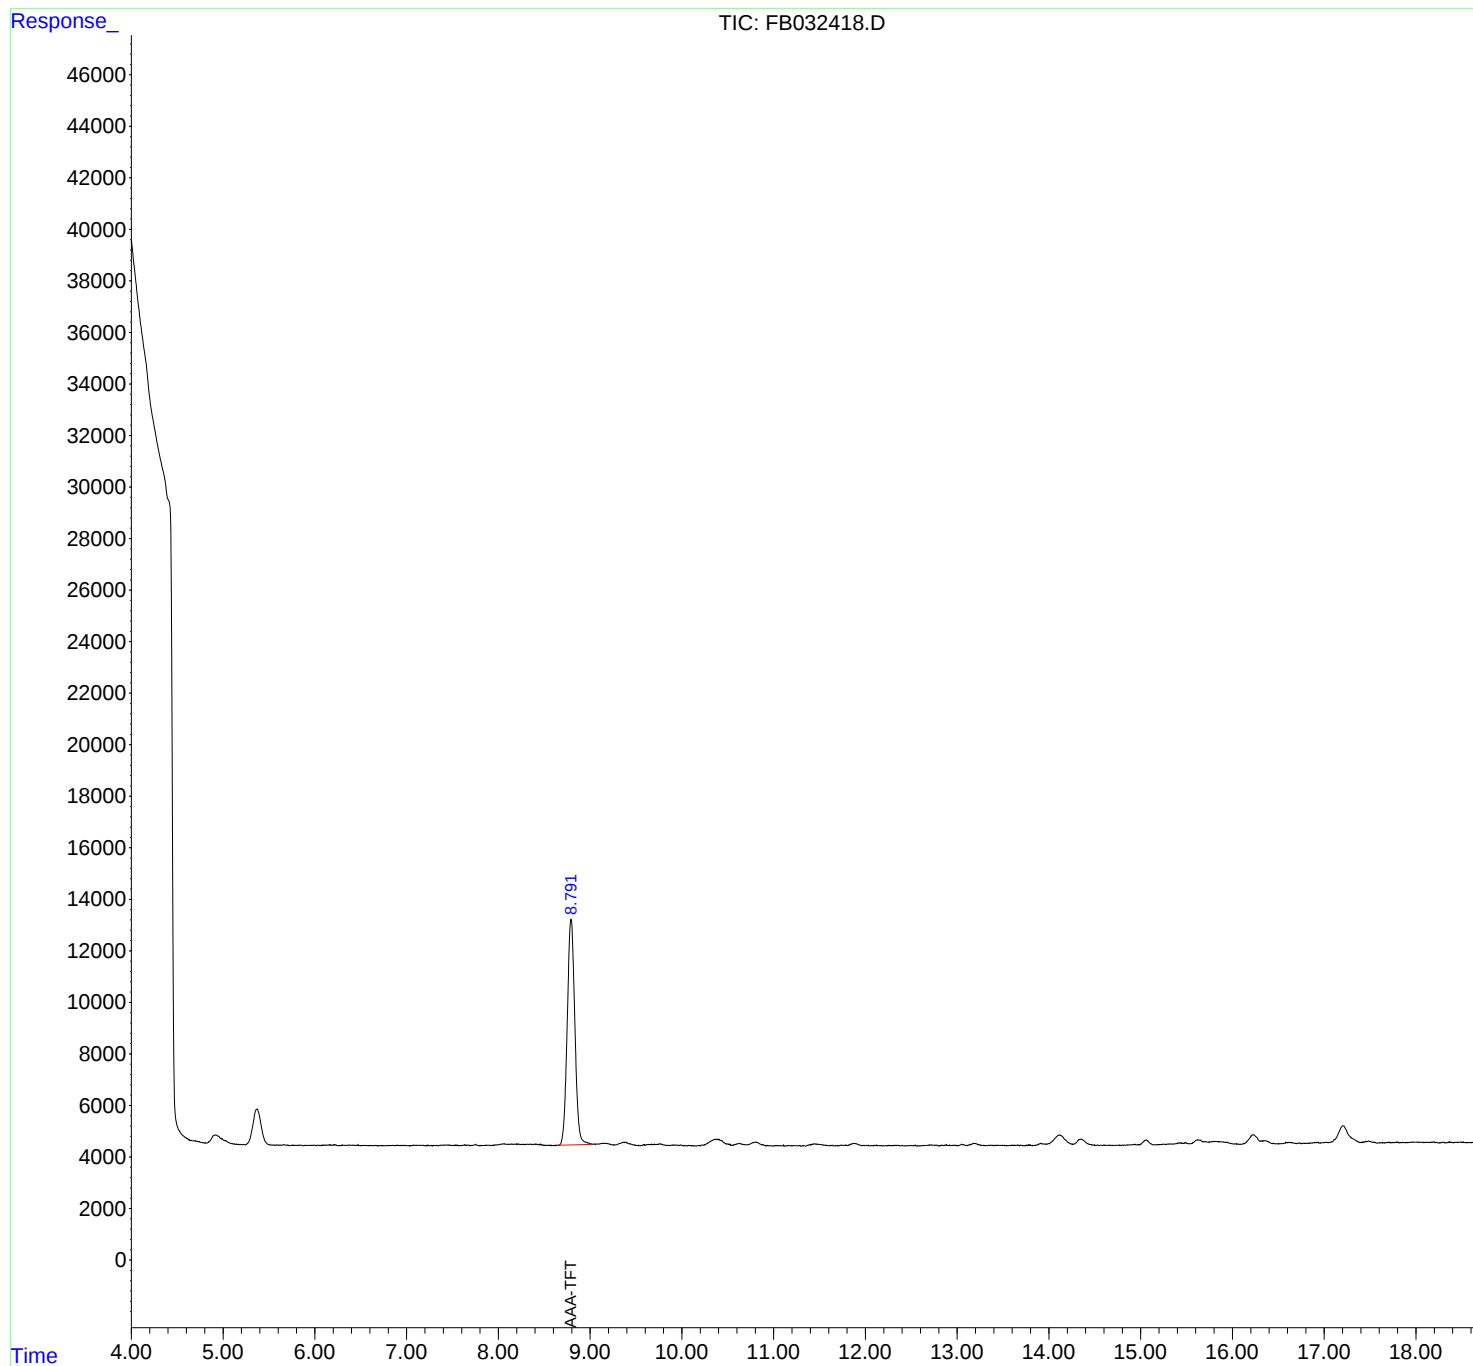

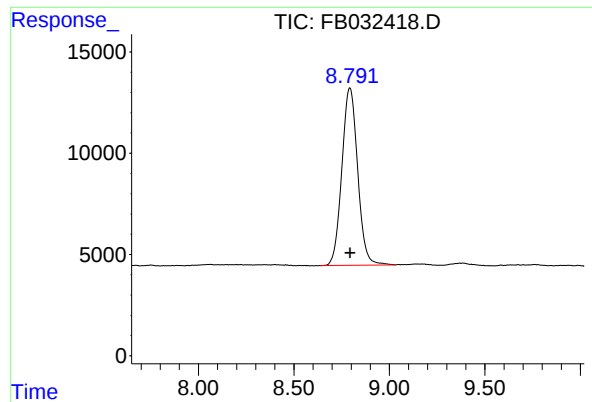

#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 502622
Conc: 22.31 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1209S2

rteres

Area Percent

Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032418.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 11:06
Sample : VBF1209S2 50X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	8.793	8.637	9.032	BV	8762	502622	100.00%	100.000%
Sum of corrected areas:						502622		

FB120525.M Wed Dec 10 01:16:46 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	
Project:	Building 50 Probe Investigation	Date Received:	
Client Sample ID:	BSF1208S1	SDG No.:	Q3741
Lab Sample ID:	BSF1208S1	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	100
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	170		1	8.00	45.0	ug/kg	12/08/25 11:38	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	19.5			50 - 150	98%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032403.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 11:38
 Operator : YP/AJ
 Sample : BSF1208S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1208S1

Integration File: Calibration.e
 Quant Time: Dec 08 13:01:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	439452	19.506 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	919629	26.506 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1130865	28.270 ng/ml
3) t n-Heptane	7.753	372133	9.418 ng/ml
4) t Benzene	7.893	442844	9.837 ng/ml
6) t Toluene	10.622	1296467	28.377 ng/ml
7) t Ethylbenzene	13.058	391474	9.612 ng/ml
8) t m-Xylene	13.191	821650	19.080 ng/ml
9) t O-Xylene	13.918	789105	19.061 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	671956	19.091 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032403.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 11:38
Operator : YP/AJ
Sample : BSF1208S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1208S1

Integration File: Calibration.e
Quant Time: Dec 08 13:01:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

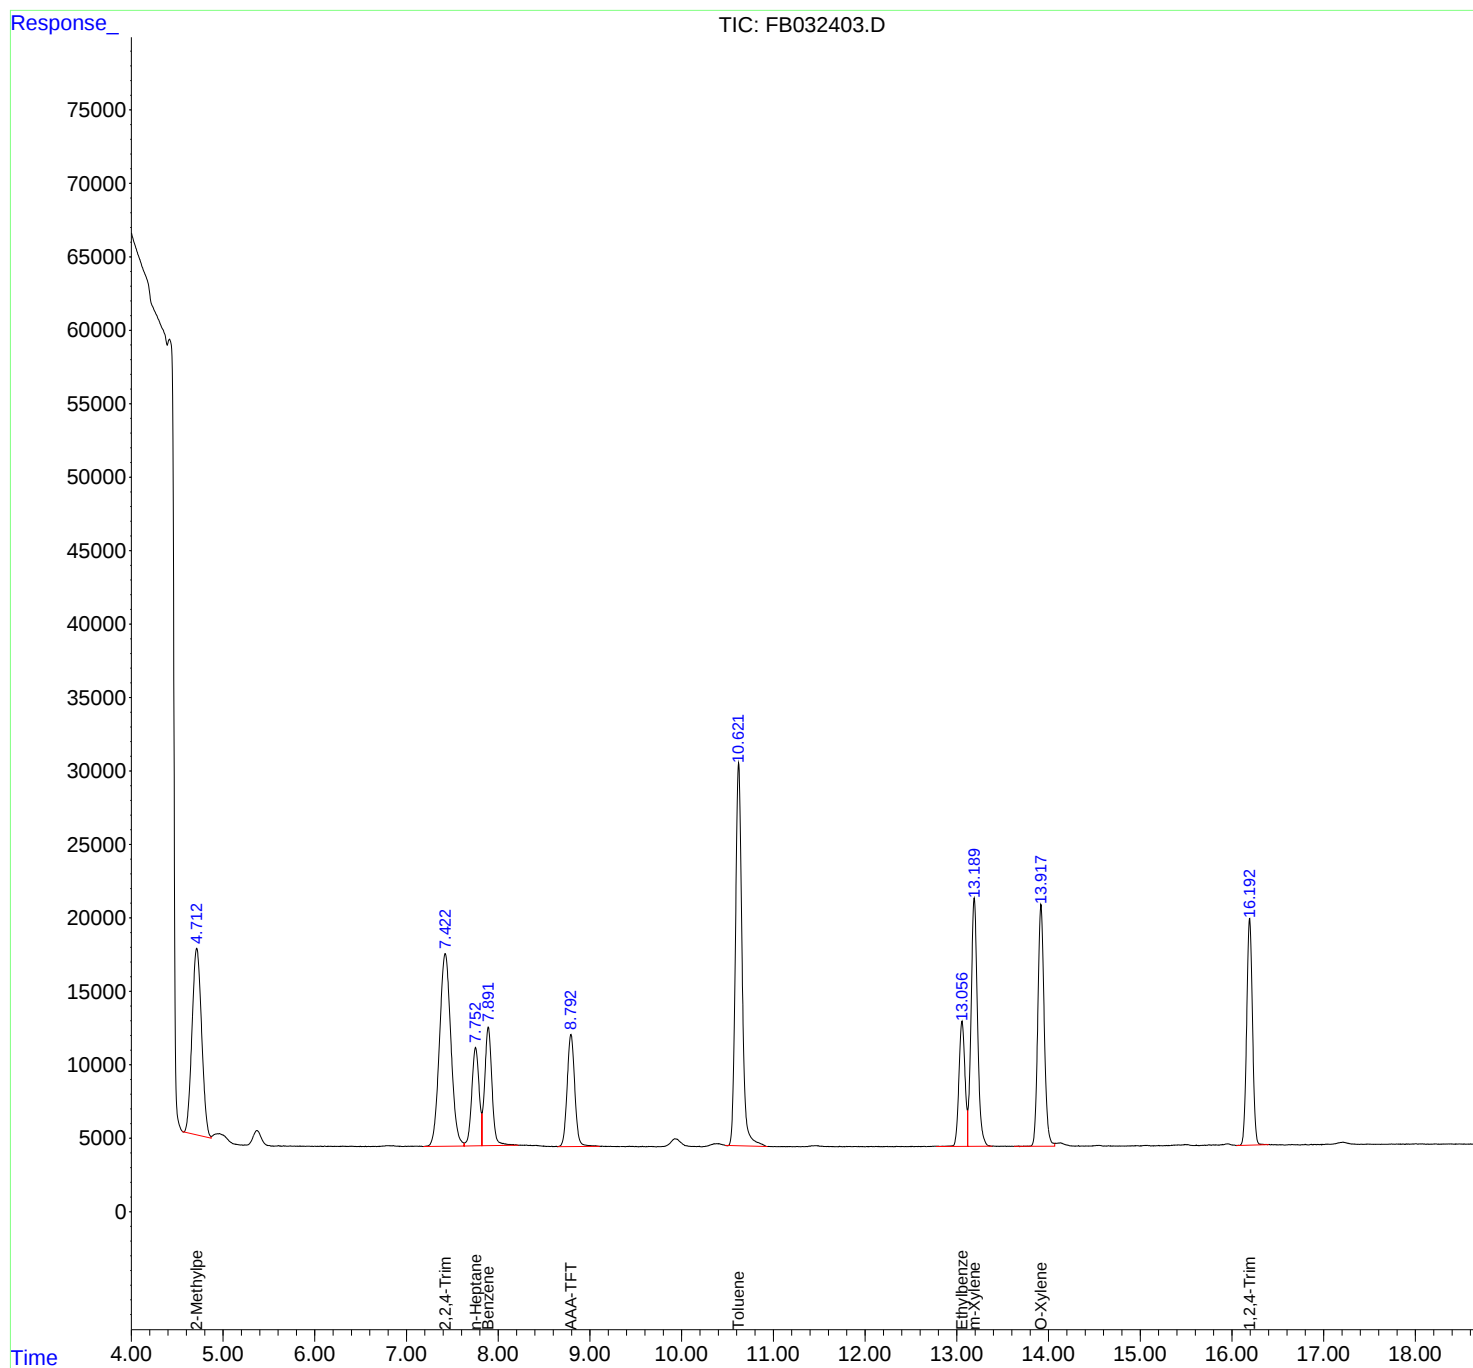

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032403.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 11:38
Sample : BSF1208S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.713	4.559	4.870	BV	12708	919629	70.93%	12.640%
2	7.423	7.184	7.629	BV	13116	1130865	87.23%	15.543%
3	7.753	7.629	7.823	VV	6703	372133	28.70%	5.115%
4	7.893	7.823	8.222	VV	8079	442844	34.16%	6.087%
5	8.794	8.646	9.107	PV	7634	439452	33.90%	6.040%
6	10.622	10.474	10.936	BV	26038	1296467	100.00%	17.819%
7	13.058	12.779	13.118	VV	8518	391474	30.20%	5.381%
8	13.191	13.118	13.388	VV	16901	821650	63.38%	11.293%
9	13.918	13.622	14.067	BV	16457	789105	60.87%	10.846%
10	16.193	16.049	16.403	PBA	15438	671956	51.83%	9.236%

Sum of corrected areas: 7275573

FB120525.M Mon Dec 08 13:08:44 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	
Project:	Building 50 Probe Investigation	Date Received:	
Client Sample ID:	BSF1209S1	SDG No.:	Q3741
Lab Sample ID:	BSF1209S1	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	100
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	183		1	8.00	45.0	ug/kg	12/09/25 11:34	FB120925
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	21.3			50 - 150	107%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032419.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 11:34
 Operator : YP/AJ
 Sample : BSF1209S1
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1209S1

Integration File: Calibration.e
 Quant Time: Dec 10 00:39:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	480380	21.322 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	1007903	29.050 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1229681	30.740 ng/ml
3) t n-Heptane	7.752	404434	10.236 ng/ml
4) t Benzene	7.892	478077	10.619 ng/ml
6) t Toluene	10.622	1410148	30.865 ng/ml
7) t Ethylbenzene	13.058	412711	10.134 ng/ml
8) t m-Xylene	13.192	871914	20.248 ng/ml
9) t O-Xylene	13.920	833028	20.122 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	714263	20.293 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032419.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 11:34
Operator : YP/AJ
Sample : BSF1209S1
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1209S1

Integration File: Calibration.e
Quant Time: Dec 10 00:39:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

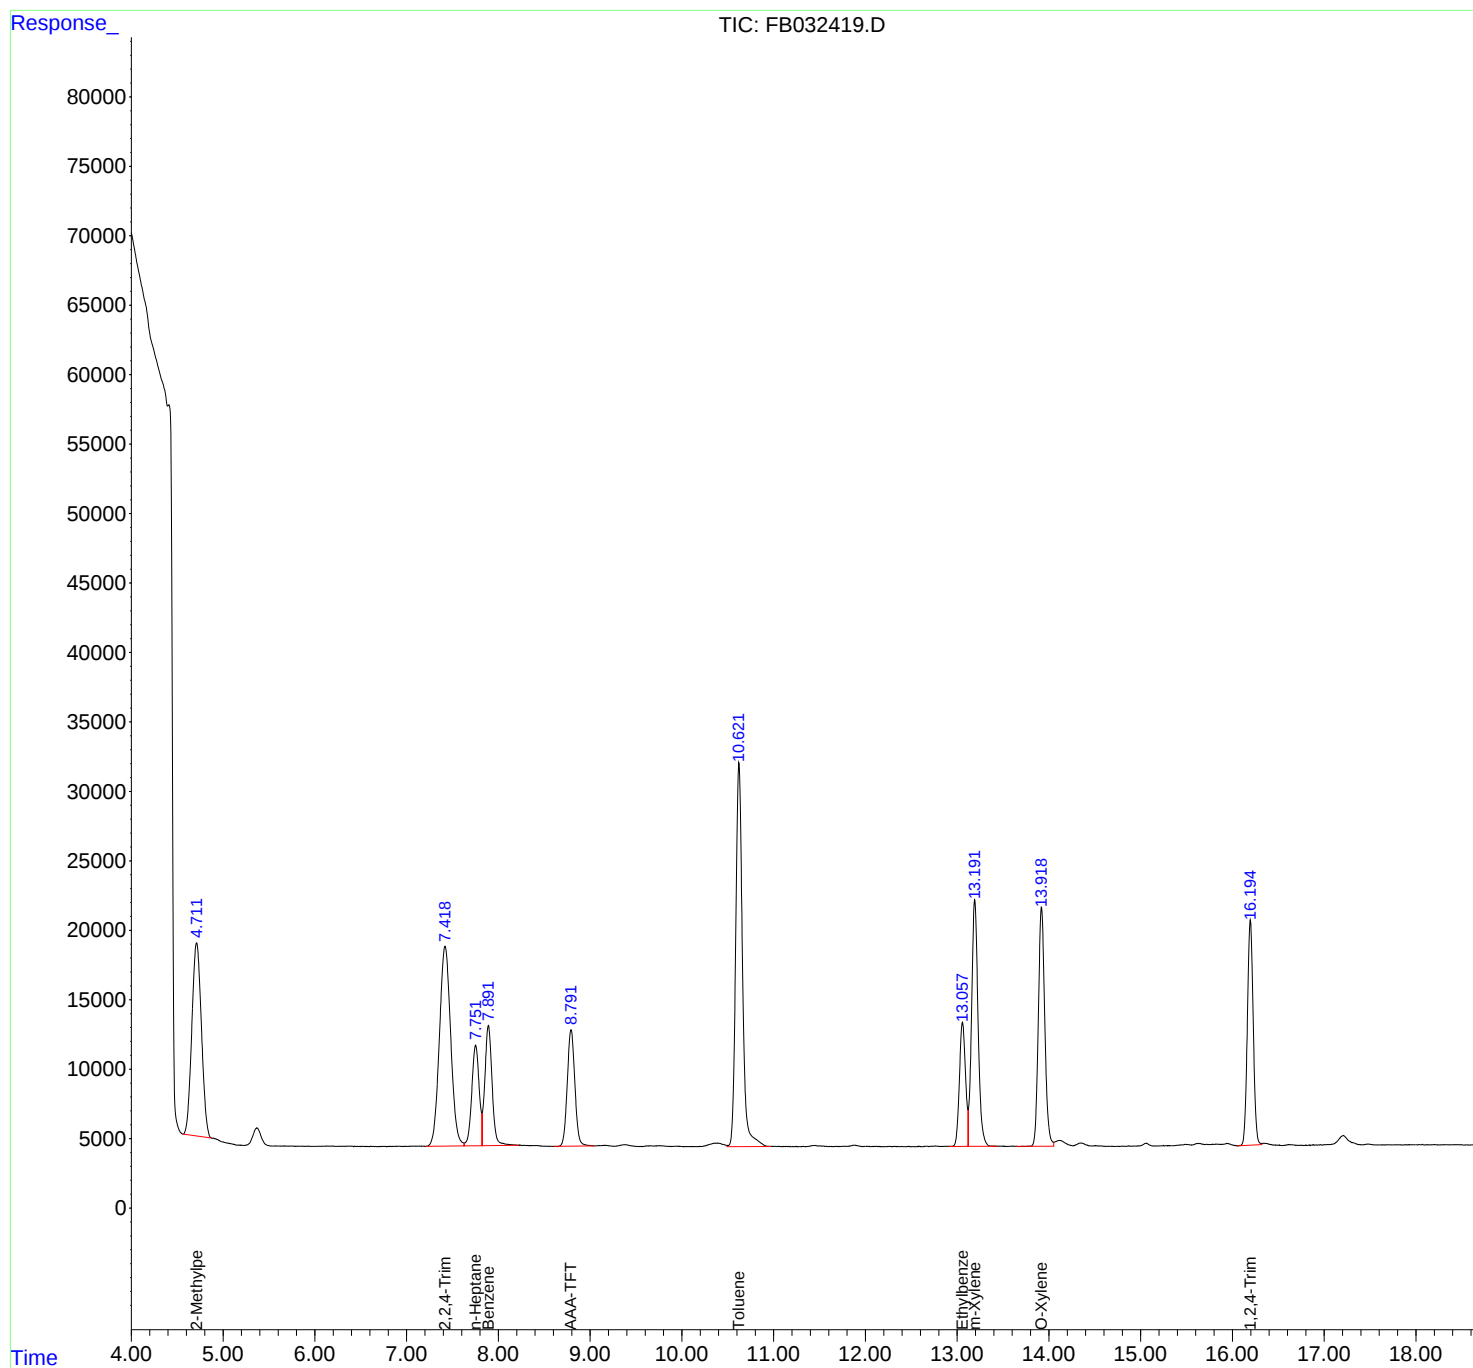

rteres

Area Percent

Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032419.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 11:34
Sample : BSF1209S1
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.712	4.559	4.875	BV	13904	1007903	71.48%	12.852%
2	7.420	7.209	7.628	BV	14402	1229681	87.20%	15.680%
3	7.752	7.628	7.822	VV	7249	404434	28.68%	5.157%
4	7.892	7.822	8.225	VB	8651	478077	33.90%	6.096%
5	8.793	8.606	9.046	BV	8390	480380	34.07%	6.125%
6	10.622	10.493	10.972	VV	27633	1410148	100.00%	17.981%
7	13.058	12.915	13.120	VV	8932	412711	29.27%	5.262%
8	13.192	13.120	13.441	VB	17760	871914	61.83%	11.118%
9	13.920	13.641	14.053	BV	17202	833028	59.07%	10.622%
10	16.196	16.052	16.319	PV	16212	714263	50.65%	9.108%

Sum of corrected areas: 7842540

FB120525.M Wed Dec 10 01:17:08 2025

Report of Analysis

Client:	Core Environmental Consultants and Services, Inc.	Date Collected:	
Project:	Building 50 Probe Investigation	Date Received:	
Client Sample ID:	BSF1208S2	SDG No.:	Q3741
Lab Sample ID:	BSF1208S2	Matrix:	SOIL
Analytical Method:	8015D GRO	% Solid:	100
Sample Wt/Vol:	5 g	Test:	Gasoline Range Organics
	Final Vol: 5 mL		

CAS Number	Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Date Ana.	BatchID
TARGETS									
GRO	GRO	174		1	8.00	45.0	ug/kg	12/08/25 14:49	FB120825
SURROGATES									
98-08-8	Alpha,Alpha,Alpha-Trifluor	20.3			50 - 150	101%	SPK: 20		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
 Data File : FB032408.D
 Signal(s) : FID2B.CH
 Acq On : 8 Dec 2025 14:49
 Operator : YP/AJ
 Sample : BSF1208S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :

FID_B

ClientSampleId :

BSF1208S2

Manual Integrations**APPROVED**

Reviewed By :Rahul Chavli 12/09/2025

Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
 Quant Time: Dec 09 03:05:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	457065	20.288 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	975936	28.129 ng/mlm
2) t 2,2,4-Trimethylpentane	7.423	1195665	29.890 ng/ml
3) t n-Heptane	7.753	401414	10.159 ng/ml
4) t Benzene	7.892	457605	10.165 ng/ml
6) t Toluene	10.622	1314299	28.767 ng/ml
7) t Ethylbenzene	13.058	391586	9.615 ng/ml
8) t m-Xylene	13.191	826969	19.204 ng/ml
9) t O-Xylene	13.918	792506	19.144 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	670950	19.062 ng/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120825\
Data File : FB032408.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 14:49
Operator : YP/AJ
Sample : BSF1208S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
BSF1208S2

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/09/2025
Supervised By :Yogesh Patel 12/09/2025

Integration File: Calibration.e
Quant Time: Dec 09 03:05:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

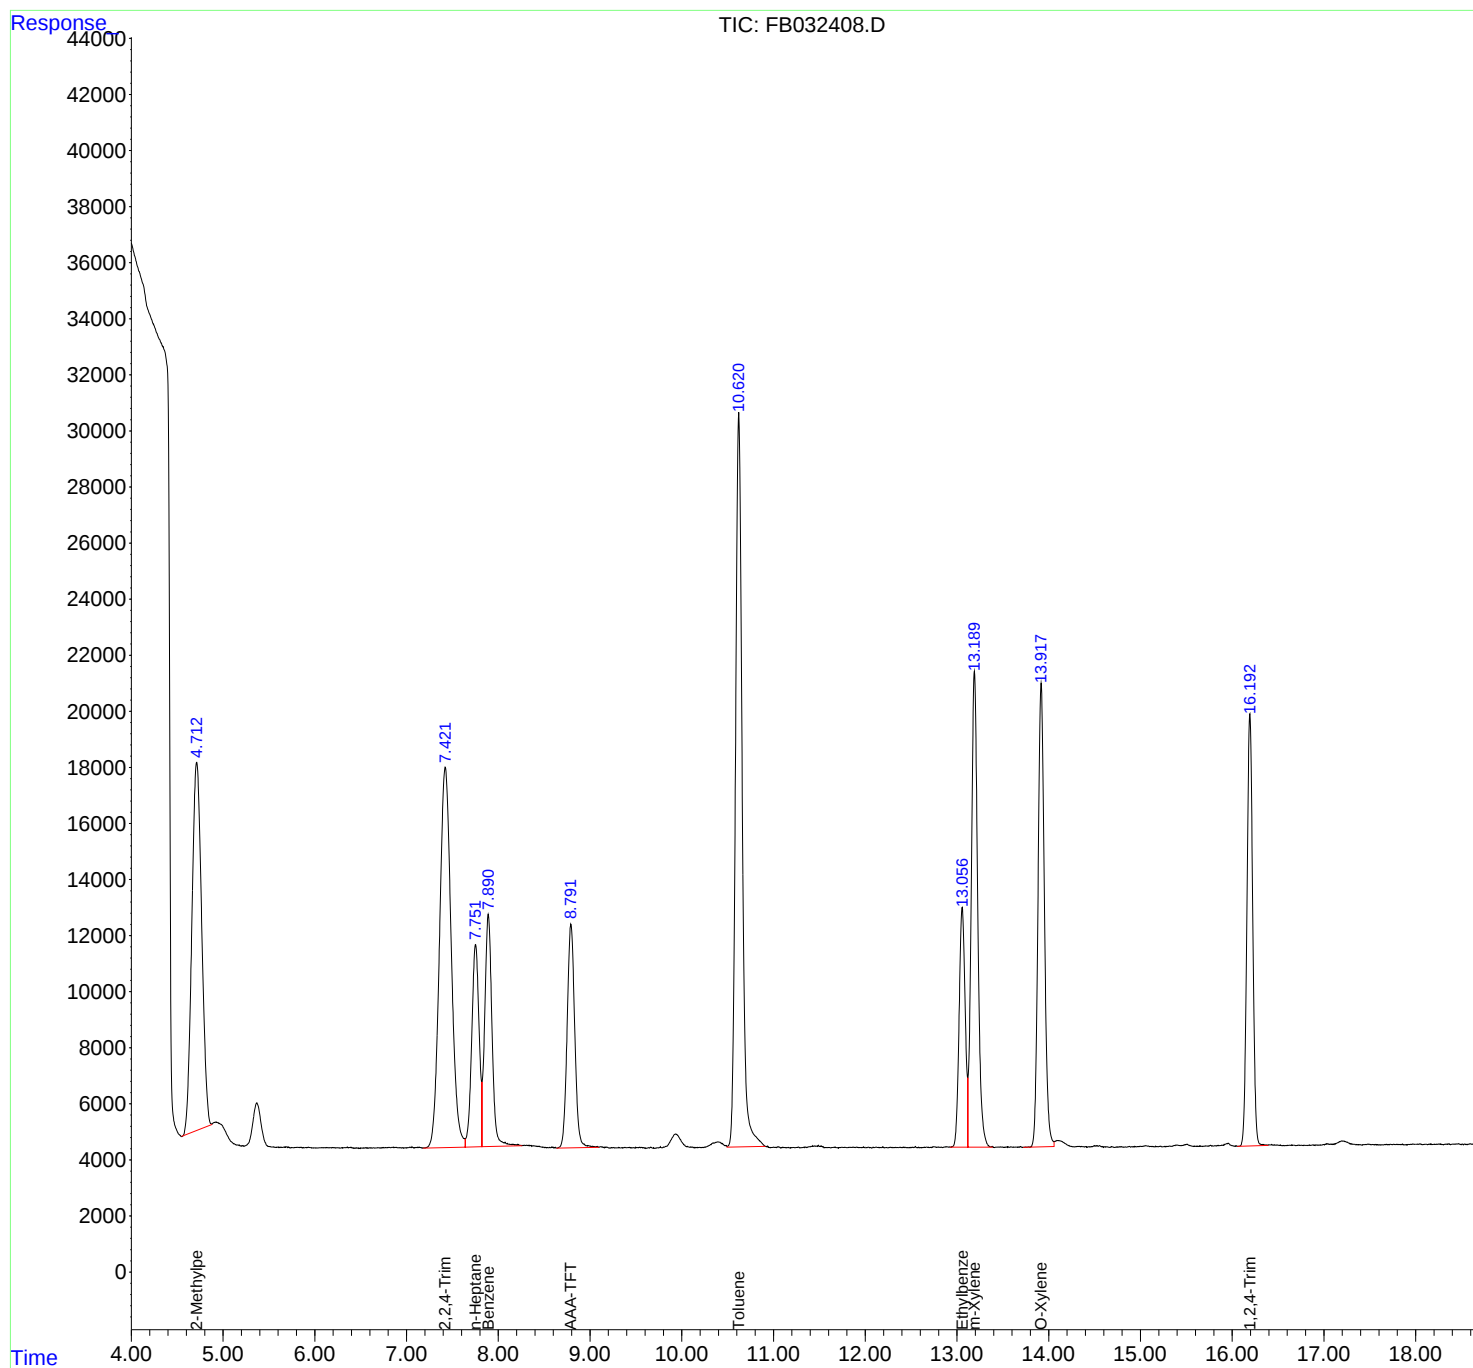

rteres

Instrument :

FID_B

ClientSampleId :

BSF1208S2

Area Percent Report

Manual IntegrationsAPPROVED

Reviewed By :Rahul Chavli 12/09/2025

Supervised By :Yogesh Patel 12/09/2025

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB12082
Data File : FB032408.D
Signal(s) : FID2B.CH
Acq On : 8 Dec 2025 14:49
Sample : BSF1208S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibrat.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Title :

Signal : FID2B.CH

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	4.712	4.551	4.878	M	13135	974631	74.16%	13.025%
2	7.423	7.181	7.640	BV	13563	1195665	90.97%	15.979%
3	7.753	7.640	7.822	VV	7214	401414	30.54%	5.365%
4	7.892	7.822	8.258	VB	8279	457605	34.82%	6.116%
5	8.792	8.637	9.093	BV	7976	457065	34.78%	6.108%
6	10.622	10.494	10.911	VBA	26174	1314299	100.00%	17.565%
7	13.058	12.923	13.119	BV	8549	391586	29.79%	5.233%
8	13.191	13.119	13.391	VBA	16960	826969	62.92%	11.052%
9	13.918	13.725	14.059	BV	16518	792506	60.30%	10.591%
10	16.193	16.055	16.391	PB	15411	670950	51.05%	8.967%

Sum of corrected areas: 7482691

FB120525.M Tue Dec 09 03:45:58 2025

Manual Integration Report

Sample ID	ClientId ID	File ID	Sequence ID	Parameter	Supervised By	Supervised On	Reason
20 PPB GRO STD		FB032399.D	FB120525	2-Methylpentane	yogesh	12/8/2025 11:22:28 AM	Peak Integrated by Software incorrectly

Manual Integration Report

Sample ID	ClientID ID	File ID	Sequence ID	Parameter	Supervised By	Supervised On	Reason
BSF1208S2		FB032408.D	FB120825	2-Methylpentane	yogesh	12/9/2025 10:13:20 AM	Peak Integrated by Software incorrectly
20 PPB GRO STD		FB032409.D	FB120825	2-Methylpentane	yogesh	12/9/2025 10:13:21 AM	Peak Integrated by Software incorrectly
Q3741-05		FB032413.D	FB120825	AAA-TFT	yogesh	12/9/2025 10:13:23 AM	Peak Integrated by Software incorrectly
BSF1208S3		FB032414.D	FB120825	2-Methylpentane	yogesh	12/9/2025 10:13:24 AM	Peak Integrated by Software incorrectly
BSF1208S3		FB032414.D	FB120825	AAA-TFT	yogesh	12/9/2025 10:13:24 AM	Peak Integrated by Software incorrectly
20 PPB GRO STD		FB032415.D	FB120825	2-Methylpentane	yogesh	12/9/2025 10:13:26 AM	Peak Integrated by Software incorrectly

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120525

Review By	rahul	Review On	12/8/2025 3:14:36 PM
Supervise By	yogesh	Supervise On	12/8/2025 3:42:04 PM
SubDirectory	FB120525	HP Acquire Method	FID_B
		HP Processing Method	FB120525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24717,PP25079,PP25080,PP25081,PP25082,PP25083		
CCC Internal Standard/PEM	PP25085		
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24718,PP25084		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	5 GRO STD	FB032390.D	5 Dec 2025 15:41	YP/AJ	Ok
2	10 GRO STD	FB032391.D	5 Dec 2025 16:10	YP/AJ	Ok
3	20 GRO STD	FB032392.D	5 Dec 2025 16:39	YP/AJ	Ok
4	50 GRO STD	FB032393.D	5 Dec 2025 17:08	YP/AJ	Ok
5	100 GRO STD	FB032394.D	5 Dec 2025 17:37	YP/AJ	Ok
6	FB120525GROICV	FB032395.D	5 Dec 2025 18:05	YP/AJ	Ok
7	VBF1205S1	FB032396.D	5 Dec 2025 18:34	YP/AJ	Ok
8	VBF1205S2	FB032397.D	5 Dec 2025 19:03	YP/AJ	Ok
9	Q3735-01	FB032398.D	5 Dec 2025 19:32	YP/AJ	Ok
10	20 PPB GRO STD	FB032399.D	5 Dec 2025 20:15	YP/AJ	Ok,M

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120825

Review By	rahul	Review On	12/9/2025 9:20:57 AM
Supervise By	yogesh	Supervise On	12/9/2025 10:13:36 AM
SubDirectory	FB120825	HP Acquire Method	HP Processing Method FB120525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24717,PP25079,PP25080,PP25081,PP25082,PP25083		
CCC Internal Standard/PEM	PP25086,PP25087,PP25088		
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24718,PP25084		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	20 PPB GRO STD	FB032400.D	8 Dec 2025 9:16	YP/AJ	Ok
2	VBF1208S1	FB032401.D	8 Dec 2025 10:40	YP/AJ	Ok
3	VBF1208S2	FB032402.D	8 Dec 2025 11:09	YP/AJ	Ok
4	BSF1208S1	FB032403.D	8 Dec 2025 11:38	YP/AJ	Ok
5	Q3748-01	FB032404.D	8 Dec 2025 12:28	YP/AJ	Ok
6	Q3741-06	FB032405.D	8 Dec 2025 13:19	YP/AJ	Ok
7	Q3741-05	FB032406.D	8 Dec 2025 13:48	YP/AJ	Not Ok
8	Q3741-04	FB032407.D	8 Dec 2025 14:17	YP/AJ	Ok
9	BSF1208S2	FB032408.D	8 Dec 2025 14:49	YP/AJ	Ok,M
10	20 PPB GRO STD	FB032409.D	8 Dec 2025 15:18	YP/AJ	Ok,M
11	Q3741-01	FB032410.D	8 Dec 2025 16:05	YP/AJ	Ok
12	Q3741-02	FB032411.D	8 Dec 2025 16:34	YP/AJ	Ok
13	Q3741-03	FB032412.D	8 Dec 2025 17:03	YP/AJ	Ok
14	Q3741-05	FB032413.D	8 Dec 2025 17:32	YP/AJ	Dilution
15	BSF1208S3	FB032414.D	8 Dec 2025 18:01	YP/AJ	Ok,M
16	20 PPB GRO STD	FB032415.D	8 Dec 2025 18:30	YP/AJ	Ok,M

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120925

Review By	rahul	Review On	12/9/2025 11:44:18 AM
Supervise By		Supervise On	
SubDirectory	FB120925	HP Acquire Method	HP Processing Method FB120525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24717,PP25079,PP25080,PP25081,PP25082,PP25083		
CCC Internal Standard/PEM	PP25086,PP25087,PP25088		
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24718,PP25084		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	20 PPB GRO STD	FB032416.D	9 Dec 2025 9:26	YP/AJ	Ok
2	VBF1209S1	FB032417.D	9 Dec 2025 10:37	YP/AJ	Ok
3	VBF1209S2	FB032418.D	9 Dec 2025 11:06	YP/AJ	Ok
4	BSF1209S1	FB032419.D	9 Dec 2025 11:34	YP/AJ	Ok
5	Q3741-05	FB032420.D	9 Dec 2025 12:25	YP/AJ	Ok
6	BSF1209S2	FB032421.D	9 Dec 2025 13:16	YP/AJ	Ok
7	20 PPB GRO STD	FB032422.D	9 Dec 2025 13:45	YP/AJ	Ok

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120525

Review By	rahul	Review On	12/8/2025 3:14:36 PM		
Supervise By	yogesh	Supervise On	12/8/2025 3:42:04 PM		
SubDirectory	FB120525	HP Acquire Method	FID_B	HP Processing Method	FB120525
STD. NAME		STD REF.#			
Tune/Reschk					
Initial Calibration Stds		PP24717,PP25079,PP25080,PP25081,PP25082,PP25083			
CCC		PP25085			
Internal Standard/PEM					
ICV/I.BLK		PP24718,PP25084			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	5 GRO STD		FB032390.D	5 Dec 2025 15:41		YP/AJ	Ok
2	10 GRO STD		FB032391.D	5 Dec 2025 16:10		YP/AJ	Ok
3	20 GRO STD		FB032392.D	5 Dec 2025 16:39		YP/AJ	Ok
4	50 GRO STD		FB032393.D	5 Dec 2025 17:08		YP/AJ	Ok
5	100 GRO STD		FB032394.D	5 Dec 2025 17:37		YP/AJ	Ok
6	FB120525GROICV		FB032395.D	5 Dec 2025 18:05		YP/AJ	Ok
7	VBF1205S1		FB032396.D	5 Dec 2025 18:34		YP/AJ	Ok
8	VBF1205S2		FB032397.D	5 Dec 2025 19:03		YP/AJ	Ok
9	Q3735-01		FB032398.D	5 Dec 2025 19:32		YP/AJ	Ok
10	20 PPB GRO STD		FB032399.D	5 Dec 2025 20:15		YP/AJ	Ok,M

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120825

Review By	rahul	Review On	12/9/2025 9:20:57 AM
Supervise By	yogesh	Supervise On	12/9/2025 10:13:36 AM
SubDirectory	FB120825	HP Acquire Method	HP Processing Method FB120525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24717,PP25079,PP25080,PP25081,PP25082,PP25083		
CCC	PP25086,PP25087,PP25088		
Internal Standard/PEM			
ICV/I.BLK	PP24718,PP25084		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	20 PPB GRO STD		FB032400.D	8 Dec 2025 9:16		YP/AJ	Ok
2	VBF1208S1		FB032401.D	8 Dec 2025 10:40		YP/AJ	Ok
3	VBF1208S2		FB032402.D	8 Dec 2025 11:09		YP/AJ	Ok
4	BSF1208S1		FB032403.D	8 Dec 2025 11:38		YP/AJ	Ok
5	Q3748-01		FB032404.D	8 Dec 2025 12:28	Vial A	YP/AJ	Ok
6	Q3741-06		FB032405.D	8 Dec 2025 13:19	Vial A	YP/AJ	Ok
7	Q3741-05		FB032406.D	8 Dec 2025 13:48	Not Purge,Vial A	YP/AJ	Not Ok
8	Q3741-04		FB032407.D	8 Dec 2025 14:17	Vial A	YP/AJ	Ok
9	BSF1208S2		FB032408.D	8 Dec 2025 14:49		YP/AJ	Ok,M
10	20 PPB GRO STD		FB032409.D	8 Dec 2025 15:18		YP/AJ	Ok,M
11	Q3741-01		FB032410.D	8 Dec 2025 16:05	Vial A	YP/AJ	Ok
12	Q3741-02		FB032411.D	8 Dec 2025 16:34	Vial A	YP/AJ	Ok
13	Q3741-03		FB032412.D	8 Dec 2025 17:03	Vial A	YP/AJ	Ok
14	Q3741-05		FB032413.D	8 Dec 2025 17:32	Need dilution,Vial B	YP/AJ	Dilution
15	BSF1208S3		FB032414.D	8 Dec 2025 18:01		YP/AJ	Ok,M
16	20 PPB GRO STD		FB032415.D	8 Dec 2025 18:30		YP/AJ	Ok,M

M : Manual Integration

Instrument ID: FID_B

Daily Analysis Runlog For Sequence/QC Batch ID # FB120925

Review By	rahul	Review On	12/9/2025 11:44:18 AM
Supervise By		Supervise On	
SubDirectory	FB120925	HP Acquire Method	HP Processing Method FB120525

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	PP24717,PP25079,PP25080,PP25081,PP25082,PP25083
CCC Internal Standard/PEM	PP25086,PP25087,PP25088
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24718,PP25084

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	20 PPB GRO STD		FB032416.D	9 Dec 2025 9:26		YP/AJ	Ok
2	VBF1209S1		FB032417.D	9 Dec 2025 10:37		YP/AJ	Ok
3	VBF1209S2		FB032418.D	9 Dec 2025 11:06		YP/AJ	Ok
4	BSF1209S1		FB032419.D	9 Dec 2025 11:34		YP/AJ	Ok
5	Q3741-05		FB032420.D	9 Dec 2025 12:25		YP/AJ	Ok
6	BSF1209S2		FB032421.D	9 Dec 2025 13:16		YP/AJ	Ok
7	20 PPB GRO STD		FB032422.D	9 Dec 2025 13:45		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 12/2/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:30
In Date: 12/01/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 12/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB138066

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q3741-01	B50-SP3-111925	1	1.15	10.38	11.53	10.66	91.6	
Q3741-02	B50-SP13-112025	2	1.18	10.33	11.51	10.1	86.4	
Q3741-03	B50-SP14-112025	3	1.19	10.25	11.44	10.14	87.3	
Q3741-04	B50-SP9-112425	4	1.16	10.61	11.77	10.2	85.2	
Q3741-05	B50-SP11-112525	5	1.16	10.47	11.63	10.02	84.6	
Q3741-06	B50-SP4-112525	6	1.18	10.50	11.68	10.2	85.9	
Q3742-01	SB-1125-23	7	1.11	10.61	11.72	8.55	70.1	
Q3742-02	SB-1125-19	8	1.19	11.07	12.26	5.72	40.9	
Q3742-03	SB-1125-8	9	1.17	10.55	11.72	10.16	85.2	
Q3742-04	SB-1125-9	10	1.19	10.57	11.76	9.5	78.6	
Q3742-05	SB-1125-21	11	1.16	10.61	11.77	9.6	79.5	
Q3742-06	SB-1125-13	12	1.18	10.18	11.36	9.88	85.5	
Q3742-07	SB-1125-18	13	1.11	10.19	11.3	8.07	68.3	
Q3742-08	SB-1125-20	14	1.15	10.84	11.99	9.86	80.4	
Q3742-09	SB-1125-22	15	1.12	10.90	12.02	9.05	72.8	
Q3742-10	SB-1125-2	16	1.16	10.76	11.92	9.38	76.4	
Q3742-11	SB-1125-3A	17	1.19	10.58	11.77	8.93	73.2	
Q3742-12	SB-1125-3B	18	1.17	10.50	11.67	10.55	89.3	
Q3742-13	SB-1125-3C	19	1.16	10.50	11.66	9.31	77.6	
Q3742-14	SB-1125-3D	20	1.13	10.45	11.58	8.5	70.5	
Q3742-14D	SB-1125-3DDUP	21	1.15	10.45	11.6	8.53	70.6	
Q3742-15	SB-1125-3E	22	1.13	10.39	11.52	8.05	66.6	
Q3742-16	SB-1125-1	23	1.19	10.33	11.52	8.78	73.5	
Q3742-17	SB-1125-25	24	1.18	11.18	12.36	8.26	63.3	
Q3742-18	SB-1125-24	25	1.15	10.90	12.05	7.99	62.8	
Q3745-05	SVOC-GPC-BLANK	31	1.00	1.00	2.00	2.00	100.0	
Q3745-06	PEST-GPC-BLANK	32	1.00	1.00	2.00	2.00	100.0	
Q3745-07	PEST-GPC-BLANK-SPIKE	33	1.00	1.00	2.00	2.00	100.0	



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 12/2/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:30
In Date: 12/01/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 12/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB138066

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q3745-08	SVOC-GPC2-BLANK	34	1.00	1.00	2.00	2.00	100.0	
Q3745-09	PEST-GPC2-BLANK	35	1.00	1.00	2.00	2.00	100.0	
Q3745-10	PEST -GPC2-BLANK-SPIKE	36	1.00	1.00	2.00	2.00	100.0	
Q3746-01	ROW	26	1.15	10.84	11.99	8.59	68.6	
Q3746-02	ROW-E2	27	1.14	10.58	11.72	5.2	38.4	
Q3747-01	1	28	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3747-02	2	29	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3747-03	3	30	1.00	1.00	2.00	2.00	100.0	WIPE SAMPLE
Q3748-01	AU-05-12-1-2025	37	1.18	10.75	11.93	11.03	91.6	
Q3748-02	AU-05-12-1-2025	38	1.18	10.55	11.73	10.88	91.9	
Q3750-01	FENCE WC-1	39	1.15	10.77	11.92	10.5	86.8	
Q3750-02	FENCE WC-1-EPH	40	1.19	10.31	11.5	10.15	86.9	
Q3750-03	FENCE WC-1-VOC	41	1.16	10.58	11.74	9.72	80.9	
Q3750-04	FENCE WC-2	42	1.11	10.51	11.62	10.2	86.5	
Q3750-05	FENCE WC-2-EPH	43	1.13	10.21	11.34	9.97	86.6	
Q3750-06	FENCE WC-2-VOC	44	1.19	10.38	11.57	10.52	89.9	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

128066

WorkList Name : %1-120125 WorkList ID : 193391 Department : Wet-Chemistry Date : 12-01-2025 08:55:16

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3741-01	B50-SP3-111925	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/19/2025	Chemtech -SO
Q3741-02	B50-SP13-112025	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/20/2025	Chemtech -SO
Q3741-03	B50-SP14-112025	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/20/2025	Chemtech -SO
Q3741-04	B50-SP9-112425	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/24/2025	Chemtech -SO
Q3741-05	B50-SP11-112525	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/25/2025	Chemtech -SO
Q3741-06	B50-SP4-112525	Solid	Percent Solids	Cool 4 deg C	CORE02	--Sele	11/25/2025	Chemtech -SO
Q3742-01	SB-1125-23	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/6025	Chemtech -SO
Q3742-02	SB-1125-19	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-03	SB-1125-8	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-04	SB-1125-9	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-05	SB-1125-21	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-06	SB-1125-13	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-07	SB-1125-18	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-08	SB-1125-20	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-09	SB-1125-22	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-10	SB-1125-2	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-11	SB-1125-3A	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-12	SB-1125-3B	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-13	SB-1125-3C	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-14	SB-1125-3D	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-15	SB-1125-3E	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO

Date/Time 12/01/25 15:13
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]
 Date/Time 12/01/25 17:40
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

g 172066

WorkList Name : %1-120125

WorkList ID : 193391

Department : Wet-Chemistry

Date : 12-01-2025 08:55:16

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3742-16	SB-1125-1	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-17	SB-1125-25	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3742-18	SB-1125-24	Solid	Percent Solids	Cool 4 deg C	REMI01	A21	11/25/2025	Chemtech -SO
Q3745-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3745-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3745-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3745-08	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3745-09	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3745-10	PEST -GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	A12	11/21/2025	Chemtech -SO
Q3746-01	ROW	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/02/2025	Chemtech -SO
Q3746-02	ROW-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/02/2025	Chemtech -SO
Q3747-01	1	Solid	Percent Solids	Cool 4 deg C	PSEG03	A11	12/01/2025	Chemtech -SO
Q3747-02	2	Solid	Percent Solids	Cool 4 deg C	PSEG03	A11	12/01/2025	Chemtech -SO
Q3747-03	3	Solid	Percent Solids	Cool 4 deg C	PSEG03	A11	12/01/2025	Chemtech -SO
Q3748-01	AU-05-12-1-2025	Solid	Percent Solids	Cool 4 deg C	PSEG03	A11	12/01/2025	Chemtech -SO
Q3748-02	AU-05-12-1-2025	Solid	Percent Solids	Cool 4 deg C	PSEG05	A12	12/01/2025	Chemtech -SO
Q3750-01	FENCE WC-1	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO
Q3750-02	FENCE WC-1-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO
Q3750-03	FENCE WC-1-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO
Q3750-04	FENCE WC-2	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO
Q3750-05	FENCE WC-2-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO

Date/Time 12/01/25 15:15
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

Date/Time 12/01/25 17:40
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

138066

WorkList Name : %1-120125

WorkList ID : 193391

Department : Wet-Chemistry

Date : 12-01-2025 08:55:16

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q3750-06	FENCE WC-2-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG05	A11	12/01/2025	Chemtech -SO

Date/Time 12/01/25 13:15
Raw Sample Received by: SB WPC
Raw Sample Relinquished by: CR 8

Date/Time 12/01/25 17:40
Raw Sample Received by: CR 8
Raw Sample Relinquished by: SB WPC



SHIPPING DOCUMENTS



284 Sheffield Street, Mountainside, NJ 07092

(908) 789-8900 Fax: (908) 788-9222

www.chemtech.net

CHAIN OF CUSTODY RECORD

Alliance Project Number:

23741

COC Number:

CLIENT INFORMATION

COMPANY: CORE ENVIRONMENTAL CONSULTANTS

ADDRESS: 22-48 119TH STREET

CITY: COLLEGE POINT STATE: NY ZIP: 11356

ATTENTION: ROLAND SCARDINO

PHONE: 609-781-8074

FAX:

PROJECT INFORMATION

PROJECT NAME: BNY - Building 50 Probe Investigation

PROJECT #:

LOCATION: Bldg 50. 63 Flushing Ave.
Brooklyn, NY

PROJECT MANAGER: ROLAND SCARDINO

E-MAIL: rscardino@coreenv.com

PHONE: 609-781-8074

FAX:

BILLING INFORMATION

BILL TO: CORE ENVIRONMENTAL CONSULTANTS PO#

ADDRESS: 2312 WEHRLE DR

CITY: BUFFALO

STATE: NY ZIP: 14221

ATTENTION: JOSEPH ZAHEER

PHONE: 716-204-8054

DATA TURNAROUND INFORMATION

FAX: STANDARD DAYS*
HARD COPY: STANDARD DAYS*
EDD STANDARD DAYS*

* TO BE APPROVED BY ALLIANCE

STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

- ☐ RESULTS ONLY ☐ USEPA CLP
☐ RESULTS + QC ☐ New York State ASP "B"
☐ New Jersey REDUCED ☐ New York State ASP "A"
☐ New Jersey CLP ☐ Other _____
☐ EDD Format _____

ANALYSIS

GRO	DRO	VOCs	SVOCs	TAL Metals	PCBs				
1	2	3	4	5	6	7	8	9	

If any metals exceed the 20x
rule, run the TCLP analysis
on 72-hr TAT

PRESERVATIVES

1	2	3	4	5	6	7	8	9
✓	✓	✓	✓	✓	✓			
✓	✓	✓	✓	✓	✓			
✓	✓	✓	✓	✓	✓			
✓	✓	✓	✓	✓	✓			
✓	✓	✓	✓	✓	✓			

COMMENTS

← Specify Preservatives
A-HCl B-HNO3
C-H2SO4 D-NaOH
E-ICE F-Other

CHEMTECH
SAMPLE
IDPROJECT
SAMPLE IDENTIFICATIONSAMPLE
MATRIXSAMPLE
TYPESAMPLE
COLLECTION

of Bottles

COMP

GRAB

DATE

TIME

1.	B50-SP3-111925	SOIL	✓		11/19/25	13:00	
2.	B50-SP3-112025	SOIL	✓		11/20/25	13:00	
3.	B50-SP4-112025	SOIL	✓		11/20/25	13:15	
4.	B50-SP9-112425	SOIL	✓		11/24/25	13:30	
5.	B50-SP11-112525	SOIL	✓		11/25/25	13:30	
6.	B50-SP4-112525	SOIL	✓		11/25/25	14:00	
7.							
8.							
9.							
10.							

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER	DATE/TIME	RECEIVED BY
1.	11/26 12:10p	1.
RELINQUISHED BY	DATE/TIME	RECEIVED BY
2.		2.
RELINQUISHED BY	DATE/TIME	RECEIVED FOR LAB BY
3.	11-26-25	3.

Conditions of bottles or coolers at receipt:

☐ Compliant ☐ Non Compliant☐ Cooler Temp 3.1°C

MeOH extraction requires an additional 4oz. Jar for percent solid

☐ Ice in Cooler?: _____

Comments:

SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ OvernightALLIANCE: ☐ Picked Up ☐ Overnight

Shipment Complete

☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT

YELLOW - ALLIANCE COPY

PINK - SAMPLER COPY

Shreena

From: Roland Scardino <rscardino@coreenv.com>
Sent: Monday, December 01, 2025 10:47 AM
Subject: RE: TB SAMPLES

EXTERNAL EMAIL - This email was sent by a person from outside your organization. Exercise caution when clicking links, opening attachments or taking further action, before validating its authenticity.

Secured by Check Point

Good morning Deepak,

We received 2 TB's in the cooler, so two were sent back to the lab. Please use one of them for the analysis.

Thank you,

Roland Scardino
Project Manager
CORE Environmental Consultants, Inc.
C: 609-781-8074
O: 718-786-4730 ext 114

22-48 119 th Street	2312 Wehrle Drive
College Point, NY 11356	Buffalo, NY 14221
P: 718.786.4730	P: 716.204.8054
F: 718.786.4764	F: 716.204.8557



www.COREenv.com

Innovative Engineering and Environmental Solutions

Laboratory Certification

Certified By	License No.
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255425
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	TX-C25-00189
Virginia	460312

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3741	CORE02	Order Date : 11/26/2025 4:57:55 PM	Project Mgr :
Client Name : Core Environmental Consul		Project Name : Building 50 Probe Investiga	Report Type : Results+QC
Client Contact : Roland Scardino		Receive DateTime : 11/26/2025 6:20:00 PM	EDD Type : Excel NY
Invoice Name : Core Environmental Consul		Purchase Order :	Hard Copy Date :
Invoice Contact : Roland Scardino			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q3741-01	B50-SP3-111925	Solid	11/19/2025	13:00					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-02	B50-SP13-112025	Solid	11/20/2025	13:00					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-03	B50-SP14-112025	Solid	11/20/2025	13:15					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-04	B50-SP9-112425	Solid	11/24/2025	13:30					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-05	B50-SP11-112525	Solid	11/25/2025	13:30					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-06	B50-SP4-112525	Solid	11/25/2025	14:00					
					VOC-TCLVOA-10		8260C		10 Bus. Days
Q3741-07	TB-1	Water	11/25/2025	14:00					
					VOC-TCLVOA-10		8260-Low		10 Bus. Days


LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q3741	CORE02	Order Date : 11/26/2025 4:57:55 PM	Project Mgr :
Client Name : Core Environmental Consul		Project Name : Building 50 Probe Investiga	Report Type : Results+QC
Client Contact : Roland Scardino		Receive DateTime : 11/26/2025 6:20:00 PM	EDD Type : Excel NY
Invoice Name : Core Environmental Consul		Purchase Order :	Hard Copy Date :
Invoice Contact : Roland Scardino			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
--------	-----------	--------	----------------	----------------	------	------------	--------	----------	--------------

Relinquished By : 

Date / Time : 12/1/25 11:05

Received By : 

Date / Time : 12/01/25 11:05

Storage Area : VOA Refridgerator Room