
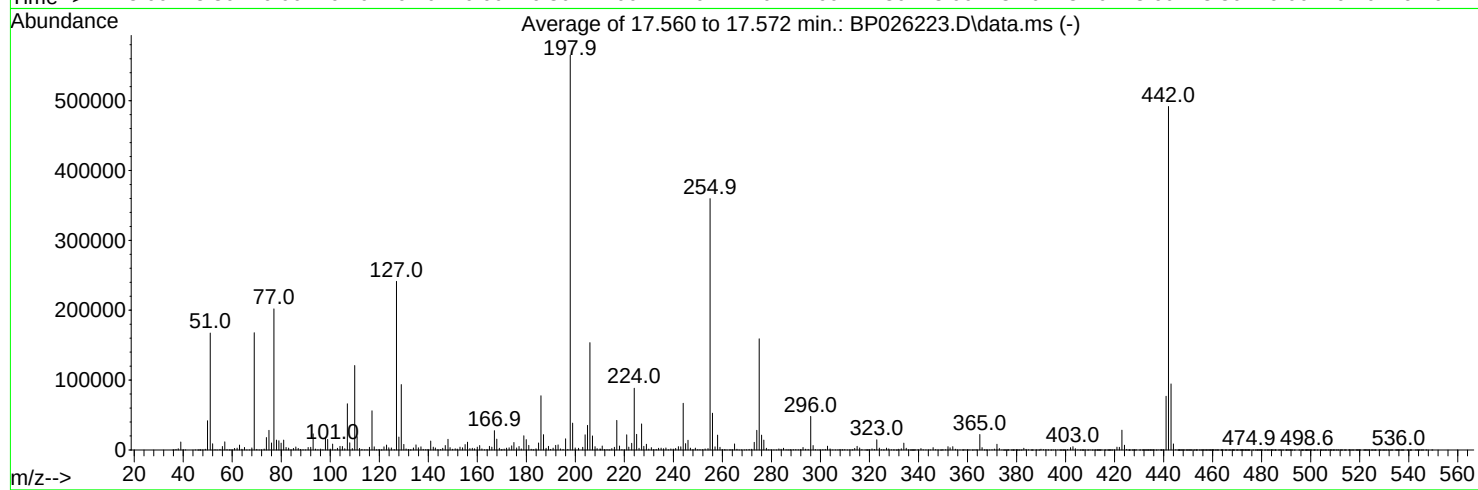


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120325\
Data File : BP026223.D
Acq On : 03 Dec 2025 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

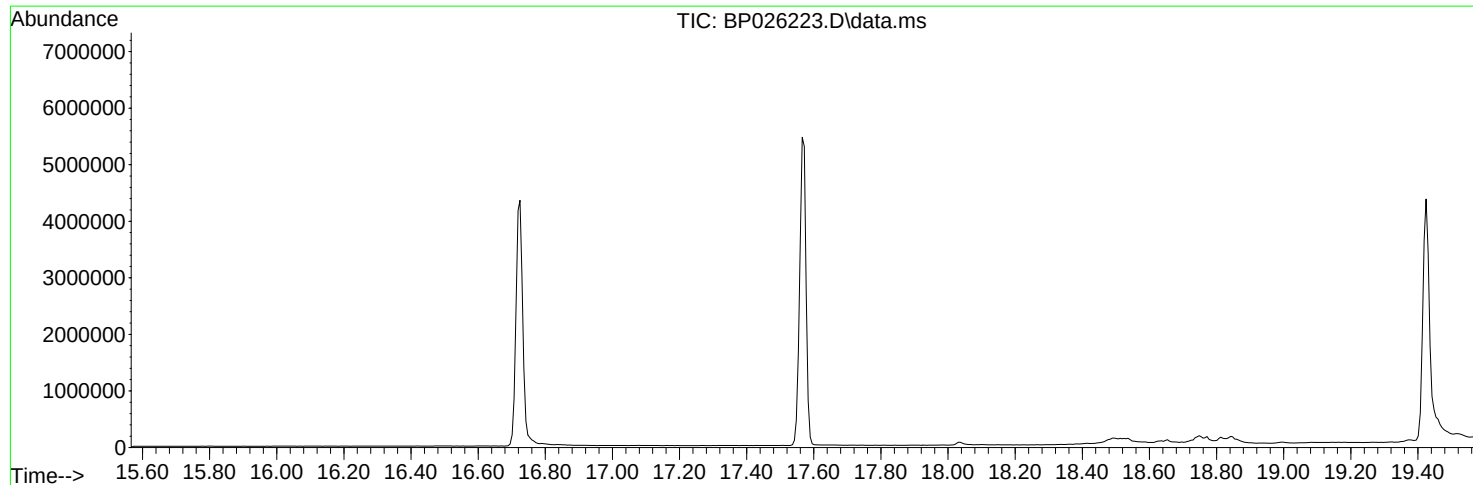




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	2821	PASS
69	69	100	100	100.0	167728	PASS
70	69	0.00	2	0.5	841	PASS
197	198	0.00	2	0.1	771	PASS
198	198	100	100	100.0	565248	PASS
199	198	5	9	6.8	38282	PASS
365	198	1	100	3.9	22129	PASS
441	443	0.01	150	81.3	76854	PASS
442	442	100	100	100.0	491627	PASS
443	442	15	24	19.2	94587	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120325\
Data File : BP026223.D
Acq On : 03 Dec 2025 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 03 13:04:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

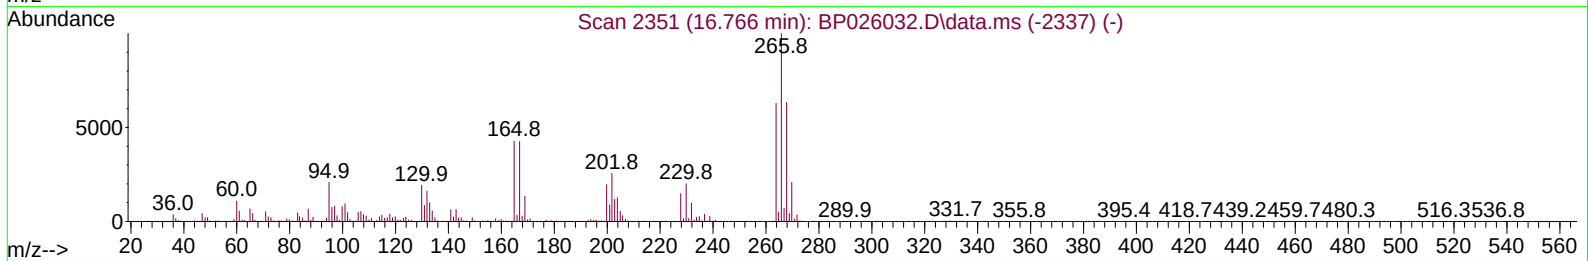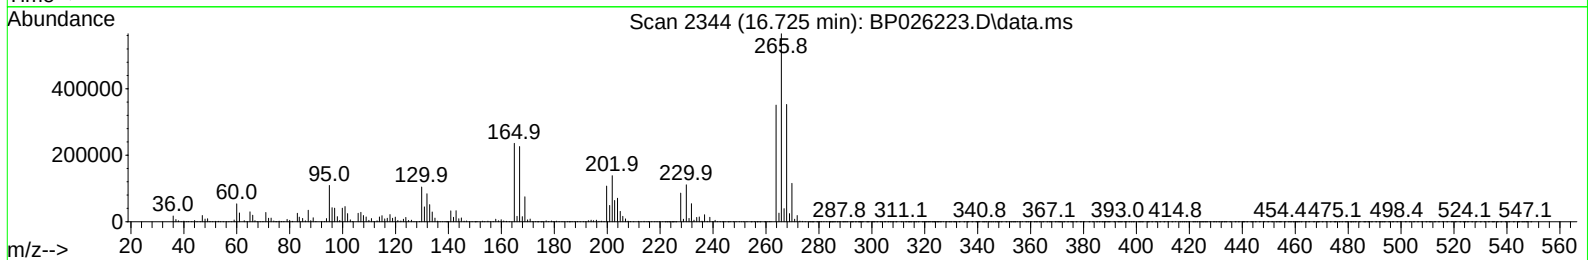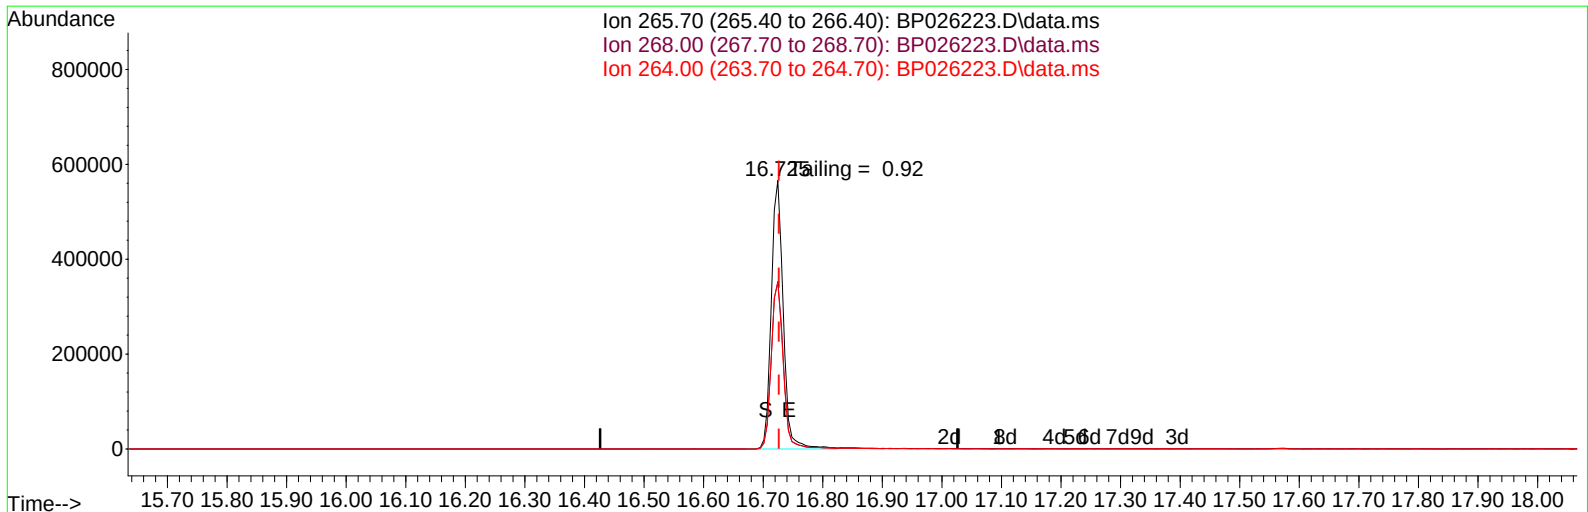

TIC: BP026223.D\data.ms

(70) Pentachlorophenol (C)

16.725min (-0.002) 23877.06 ng m




response 803180

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.35
264.00	62.70	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120325\
Data File : BP026223.D
Acq On : 03 Dec 2025 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 03 13:08:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

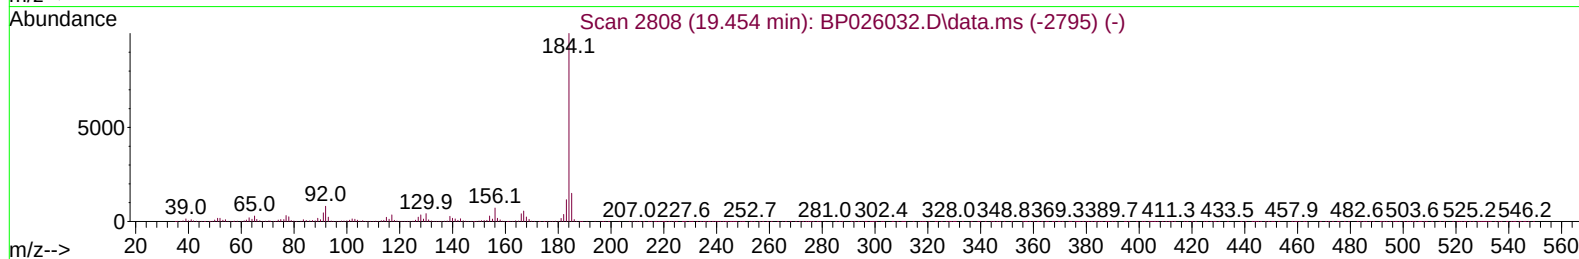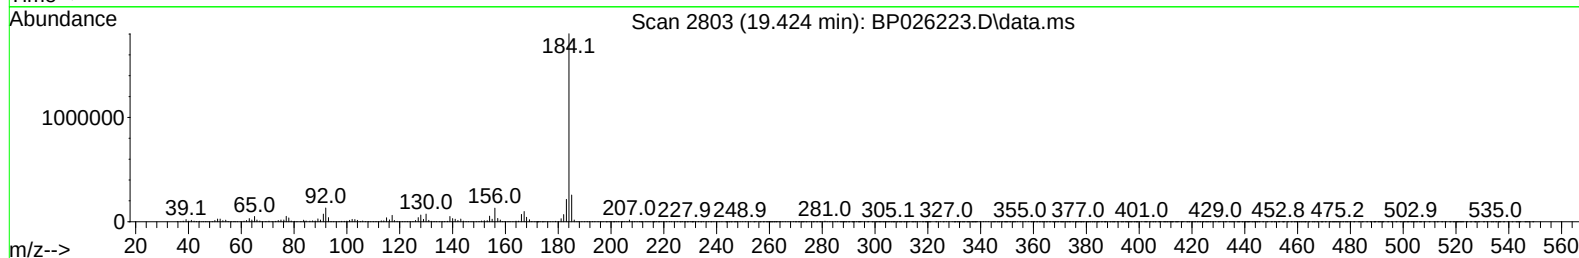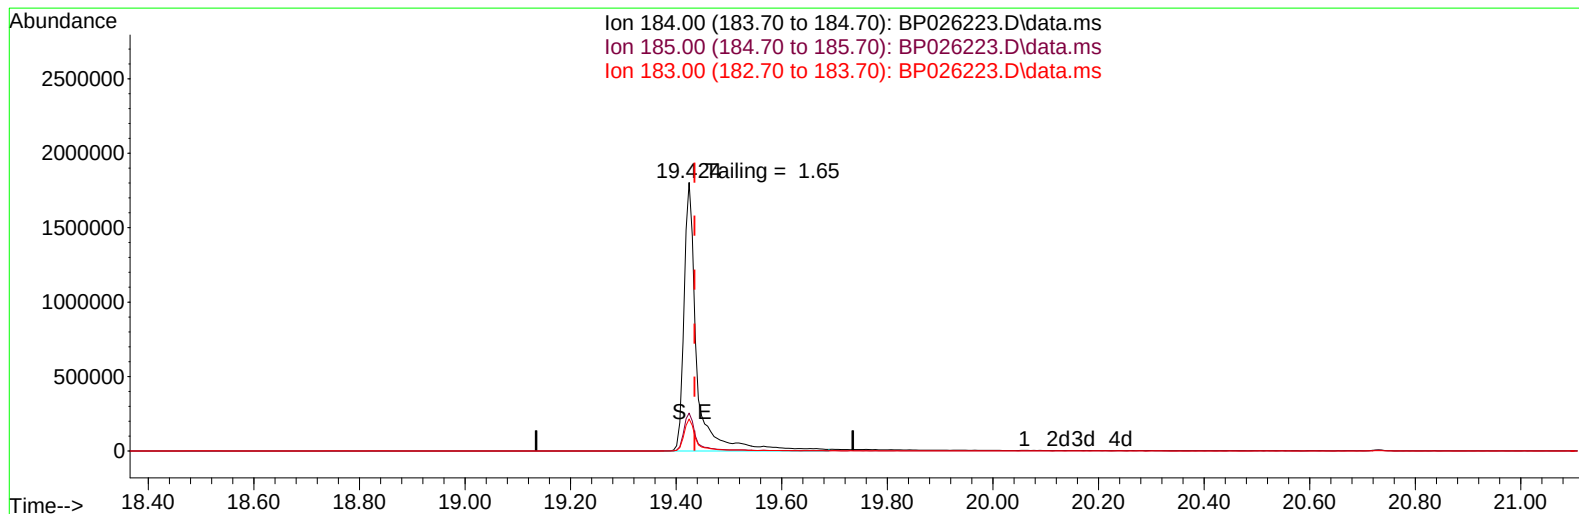

TIC: BP026223.D\data.ms

(77) Benzidine

19.424min (-0.010) 582608.37 ng m

response 3235664

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.14
183.00	11.30	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/3/2025	BNA_P	<u>BP026223.D</u>
Compound Name	Response	Retention Time
DDT	1847364	20.73
DDD	58978	20.266
DDE	3263	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
62241	1909605	3.26

Instrument :
BNA_P
ClientSampleId :
DFTPP