
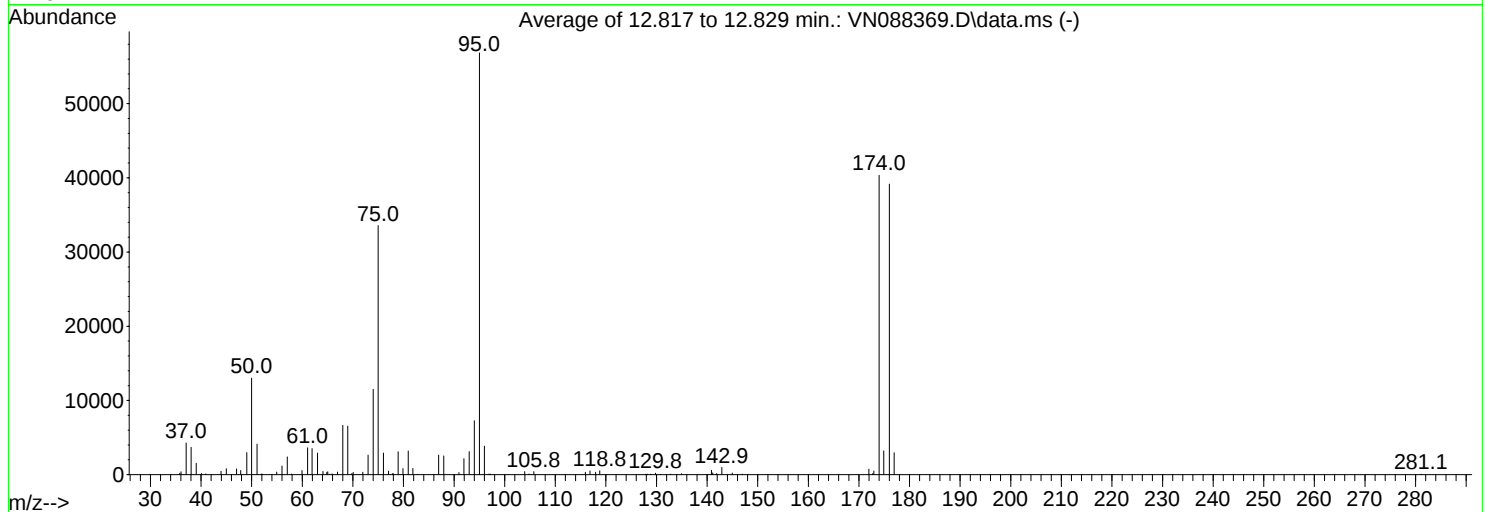


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN120125\  
Data File : VN088369.D  
Acq On : 01 Dec 2025 08:49  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N112425W.M  
Title : SW846 8260  
Last Update : Tue Nov 25 01:34:52 2025

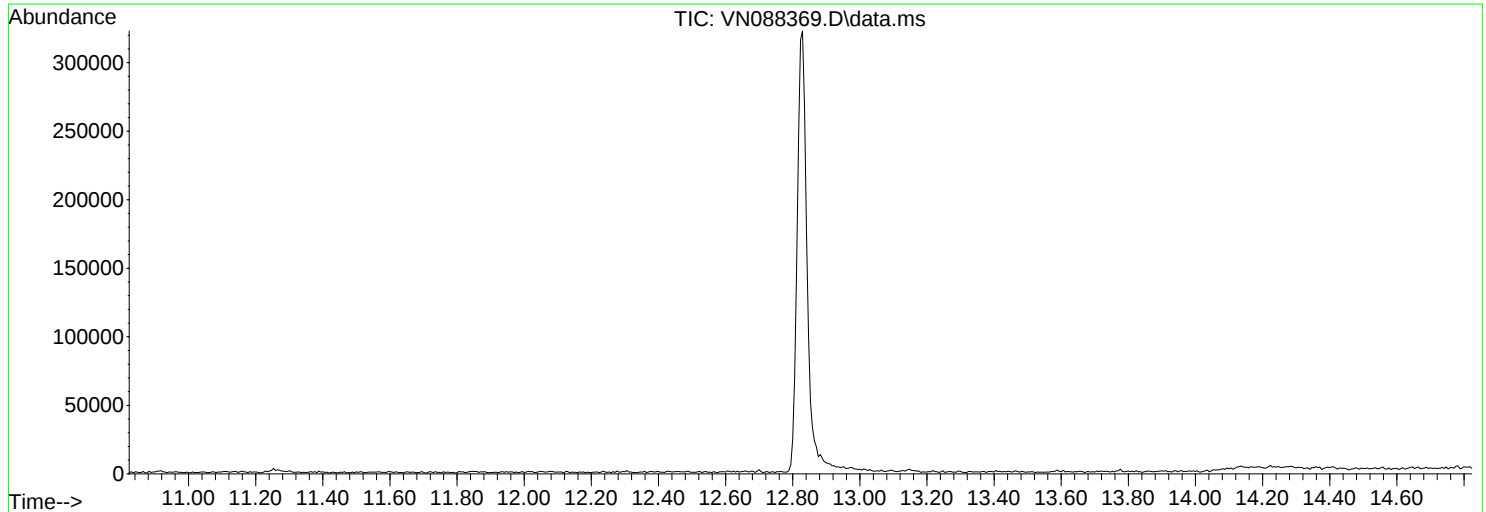

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1838

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 22.9         | 13006      | PASS                |
| 75             | 95              | 30              | 60              | 59.1         | 33576      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 56845      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 3835       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 489        | PASS                |
| 174            | 95              | 50              | 100             | 71.0         | 40341      | PASS                |
| 175            | 174             | 5               | 9               | 8.0          | 3213       | PASS                |
| 176            | 174             | 95              | 101             | 97.1         | 39165      | PASS                |
| 177            | 176             | 5               | 9               | 7.5          | 2949       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.80 | 190    | 49.05 | 2976   | 61.95 | 3517   | 70.05 | 311    |
| 36.05 | 384    | 50.00 | 13006  | 63.00 | 2917   | 71.95 | 331    |
| 37.05 | 4272   | 51.05 | 4113   | 64.10 | 433    | 73.00 | 263    |
| 38.05 | 3684   | 51.90 | 88     | 64.85 | 304    | 74.00 | 1149   |
| 39.05 | 1525   | 52.10 | 68     | 65.05 | 399    | 75.00 | 33576  |
| 40.10 | 142    | 54.95 | 339    | 65.40 | 72     | 76.05 | 2917   |
| 40.95 | 105    | 56.00 | 1161   | 65.90 | 102    | 77.05 | 468    |
| 43.95 | 455    | 57.05 | 2400   | 66.95 | 355    | 77.80 | 128    |
| 45.00 | 808    | 57.90 | 81     | 68.00 | 6639   | 78.00 | 126    |
| 47.00 | 782    | 59.95 | 560    | 69.00 | 6543   | 78.95 | 3079   |
| 47.85 | 567    | 61.05 | 3625   | 69.80 | 174    | 79.90 | 824    |

Average of 12.817 to 12.829 min.: VN088369.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|-------|--------|--------|--------|--------|--------|--------|--------|
| 80.95 | 3198   | 96.00  | 3835   | 128.20 | 67     | 147.00 | 61     |
| 81.85 | 841    | 96.90  | 89     | 128.80 | 61     | 148.00 | 50     |
| 82.80 | 51     | 97.20  | 58     | 129.80 | 188    | 171.95 | 743    |
| 86.00 | 50     | 103.95 | 408    | 130.80 | 50     | 172.70 | 124    |
| 86.95 | 2627   | 104.80 | 82     | 132.80 | 67     | 172.95 | 489    |
| 87.95 | 2534   | 105.75 | 414    | 134.95 | 138    | 174.00 | 40341  |
| 90.95 | 286    | 115.95 | 332    | 140.85 | 577    | 174.90 | 3213   |
| 91.95 | 2167   | 116.85 | 505    | 141.10 | 238    | 176.00 | 39165  |
| 93.00 | 3106   | 117.95 | 315    | 141.90 | 151    | 176.95 | 2949   |
| 94.00 | 7272   | 118.80 | 513    | 142.90 | 969    | 281.10 | 73     |
| 95.00 | 56845  | 127.80 | 56     | 144.95 | 206    |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB