
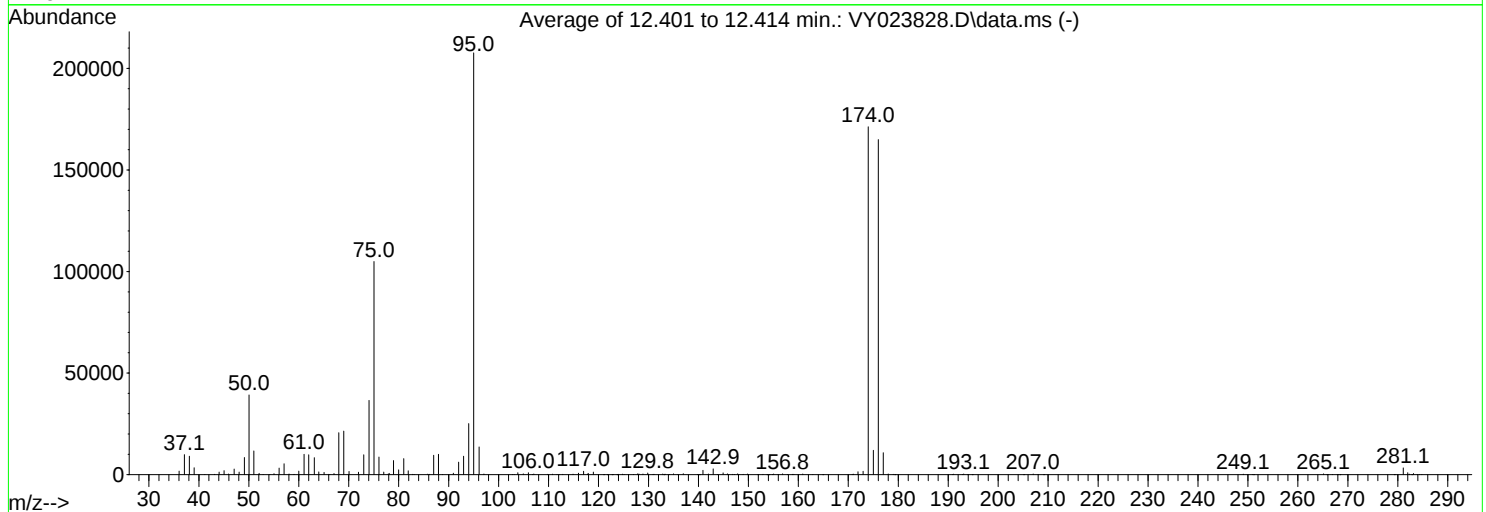


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120125\
Data File : VY023828.D
Acq On : 01 Dec 2025 07:24
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y112625S.M
Title : SW846 8260
Last Update : Thu Nov 27 01:14:36 2025

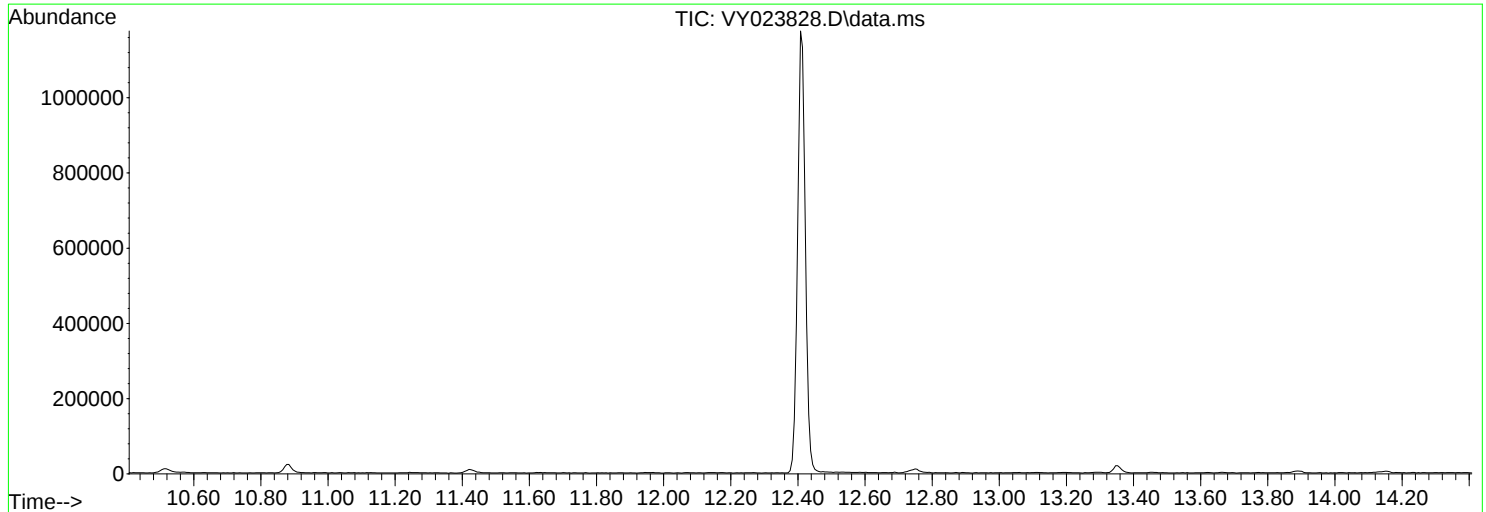

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	39200	PASS
75	95	30	60	50.5	104963	PASS
95	95	100	100	100.0	207680	PASS
96	95	5	9	6.6	13621	PASS
173	174	0.00	2	1.0	1686	PASS
174	95	50	100	82.5	171261	PASS
175	174	5	9	7.0	12023	PASS
176	174	95	101	96.3	164952	PASS
177	176	5	9	6.5	10787	PASS