
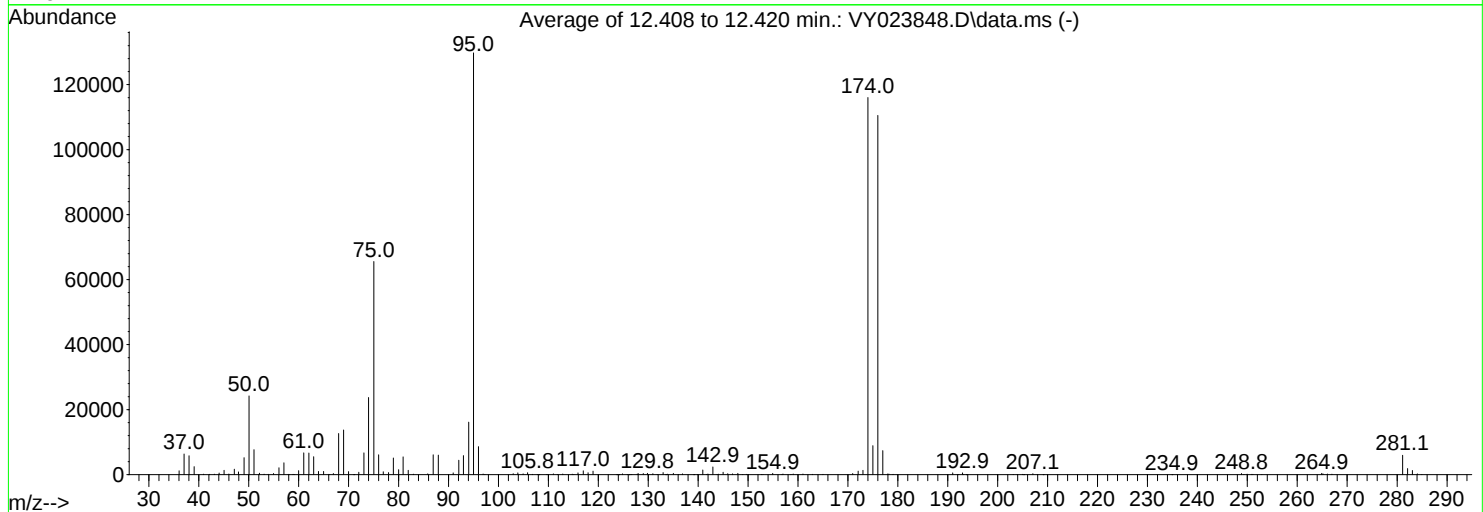


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120225\
Data File : VY023848.D
Acq On : 02 Dec 2025 06:50
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y112625S.M
Title : SW846 8260
Last Update : Thu Nov 27 01:14:36 2025

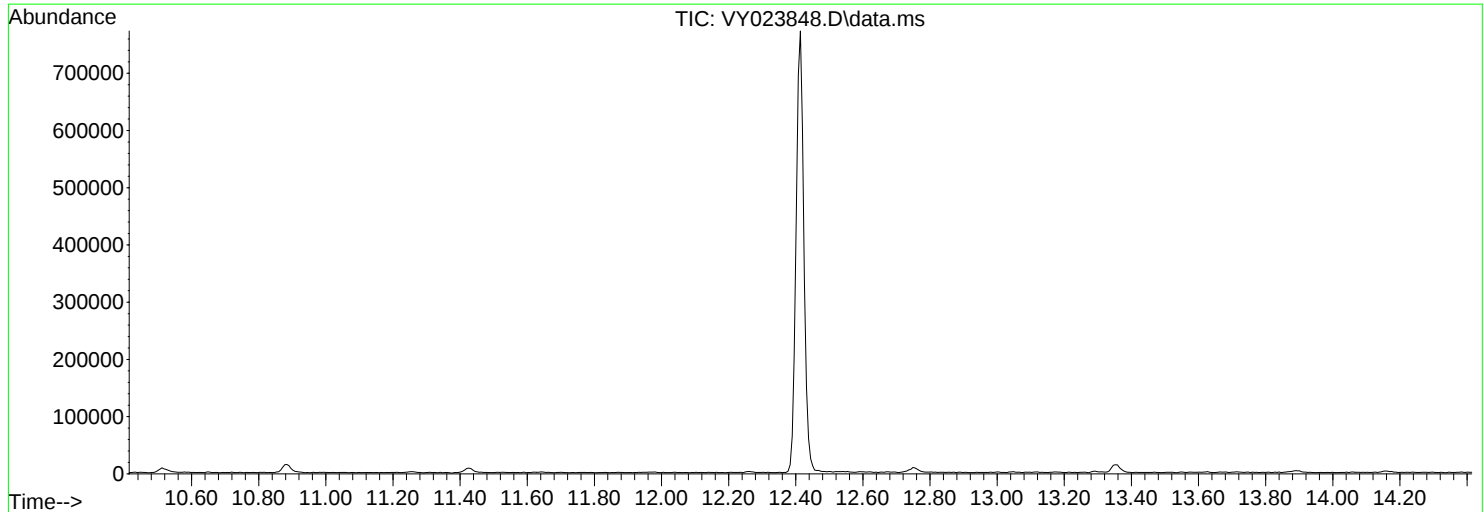

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	24219	PASS
75	95	30	60	50.5	65573	PASS
95	95	100	100	100.0	129781	PASS
96	95	5	9	6.6	8615	PASS
173	174	0.00	2	1.1	1334	PASS
174	95	50	100	89.4	116061	PASS
175	174	5	9	7.7	8934	PASS
176	174	95	101	95.2	110509	PASS
177	176	5	9	6.7	7407	PASS