

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
 Data File : PO115517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 16:42
 Operator : YP/AJ
 Sample : Q3742-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-1125-18

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 17:05:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.642	143.8E6	88902617	20.437m	19.903m
2) SA Decachlor...	9.919	8.627	102.6E6	82887690	23.214	21.232

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
Data File : PO115517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 16:42
Operator : YP/AJ
Sample : Q3742-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-1125-18


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 17:05:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

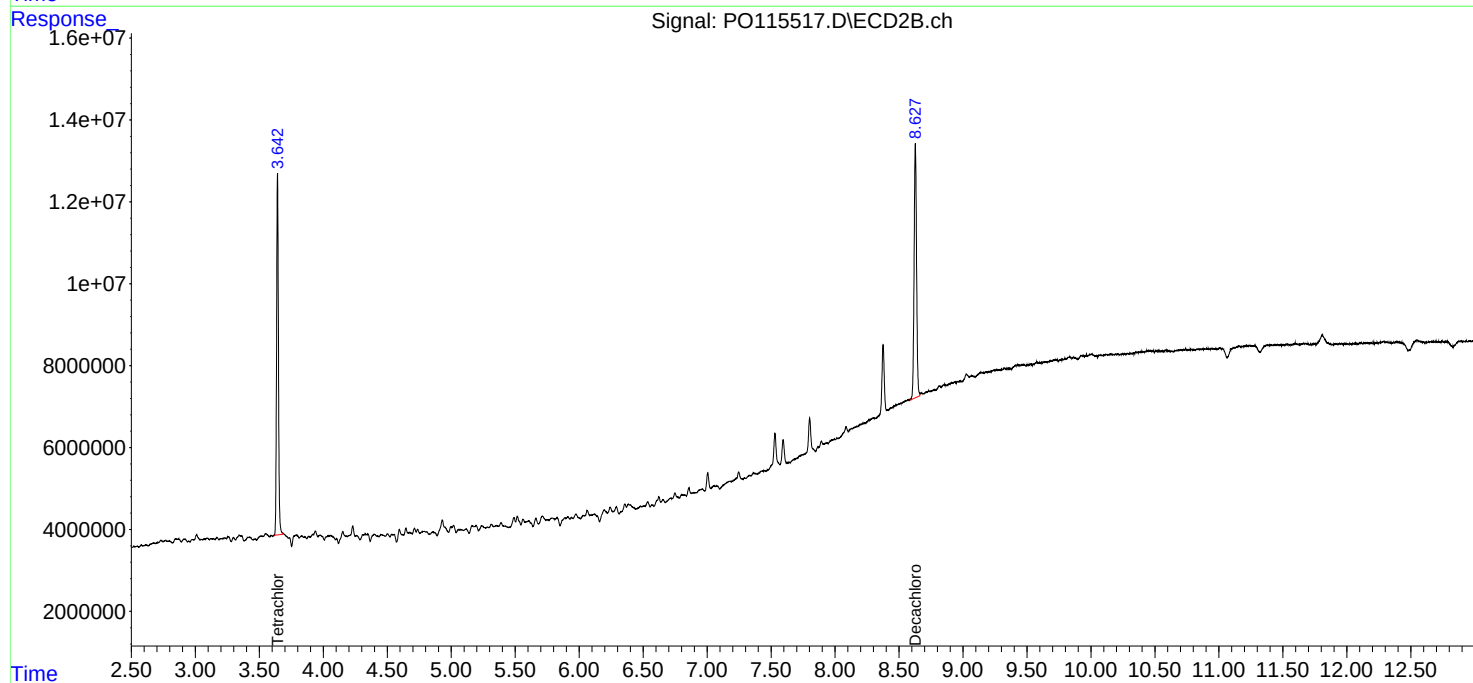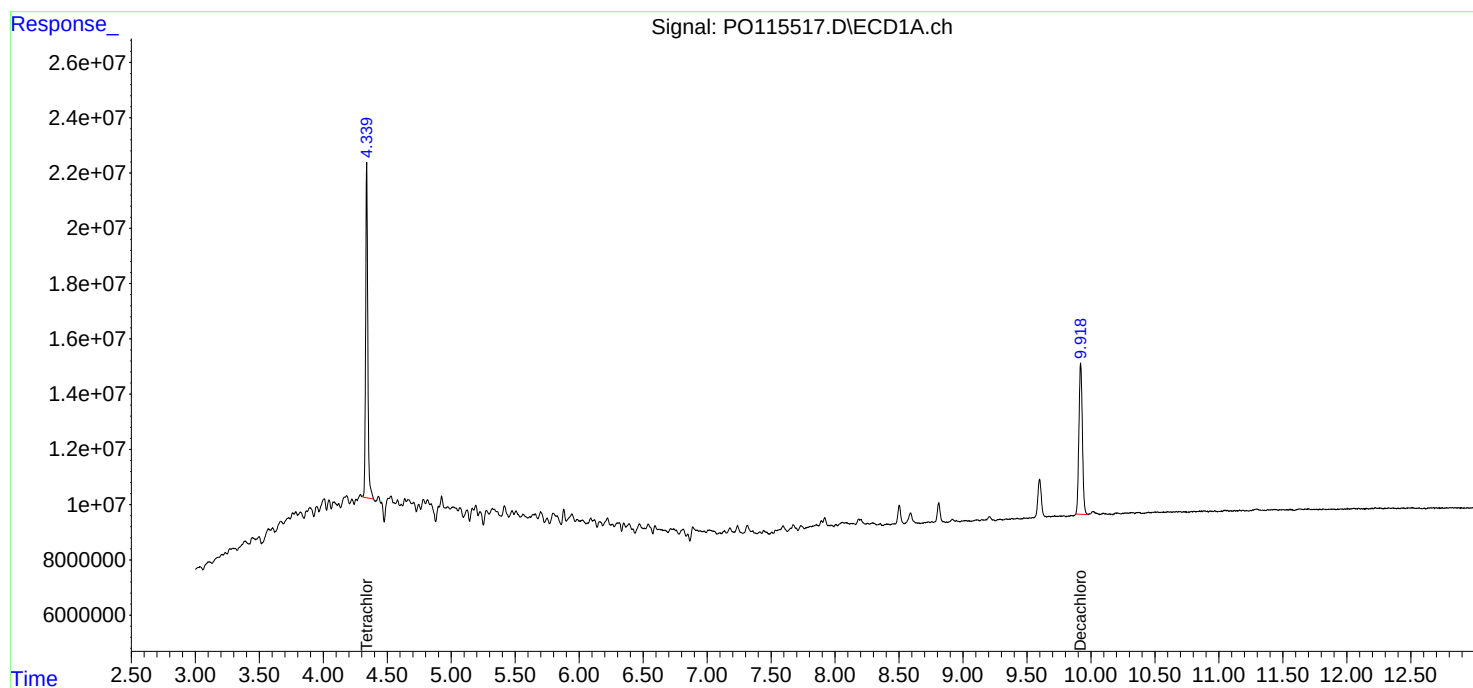

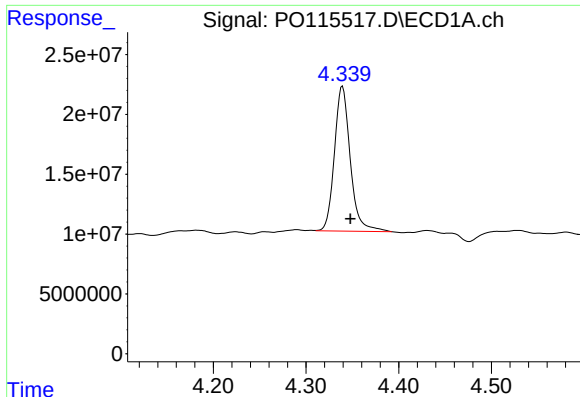


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.009 min
Response: 143837918
Conc: 20.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-1125-18


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

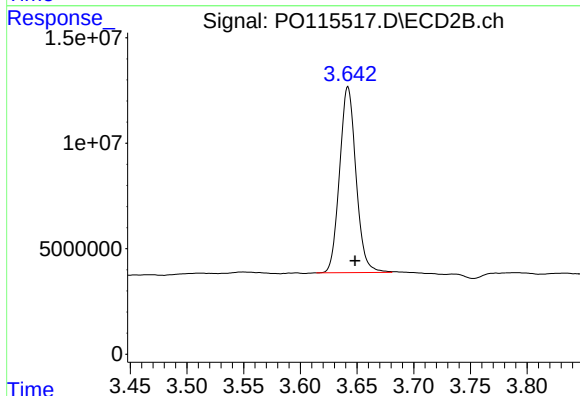


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.007 min
Response: 88902617
Conc: 19.90 ng/ml m

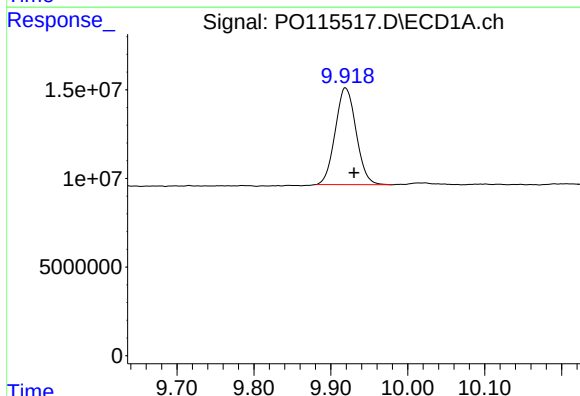

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.011 min
Response: 102612279
Conc: 23.21 ng/ml

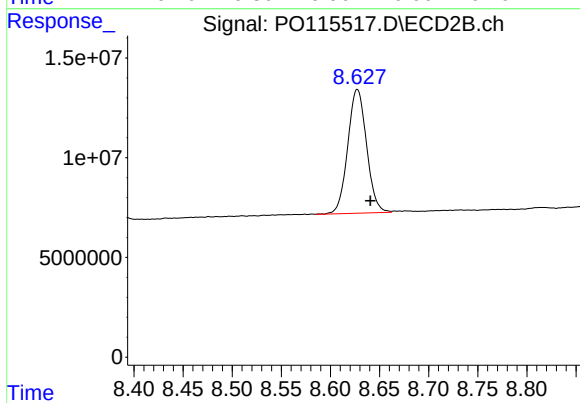

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.013 min
Response: 82887690
Conc: 21.23 ng/ml