

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
 Data File : PO115528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 20:20
 Operator : YP/AJ
 Sample : Q3742-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-1125-1

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:22:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.641	171.6E6	106.0E6	24.379	23.733
2) SA Decachlor...	9.914	8.626	109.5E6	90830503	24.763m	23.267

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
Data File : PO115528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 20:20
Operator : YP/AJ
Sample : Q3742-16
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-1125-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:22:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

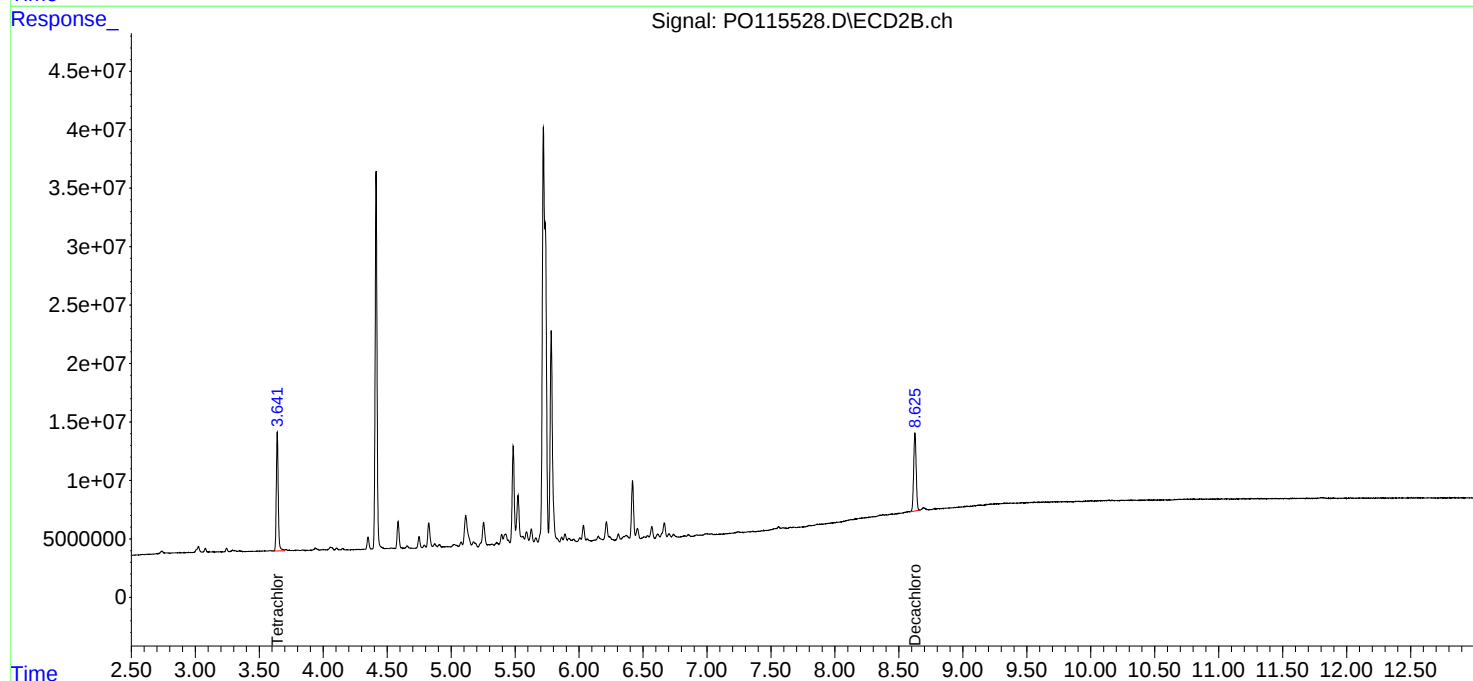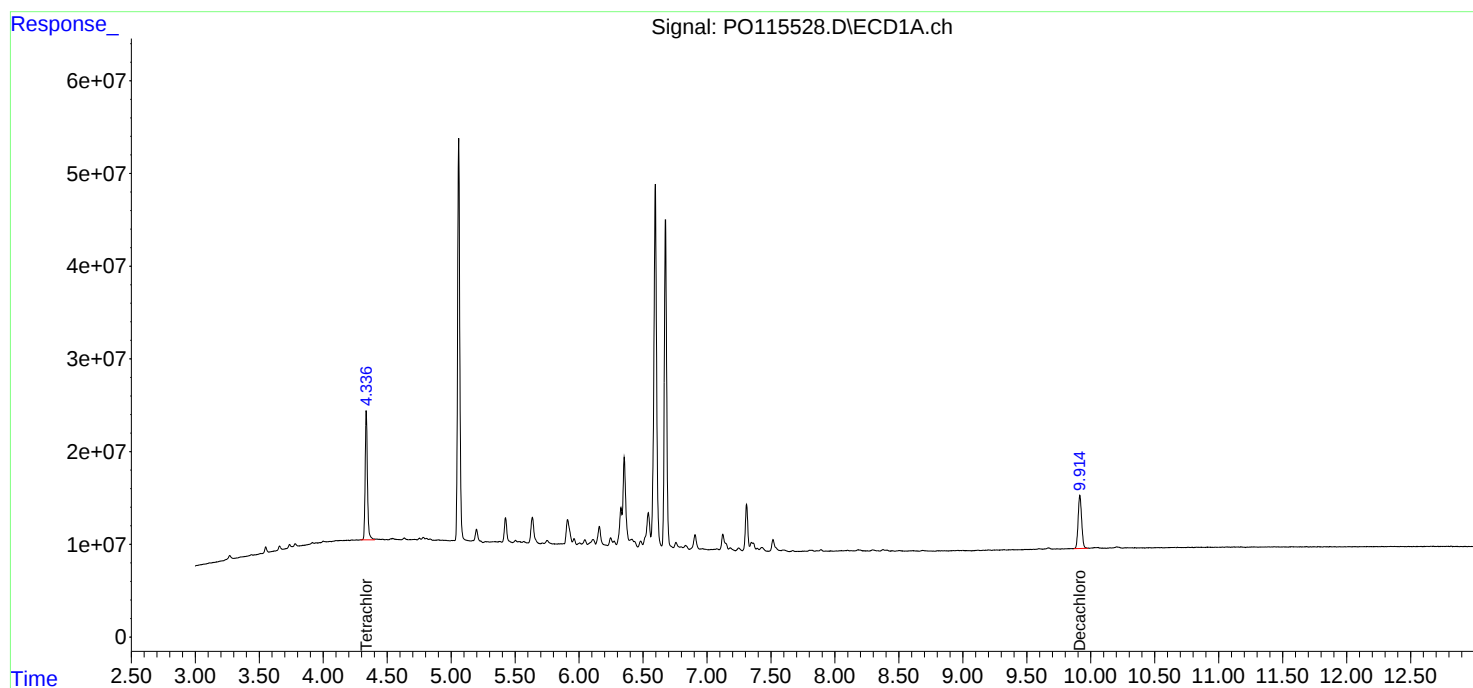

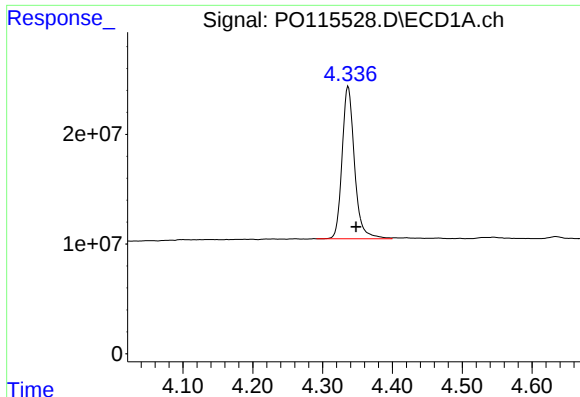


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.011 min
Response: 171584462
Conc: 24.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-1125-1


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

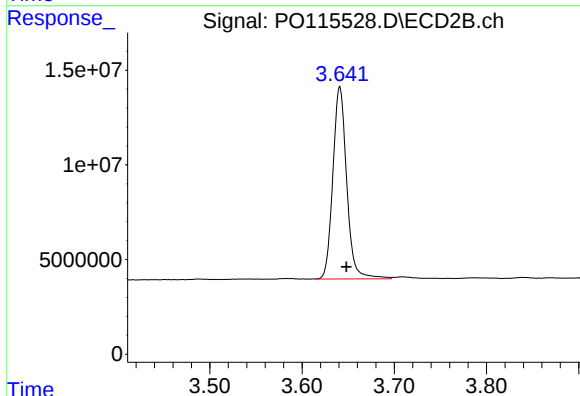


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: -0.007 min
Response: 106011286
Conc: 23.73 ng/ml

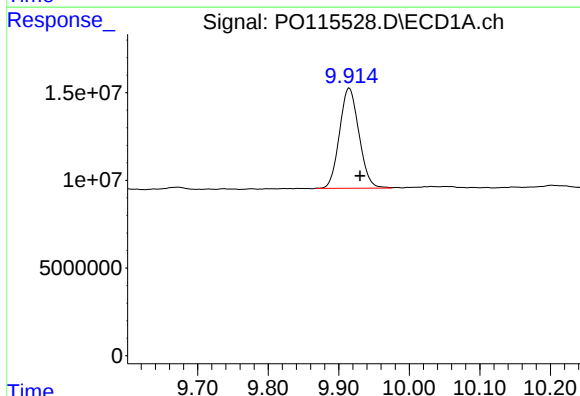

#2 Decachlorobiphenyl

R.T.: 9.914 min
Delta R.T.: -0.016 min
Response: 109459592
Conc: 24.76 ng/ml m

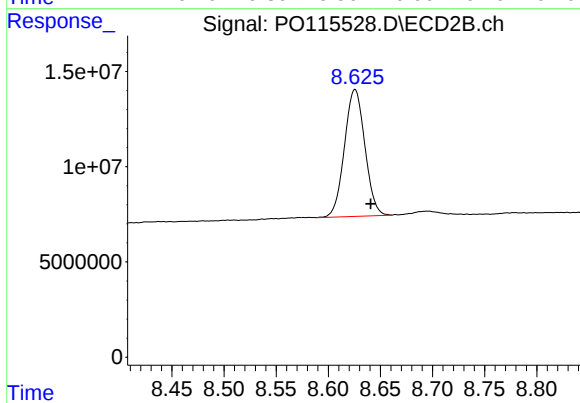

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.015 min
Response: 90830503
Conc: 23.27 ng/ml