

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
 Data File : PD091427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 17:23
 Operator : AR\AJ
 Sample : Q3742-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-1125-23

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/03/2025
 Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:09:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.871	61999307	772.5E6	17.978m	21.090
28) SA Decachlor...	9.075	8.061	79869136	651.3E6	16.032	16.459

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
Data File : PD091427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 17:23
Operator : AR\AJ
Sample : Q3742-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-1125-23


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:09:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

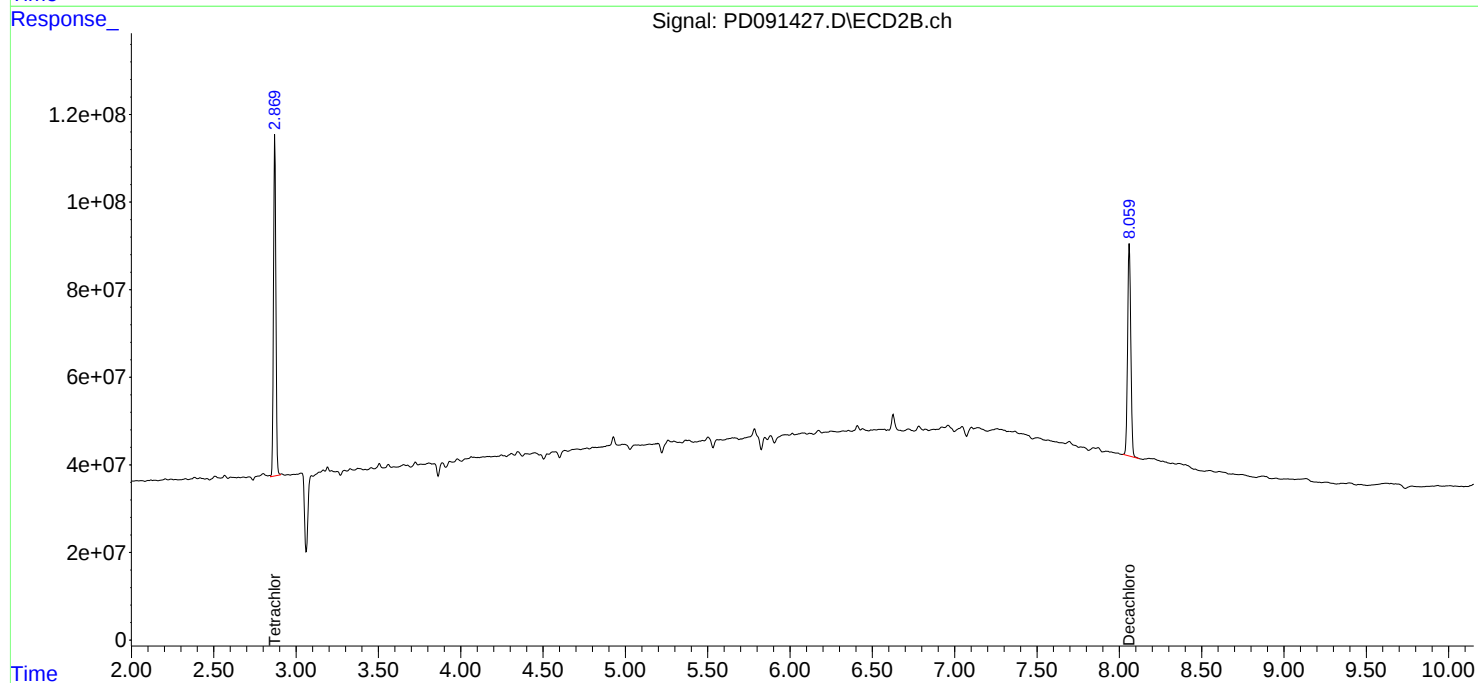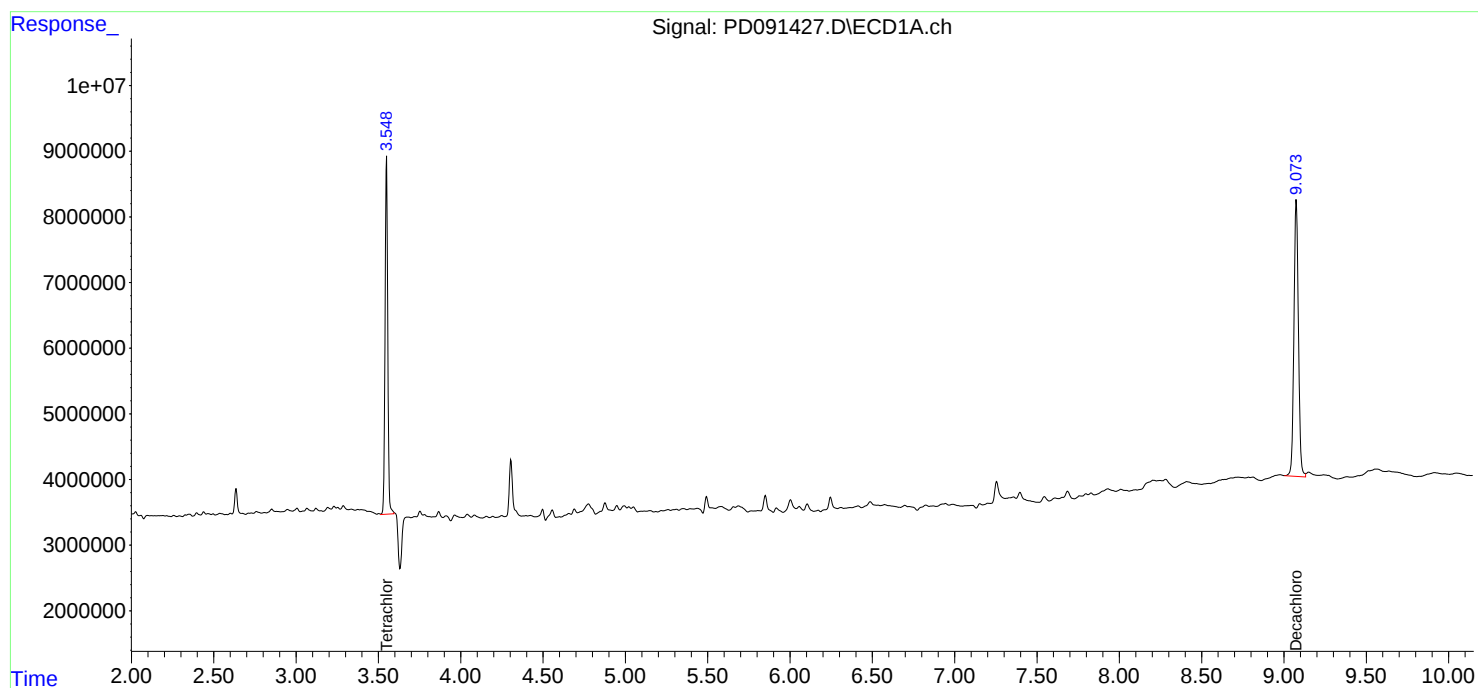

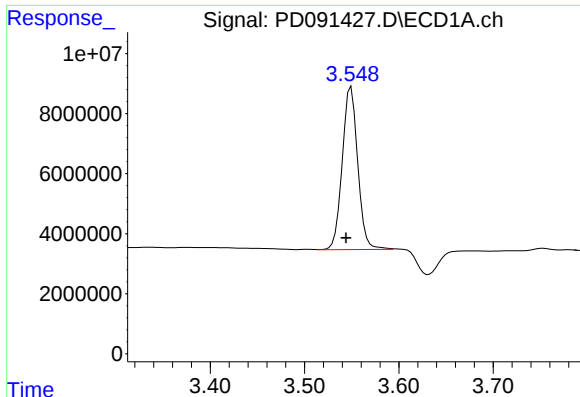


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.004 min
Response: 61999307
Conc: 17.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-1125-23


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

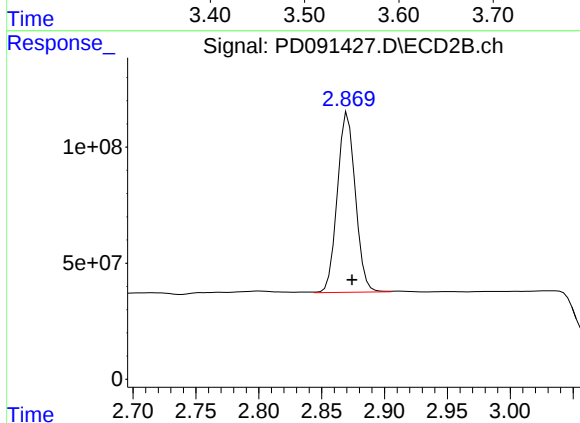


#1 Tetrachloro-m-xylene

R.T.: 2.871 min
Delta R.T.: -0.003 min
Response: 772515638
Conc: 21.09 ng/ml

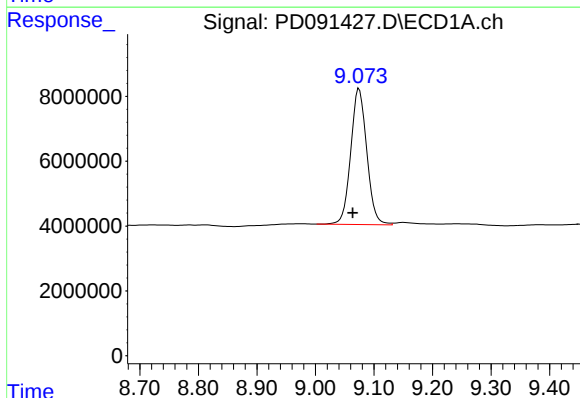

#28 Decachlorobiphenyl

R.T.: 9.075 min
Delta R.T.: 0.011 min
Response: 79869136
Conc: 16.03 ng/ml

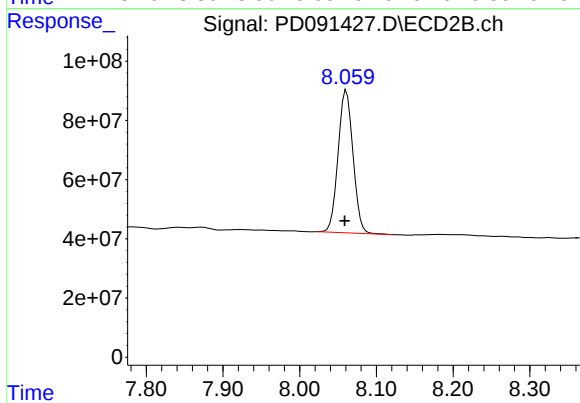

#28 Decachlorobiphenyl

R.T.: 8.061 min
Delta R.T.: 0.002 min
Response: 651344172
Conc: 16.46 ng/ml