

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
 Data File : PD091443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 21:15
 Operator : AR\AJ
 Sample : Q3742-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-1125-25

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/03/2025
 Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:12:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.870	48829556	583.8E6	14.159m	15.938m
28)	SA Decachlor...	9.063	8.057	72839292	498.0E6	14.621	12.583

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120225\
Data File : PD091443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 21:15
Operator : AR\AJ
Sample : Q3742-17
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-1125-25


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/03/2025
Supervised By : Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:12:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

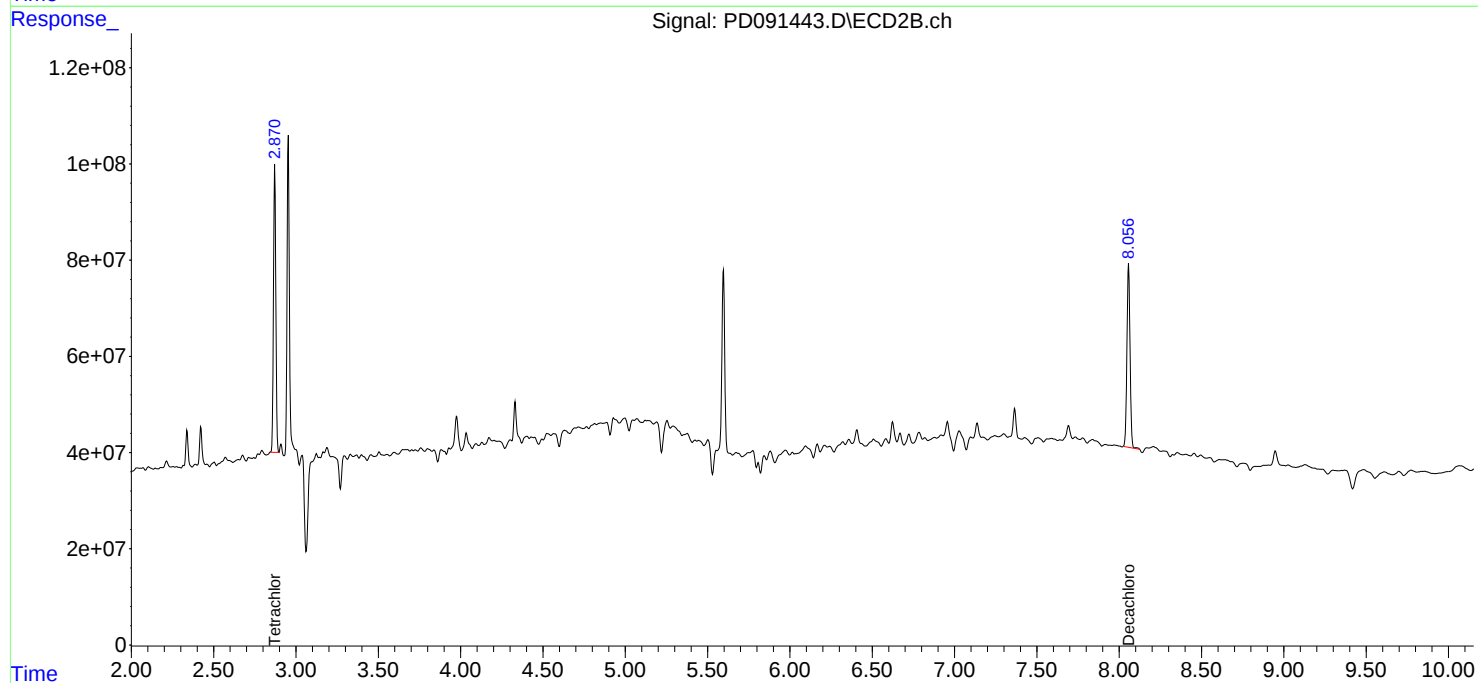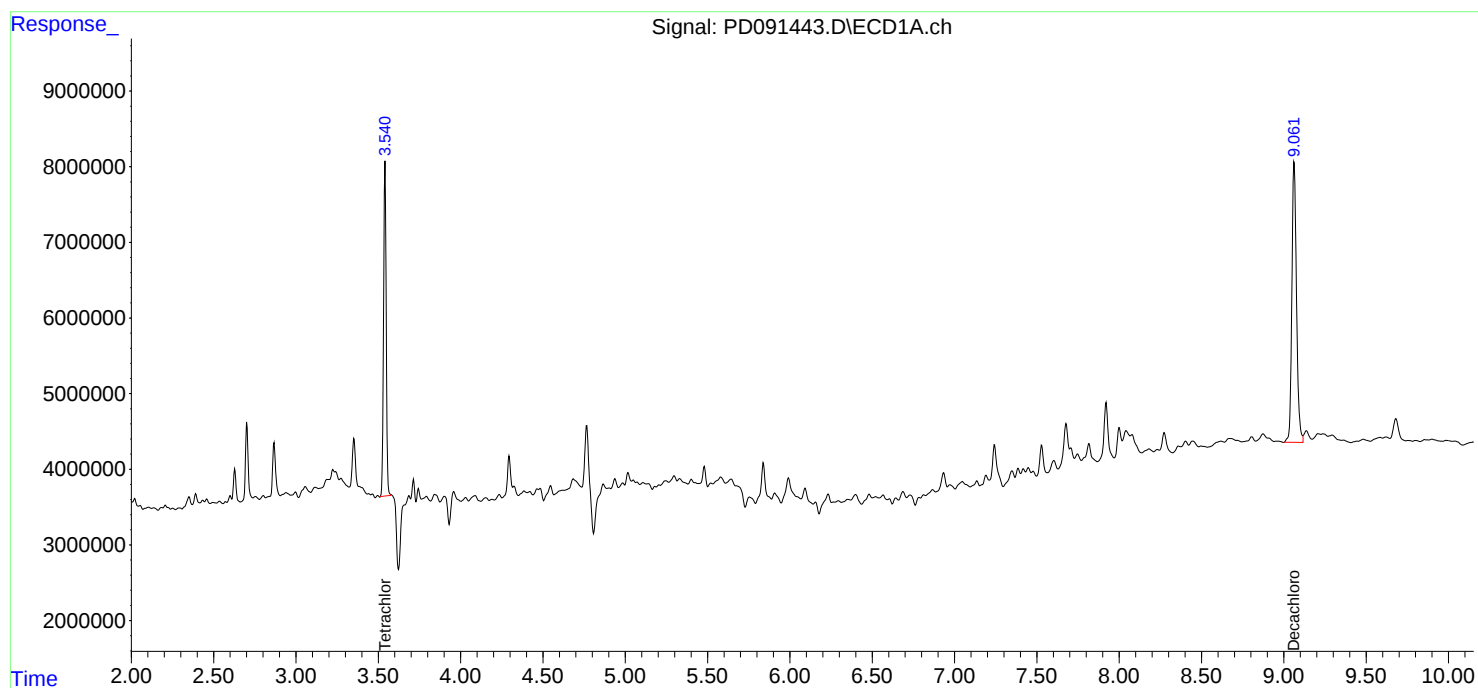

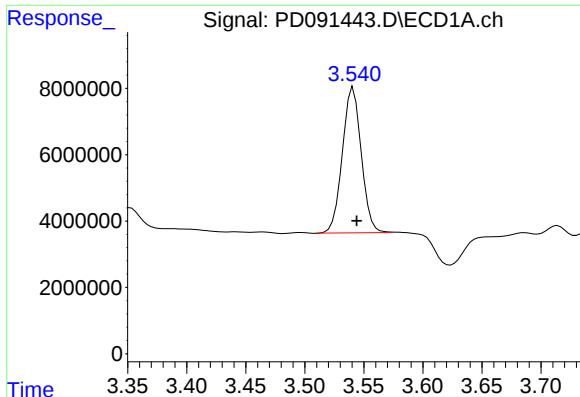


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 48829556
Conc: 14.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-1125-25


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

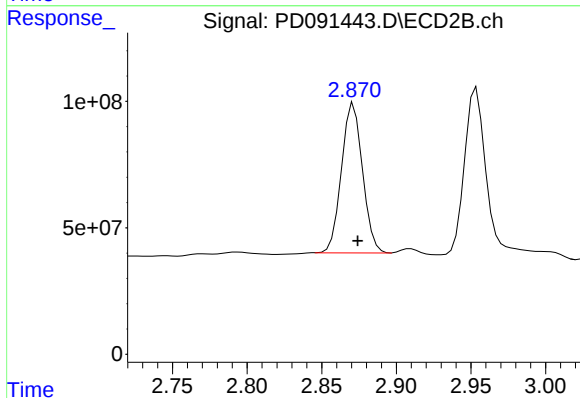


#1 Tetrachloro-m-xylene

R.T.: 2.870 min
Delta R.T.: -0.004 min
Response: 583805489
Conc: 15.94 ng/ml m

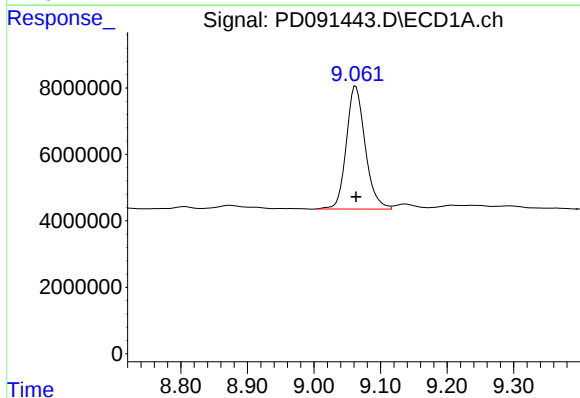

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 72839292
Conc: 14.62 ng/ml

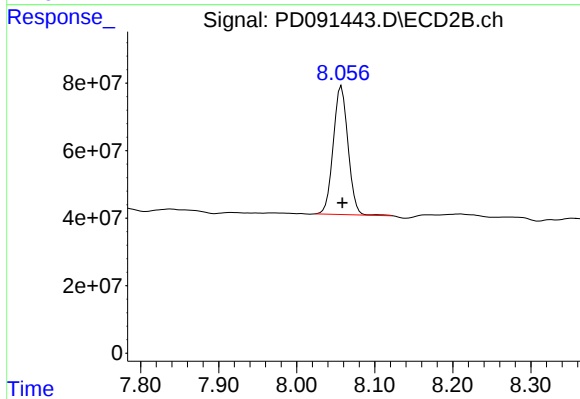

#28 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: -0.001 min
Response: 497953596
Conc: 12.58 ng/ml