


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144397.D
Acq On : 02 Dec 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

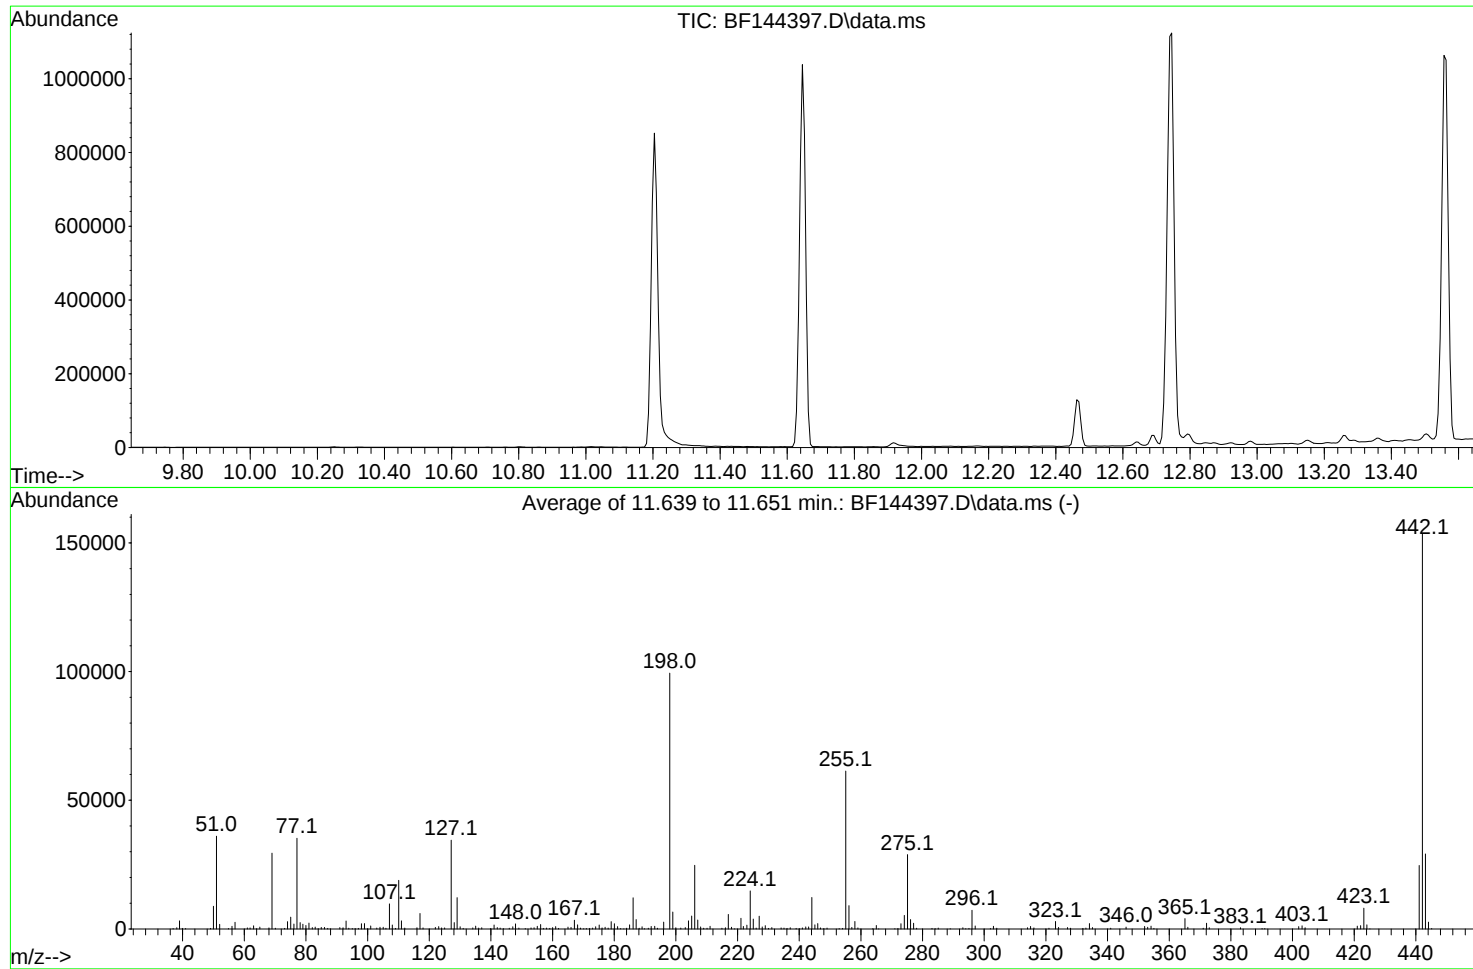




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	437	PASS
69	69	100	100	100.0	29459	PASS
70	69	0.00	2	1.1	316	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99365	PASS
199	198	5	9	6.6	6573	PASS
365	198	1	100	4.0	4014	PASS
441	443	0.01	150	84.5	24640	PASS
442	442	100	100	100.0	153424	PASS
443	442	15	24	19.0	29152	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144397.D
Acq On : 02 Dec 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 10:51:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

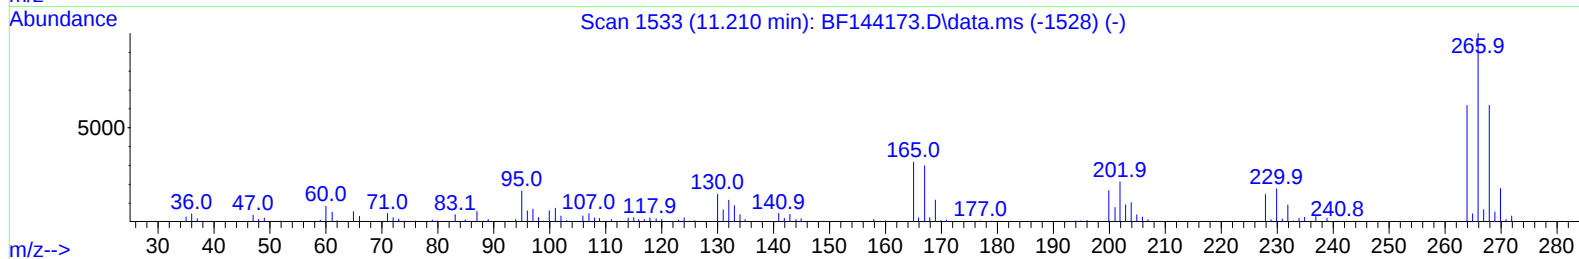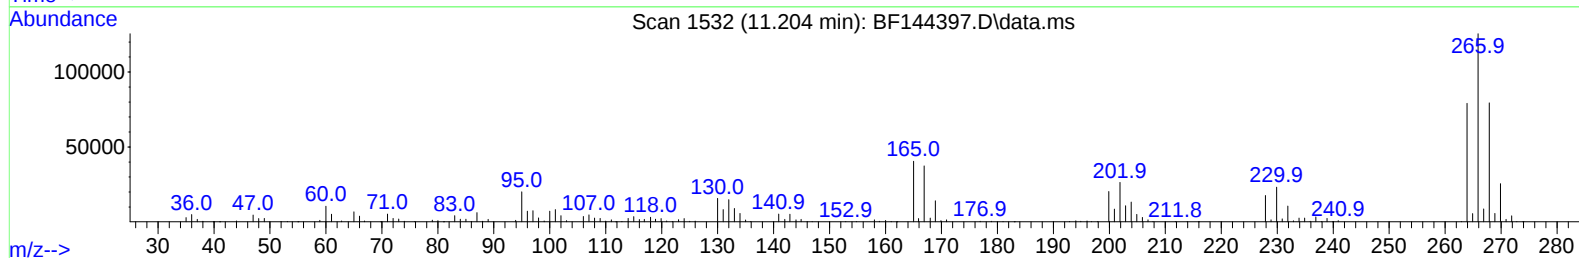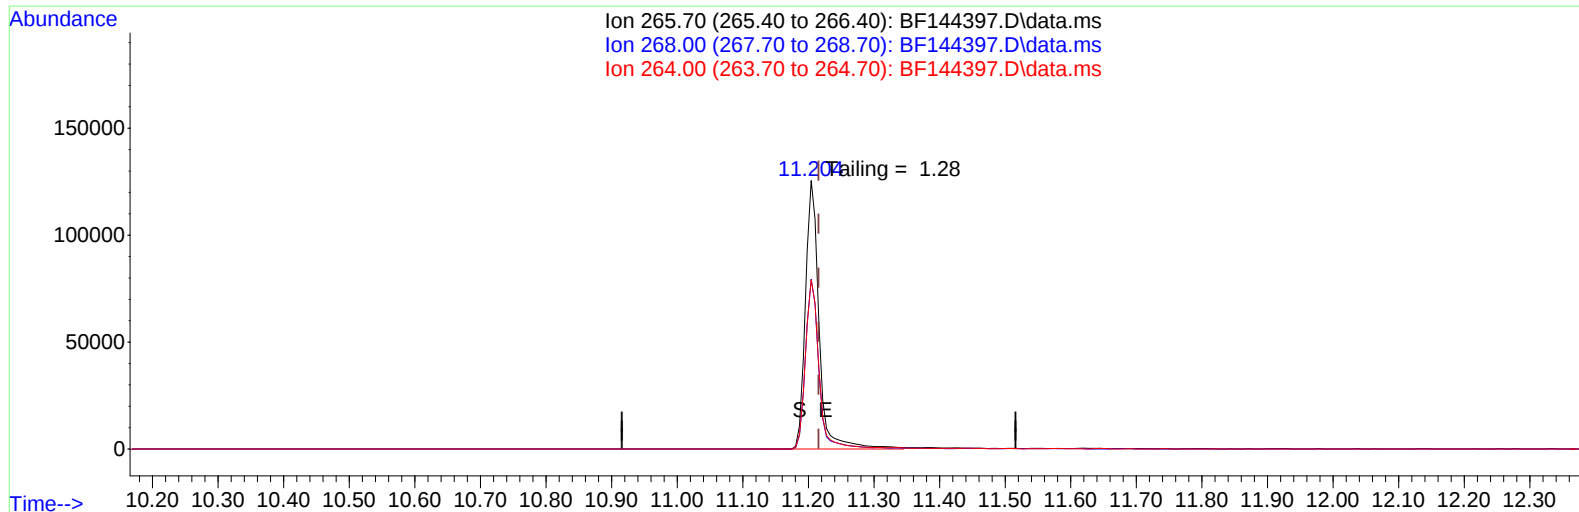

TIC: BF144397.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 36284.74 ng




response 183362

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.26
264.00	61.80	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144397.D
Acq On : 02 Dec 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 10:51:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

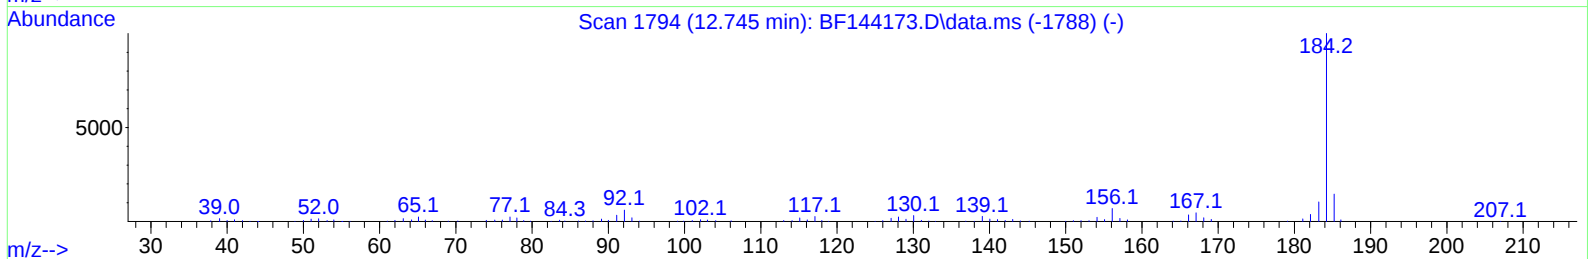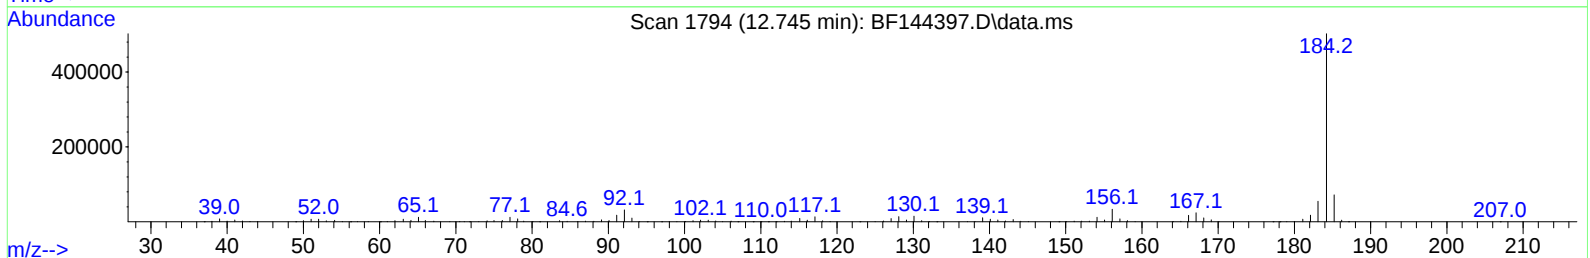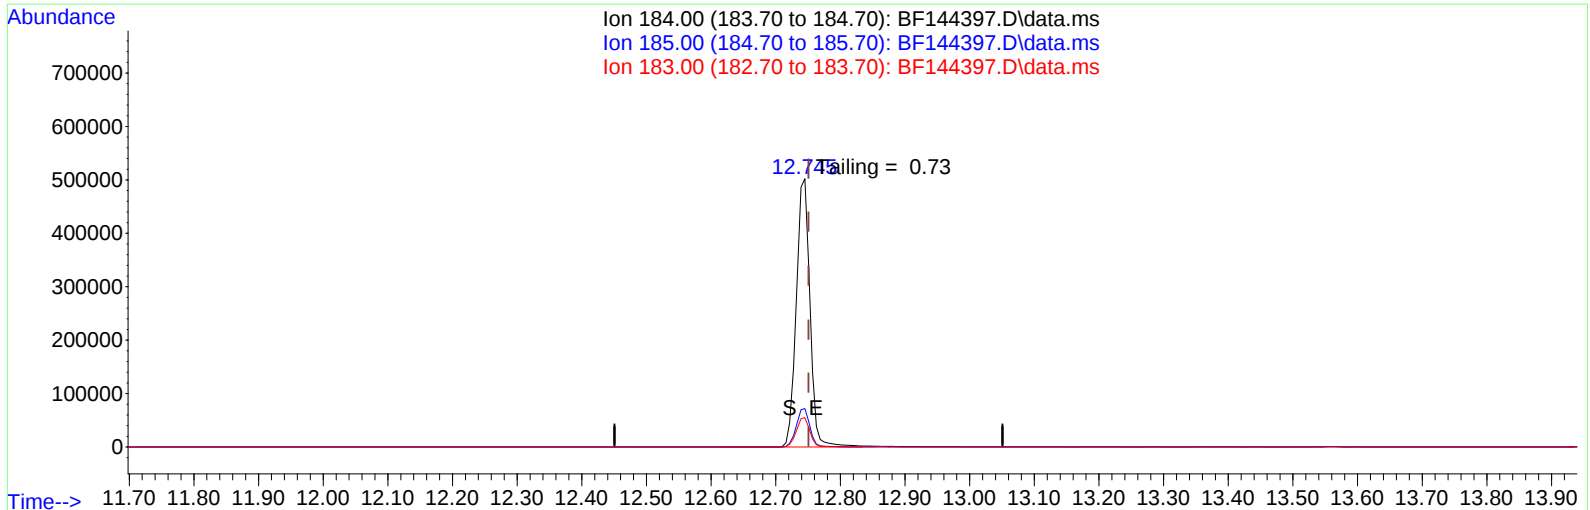

TIC: BF144397.D\data.ms

(77) Benzidine

12.745min (-0.006) 20356.93 ng

response 746056

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.40	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2025	BNA_F	<u>BF144397.D</u>
Compound Name	Response	Retention Time
DDT	313350	13.563
DDD	7988	13.263
DDE	1105	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9093	322443	2.82

Instrument :
BNA_F
ClientSampleId :
DFTPP