


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120225\
Data File : BP026206.D
Acq On : 02 Dec 2025 13:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

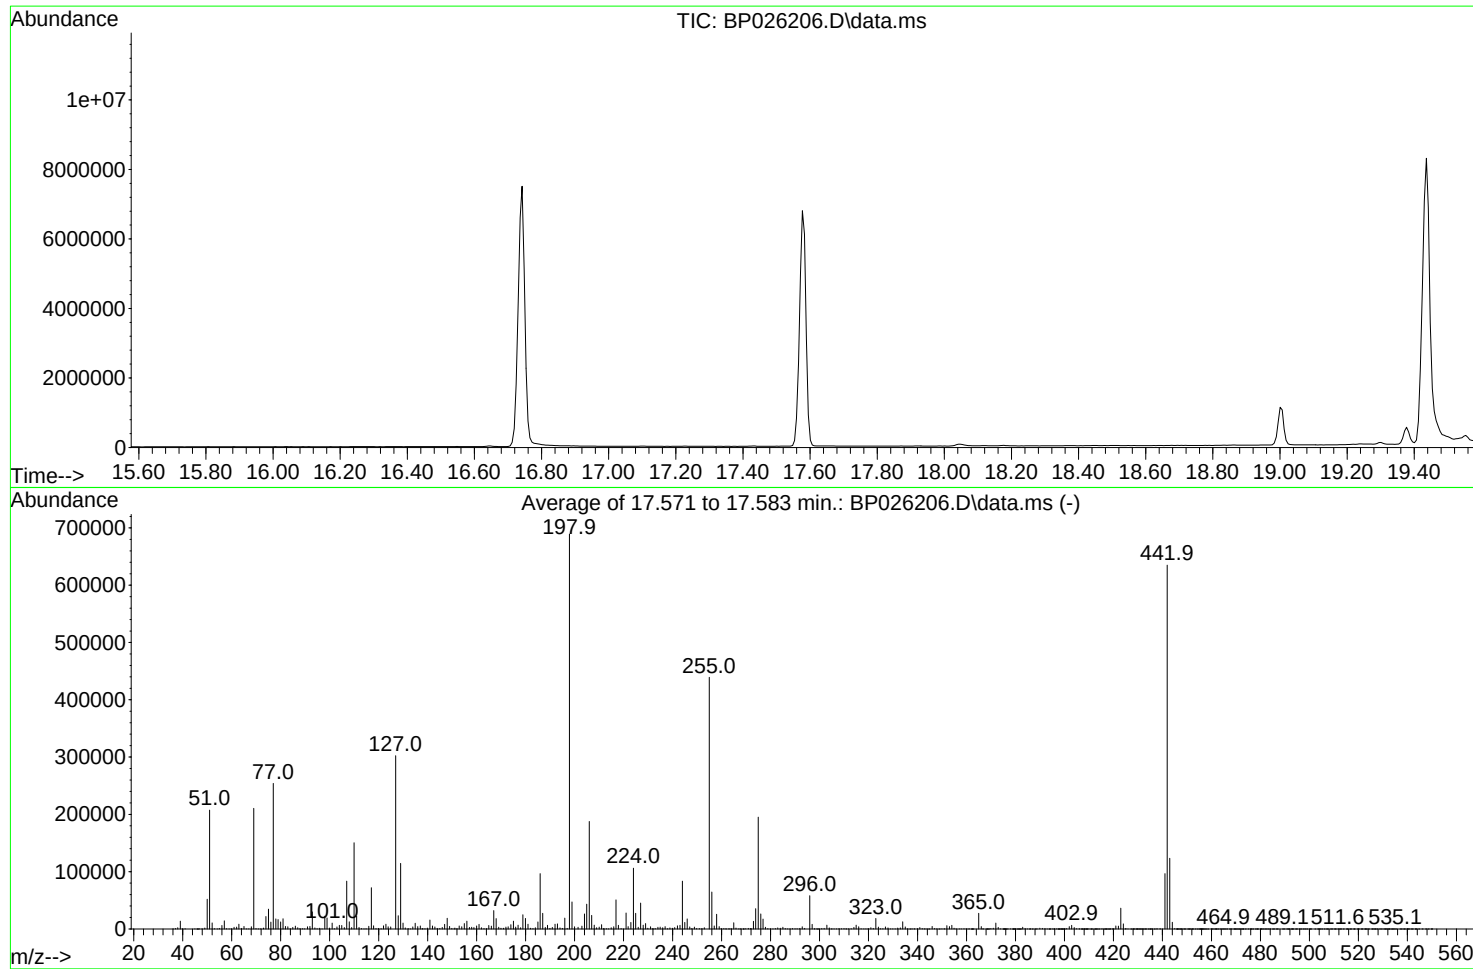




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2479

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3677	PASS
69	69	100	100	100.0	210501	PASS
70	69	0.00	2	0.4	763	PASS
197	198	0.00	2	0.2	1103	PASS
198	198	100	100	100.0	689278	PASS
199	198	5	9	6.8	47037	PASS
365	198	1	100	4.0	27229	PASS
441	443	0.01	150	78.3	96541	PASS
442	442	100	100	100.0	635043	PASS
443	442	15	24	19.4	123291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120225\
Data File : BP026206.D
Acq On : 02 Dec 2025 13:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 02 14:15:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

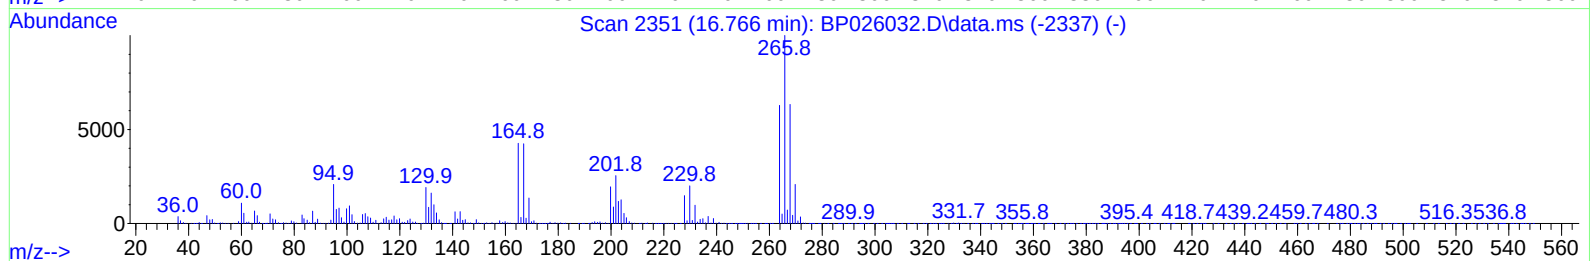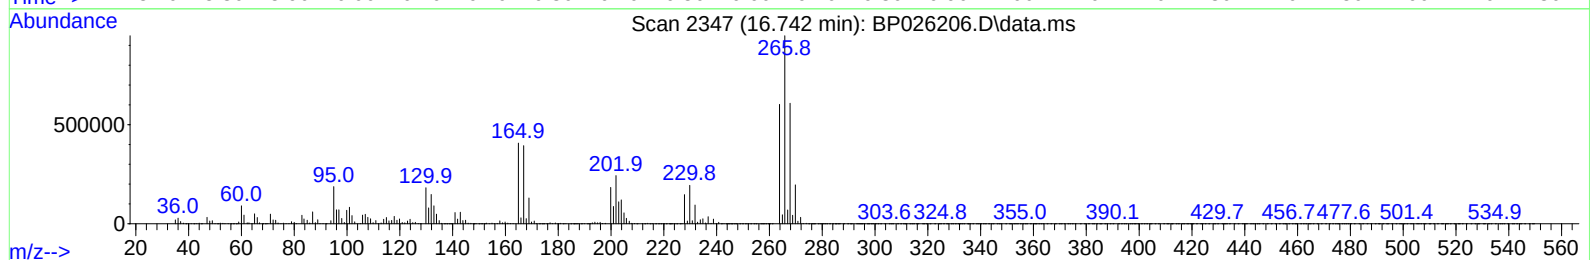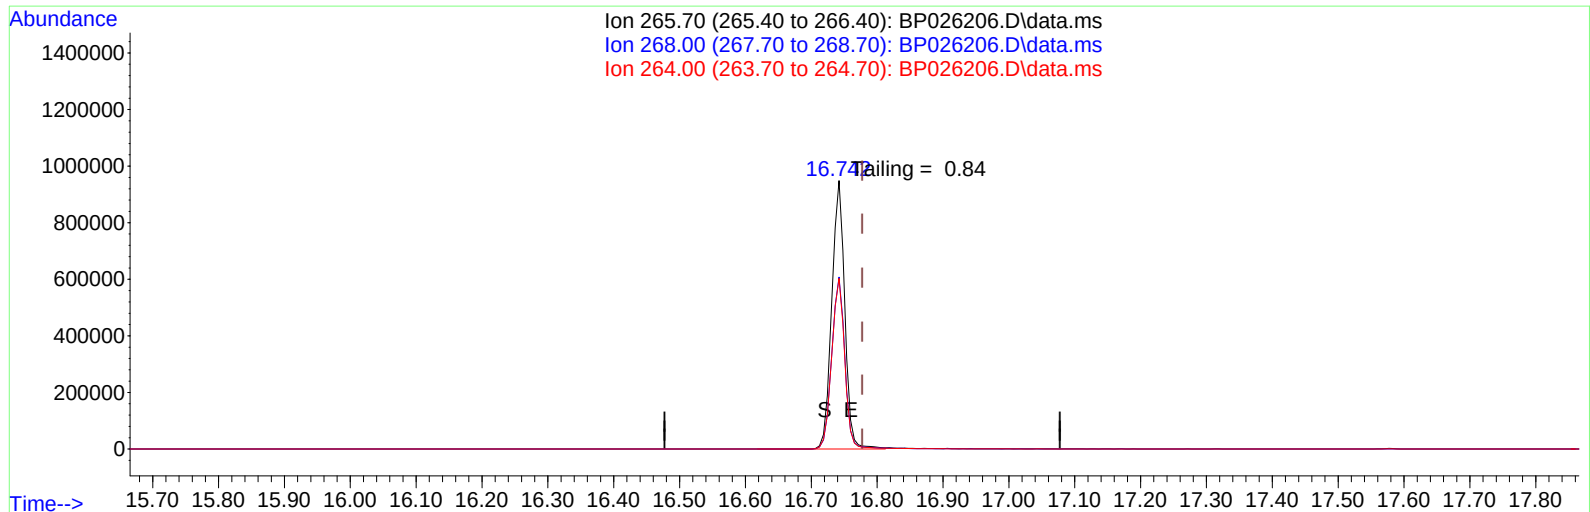

TIC: BP026206.D\data.ms

(70) Pentachlorophenol (C)

16.742min (-0.036) 44471.14 ng




response 1312034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.07
264.00	62.70	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120225\
Data File : BP026206.D
Acq On : 02 Dec 2025 13:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 02 14:15:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

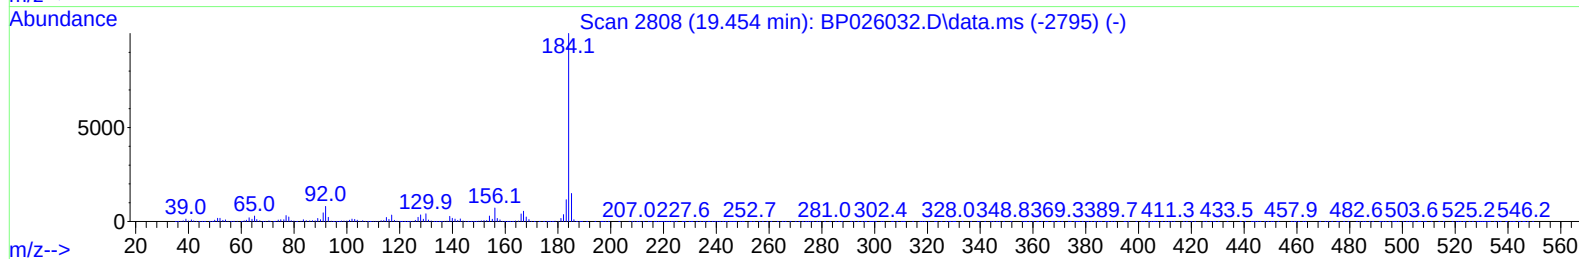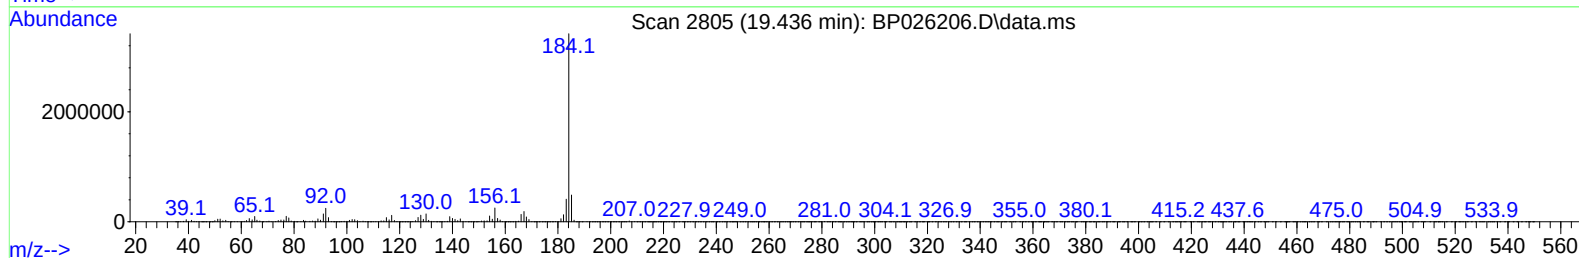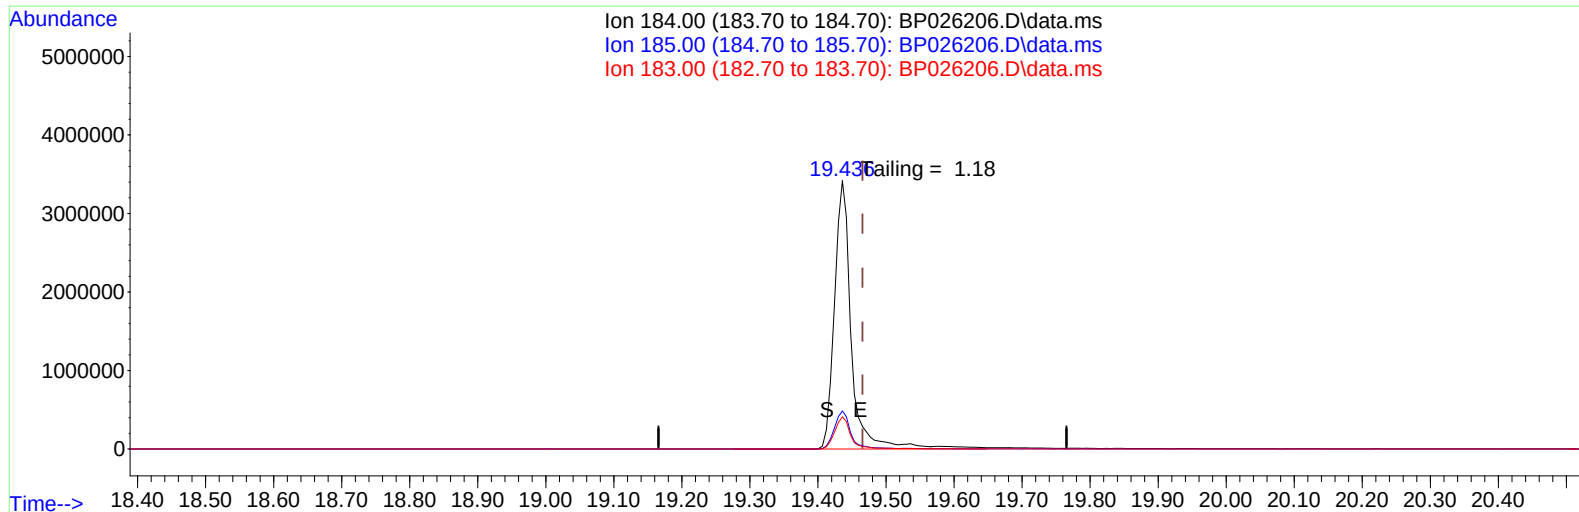

TIC: BP026206.D\data.ms

(77) Benzidine

19.436min (-0.030) 23336.74 ng

response 5681950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.30	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/2/2025	BNA_P	<u>BP026206.D</u>
Compound Name	Response	Retention Time
DDT	3006140	20.736
DDD	68650	20.277
DDE	5960	19.742
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74610	3080750	2.42

Instrument :
BNA_P
ClientSampleId :
DFTPP