

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
 Data File : BF144399.D
 Acq On : 02 Dec 2025 13:16
 Operator : RC/JU
 Sample : PB170788BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB170788BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	485	492	513	rBV	261580	432030	26.79%	3.857%
2	5.493	556	561	584	rBV	977123	1352981	83.91%	12.078%
3	6.498	726	732	759	rBV	952575	1355672	84.07%	12.102%
4	6.863	789	794	804	rBV	349536	438980	27.22%	3.919%
5	7.422	884	889	908	rBV	617969	864637	53.62%	7.718%
6	8.145	1006	1012	1026	rBV	437808	570897	35.40%	5.096%
7	9.222	1189	1195	1214	rBV	1240100	1612510	100.00%	14.394%
8	9.904	1305	1311	1324	rBV	510148	655566	40.66%	5.852%
9	10.698	1440	1446	1467	rBV	678292	960620	59.57%	8.575%
10	11.392	1559	1564	1573	rBV	445547	613478	38.04%	5.476%
11	12.980	1829	1834	1840	rBV	1019221	1353350	83.93%	12.081%
12	14.045	2010	2015	2023	rBV	318671	432061	26.79%	3.857%
13	15.533	2261	2268	2277	rBV	318071	559710	34.71%	4.996%




Sum of corrected areas: 11202492

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144399.D
Acq On : 02 Dec 2025 13:16
Operator : RC/JU
Sample : PB170788BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170788BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

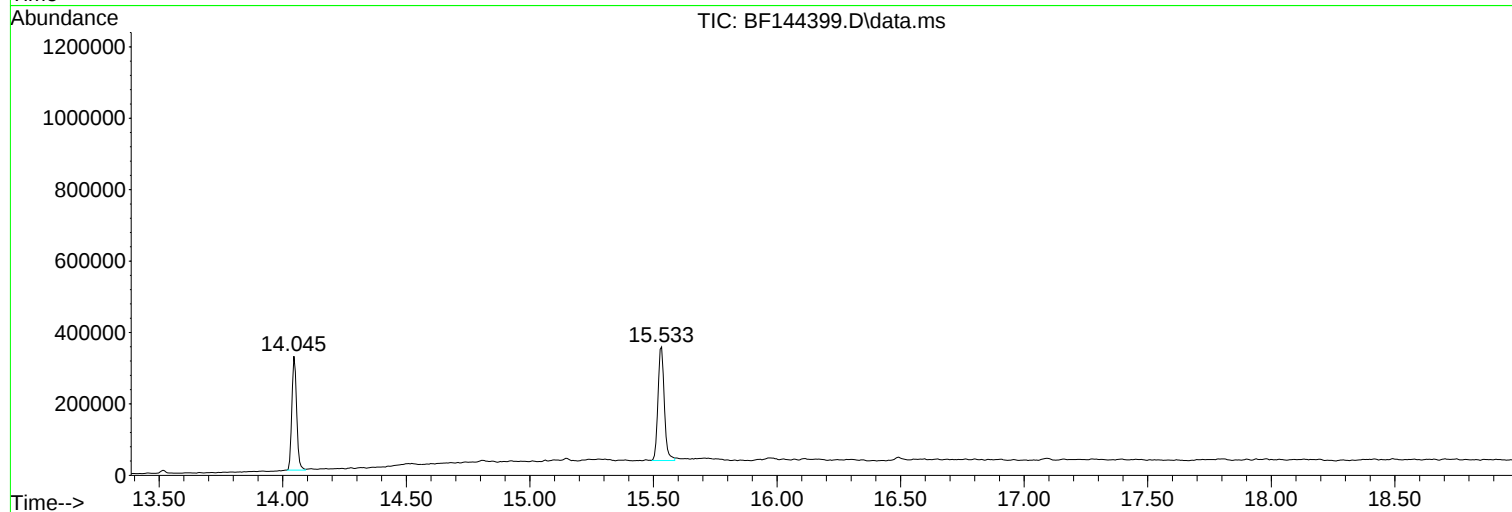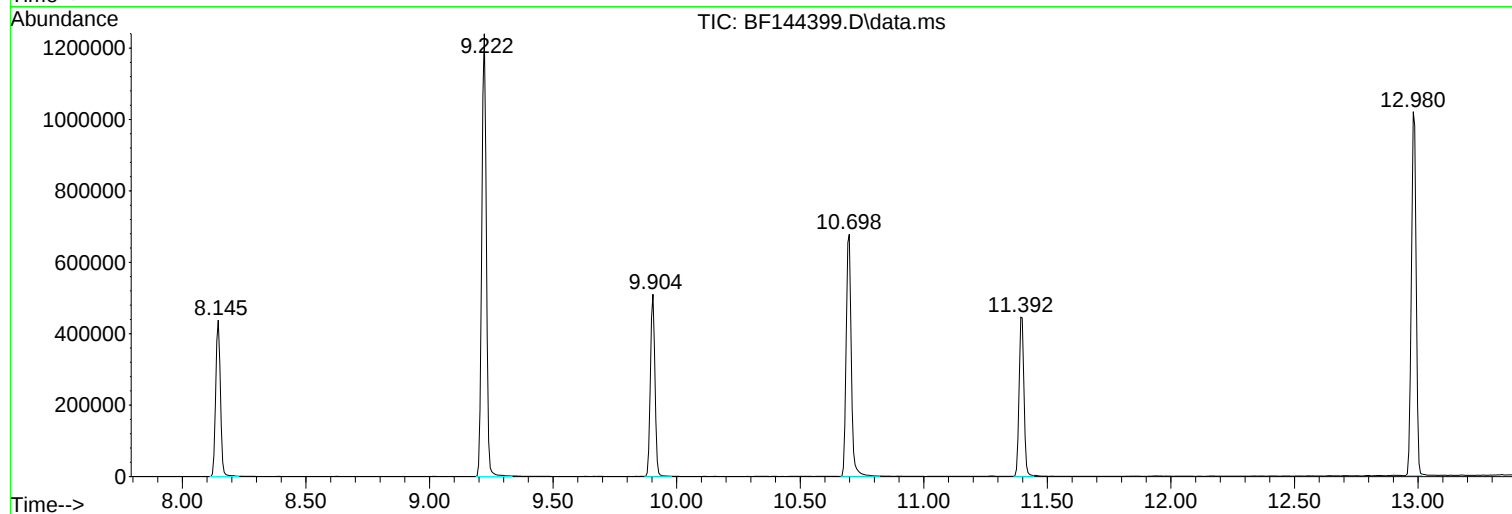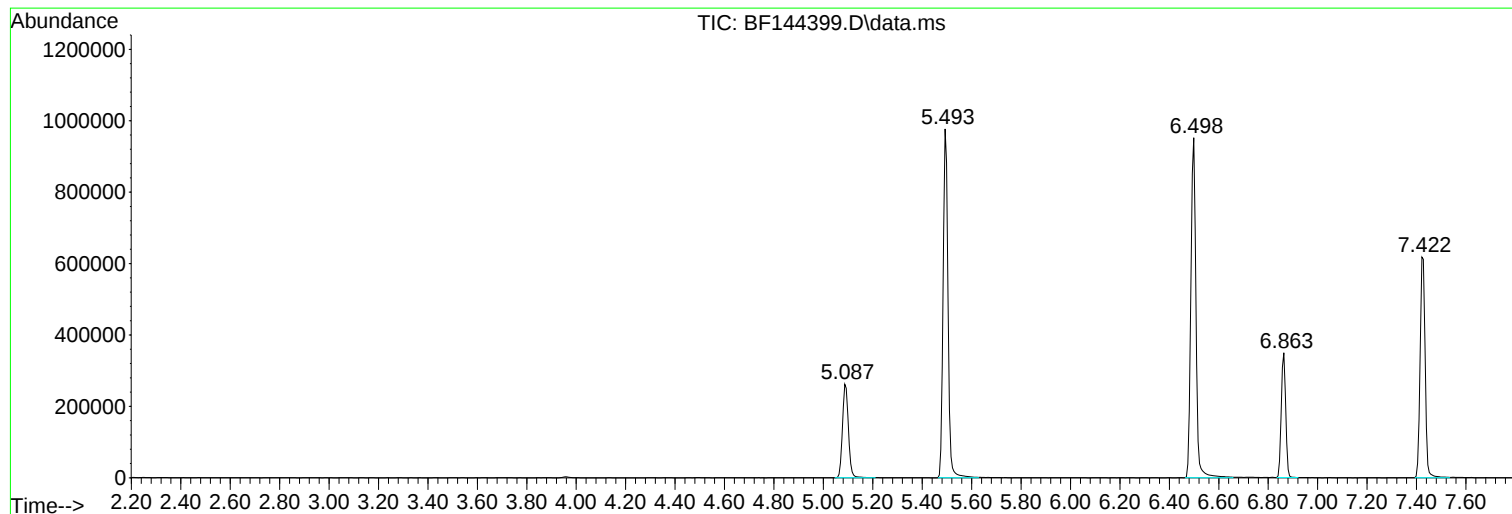

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144399.D
Acq On : 02 Dec 2025 13:16
Operator : RC/JU
Sample : PB170788BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170788BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144399.D
Acq On : 02 Dec 2025 13:16
Operator : RC/JU
Sample : PB170788BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170788BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------