

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
 Data File : BF144401.D
 Acq On : 02 Dec 2025 14:21
 Operator : RC/JU
 Sample : Q3742-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1125-23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	483	490	500	rBV	182687	266291	24.53%	1.635%
2	5.487	555	560	575	rBV	584977	823787	75.88%	5.057%
3	6.498	726	732	748	rBV	610303	839387	77.32%	5.152%
4	6.863	789	794	799	rBV	224643	284348	26.19%	1.745%
5	7.422	881	889	899	rBV	423588	541365	49.86%	3.323%
6	8.145	1006	1012	1022	rBV2	292495	471933	43.47%	2.897%
7	8.857	1128	1133	1139	rVB	68661	84319	7.77%	0.518%
8	8.957	1145	1150	1158	rVB	57129	71677	6.60%	0.440%
9	9.216	1189	1194	1200	rBV	809573	1022248	94.16%	6.275%
10	9.322	1208	1212	1217	rVB	15922	20950	1.93%	0.129%
11	9.416	1222	1228	1233	rVB	15340	24735	2.28%	0.152%
12	9.486	1233	1240	1245	rBV	35817	57802	5.32%	0.355%
13	9.557	1247	1252	1255	rBV	55664	80027	7.37%	0.491%
14	9.586	1255	1257	1261	rVB	29542	30107	2.77%	0.185%
15	9.675	1268	1272	1280	rVB	25319	44398	4.09%	0.273%
16	9.757	1280	1286	1291	rBV2	24966	35629	3.28%	0.219%
17	9.898	1302	1310	1314	rBV	337144	467130	43.03%	2.867%
18	9.933	1314	1316	1320	rVV	98380	103952	9.57%	0.638%
19	10.004	1324	1328	1332	rVB	10255	15704	1.45%	0.096%
20	10.057	1332	1337	1340	rBV2	12891	19963	1.84%	0.123%
21	10.104	1340	1345	1349	rVV	90666	121536	11.19%	0.746%
22	10.139	1349	1351	1355	rVB	17335	20064	1.85%	0.123%
23	10.216	1360	1364	1367	rBV2	18079	25137	2.32%	0.154%
24	10.245	1367	1369	1374	rVB	16839	18645	1.72%	0.114%
25	10.310	1374	1380	1387	rBV3	18451	46749	4.31%	0.287%
26	10.398	1389	1395	1398	rBV6	9256	14083	1.30%	0.086%
27	10.451	1398	1404	1409	rBV2	131899	173678	16.00%	1.066%
28	10.516	1409	1415	1416	rBV3	23472	40617	3.74%	0.249%
29	10.610	1427	1431	1437	rVB2	164362	237150	21.84%	1.456%
30	10.692	1440	1445	1450	rBV	511358	654688	60.30%	4.019%
31	10.816	1460	1466	1473	rVB7	14497	32013	2.95%	0.197%
32	10.922	1481	1484	1490	rBV	23590	31180	2.87%	0.191%
33	10.998	1490	1497	1500	rBV3	41817	80961	7.46%	0.497%
34	11.027	1500	1502	1504	rBV2	10871	11548	1.06%	0.071%
35	11.127	1514	1519	1520	rBV3	20227	29106	2.68%	0.179%
36	11.198	1527	1531	1535	rVB	53233	62636	5.77%	0.384%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
 Data File : BF144401.D
 Acq On : 02 Dec 2025 14:21
 Operator : RC/JU
 Sample : Q3742-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1125-23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.245	1535	1539	1543	rVV3	34277	55662	5.13%	0.342%
38	11.286	1543	1546	1553	rVB	62666	85540	7.88%	0.525%
39	11.392	1558	1564	1565	rBV	319276	351623	32.39%	2.158%
40	11.422	1565	1569	1573	rVV	780408	1085663	100.00%	6.664%
41	11.469	1573	1577	1581	rVV	198330	253911	23.39%	1.559%
42	11.504	1581	1583	1588	rVB2	17938	20158	1.86%	0.124%
43	11.627	1598	1604	1610	rVV2	66978	121038	11.15%	0.743%
44	11.686	1611	1614	1617	rVV	17222	21932	2.02%	0.135%
45	11.727	1617	1621	1626	rVB3	30776	43368	3.99%	0.266%
46	11.804	1631	1634	1638	rVB	15617	20440	1.88%	0.125%
47	11.921	1645	1654	1659	rBV2	243145	590550	54.40%	3.625%
48	11.969	1659	1662	1665	rBV	54789	70397	6.48%	0.432%
49	12.010	1665	1669	1676	rVB2	173968	337133	31.05%	2.069%
50	12.074	1676	1680	1682	rBV3	35867	49701	4.58%	0.305%
51	12.163	1692	1695	1696	rBV3	25208	24640	2.27%	0.151%
52	12.192	1696	1700	1703	rVV	67763	77037	7.10%	0.473%
53	12.221	1703	1705	1710	rVB	49632	54139	4.99%	0.332%
54	12.263	1710	1712	1716	rVB	11832	13323	1.23%	0.082%
55	12.345	1719	1726	1727	rBV2	69051	106292	9.79%	0.652%
56	12.445	1739	1743	1746	rBV	74049	100399	9.25%	0.616%
57	12.480	1746	1749	1755	rVV3	44518	84359	7.77%	0.518%
58	12.539	1755	1759	1766	rVB3	46780	71365	6.57%	0.438%
59	12.610	1766	1771	1776	rBV	534110	704257	64.87%	4.323%
60	12.698	1783	1786	1791	rVB2	51596	69636	6.41%	0.427%
61	12.839	1804	1810	1816	rBV	442088	671869	61.89%	4.124%
62	12.892	1816	1819	1826	rVB3	40266	62978	5.80%	0.387%
63	12.980	1827	1834	1842	rVB	595804	839811	77.35%	5.155%
64	13.063	1842	1848	1851	rBV2	57046	119460	11.00%	0.733%
65	13.168	1859	1866	1870	rVB	79033	136717	12.59%	0.839%
66	13.233	1874	1877	1880	rBV2	32364	40263	3.71%	0.247%
67	13.274	1880	1884	1891	rVB3	60938	100073	9.22%	0.614%
68	13.368	1896	1900	1902	rBV	35884	43366	3.99%	0.266%
69	13.398	1902	1905	1909	rVB	38176	43666	4.02%	0.268%
70	13.680	1950	1953	1956	rBV	42798	55838	5.14%	0.343%
71	13.792	1967	1972	1974	rBV	55344	85302	7.86%	0.524%
72	14.039	2007	2014	2017	rBV2	402669	698044	64.30%	4.285%
73	14.068	2017	2019	2026	rVB	221510	262032	24.14%	1.608%
74	14.315	2057	2061	2066	rVB2	37209	65492	6.03%	0.402%
75	14.433	2077	2081	2084	rBV	51140	69236	6.38%	0.425%
76	14.462	2084	2086	2090	rVB2	28539	30819	2.84%	0.189%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144401.D
Acq On : 02 Dec 2025 14:21
Operator : RC/JU
Sample : Q3742-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1125-23

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	14.839	2147	2150	2155	rVB3	38603	57958	5.34%	0.356%
78	15.092	2188	2193	2204	rBV	191723	449297	41.38%	2.758%
79	15.398	2241	2245	2252	rBV2	107746	197112	18.16%	1.210%
80	15.462	2252	2256	2261	rVB	154202	227908	20.99%	1.399%
81	15.527	2262	2267	2279	rBV2	240112	430404	39.64%	2.642%
82	17.021	2516	2521	2529	rBV2	71577	153564	14.14%	0.943%
83	17.480	2594	2599	2613	rVB	56191	132219	12.18%	0.812%


Sum of corrected areas: 16291534

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144401.D
Acq On : 02 Dec 2025 14:21
Operator : RC/JU
Sample : Q3742-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1125-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

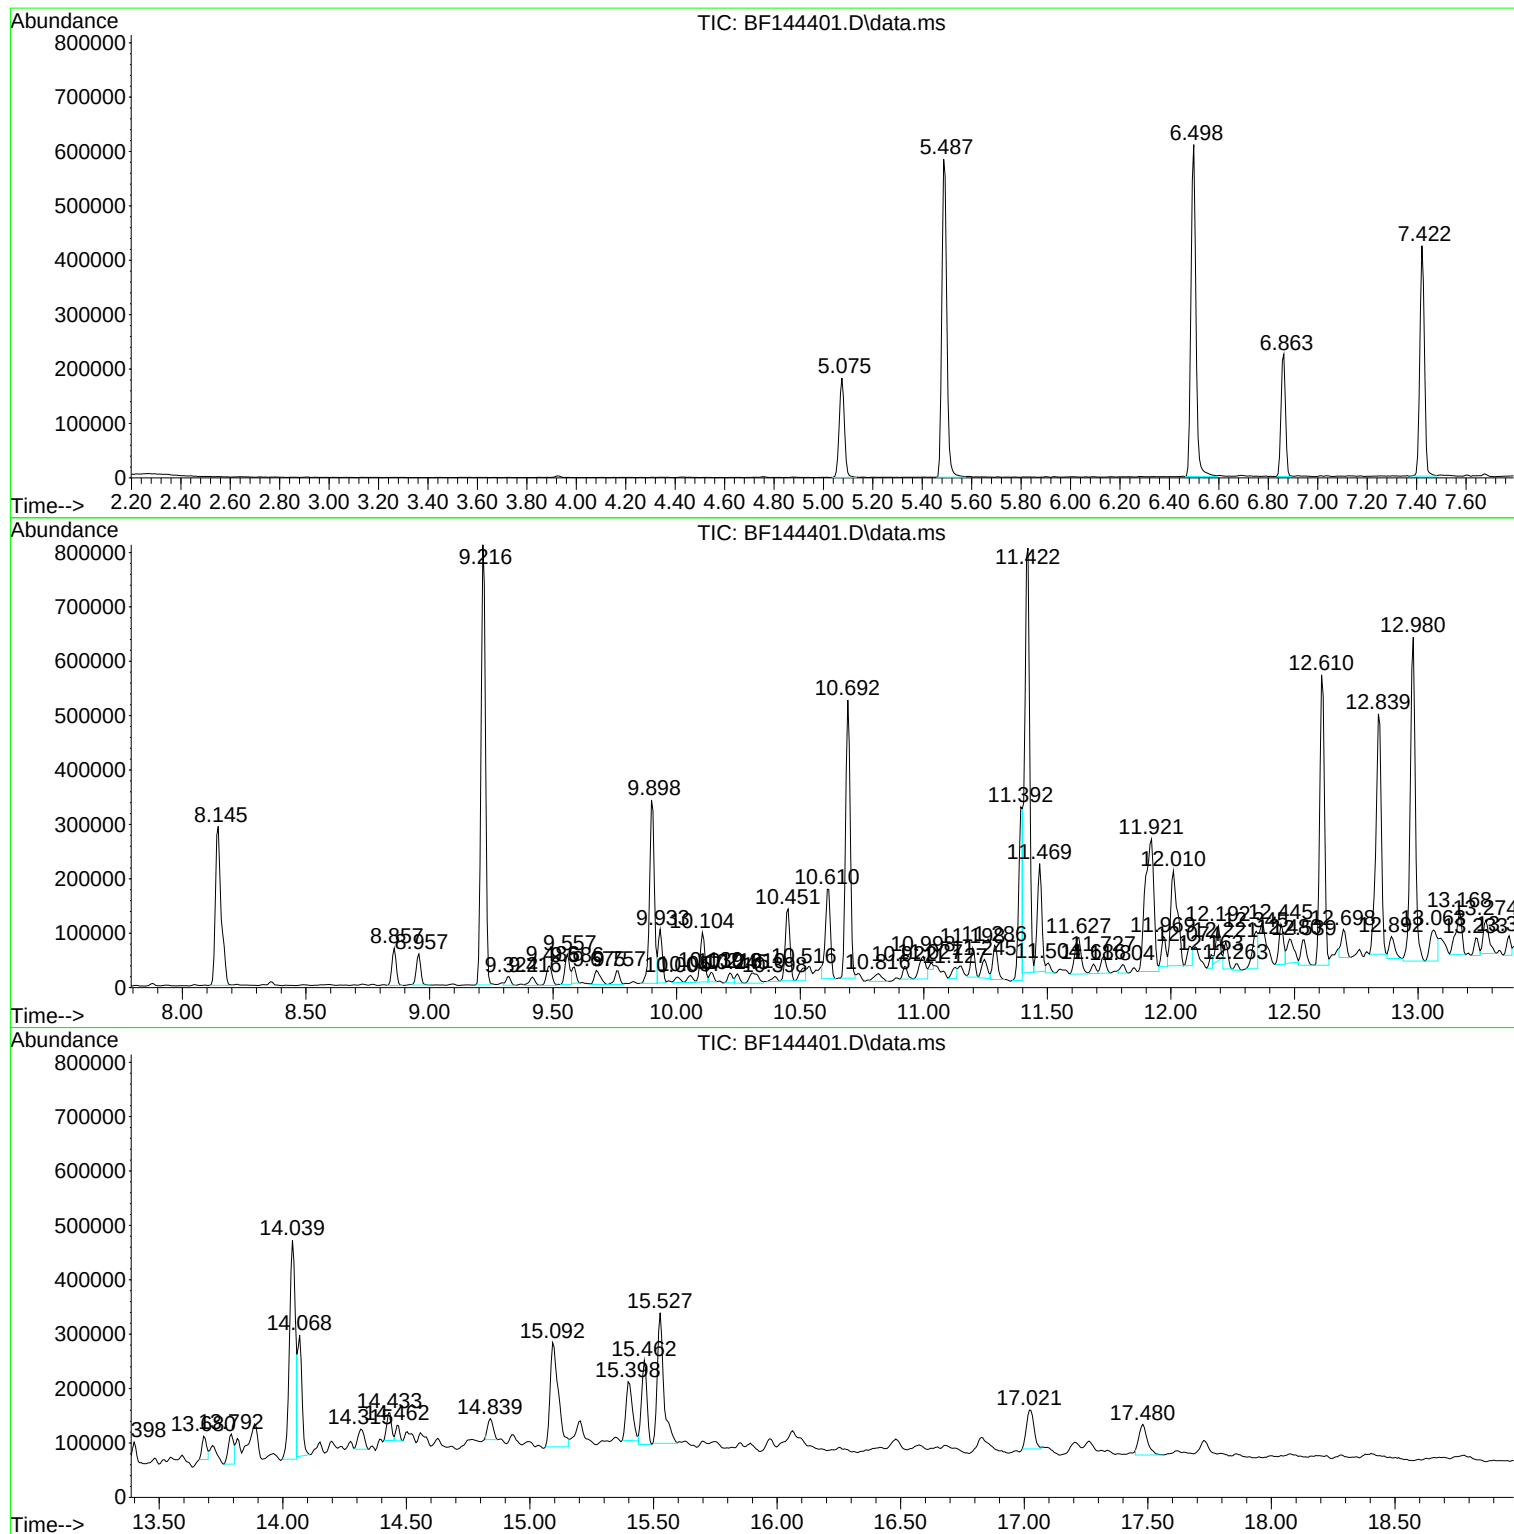

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144401.D
Acq On : 02 Dec 2025 14:21
Operator : RC/JU
Sample : Q3742-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1125-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120225\
Data File : BF144401.D
Acq On : 02 Dec 2025 14:21
Operator : RC/JU
Sample : Q3742-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1125-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc