
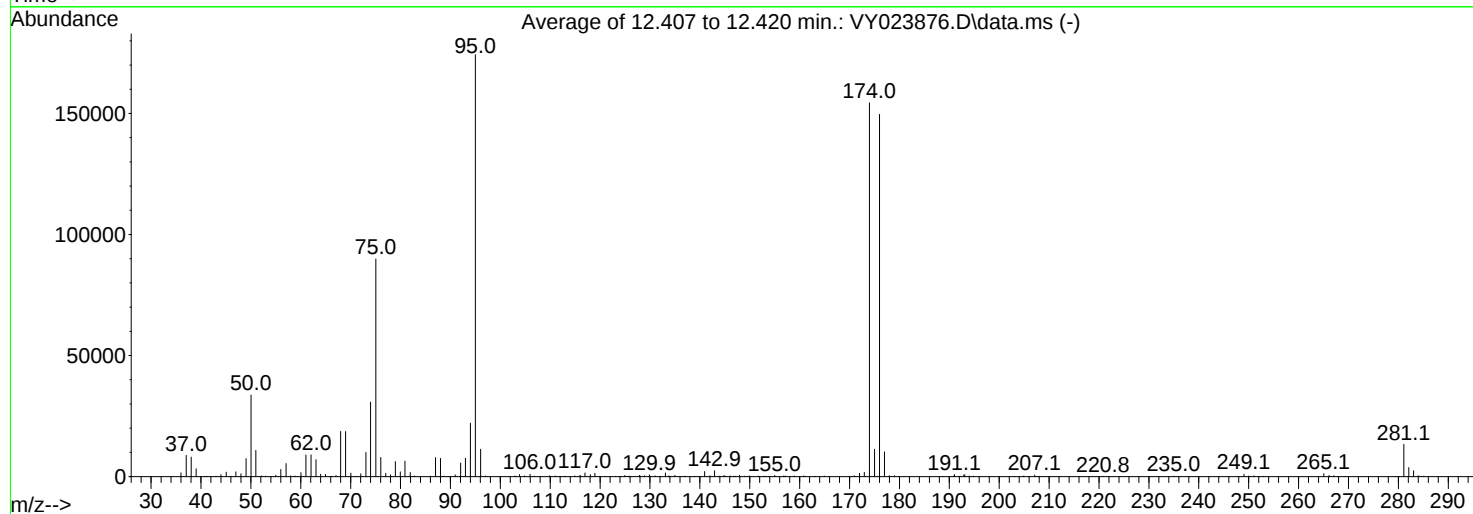


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120425\
Data File : VY023876.D
Acq On : 04 Dec 2025 07:00
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120325S.M
Title : SW846 8260
Last Update : Thu Dec 04 03:49:13 2025

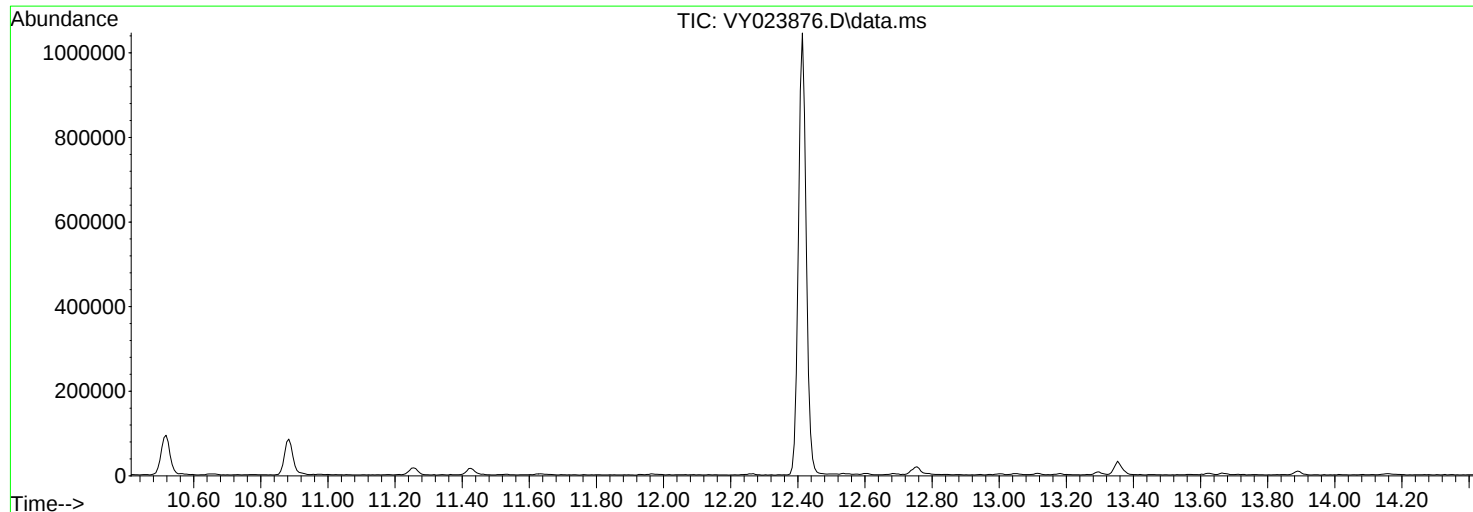

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	33653	PASS
75	95	30	60	51.6	89864	PASS
95	95	100	100	100.0	174251	PASS
96	95	5	9	6.5	11259	PASS
173	174	0.00	2	1.1	1774	PASS
174	95	50	100	88.6	154389	PASS
175	174	5	9	7.3	11277	PASS
176	174	95	101	96.9	149589	PASS
177	176	5	9	6.8	10238	PASS