

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120225\
 Data File : PL097766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 17:35
 Operator : AR\AJ
 Sample : Q3443-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TW-1125-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:04:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 26 07:07:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	2.802	65772691	91352082	12.837	12.771
28)	SA Decachlor...	8.972	7.954	53536575	256.5E6	16.680	54.494 #
Target Compounds							
3)	MA gamma-BHC...	0.000	3.640	0	3211931	N.D.	0.313 #
7)	B delta-BHC	4.717	0.000	20558996	0	2.946	N.D. #
8)	B Heptachlo...	5.625	4.746f	13281724	3816149	2.112	0.455 #
9)	A Endosulfan I	0.000	5.149f	0	4177547	N.D.	0.483 #
10)	B gamma-Chl...	5.867	0.000	2706004	0	0.453	N.D. #
11)	B alpha-Chl...	0.000	5.108f	0	4947826	N.D.	0.528 #
13)	MA Dieldrin	0.000	5.368f	0	4146151	N.D.	0.480 #
15)	B Endosulfa...	6.714	0.000	23586493	0	4.649	N.D. #
19)	B Endosulfa...	0.000	6.381f	0	9681153	N.D.	1.411 #
23)	Chlordane-1	0.000	3.808	0	2805057	N.D.	11.039 #
25)	Chlordane-3	5.867	0.000	2706004	0	3.430	N.D. #
26)	Chlordane-4	0.000	5.108f	0	4947826	N.D.	6.585 #
27)	Chlordane-5	0.000	5.997f	0	11159628	N.D.	42.594 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120225\
Data File : PL097766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 17:35
Operator : AR\AJ
Sample : Q3443-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:04:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Wed Nov 26 07:07:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

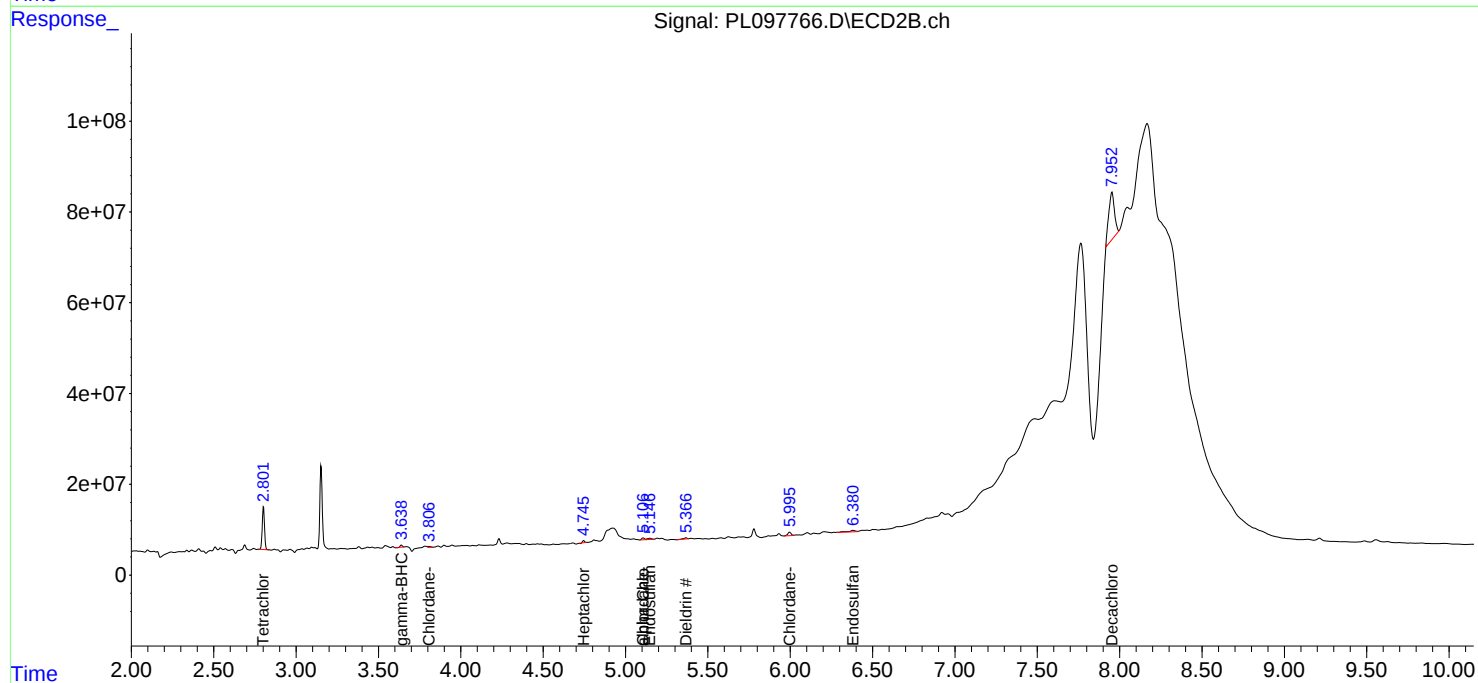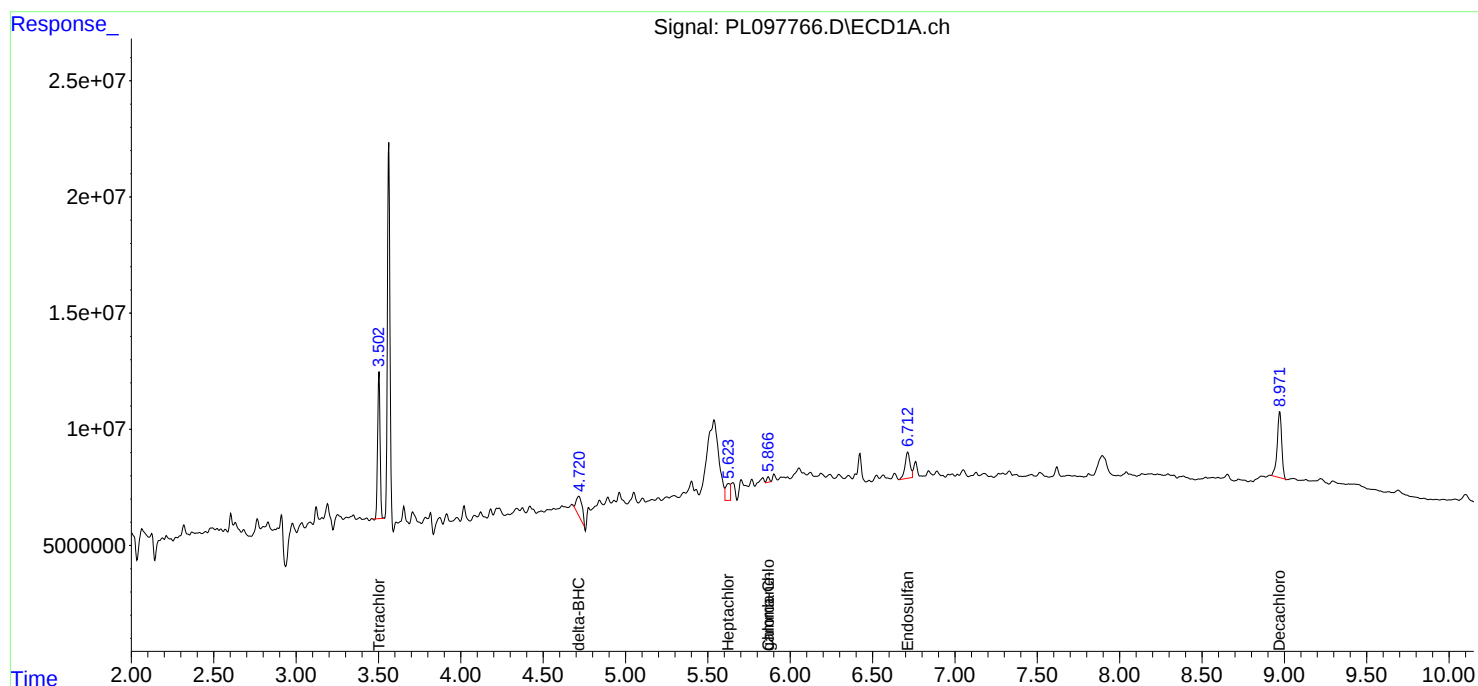


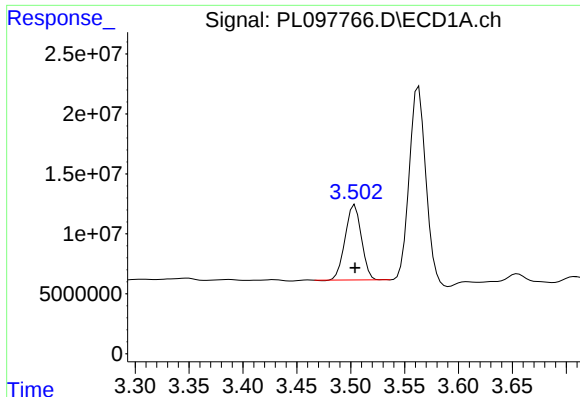

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 65772691
Conc: 12.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

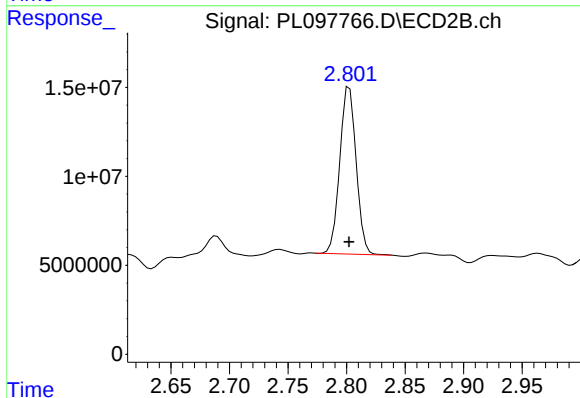


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 91352082
Conc: 12.77 ng/ml

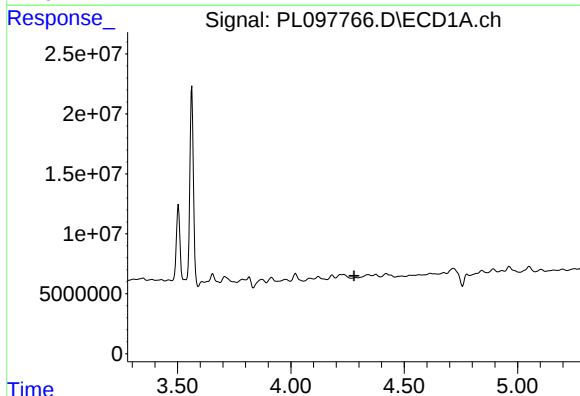


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.279 min
Response: 0
Conc: N.D.

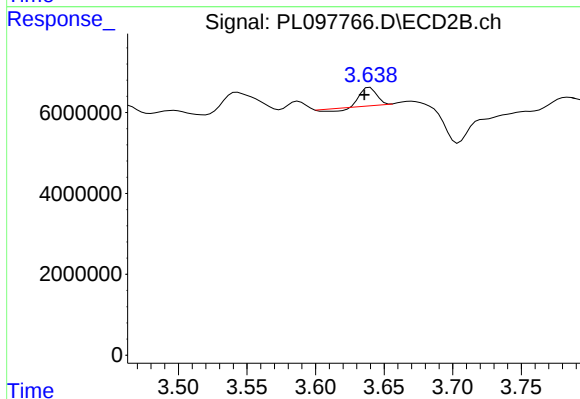

#3 gamma-BHC (Lindane)


R.T.: 3.640 min
Delta R.T.: 0.004 min
Response: 3211931
Conc: 0.31 ng/ml

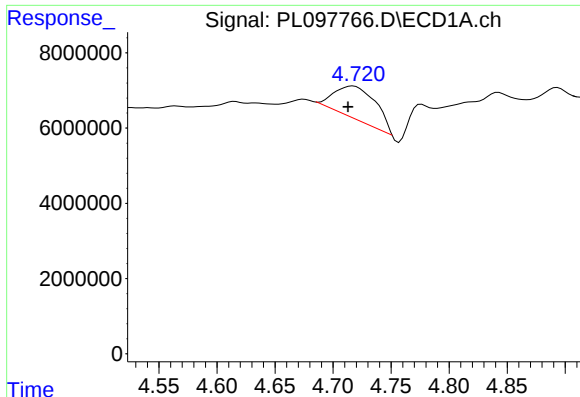

#7 delta-BHC


R.T.: 4.717 min
Delta R.T.: 0.004 min
Response: 20558996
Conc: 2.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

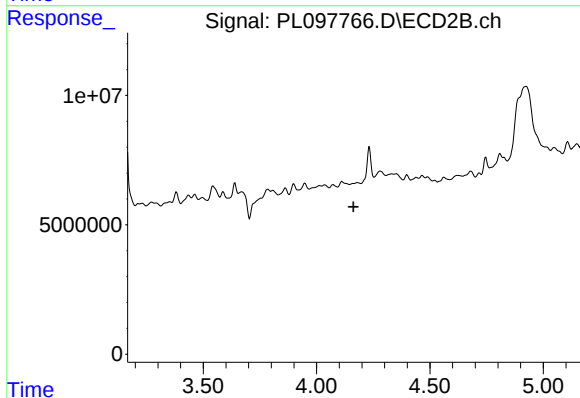


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.163 min
Response: 0
Conc: N.D.

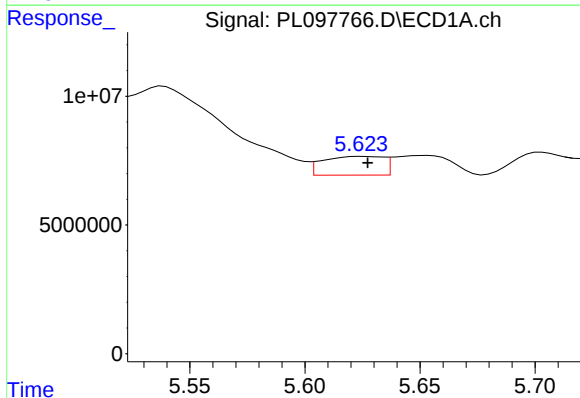


#8 Heptachlor epoxide

R.T.: 5.625 min
Delta R.T.: -0.003 min
Response: 13281724
Conc: 2.11 ng/ml

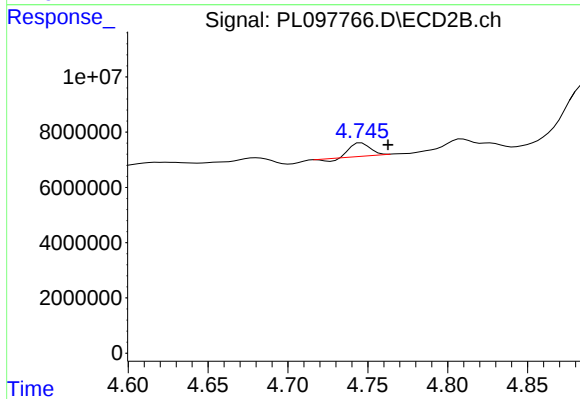

#8 Heptachlor epoxide


R.T.: 4.746 min
Delta R.T.: -0.017 min
Response: 3816149
Conc: 0.45 ng/ml

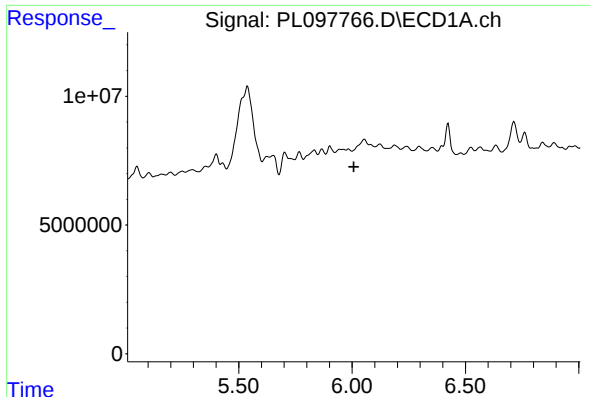

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

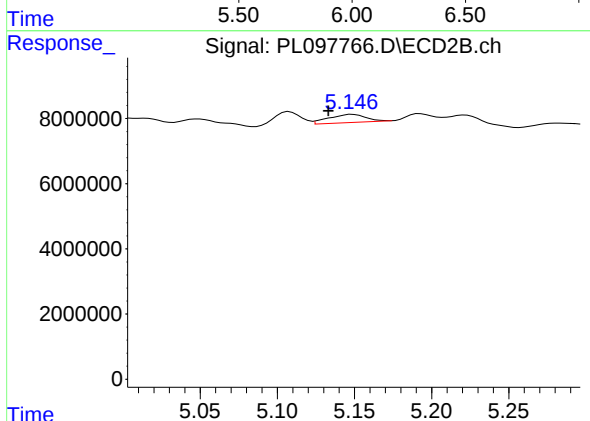


#9 Endosulfan I

R.T.: 5.149 min
Delta R.T.: 0.016 min
Response: 4177547
Conc: 0.48 ng/ml

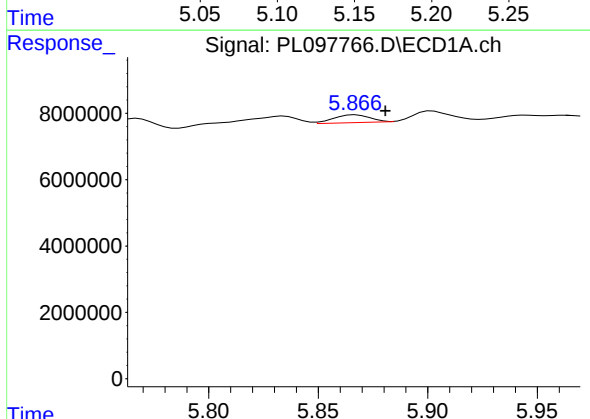


#10 gamma-Chlordane

R.T.: 5.867 min
Delta R.T.: -0.014 min
Response: 2706004
Conc: 0.45 ng/ml

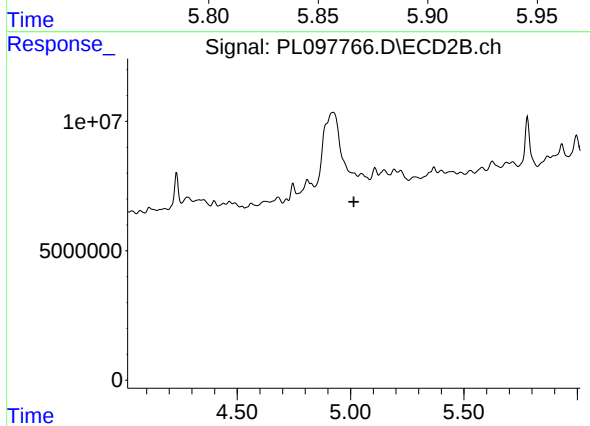

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.015 min
Response: 0
Conc: N.D.

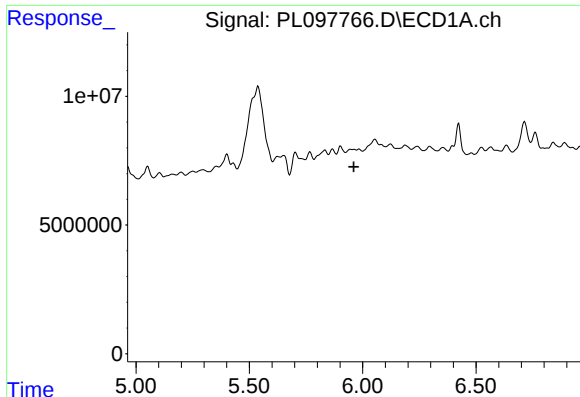

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

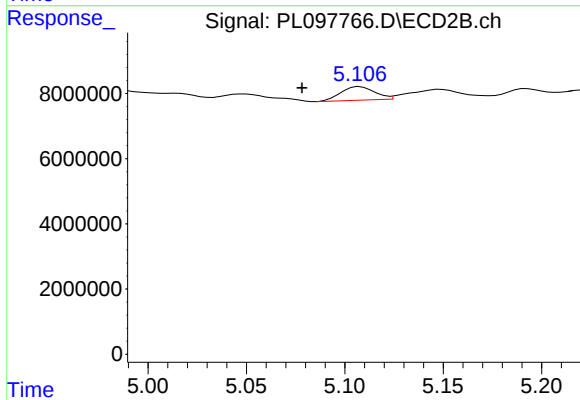


#11 alpha-Chlordane

R.T.: 5.108 min
Delta R.T.: 0.030 min
Response: 4947826
Conc: 0.53 ng/ml

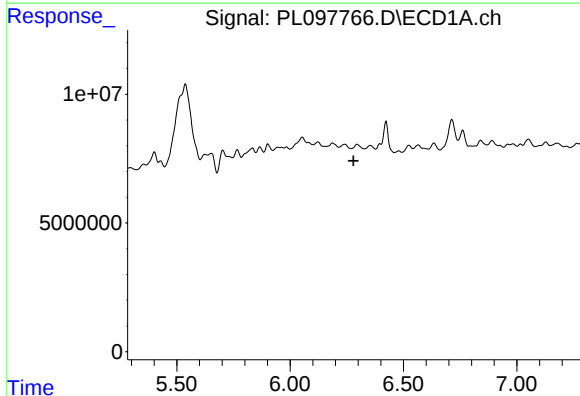


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.280 min
Response: 0
Conc: N.D.

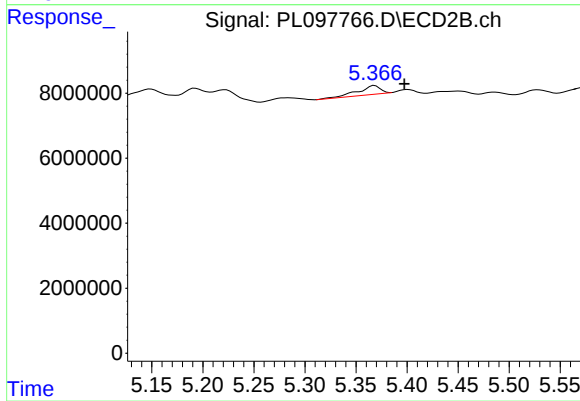

#13 Dieldrin


R.T.: 5.368 min
Delta R.T.: -0.029 min
Response: 4146151
Conc: 0.48 ng/ml

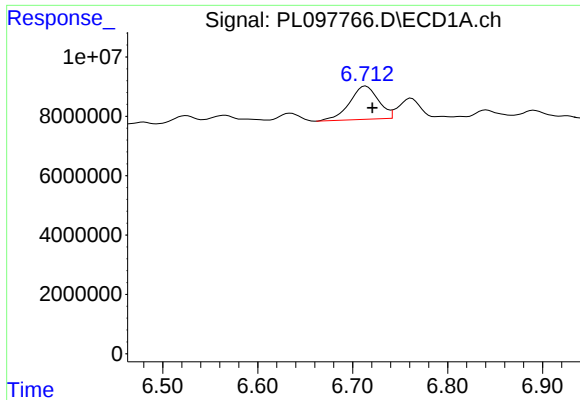

#15 Endosulfan II


R.T.: 6.714 min
Delta R.T.: -0.007 min
Response: 23586493
Conc: 4.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

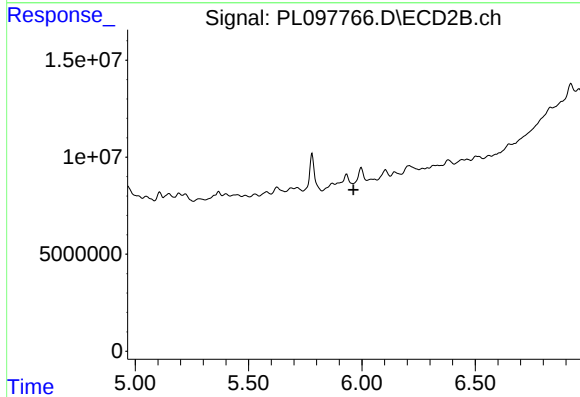


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.963 min
Response: 0
Conc: N.D.

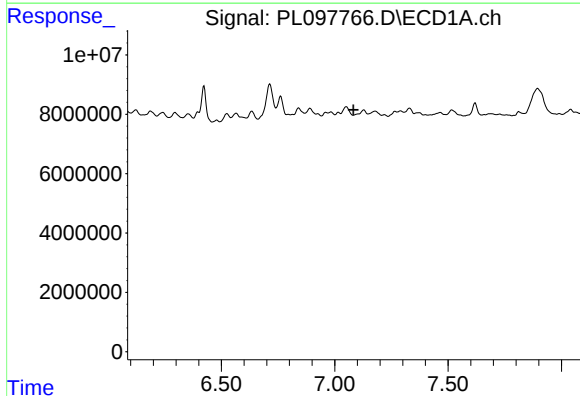


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.083 min
Response: 0
Conc: N.D.

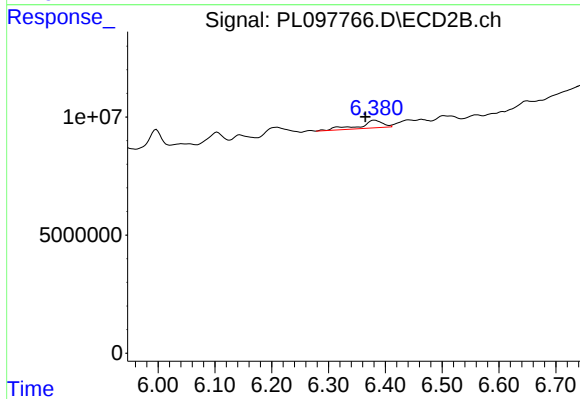

#19 Endosulfan Sulfate


R.T.: 6.381 min
Delta R.T.: 0.017 min
Response: 9681153
Conc: 1.41 ng/ml

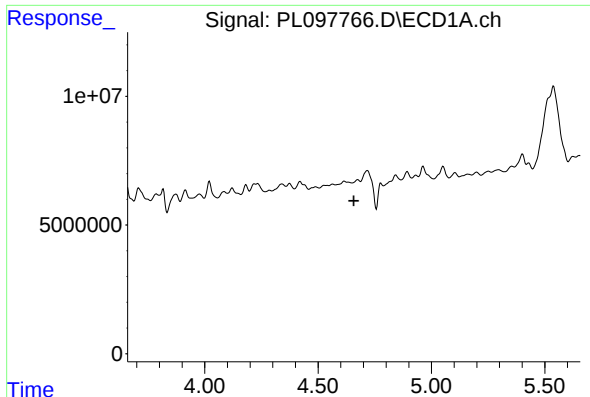

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

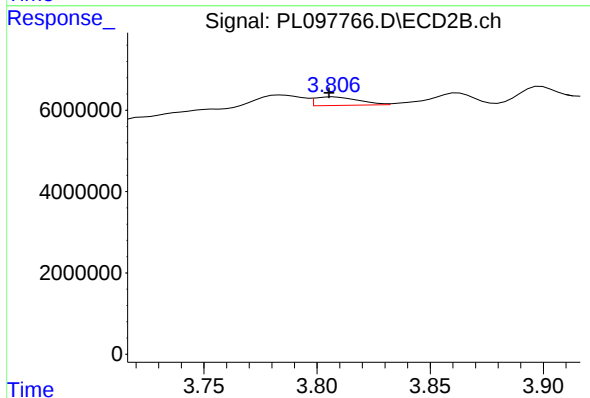


#23 Chlordane-1

R.T.: 3.808 min
Delta R.T.: 0.002 min
Response: 2805057
Conc: 11.04 ng/ml

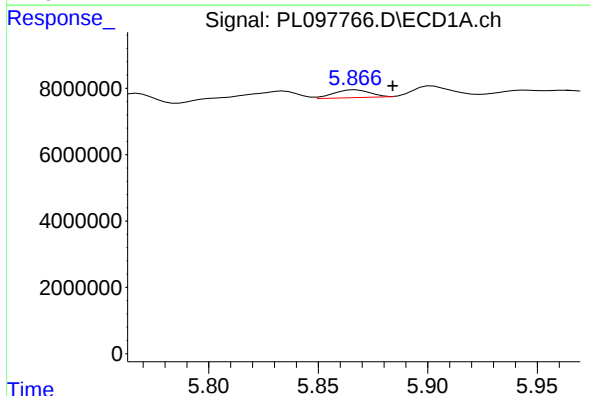


#25 Chlordane-3

R.T.: 5.867 min
Delta R.T.: -0.017 min
Response: 2706004
Conc: 3.43 ng/ml

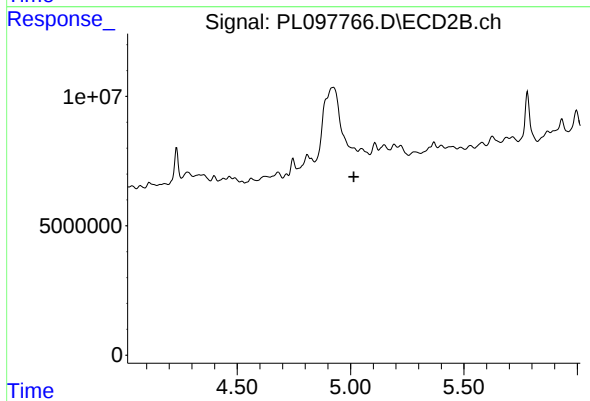

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.014 min
Response: 0
Conc: N.D.

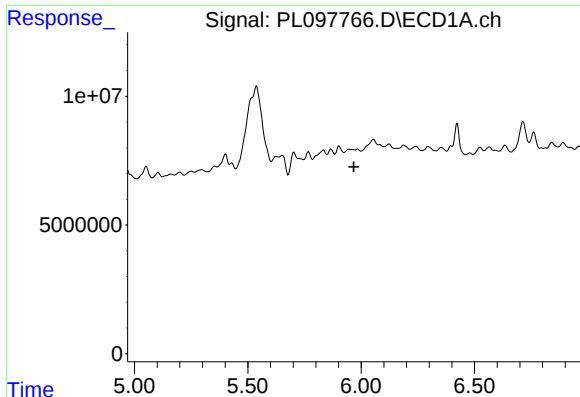

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

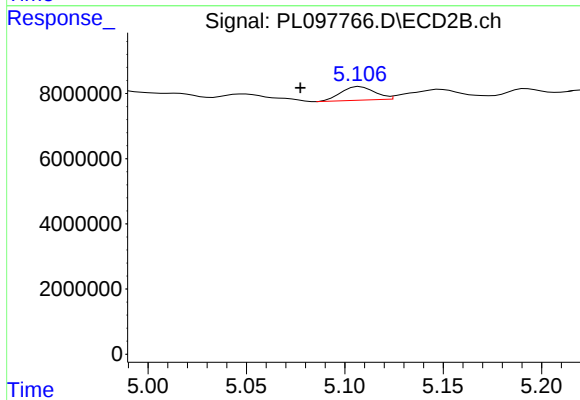


#26 Chlordane-4

R.T.: 5.108 min
Delta R.T.: 0.030 min
Response: 4947826
Conc: 6.59 ng/ml

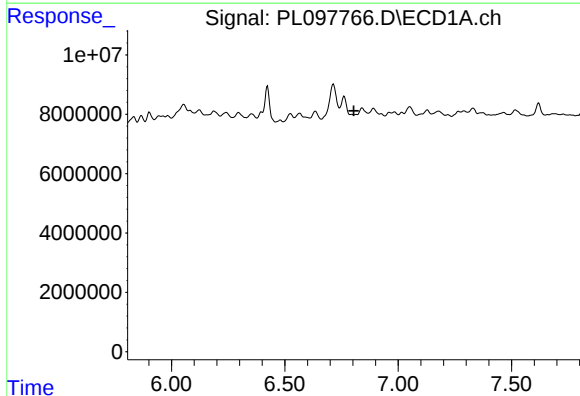


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.804 min
Response: 0
Conc: N.D.

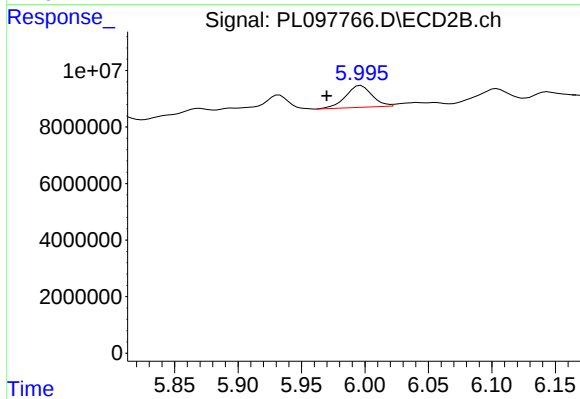

#27 Chlordane-5


R.T.: 5.997 min
Delta R.T.: 0.027 min
Response: 11159628
Conc: 42.59 ng/ml

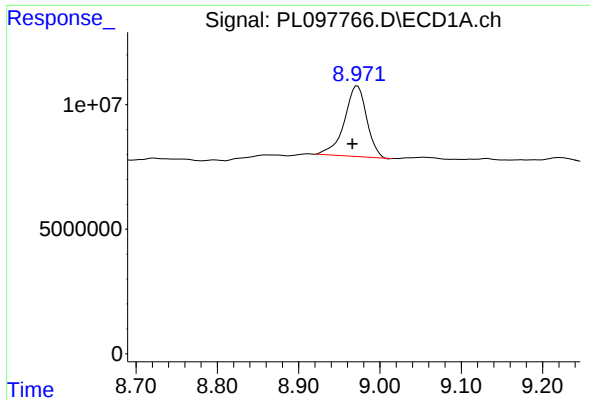

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.006 min
Response: 53536575
Conc: 16.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-1125-2

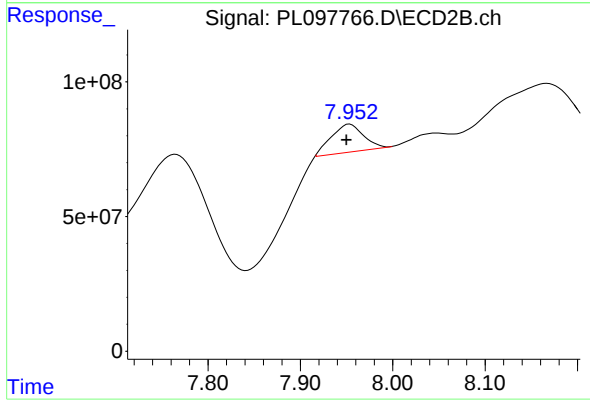

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.004 min
Response: 256490531
Conc: 54.49 ng/ml