
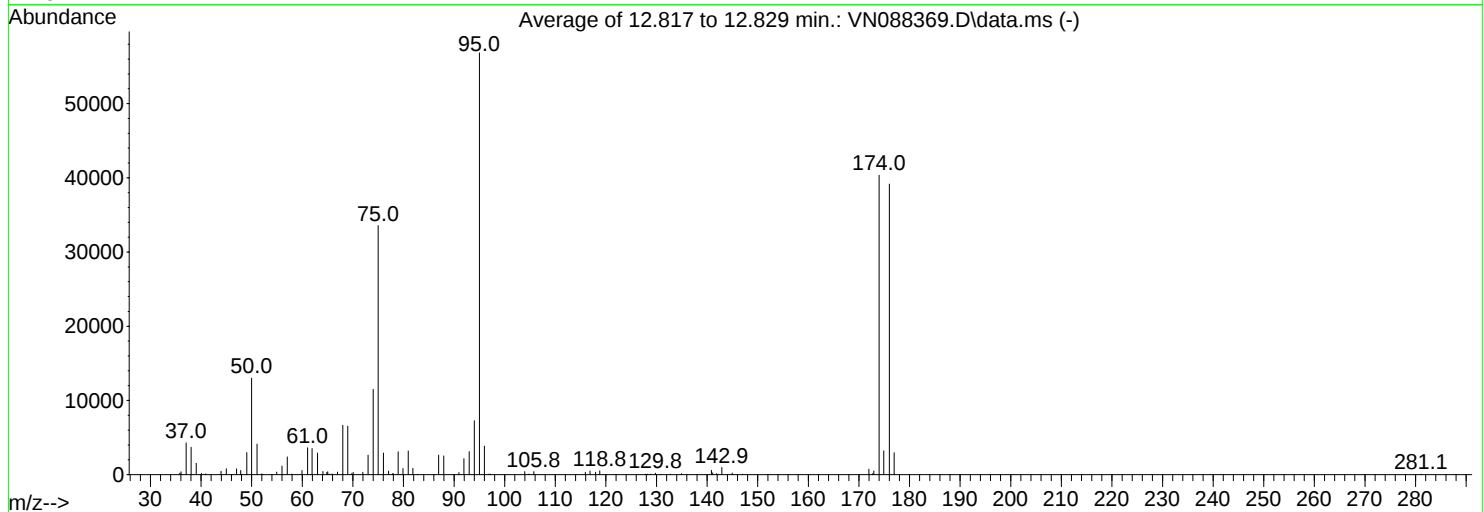


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120125\
Data File : VN088369.D
Acq On : 01 Dec 2025 08:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

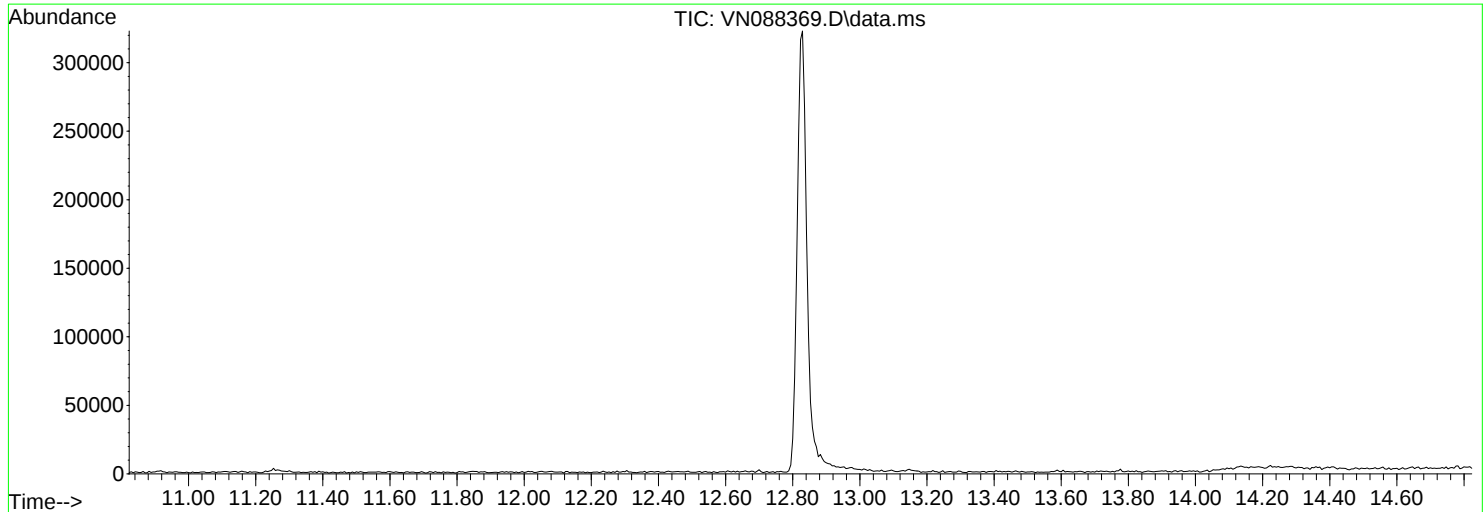

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	13006	PASS
75	95	30	60	59.1	33576	PASS
95	95	100	100	100.0	56845	PASS
96	95	5	9	6.7	3835	PASS
173	174	0.00	2	1.2	489	PASS
174	95	50	100	71.0	40341	PASS
175	174	5	9	8.0	3213	PASS
176	174	95	101	97.1	39165	PASS
177	176	5	9	7.5	2949	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	190	49.05	2976	61.95	3517	70.05	311
36.05	384	50.00	13006	63.00	2917	71.95	331
37.05	4272	51.05	4113	64.10	433	73.00	263
38.05	3684	51.90	88	64.85	304	74.00	1149
39.05	1525	52.10	68	65.05	399	75.00	33576
40.10	142	54.95	339	65.40	72	76.05	2917
40.95	105	56.00	1161	65.90	102	77.05	468
43.95	455	57.05	2400	66.95	355	77.80	128
45.00	808	57.90	81	68.00	6639	78.00	126
47.00	782	59.95	560	69.00	6543	78.95	3079
47.85	567	61.05	3625	69.80	174	79.90	824

Average of 12.817 to 12.829 min.: VN088369.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	3198	96.00	3835	128.20	67	147.00	61
81.85	841	96.90	89	128.80	61	148.00	50
82.80	51	97.20	58	129.80	188	171.95	743
86.00	50	103.95	408	130.80	50	172.70	124
86.95	2627	104.80	82	132.80	67	172.95	489
87.95	2534	105.75	414	134.95	138	174.00	40341
90.95	286	115.95	332	140.85	577	174.90	3213
91.95	2167	116.85	505	141.10	238	176.00	39165
93.00	3106	117.95	315	141.90	151	176.95	2949
94.00	7272	118.80	513	142.90	969	281.10	73
95.00	56845	127.80	56	144.95	206		

Instrument :

MSVOA_N

ClientSampleId :

BFB