


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL120225\
Data File : VL043291.D
Acq On : 02 Dec 2025 08:38
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL111825AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Nov 19 01:11:25 2025

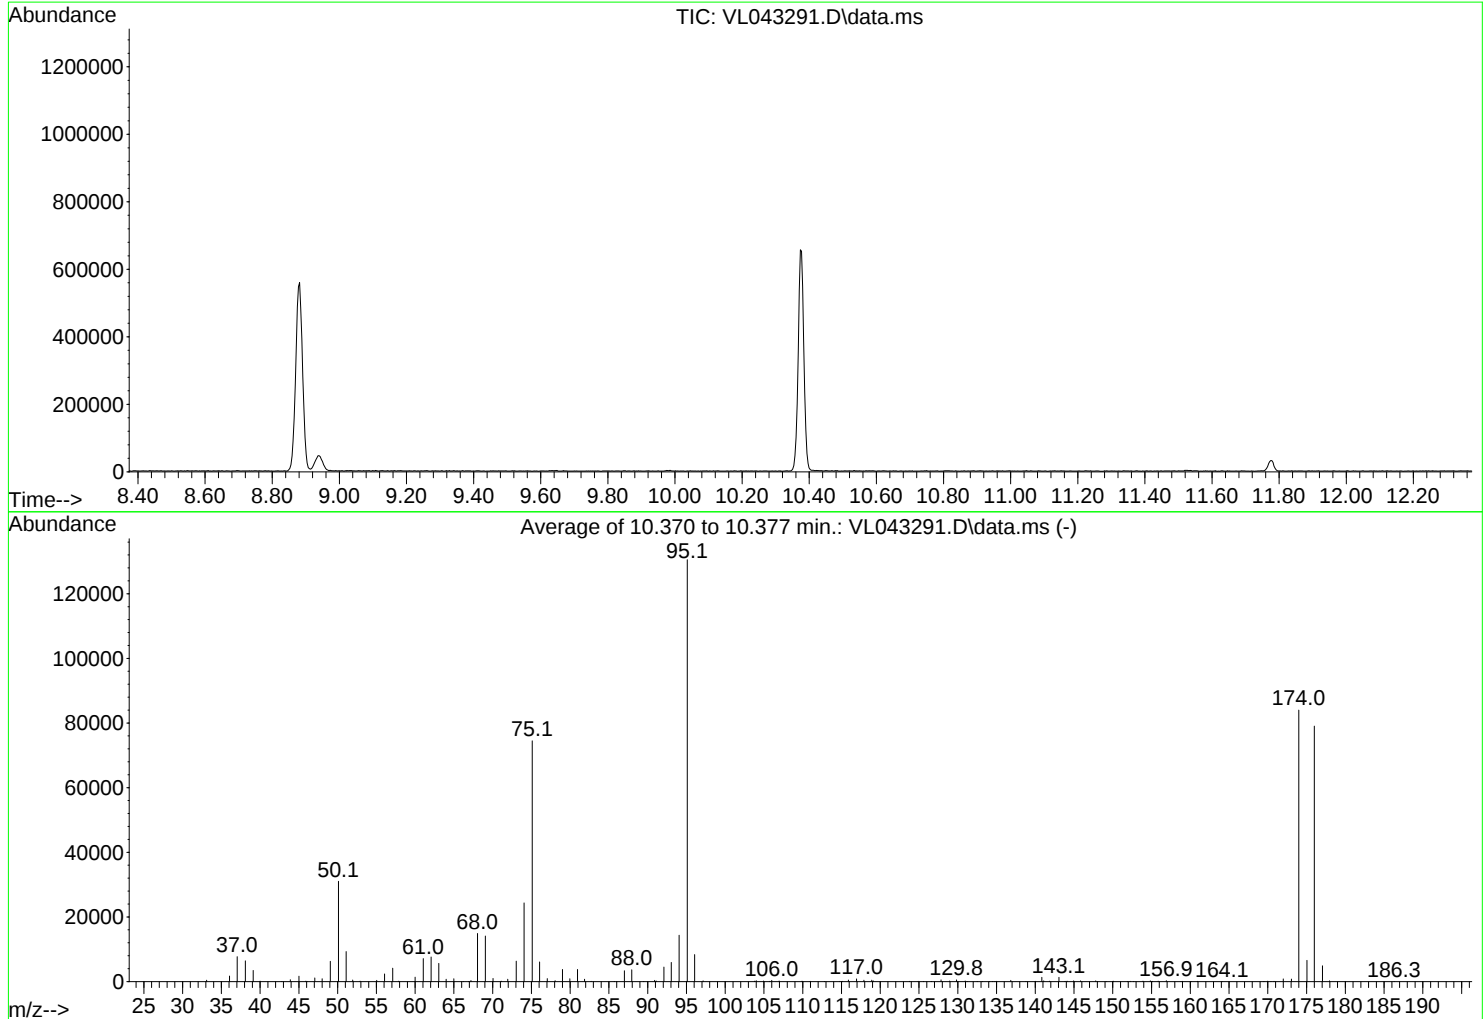

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	31024	PASS
75	95	30	66	57.1	74475	PASS
95	95	100	100	100.0	130520	PASS
96	95	5	9	6.4	8369	PASS
173	174	0.00	2	0.9	796	PASS
174	95	50	120	64.3	83984	PASS
175	174	4	9	7.8	6548	PASS
176	174	93	101	94.1	79069	PASS
177	176	5	9	6.2	4882	PASS

Average of 10.370 to 10.377 min.: VL043291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	424	47.05	1140	60.00	1351	70.05	951
36.05	1694	48.00	882	61.05	7092	71.10	111
37.05	7695	49.05	6286	62.05	7621	71.95	701
38.10	6427	50.10	31024	63.05	5631	73.05	630
39.10	3429	51.10	9311	64.00	698	74.05	24312
40.00	107	51.95	471	65.00	889	75.10	74475
42.80	48	52.90	108	66.20	46	76.05	6095
43.90	588	55.05	354	66.90	26	77.05	906
45.00	1676	56.05	2346	67.20	317	78.05	302
45.90	127	57.10	4136	68.05	14867	79.00	3750
46.05	60	57.90	136	69.05	14105	79.95	876

Average of 10.370 to 10.377 min.: VL043291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	3756	93.05	5935	109.90	143	124.90	92
81.85	744	94.05	14353	110.95	87	125.60	19
82.70	61	95.10	130520	112.80	28	126.60	18
85.70	26	96.05	8369	114.80	72	127.85	526
86.00	53	97.15	219	115.10	82	128.95	186
87.00	3354	103.80	113	115.90	484	129.85	530
87.95	3639	104.00	276	116.95	804	130.95	157
89.50	22	104.95	167	117.90	413	131.20	34
90.90	363	105.75	63	118.90	421	132.50	46
91.10	192	106.00	398	119.10	242	133.20	19
92.10	4503	106.95	157	123.80	102	134.10	30

Average of 10.370 to 10.377 min.: VL043291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
134.50	26	144.10	104	154.85	209	170.40	40
134.80	52	144.95	204	155.10	63	170.80	70
135.00	94	145.85	228	155.85	127	172.00	827
136.85	380	147.80	220	156.90	271	173.05	796
138.80	21	148.00	21	158.80	55	174.00	83984
140.00	95	149.15	45	159.00	90	175.05	6548
140.85	1296	150.05	127	160.10	36	176.00	79069
141.10	236	151.90	22	160.90	100	177.05	4882
141.85	142	152.25	67	164.10	49	177.95	213
143.05	1316	152.70	19	169.50	21	186.30	21
143.85	72	153.90	112	170.00	117		