


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121025\
Data File : BN038297.D
Acq On : 10 Dec 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

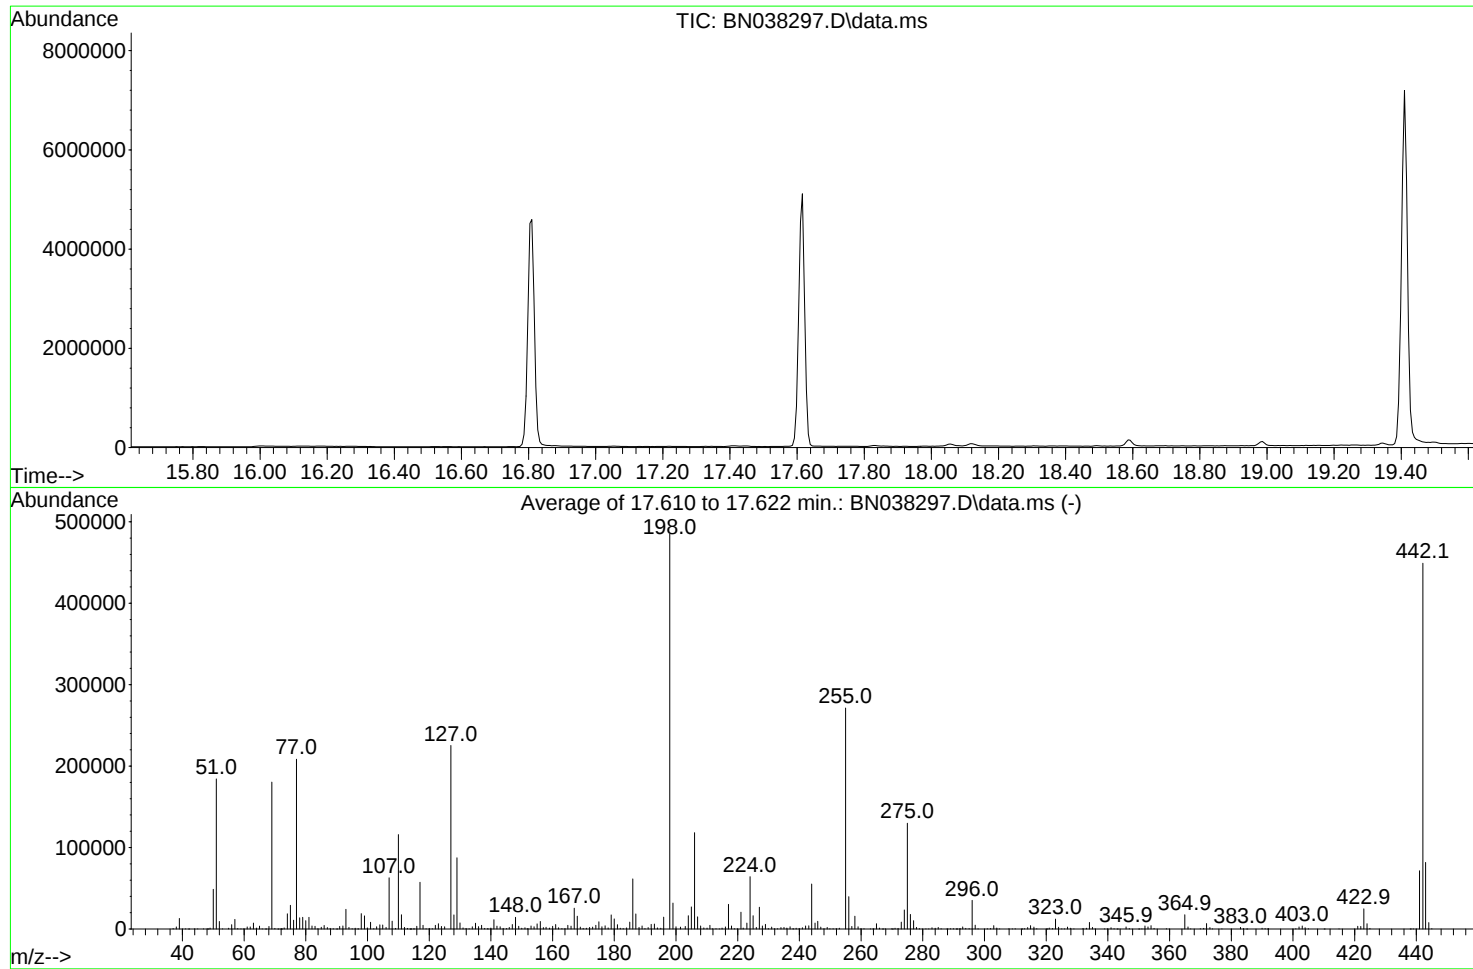

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3142	PASS
69	69	100	100	100.0	180342	PASS
70	69	0.00	2	0.5	866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	484821	PASS
199	198	5	9	6.6	31797	PASS
365	198	1	100	3.6	17415	PASS
441	443	0.01	150	87.6	71624	PASS
442	442	100	100	100.0	449131	PASS
443	442	15	24	18.2	81797	PASS