
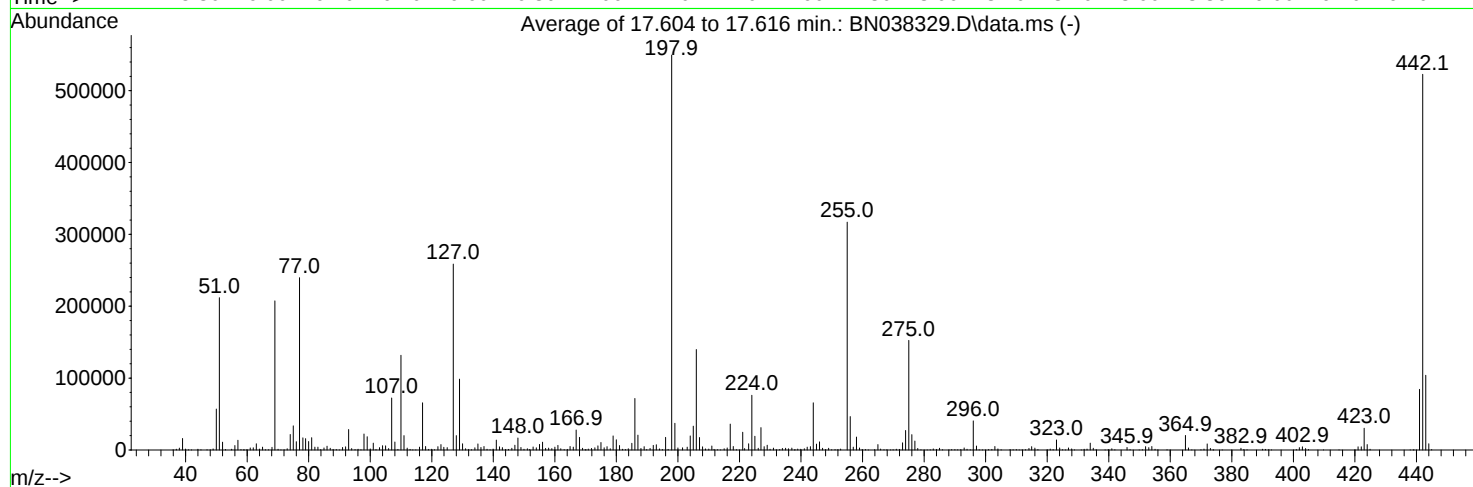


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038329.D
Acq On : 11 Dec 2025 23:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

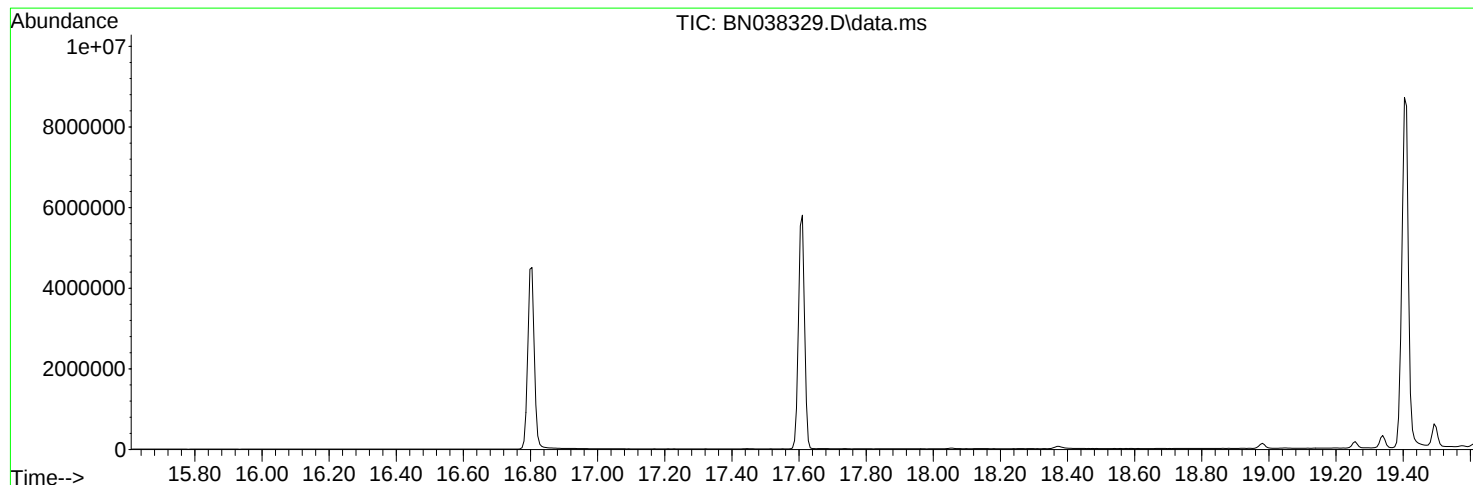




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2460

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	3777	PASS
69	69	100	100	100.0	207536	PASS
70	69	0.00	2	0.5	1066	PASS
197	198	0.00	2	0.1	776	PASS
198	198	100	100	100.0	549547	PASS
199	198	5	9	6.8	37157	PASS
365	198	1	100	3.7	20075	PASS
441	443	0.01	150	81.1	84259	PASS
442	442	100	100	100.0	522795	PASS
443	442	15	24	19.9	103896	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038329.D
Acq On : 11 Dec 2025 23:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 03:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

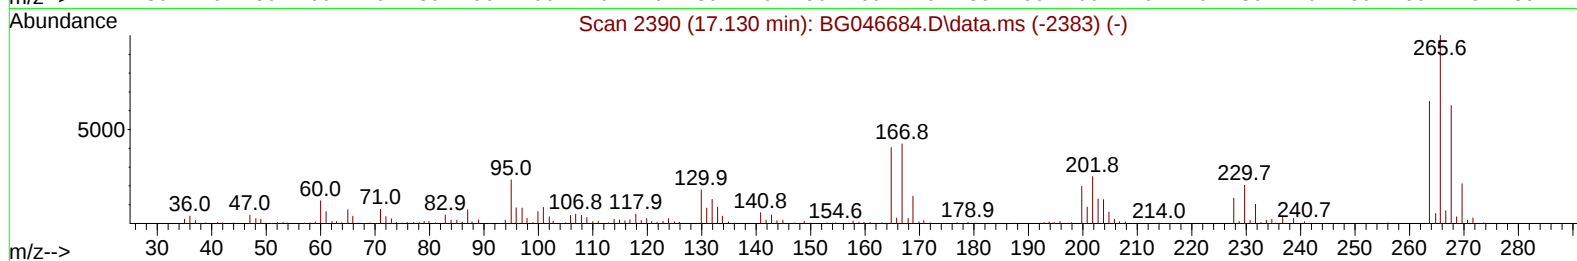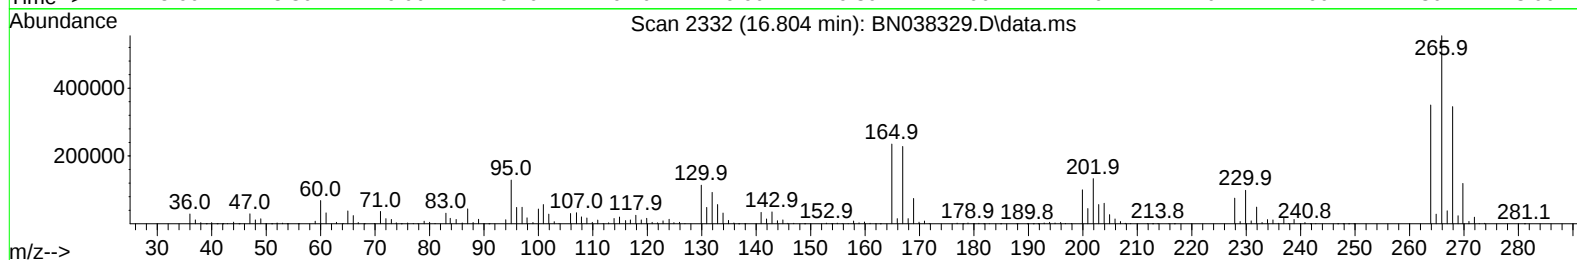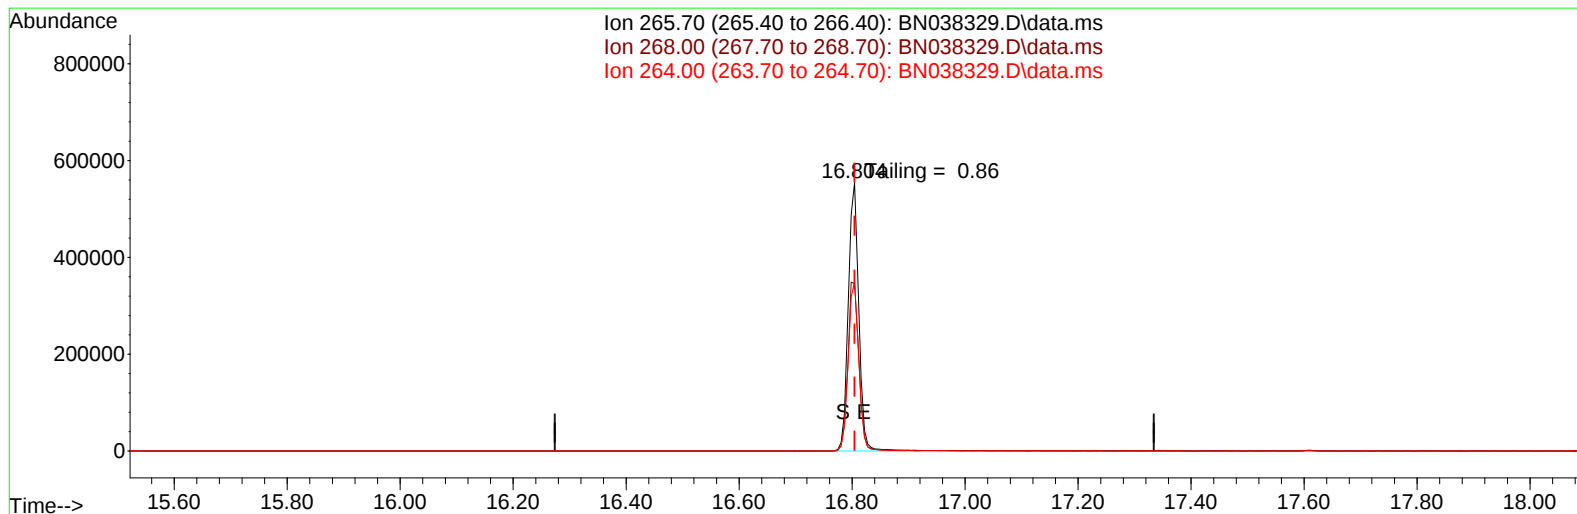

TIC: BN038329.D\data.ms

(70) Pentachlorophenol (C)

16.804min (0.000) 217492.83 ng




response 718575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.31
264.00	61.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038329.D
Acq On : 11 Dec 2025 23:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 03:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

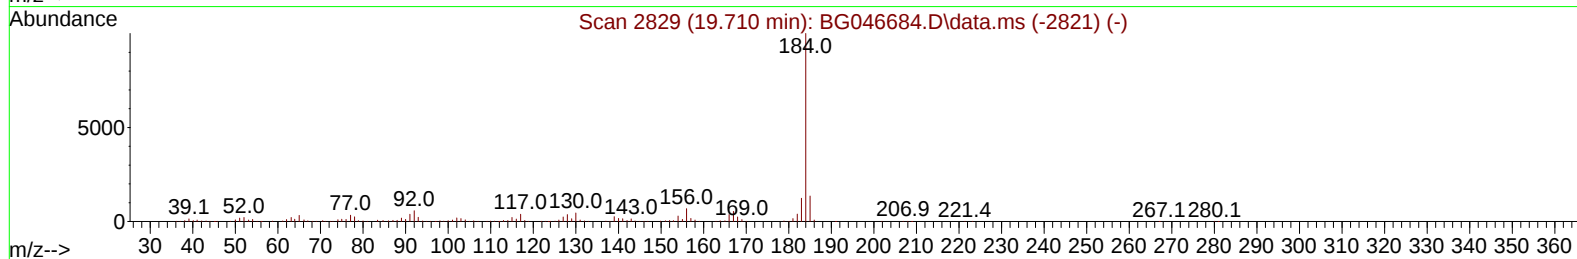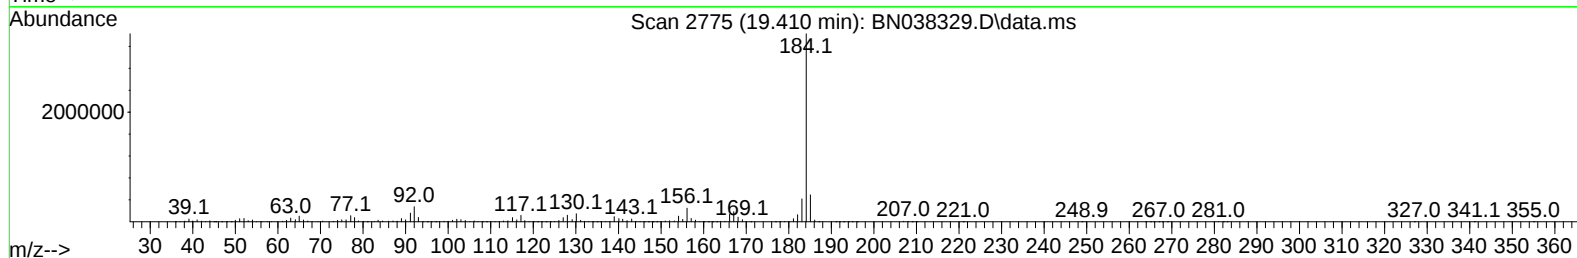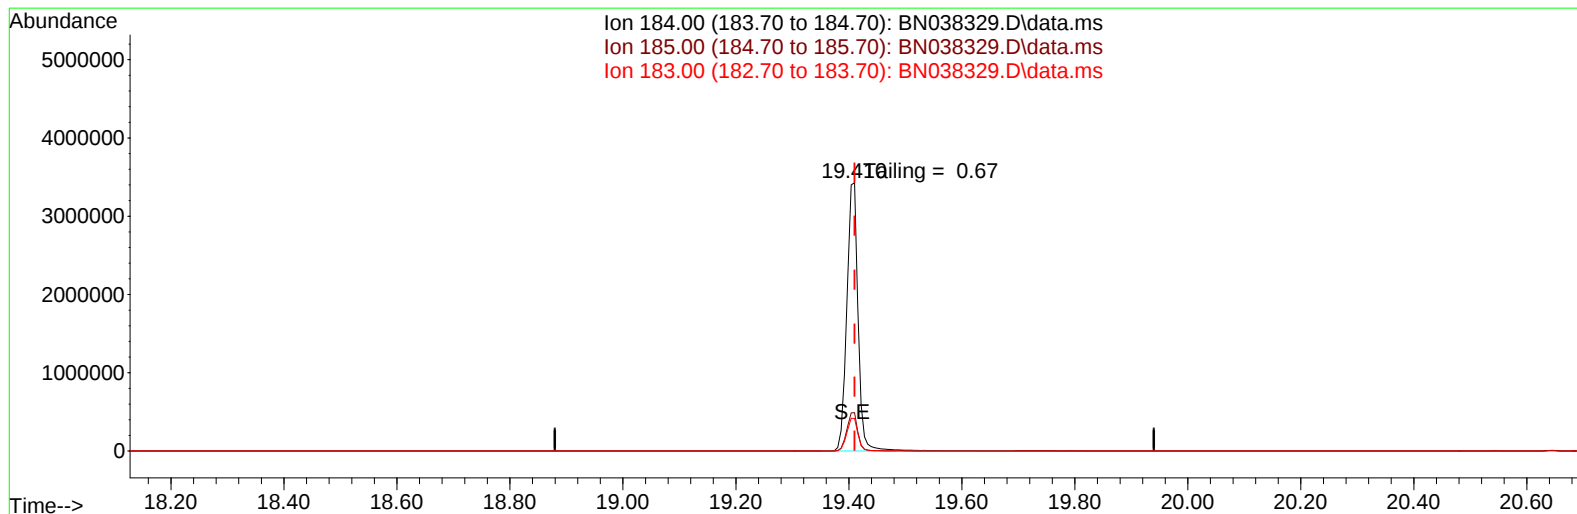

TIC: BN038329.D\data.ms

(77) Benzidine

19.410min (0.000) 4649.10 ng

response 4774950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	12.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2025	BNA_N	<u>BN038329.D</u>
Compound Name	Response	Retention Time
DDT	2196296	20.645
DDD	86752	20.204
DDE	2556	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
89308	2285604	3.91

Instrument :
BNA_N
ClientSampleId :
DFTPP