
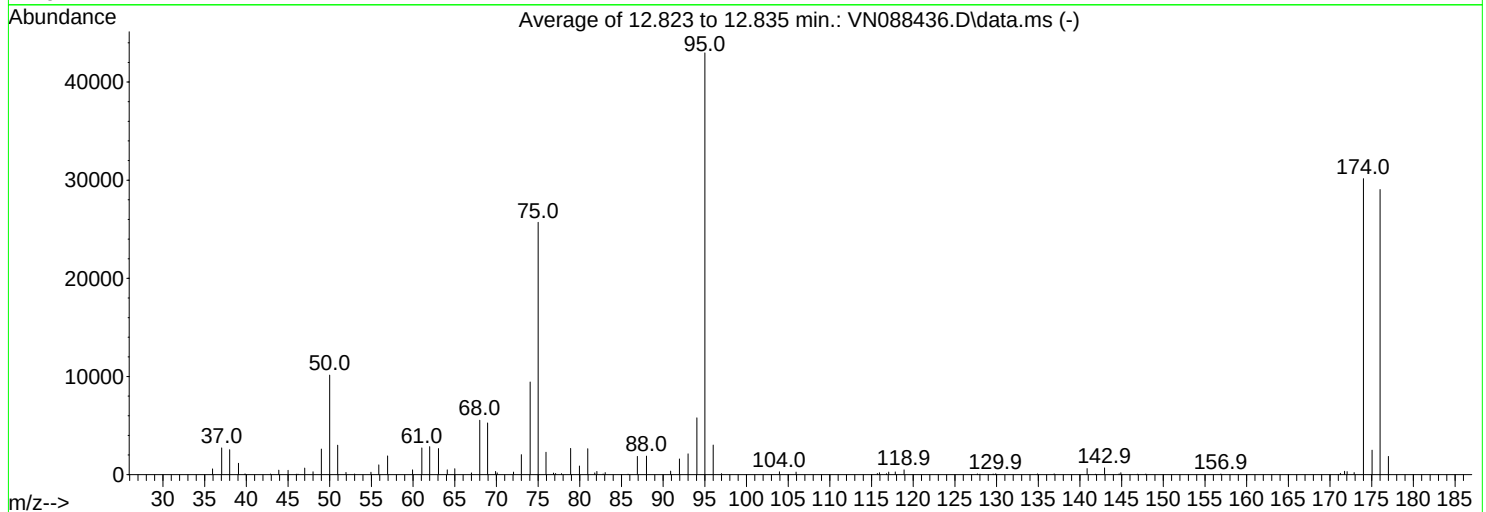


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120425\
Data File : VN088436.D
Acq On : 04 Dec 2025 11:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

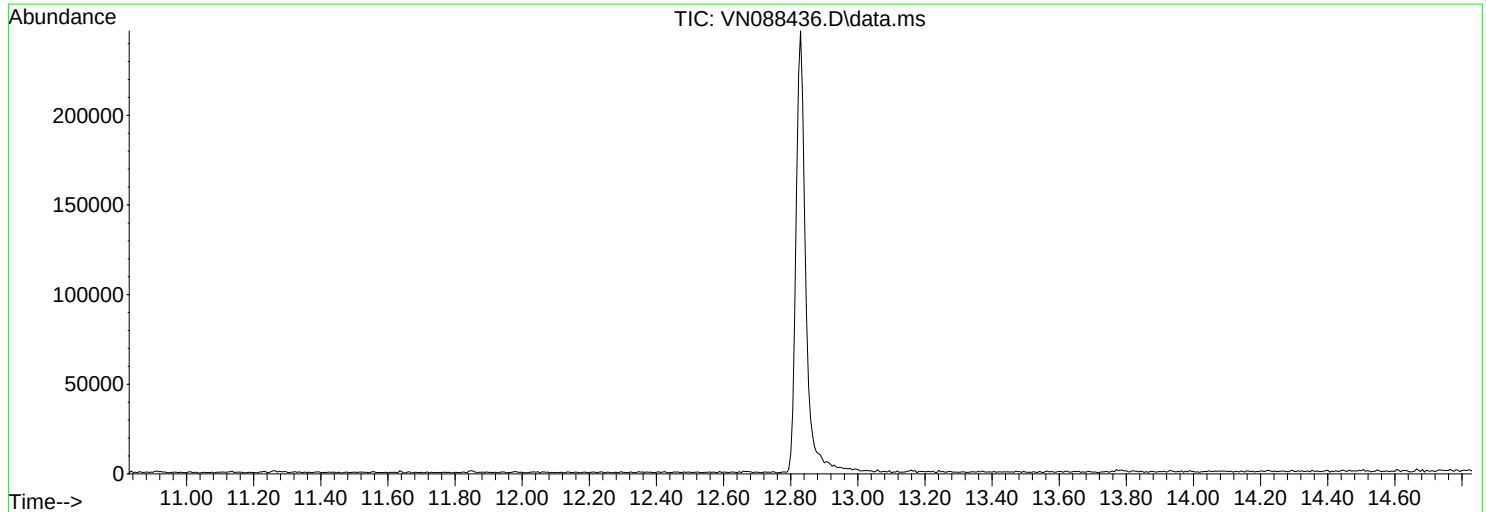

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	10147	PASS
75	95	30	60	59.8	25707	PASS
95	95	100	100	100.0	42976	PASS
96	95	5	9	7.0	3020	PASS
173	174	0.00	2	0.7	221	PASS
174	95	50	100	70.2	30165	PASS
175	174	5	9	8.3	2492	PASS
176	174	95	101	96.3	29056	PASS
177	176	5	9	6.4	1867	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	584	48.00	287	62.00	2852	74.05	943
37.05	2726	49.00	2602	63.05	2665	75.00	2570
38.00	2546	50.00	10147	64.10	494	75.95	228
39.05	1160	50.95	2998	65.00	605	76.85	17
39.85	81	51.95	228	67.00	181	77.10	110
42.90	65	53.00	65	68.00	5547	77.80	94
43.90	456	54.95	241	68.95	5266	78.90	2668
45.00	436	55.90	989	69.90	333	79.95	879
46.00	52	56.95	1910	70.10	186	80.95	2648
46.20	51	59.95	491	72.05	264	81.80	181
47.00	668	61.05	2720	73.00	2047	82.05	329

Average of 12.823 to 12.835 min.: VN088436.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.80	60	97.00	99	129.60	63	156.90	69
83.05	210	103.95	288	129.90	95	171.25	133
85.80	57	105.95	255	134.90	84	171.75	339
86.90	1861	115.70	111	136.90	80	172.05	316
88.00	1886	115.95	198	140.85	619	172.90	221
90.90	359	116.80	99	141.90	54	174.00	30165
91.95	1605	117.05	260	142.95	686	175.05	2492
93.00	2116	117.85	283	144.70	81	176.00	29056
94.05	5785	118.90	482	144.90	199	177.00	1867
95.00	42976	127.70	81	146.90	53		
96.00	3020	128.00	53	147.90	63		

Instrument :

MSVOA_N

ClientSampleId :

BFB