


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120625\
Data File : BN038286.D
Acq On : 05 Dec 2025 22:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 28 21:04:10 2025

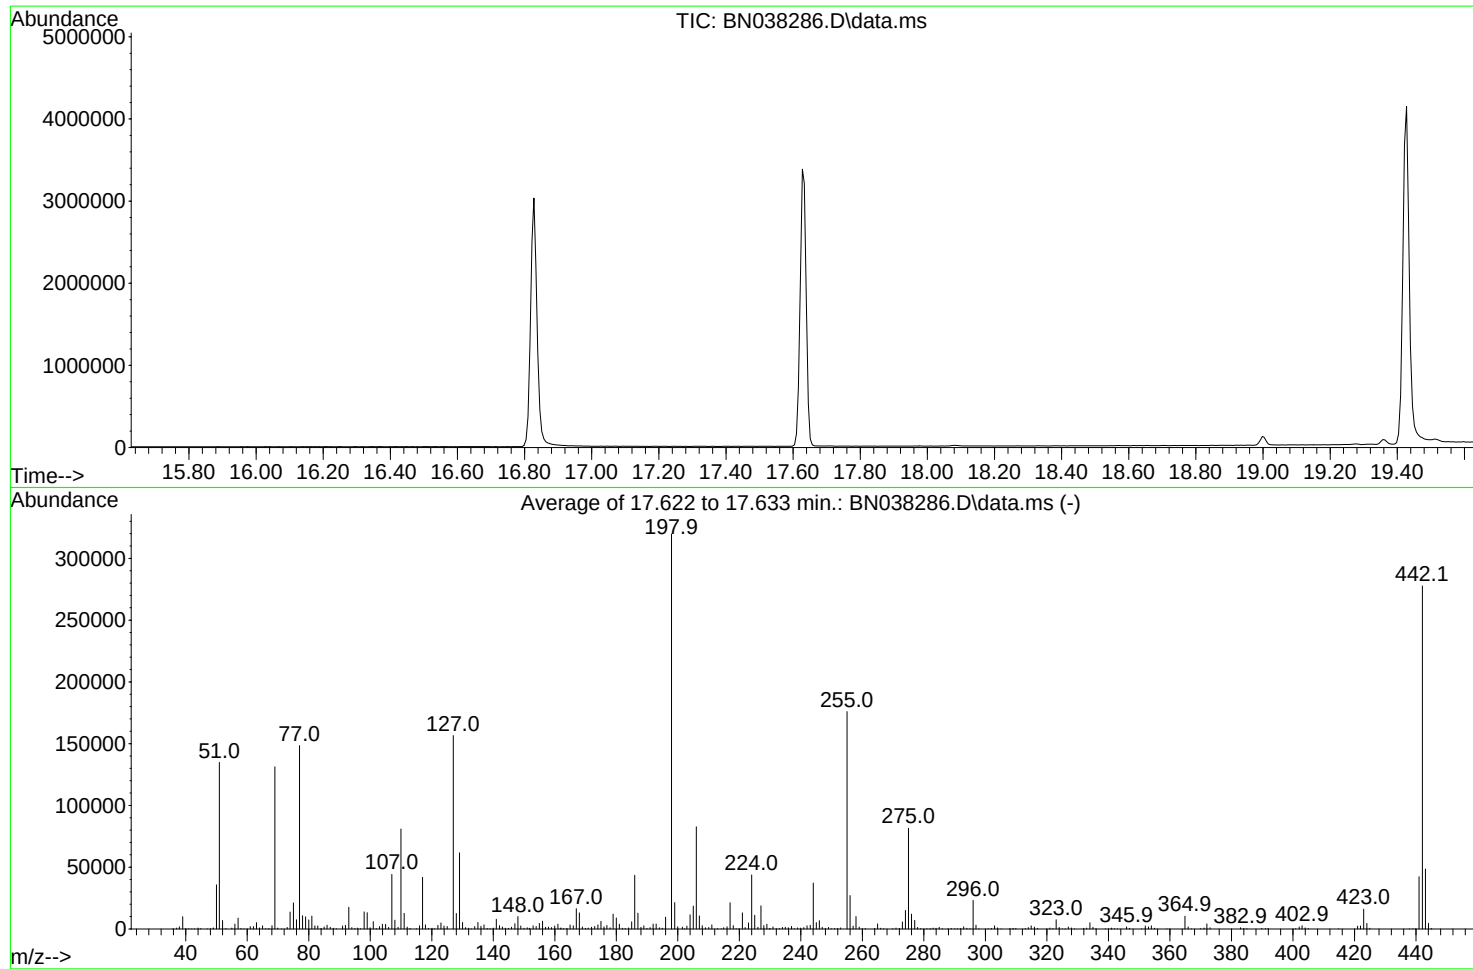




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	2623	PASS
69	69	100	100	100.0	131344	PASS
70	69	0.00	2	0.5	663	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	319659	PASS
199	198	5	9	6.7	21277	PASS
365	198	1	100	3.2	10356	PASS
441	443	0.01	150	87.1	42301	PASS
442	442	100	100	100.0	277739	PASS
443	442	15	24	17.5	48576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120625\
Data File : BN038286.D
Acq On : 05 Dec 2025 22:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 05 23:53:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 23:53:11 2025
Response via : Initial Calibration

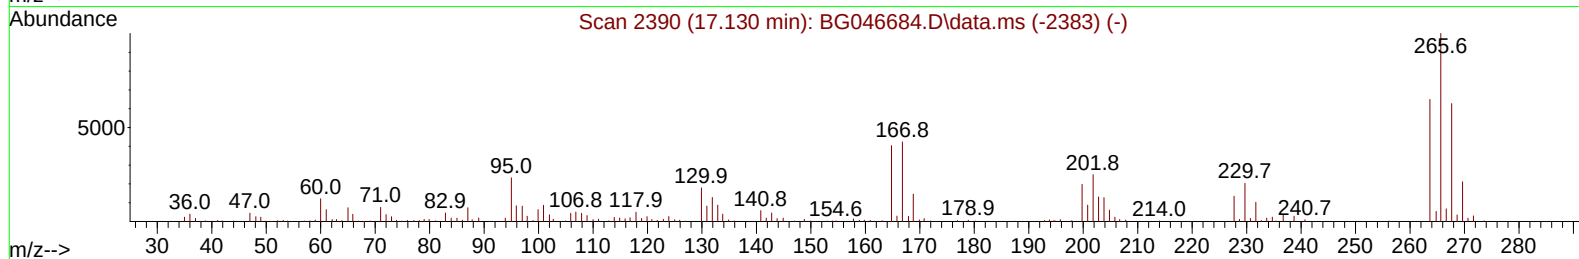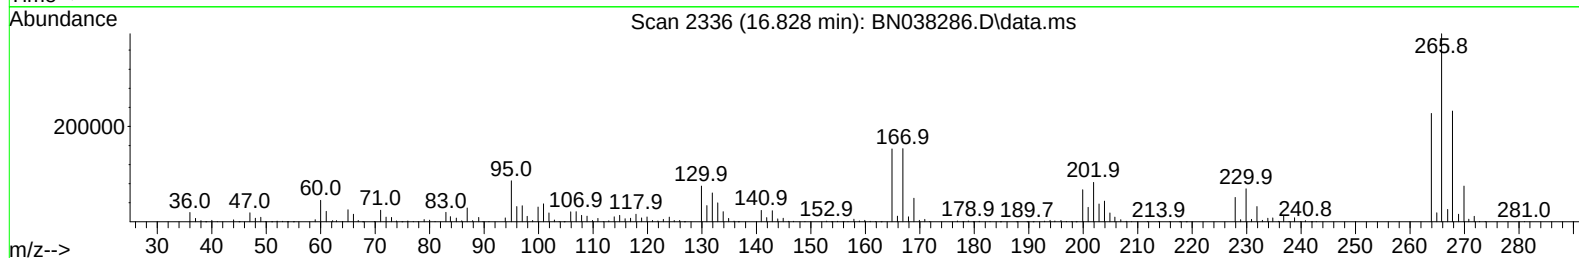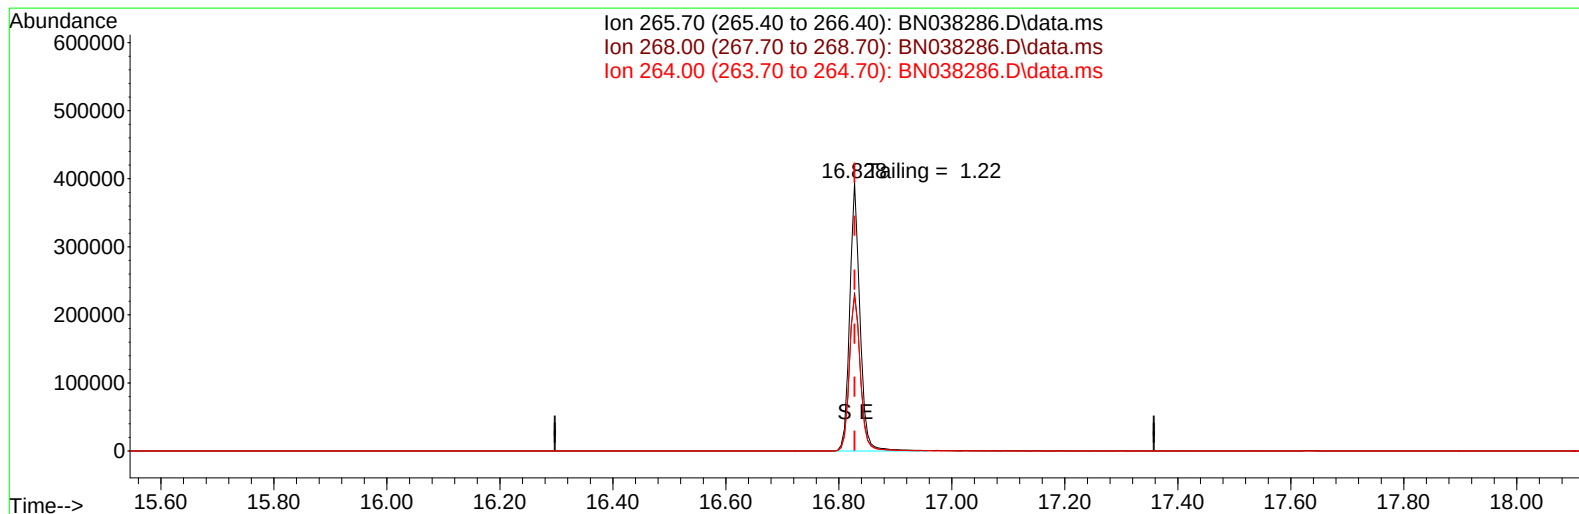

TIC: BN038286.D\data.ms

(70) Pentachlorophenol (C)

16.828min (0.000) 33987.82 ng




response 499848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.95
264.00	61.60	57.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120625\
Data File : BN038286.D
Acq On : 05 Dec 2025 22:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 05 23:53:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 23:53:11 2025
Response via : Initial Calibration

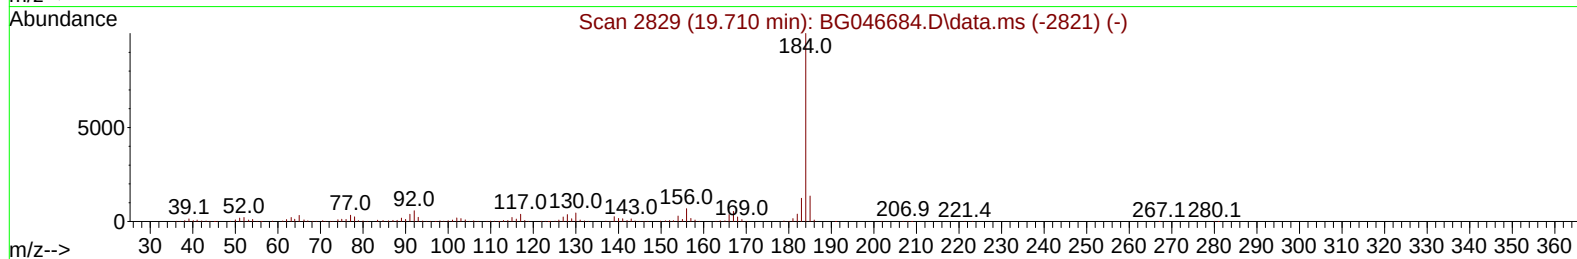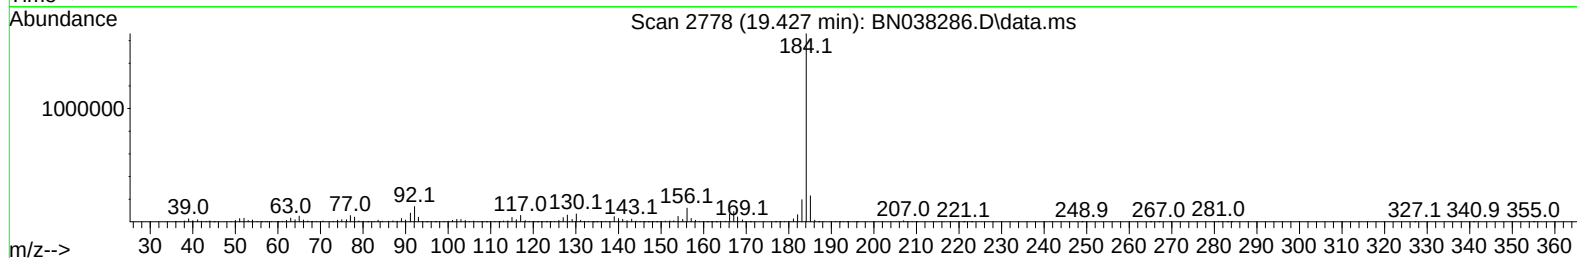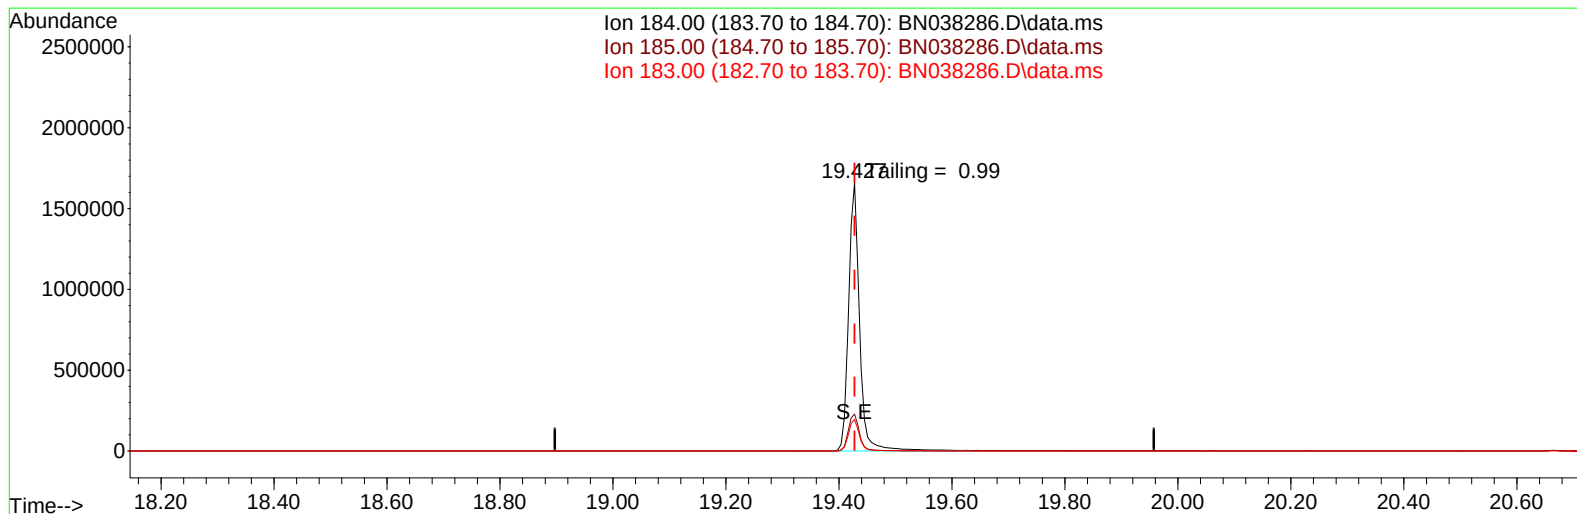

TIC: BN038286.D\data.ms

(77) Benzidine

19.427min (0.000) 0.00 ng

response 2256964

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.77
183.00	13.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2025	BNA_N	<u>BN038286.D</u>
Compound Name	Response	Retention Time
DDT	1037331	20.663
DDD	97794	20.222
DDE	3160	19.716
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
100954	1138285	8.87

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP