


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120525\
Data File : VN088462.D
Acq On : 05 Dec 2025 08:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N111325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 14 00:49:21 2025

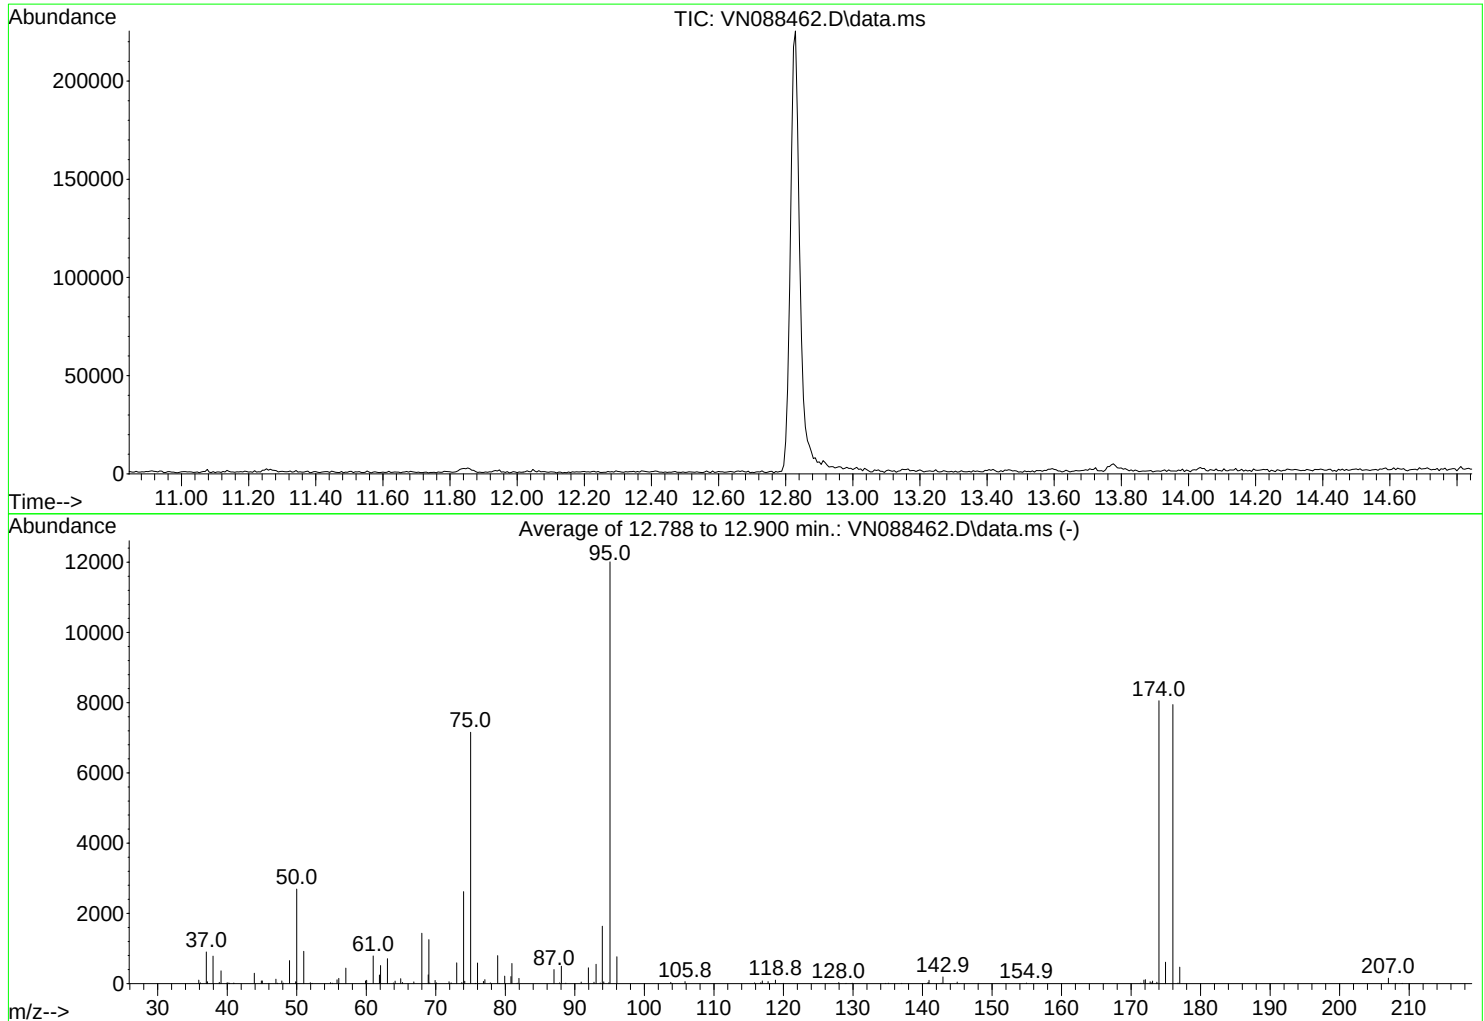

AutoFind: Averaged scan 1842 to 1861; Bkg corrected with scan 1841

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.4	2694	PASS
75	95	30	60	59.6	7156	PASS
95	95	100	100	100.0	12010	PASS
96	95	5	9	6.4	766	PASS
173	174	0.00	2	0.9	72	PASS
174	95	50	100	67.1	8054	PASS
175	174	5	9	7.6	612	PASS
176	174	95	101	98.6	7944	PASS
177	176	5	9	5.9	469	PASS