


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120825\
Data File : BP026249.D
Acq On : 08 Dec 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 05 14:52:44 2025

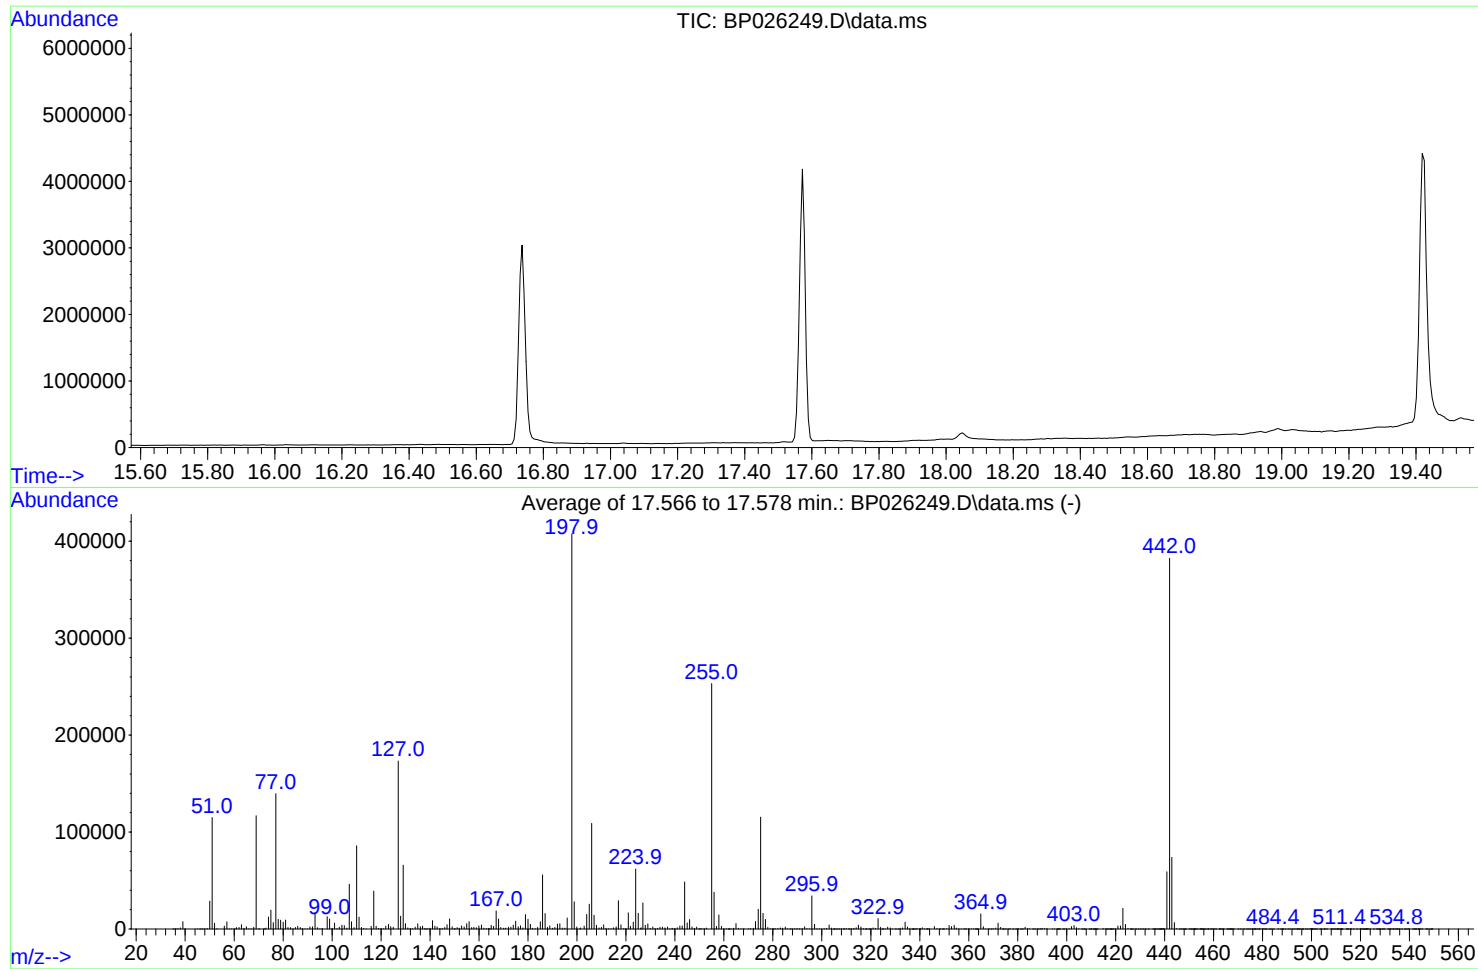

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	1878	PASS
69	69	100	100	100.0	116823	PASS
70	69	0.00	2	0.0	57	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	407264	PASS
199	198	5	9	6.9	28134	PASS
365	198	1	100	3.8	15601	PASS
441	443	0.01	150	79.8	59067	PASS
442	442	100	100	100.0	382412	PASS
443	442	15	24	19.4	74003	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/8/2025	BNA_P	<u>BP026249.D</u>
Compound Name	Response	Retention Time
DDT	1564189	20.725
DDD	32672	20.266
DDE	10232	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42904	1607093	2.67

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120825\
Data File : BP026249.D
Acq On : 08 Dec 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 08 13:36:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

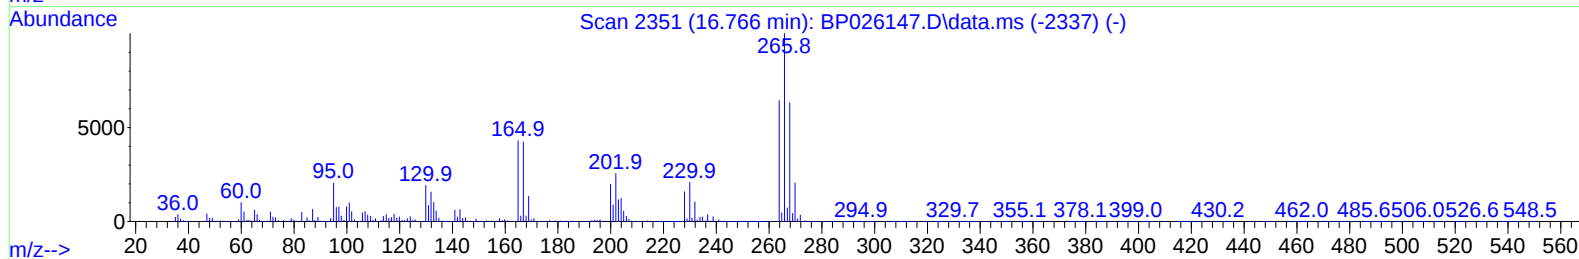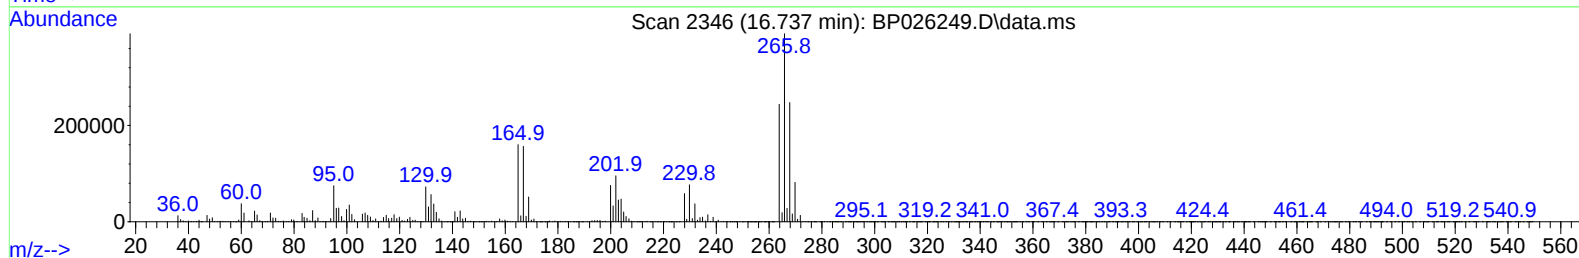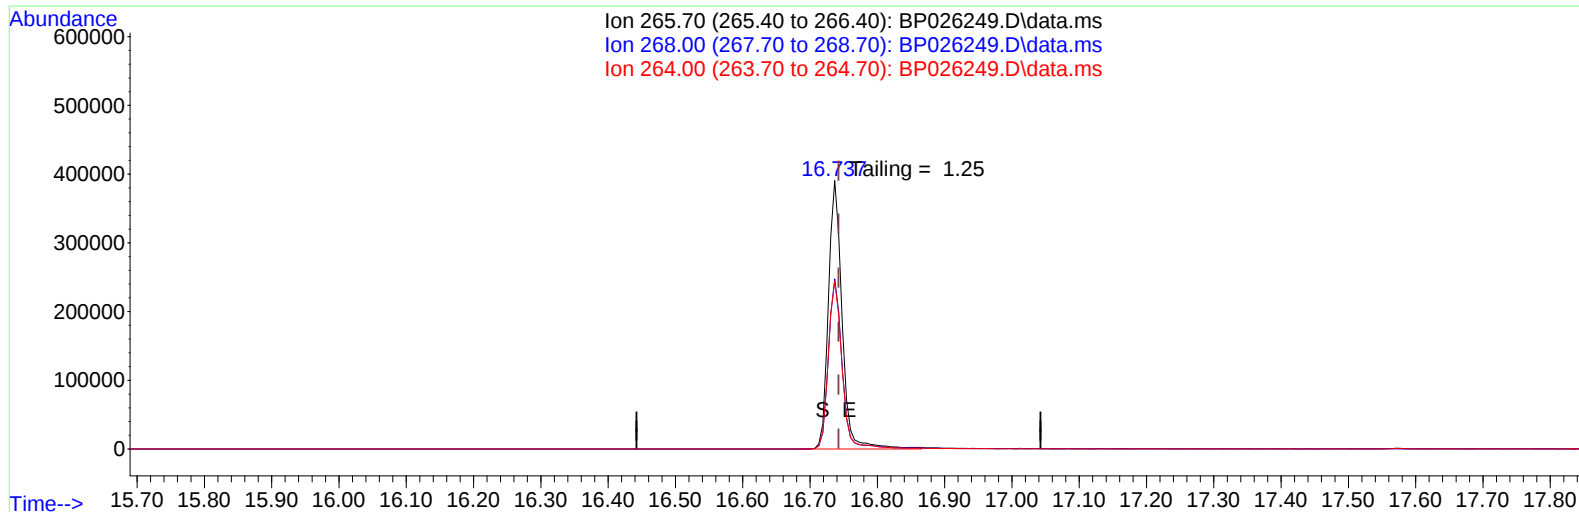

TIC: BP026249.D\data.ms

(70) Pentachlorophenol (C)

16.737min (-0.006) 52008.38 ng




response 550867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.39
264.00	62.70	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120825\
Data File : BP026249.D
Acq On : 08 Dec 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 08 13:36:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

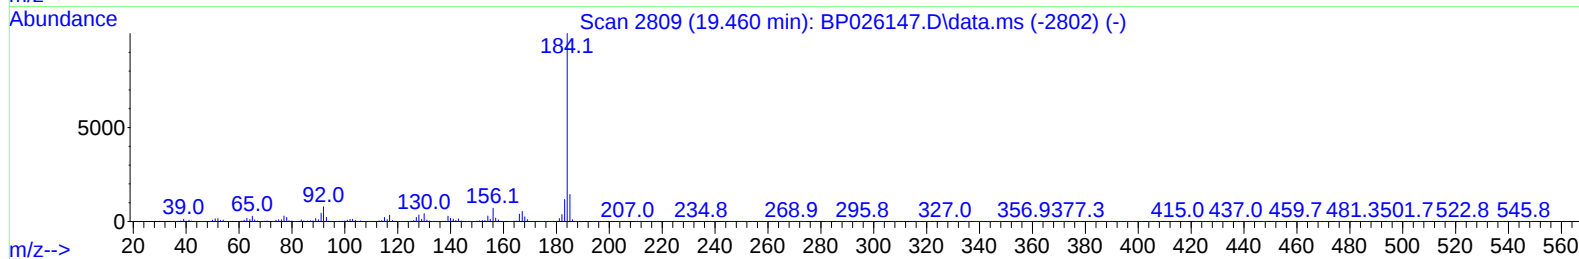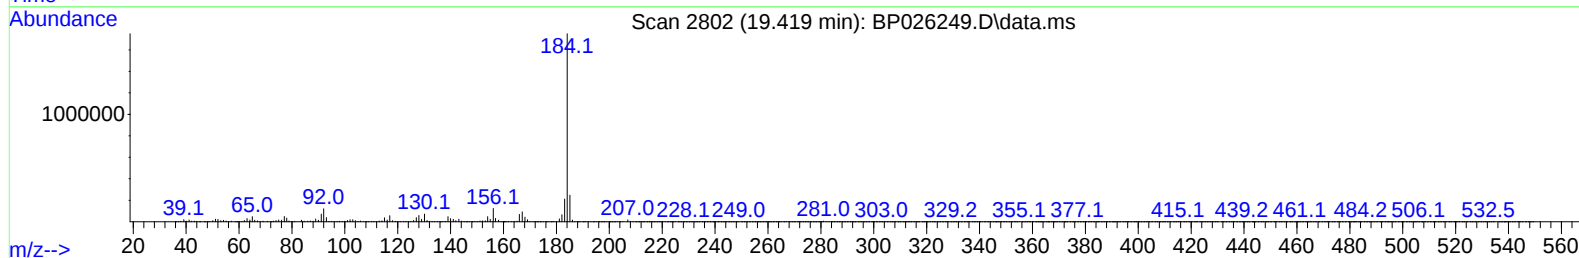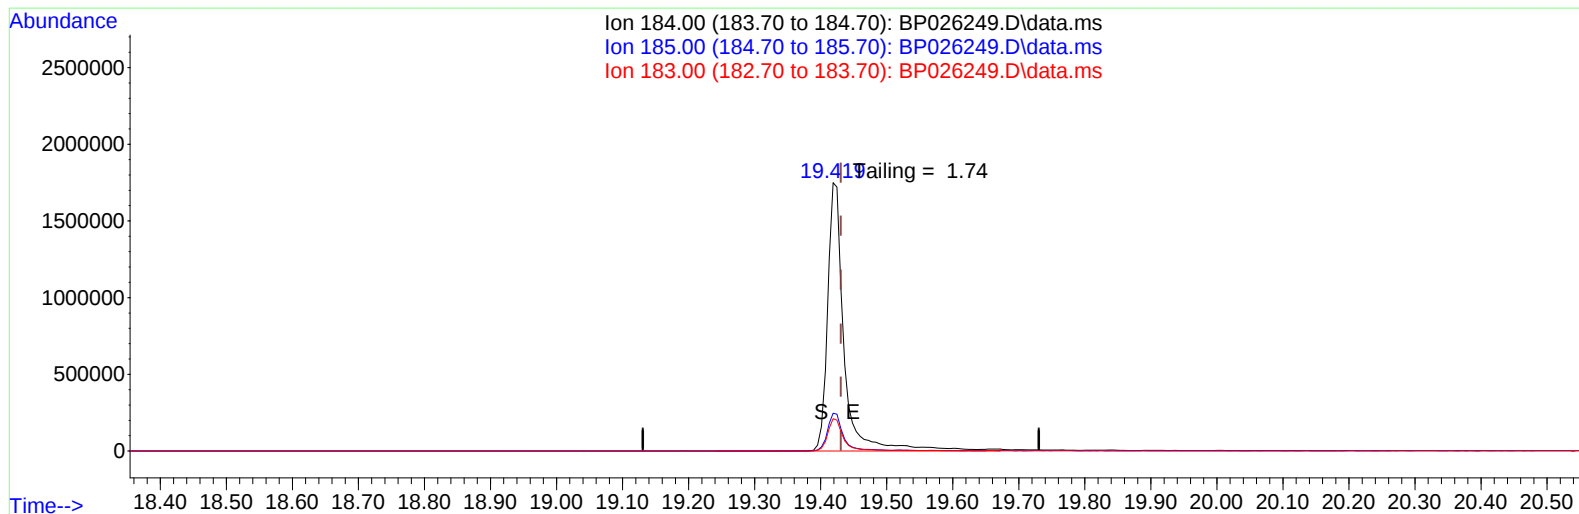

TIC: BP026249.D\data.ms

(77) Benzidine

19.419min (-0.012) 23636.55 ng

response 2964704

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.10
183.00	11.30	12.07
0.00	0.00	0.00