
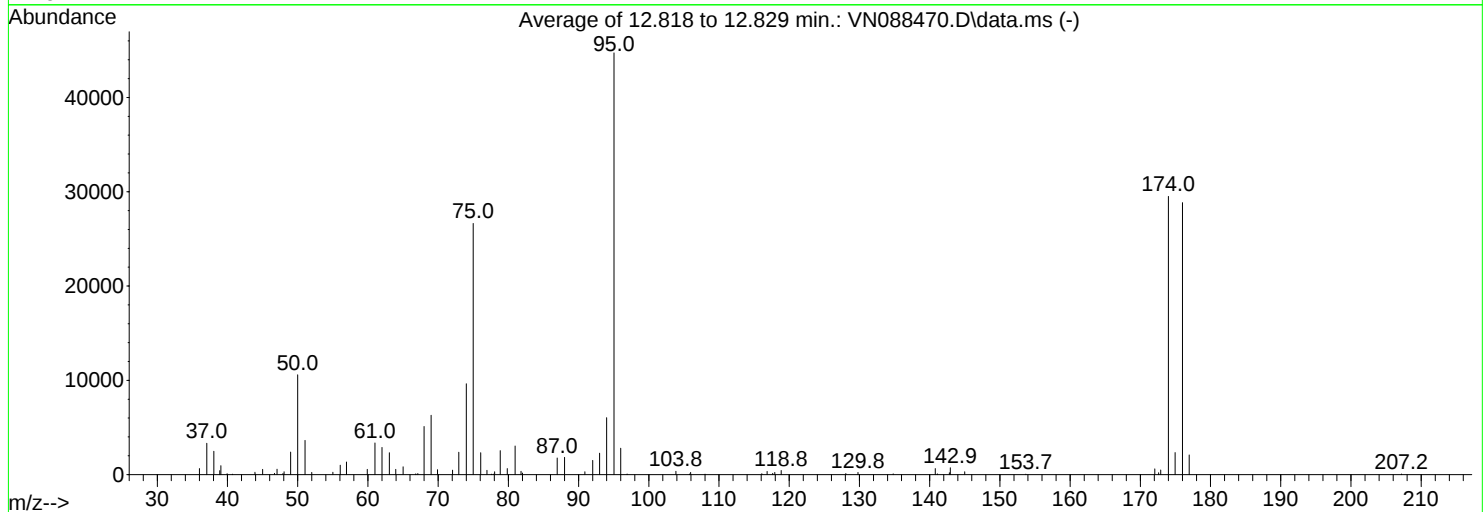


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120925\
Data File : VN088470.D
Acq On : 09 Dec 2025 10:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

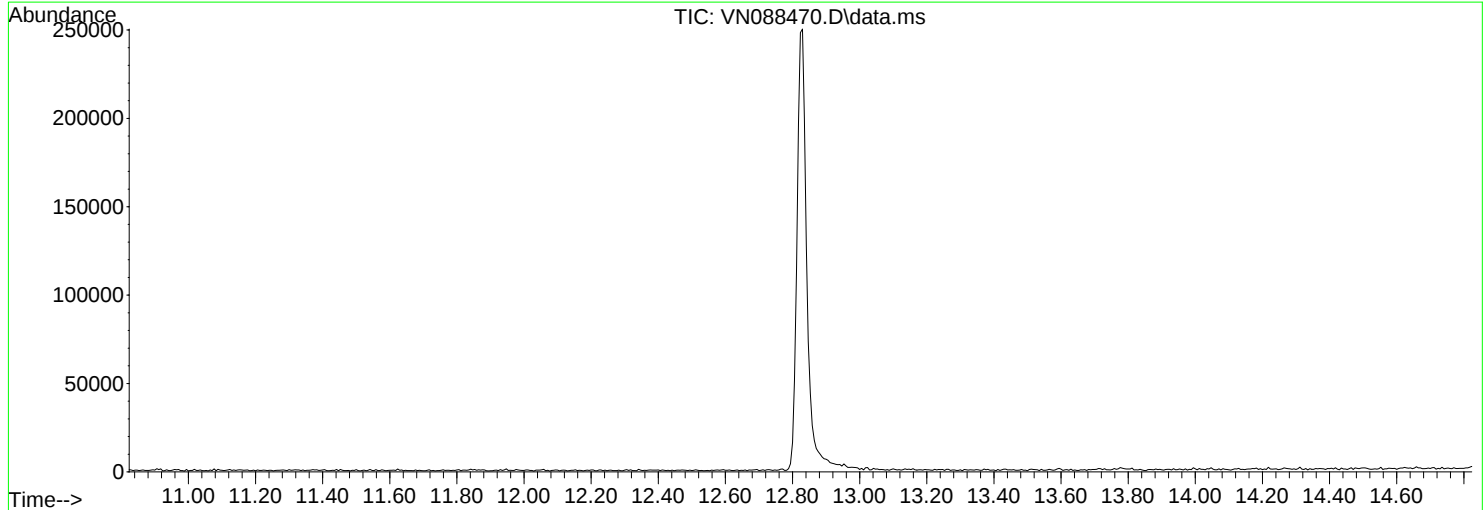

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	10596	PASS
75	95	30	60	59.6	26648	PASS
95	95	100	100	100.0	44731	PASS
96	95	5	9	6.3	2807	PASS
173	174	0.00	2	1.7	500	PASS
174	95	50	100	66.0	29515	PASS
175	174	5	9	7.9	2339	PASS
176	174	95	101	97.7	28840	PASS
177	176	5	9	7.2	2090	PASS

Average of 12.818 to 12.829 min.: VN088470.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	652	47.05	570	61.00	3358	72.95	2379
37.05	3334	47.90	115	62.00	2883	74.00	9631
38.05	2484	48.05	298	63.05	2321	75.00	2664
38.90	431	49.00	2388	63.95	561	76.05	2319
39.05	953	50.00	10596	65.00	836	76.95	460
39.95	94	51.05	3626	66.80	84	77.60	54
40.70	58	52.00	238	67.10	114	77.90	56
43.90	258	55.00	249	68.00	5116	78.05	299
44.00	44	56.05	1010	69.00	6297	78.85	2543
45.00	567	56.95	1342	69.90	534	79.85	653
46.70	129	59.90	553	72.05	476	80.95	3031

Average of 12.818 to 12.829 min.: VN088470.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	358	103.85	362	134.80	79	174.95	2339
82.00	173	105.80	74	140.80	650	176.00	28840
86.95	1761	105.95	237	141.10	85	176.95	2090
88.00	1833	108.00	51	142.80	198	207.20	75
90.90	302	116.10	104	142.95	722		
92.00	1517	116.85	348	145.00	299		
93.00	2270	117.65	143	153.70	50		
94.00	6037	117.95	246	172.05	607		
95.05	44731	118.85	447	172.60	206		
96.00	2807	128.05	120	172.90	500		
96.90	62	129.80	236	174.00	29515		