




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
Data File : VV039511.D
Acq On : 09 Dec 2025 17:48
Operator : SY/MD
Sample : Q3787-18
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 10 01:18:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

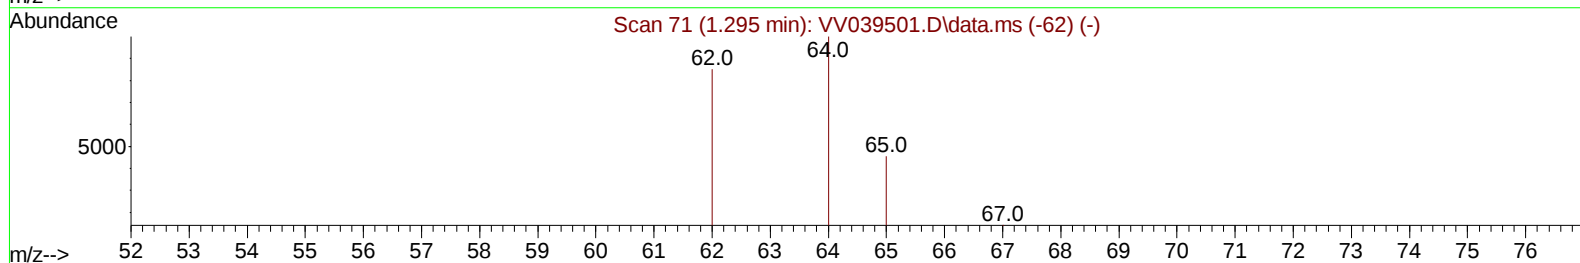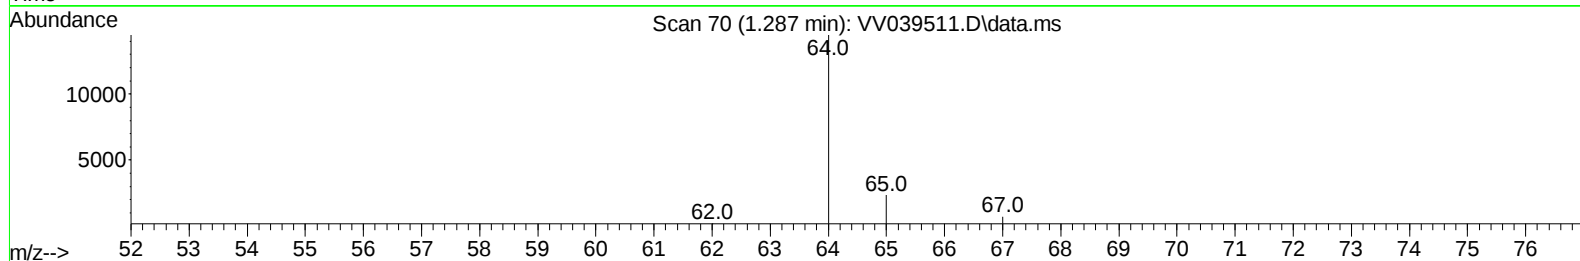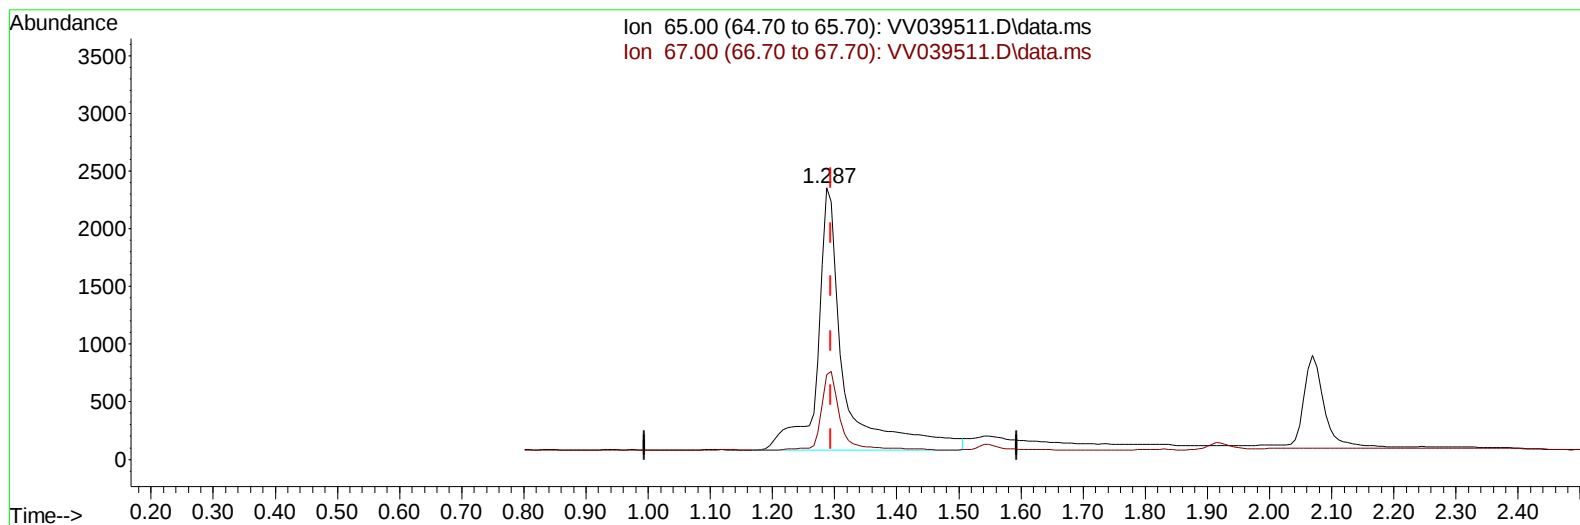

TIC: VV039511.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.287min (-0.007) 0.94 ug/L

response 6666

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	21.27#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
Data File : VV039511.D
Acq On : 09 Dec 2025 17:48
Operator : SY/MD
Sample : Q3787-18
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 10 01:18:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

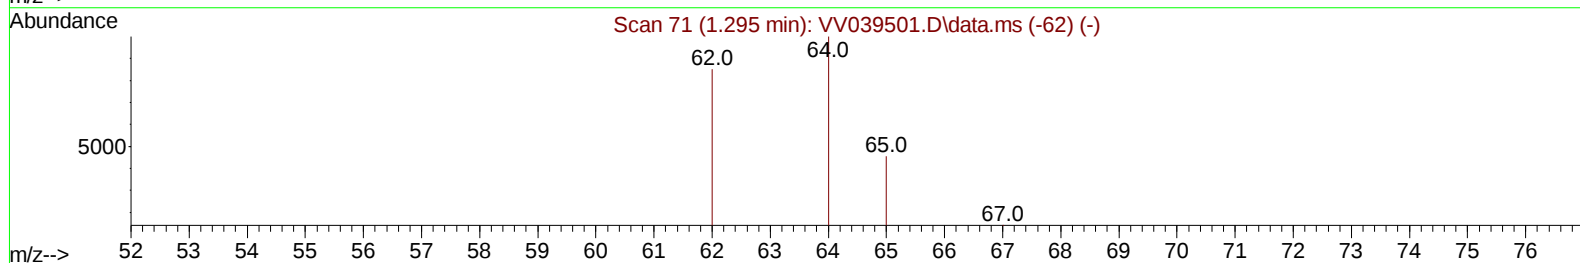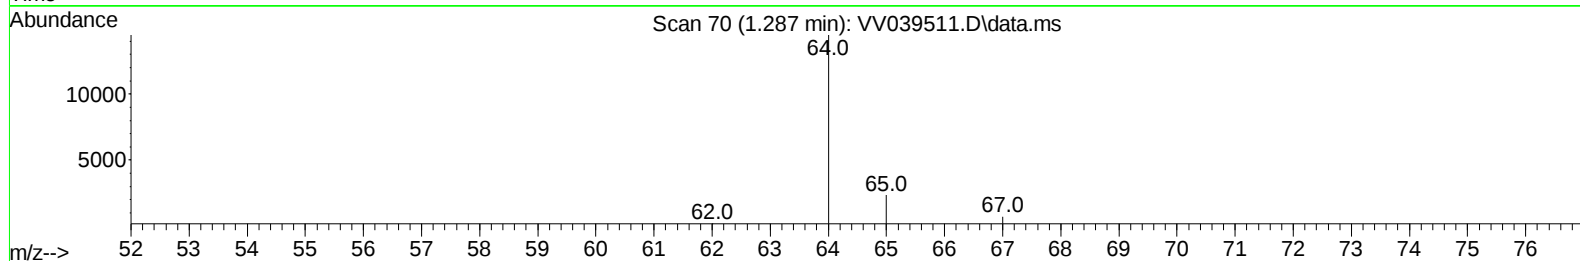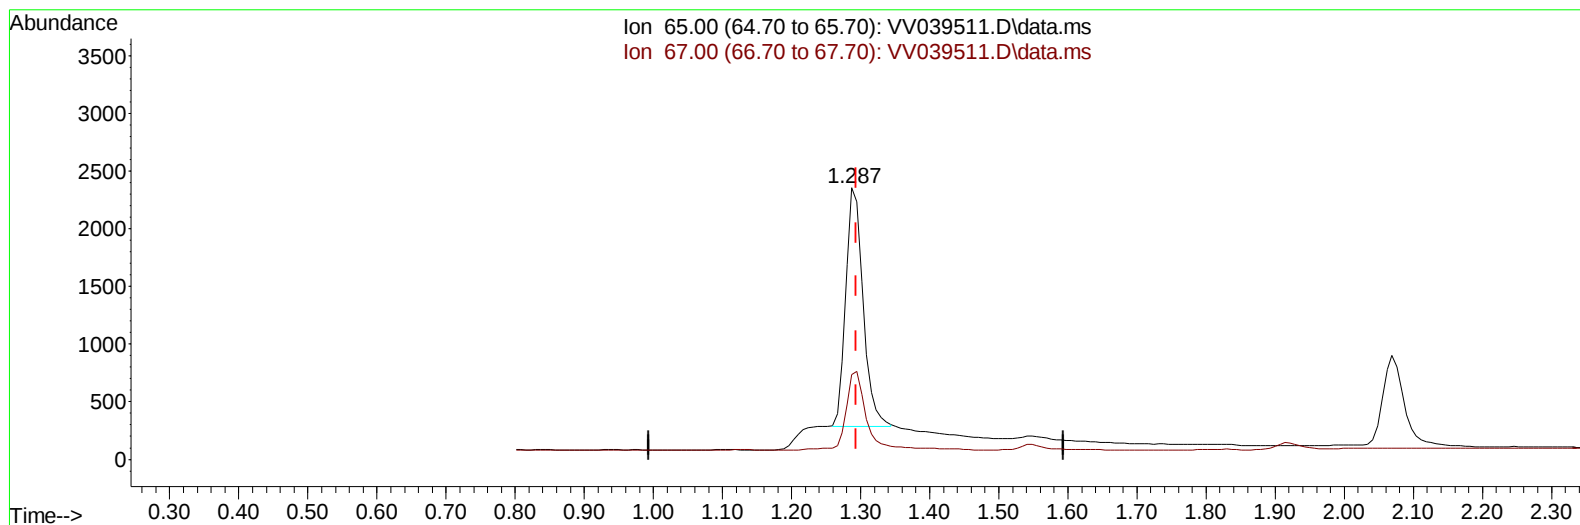

TIC: VV039511.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.287min (-0.007) 0.51 ug/L m

response 3606

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	39.32
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
 Data File : VV039511.D
 Acq On : 09 Dec 2025 17:48
 Operator : SY/MD
 Sample : Q3787-18
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-120425-SIM-FD

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 10 01:18:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7201	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	6889	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.197	152	3685	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	3606m	0.510	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	102.000%		
4) 1,2-Dichloroethane-d4	4.993	65	1983	0.414	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	82.000%		
7) 1,2-Dichloropropane-d6	5.996	67	2352	0.405	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	80.000%		
8) Toluene-d8	7.254	98	4431	0.452	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1617	0.494	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
Data File : VV039511.D
Acq On : 09 Dec 2025 17:48
Operator : SY/MD
Sample : Q3787-18
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 10 01:18:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

