

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
 Data File : VV039510.D
 Acq On : 09 Dec 2025 17:27
 Operator : SY/MD
 Sample : Q3787-16
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-120425-SIM

Quant Time: Dec 10 01:17:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/10/2025
 Supervised By : Mahesh Dadoda 12/10/2025

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)

Internal Standards					
1) 1,4-Difluorobenzene	5.566	114	6729	0.500 ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6569	0.500 ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	3453	0.500 ug/L	0.02

System Monitoring Compounds

2) Vinyl Chloride-d3	1.294	65	3797m	0.575 ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 114.000%
4) 1,2-Dichloroethane-d4	4.993	65	1999	0.446 ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	= 90.000%
7) 1,2-Dichloropropane-d6	5.996	67	2347	0.423 ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	= 84.000%
8) Toluene-d8	7.254	98	4406	0.471 ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	= 94.000%
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1655	0.530 ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 106.000%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
Data File : VV039510.D
Acq On : 09 Dec 2025 17:27
Operator : SY/MD
Sample : Q3787-16
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM

Quant Time: Dec 10 01:17:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 12/10/2025
Supervised By : Mahesh Dadoda 12/10/2025

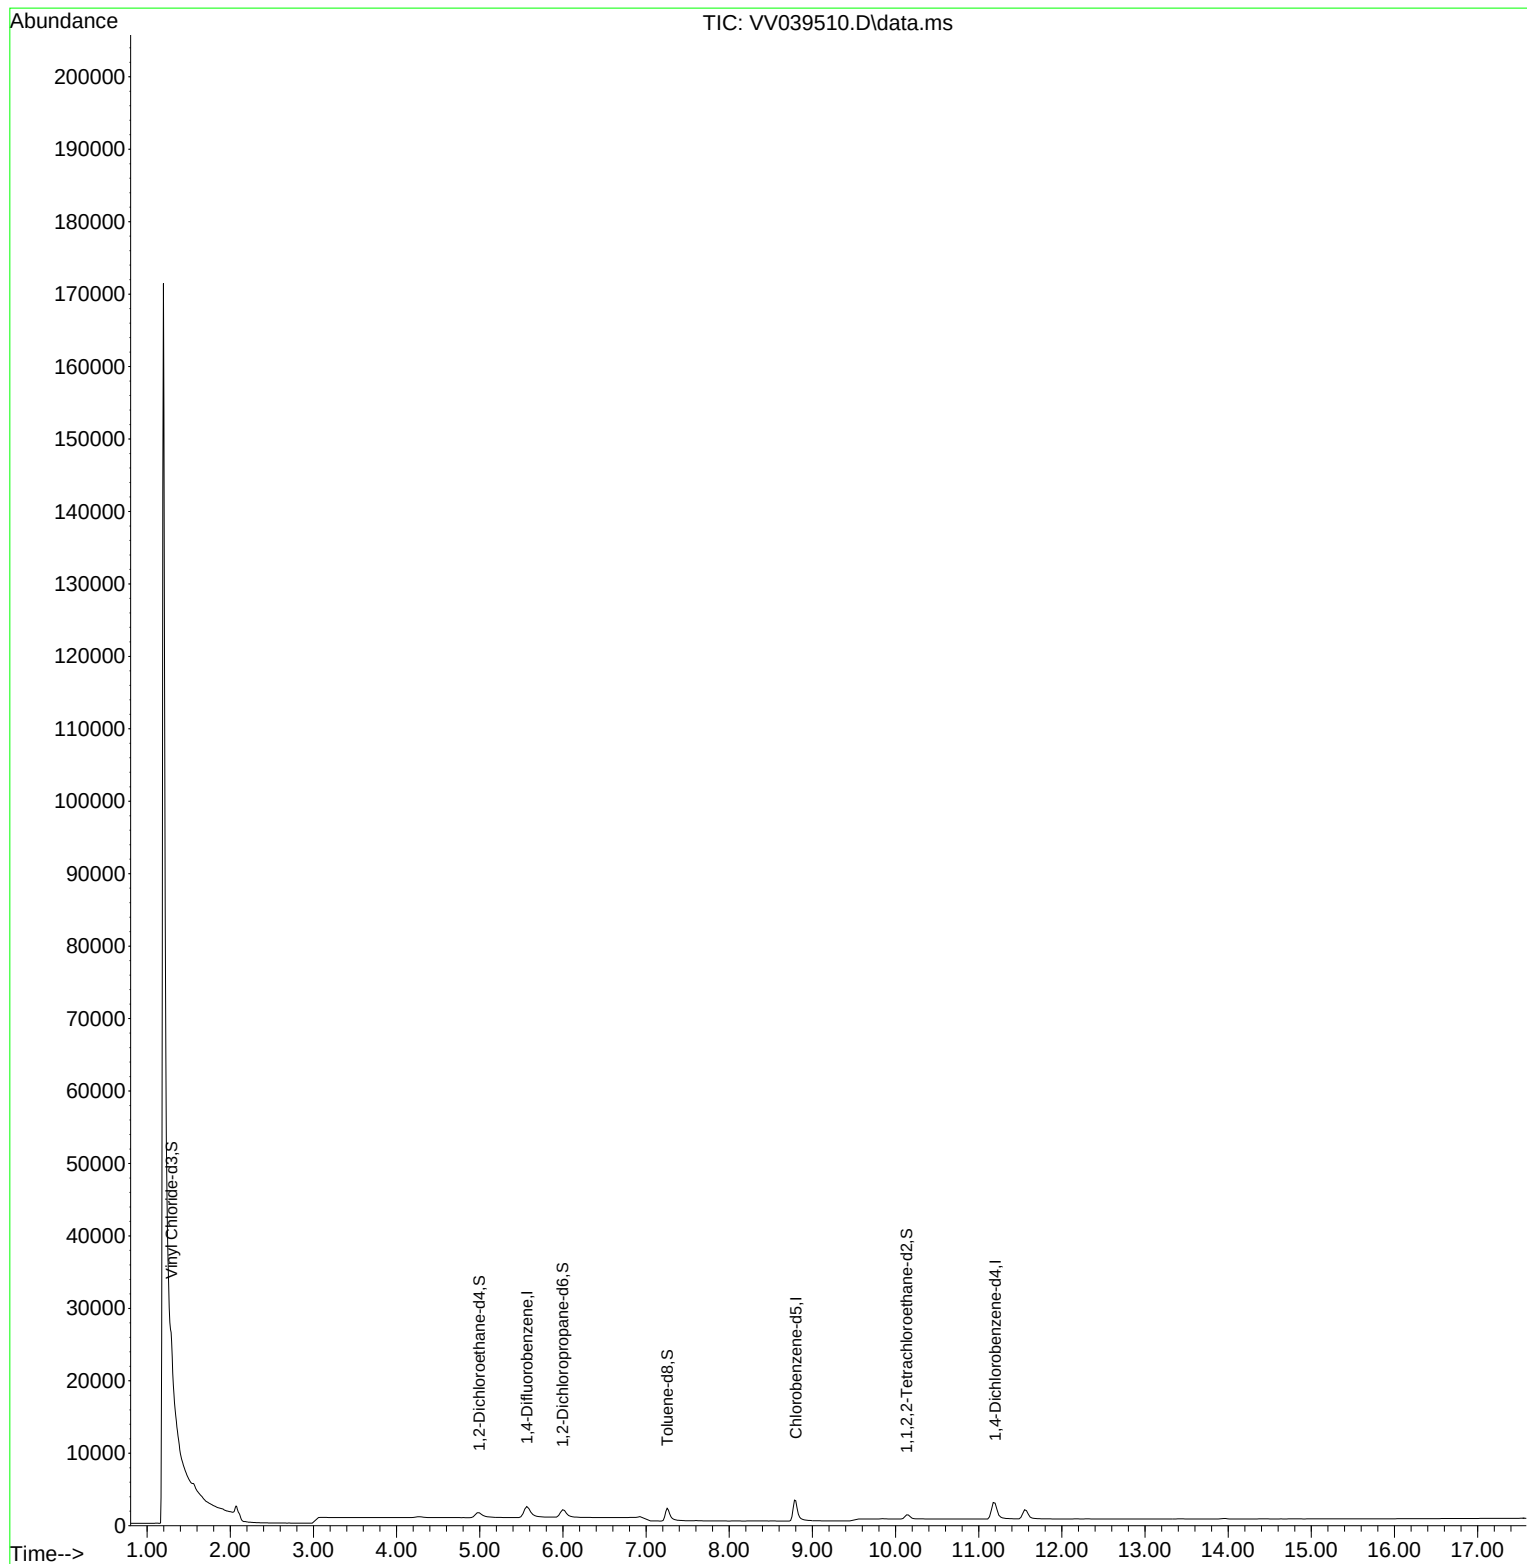

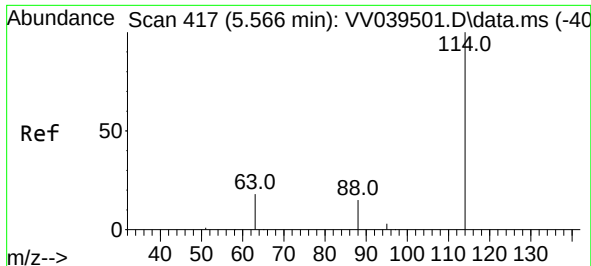

#1
1,4-Difluorobenzene
Concen: 0.500 ug/L
RT: 5.566 min Scan# 417
Delta R.T. 0.000 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27




Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM

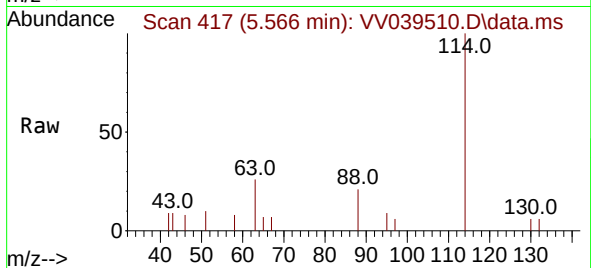

Tgt Ion:114 Resp: 6729
Ion Ratio Lower Upper
114 100
63 19.9 15.0 22.4
88 15.8 12.0 18.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

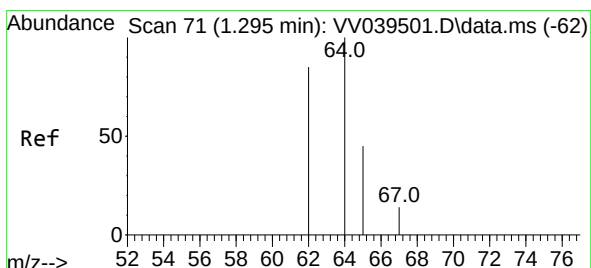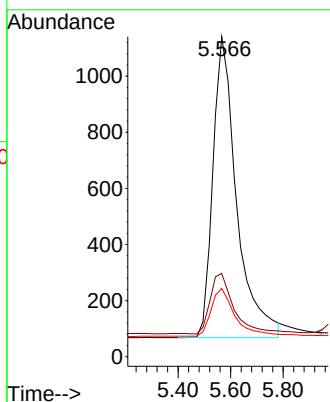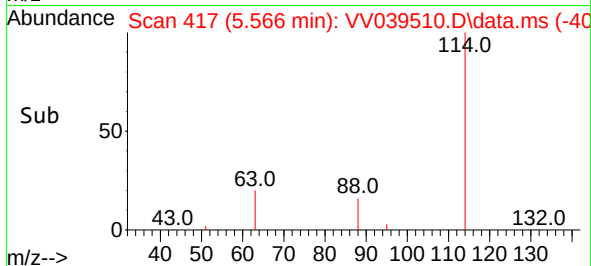

#2
Vinyl Chloride-d3
Concen: 0.575 ug/L m
RT: 1.294 min Scan# 71
Delta R.T. 0.000 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27


Tgt Ion: 65 Resp: 3797
Ion Ratio Lower Upper
65 100
67 33.3 22.3 41.5

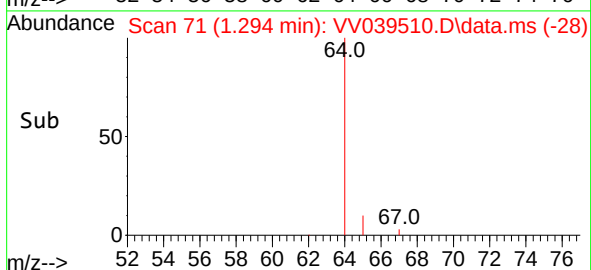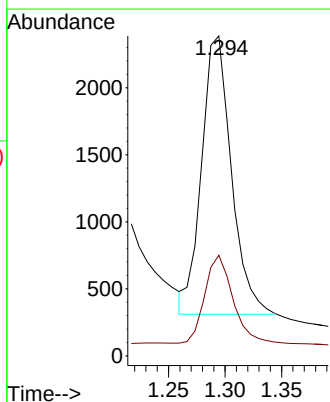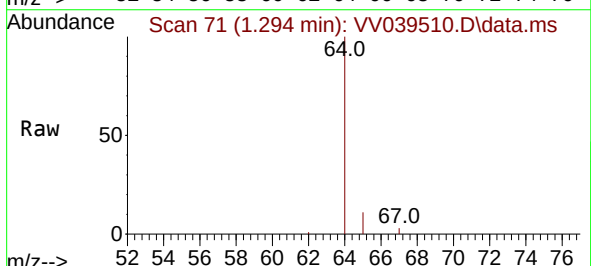

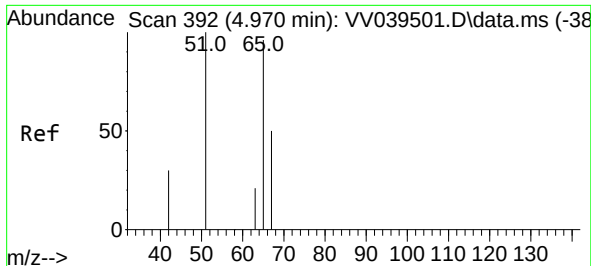

#4
1,2-Dichloroethane-d4
Concen: 0.446 ug/L
RT: 4.993 min Scan# 392
Delta R.T. 0.024 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27




Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM

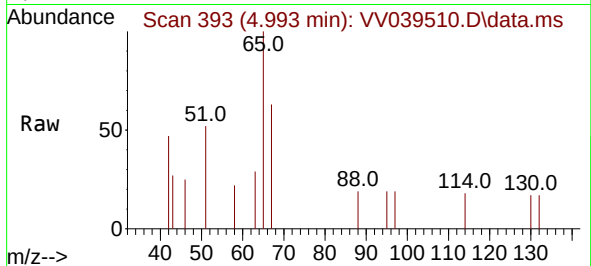

Tgt Ion: 65 Resp: 199
Ion Ratio Lower Upper
65 100
67 54.1 32.5 60.3
51 39.7 121.4 225.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

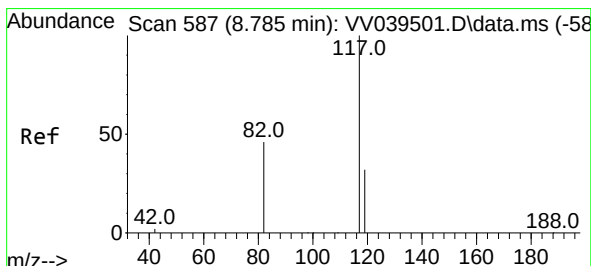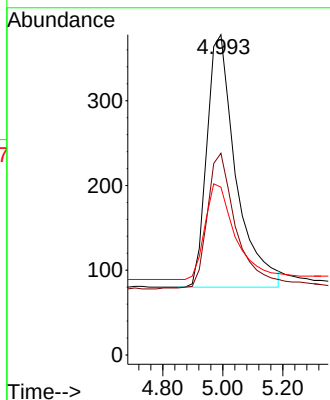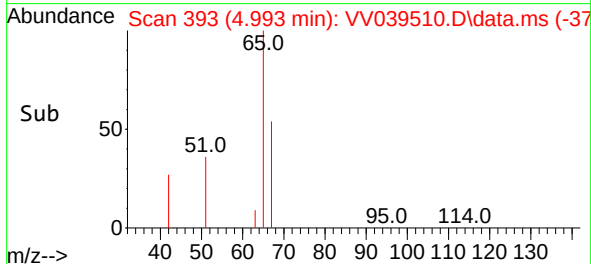

#5
Chlorobenzene-d5
Concen: 0.500 ug/L
RT: 8.800 min Scan# 588
Delta R.T. 0.015 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27


Tgt Ion:117 Resp: 6569
Ion Ratio Lower Upper
117 100
82 48.0 39.4 59.2
119 32.5 26.2 39.2

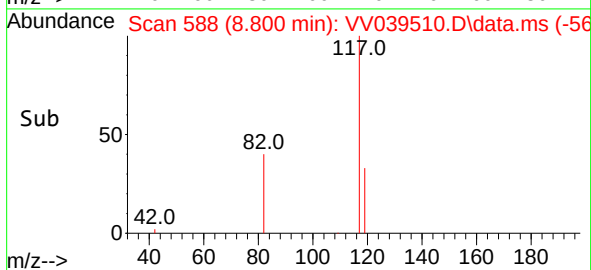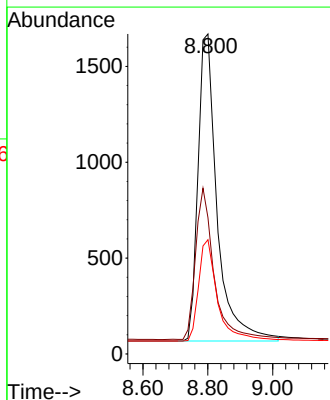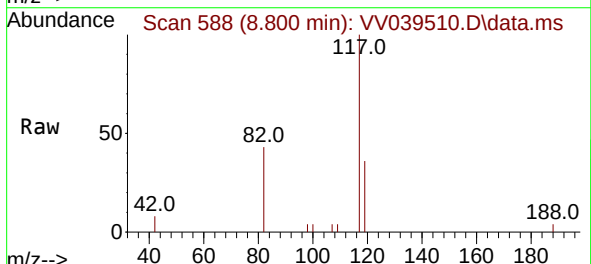

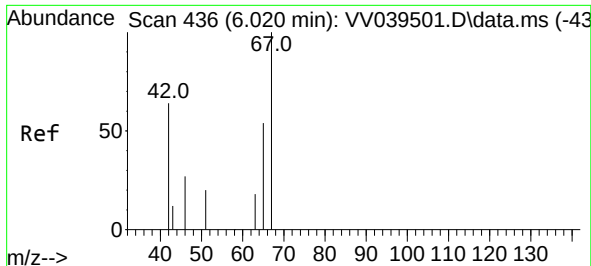

#7
1,2-Dichloropropane-d6
Concen: 0.423 ug/L
RT: 5.996 min Scan# 41
Delta R.T. -0.023 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27




Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM

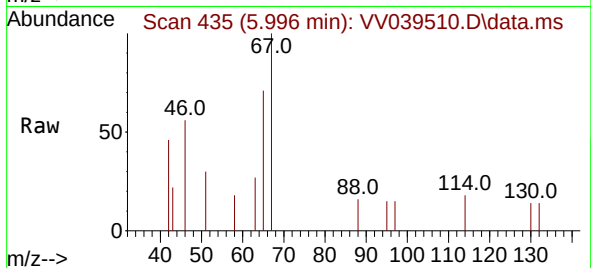

Tgt Ion:	67	Resp:	234
Ion	Ratio	Lower	Upper
67	100		
65	64.0	37.9	56.9
46	43.8	27.4	41.0
42	30.9	51.2	76.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

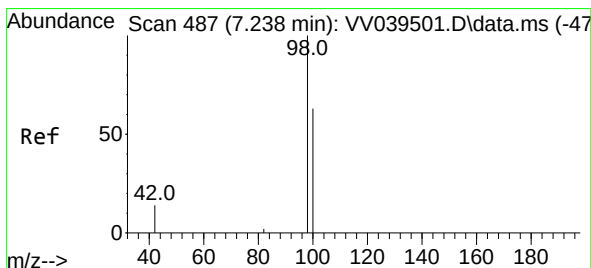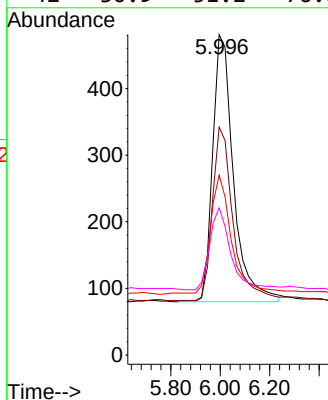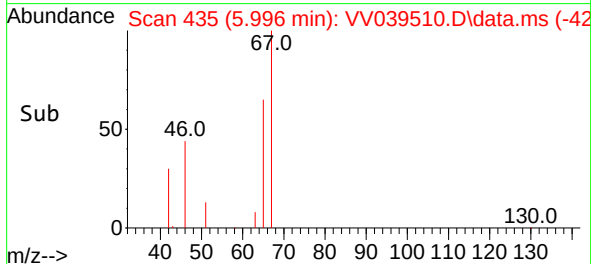

#8
Toluene-d8
Concen: 0.471 ug/L
RT: 7.254 min Scan# 488
Delta R.T. 0.016 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27

Tgt Ion:	98	Resp:	4406
Ion	Ratio	Lower	Upper
98	100		
100	62.3	44.5	82.7
42	10.7	10.1	18.7

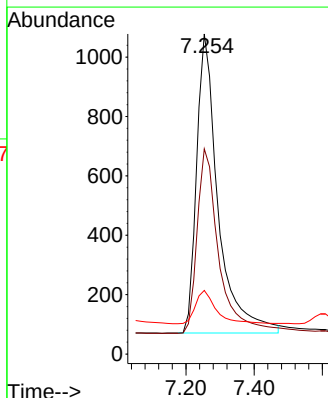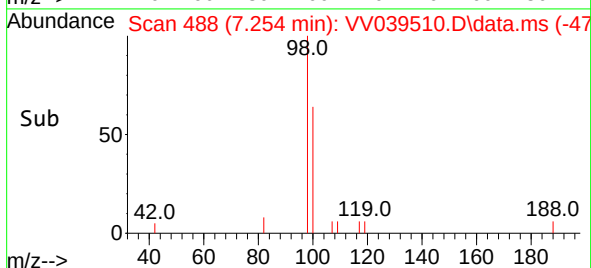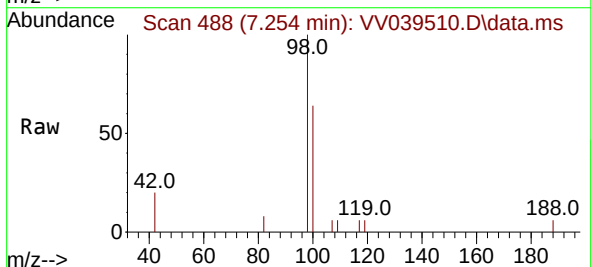

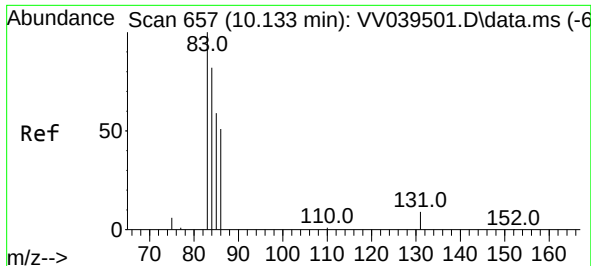





#10
1,1,2,2-Tetrachloroethane-d2
Concen: 0.530 ug/L
RT: 10.133 min Scan# 610
Delta R.T. -0.000 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM

Tgt Ion: 84 Resp: 165
Ion Ratio Lower Upper
84 100
86 62.2 44.4 82.5

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

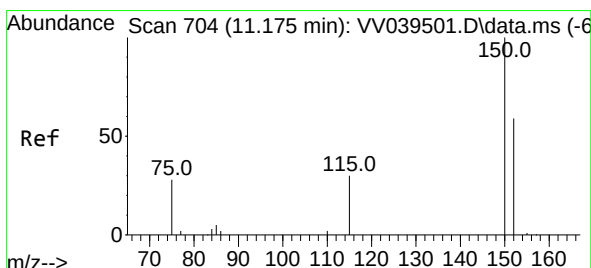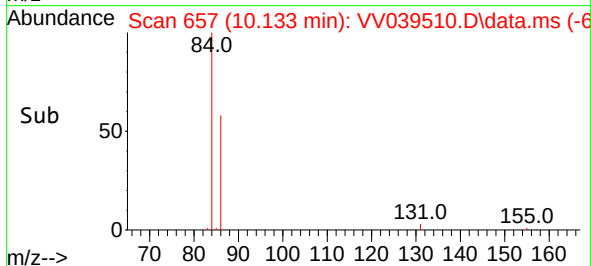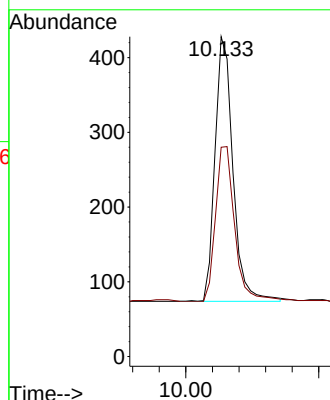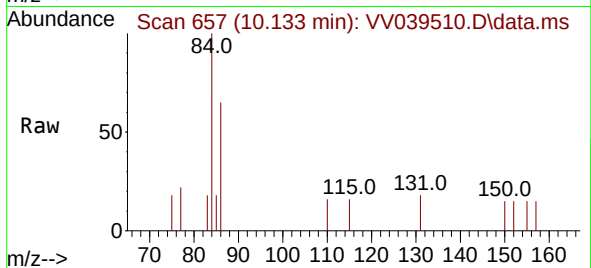

#12
1,4-Dichlorobenzene-d4
Concen: 0.500 ug/L
RT: 11.197 min Scan# 705
Delta R.T. 0.022 min
Lab File: VV039510.D
Acq: 09 Dec 2025 17:27

Tgt Ion:152 Resp: 3453
Ion Ratio Lower Upper
152 100
115 54.3 0.0 101.6
150 159.6 0.0 396.2

