

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
 Data File : VV039511.D
 Acq On : 09 Dec 2025 17:48
 Operator : SY/MD
 Sample : Q3787-18
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-120425-SIM-FD

Quant Time: Dec 10 01:18:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7201	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	6889	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.197	152	3685	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	6666	0.943	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	188.000%#
4) 1,2-Dichloroethane-d4	4.993	65	1983	0.414	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	82.000%
7) 1,2-Dichloropropane-d6	5.996	67	2352	0.405	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	80.000%
8) Toluene-d8	7.254	98	4431	0.452	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	90.000%
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1617	0.494	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	98.000%
Target Compounds						
						Qvalue
11) 1,1,2,2-Tetrachloroethane	9.556	83	384	0.056	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120925\
Data File : VV039511.D
Acq On : 09 Dec 2025 17:48
Operator : SY/MD
Sample : Q3787-18
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD

Quant Time: Dec 10 01:18:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration




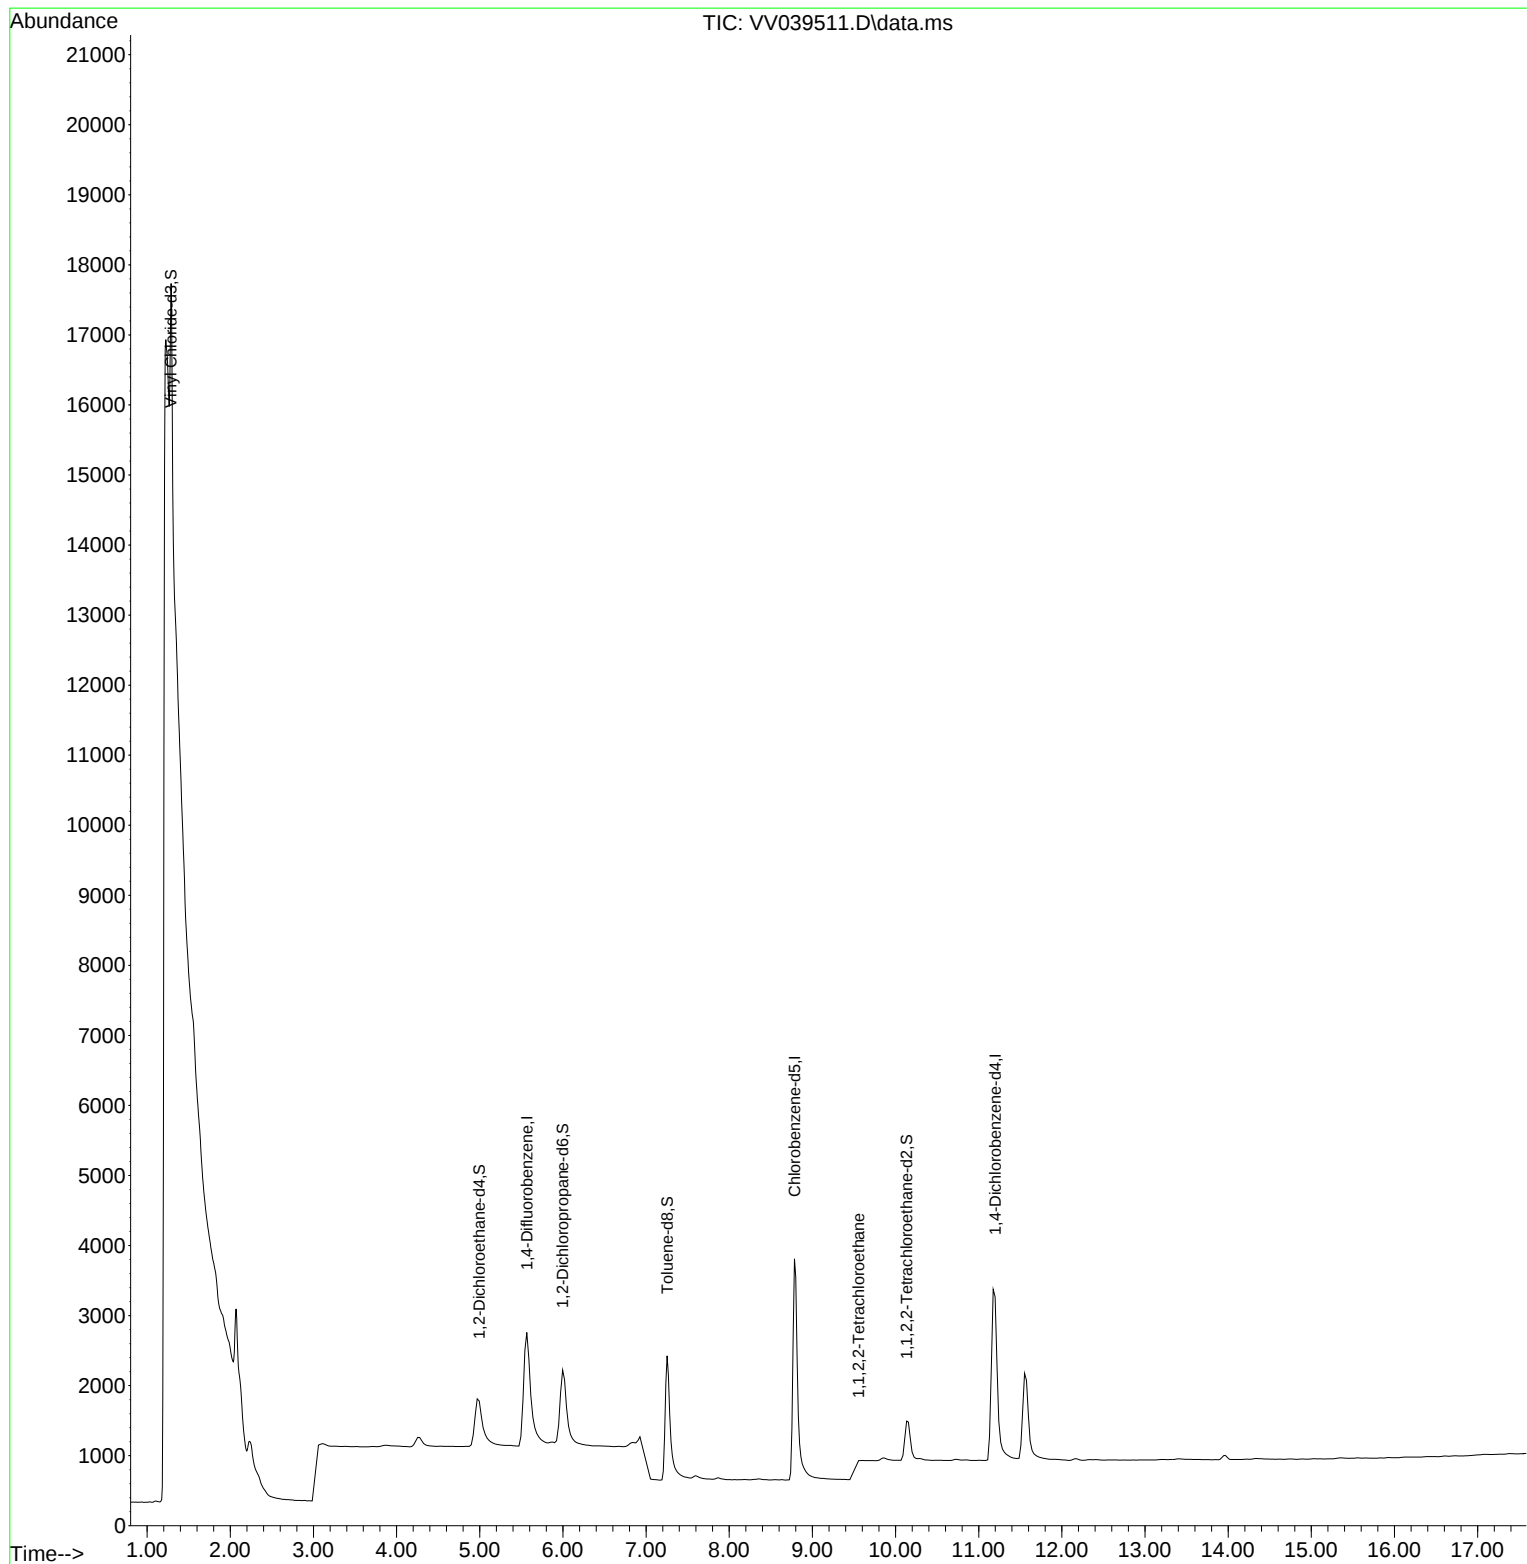


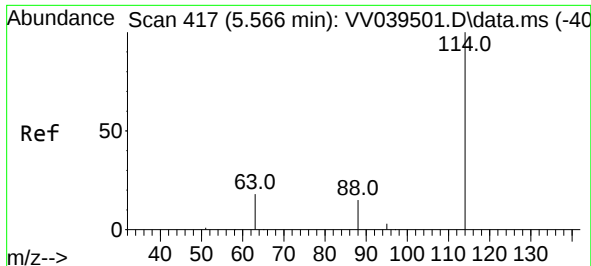

#1
 1,4-Difluorobenzene
 Concen: 0.500 ug/L
 RT: 5.566 min Scan# 417
 Delta R.T. 0.000 min
 Lab File: VV039511.D
 Acq: 09 Dec 2025 17:48




Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-120425-SIM-FD


Tgt Ion:	114	Resp:	7201
Ion	Ratio	Lower	Upper
114	100		
63	19.3	15.0	22.4
88	15.8	12.0	18.0

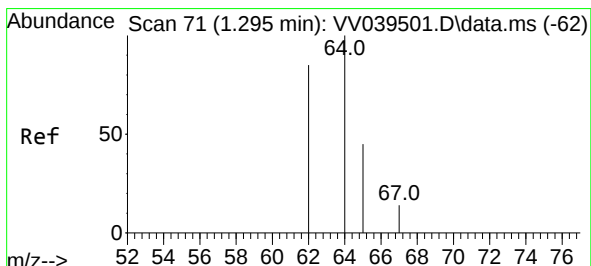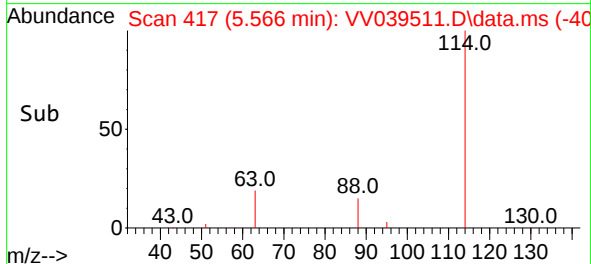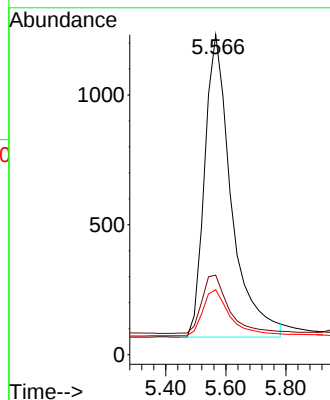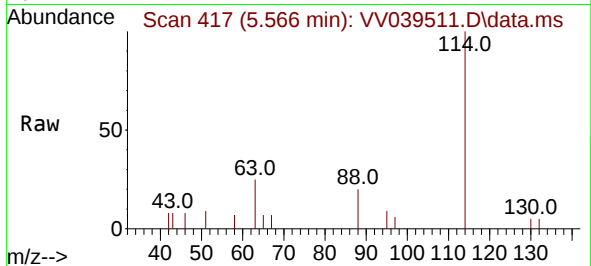

#2
 Vinyl Chloride-d3
 Concen: 0.943 ug/L
 RT: 1.287 min Scan# 70
 Delta R.T. -0.007 min
 Lab File: VV039511.D
 Acq: 09 Dec 2025 17:48

Tgt Ion:	65	Resp:	6666
Ion	Ratio	Lower	Upper
65	100		
67	21.3	22.3	41.5


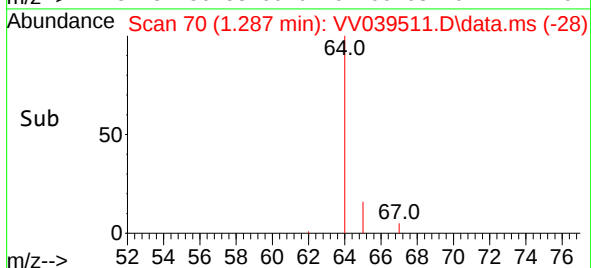
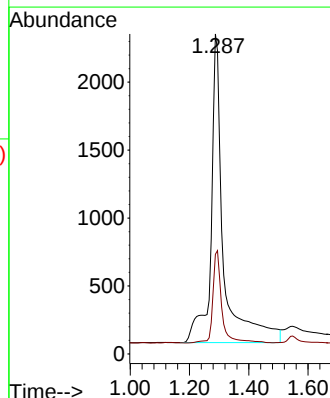
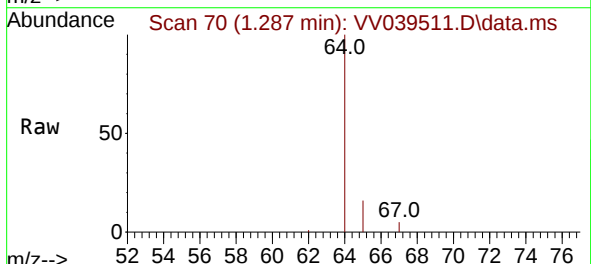


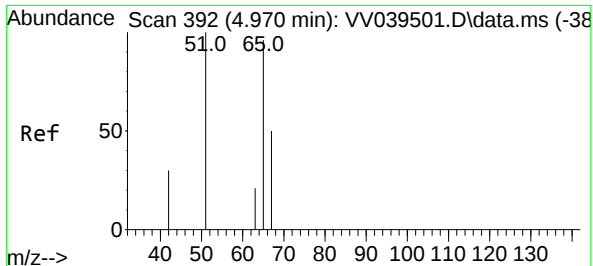

#4
1,2-Dichloroethane-d4
Concen: 0.414 ug/L
RT: 4.993 min Scan# 392
Delta R.T. 0.024 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48




Instrument : MSVOA_V
ClientSampleId : OW-08B-72.5-120425-SIM-FD


Tgt Ion: 65 Resp: 1983
Ion Ratio Lower Upper
65 100
67 51.8 32.5 60.3
51 40.7 121.4 225.6#

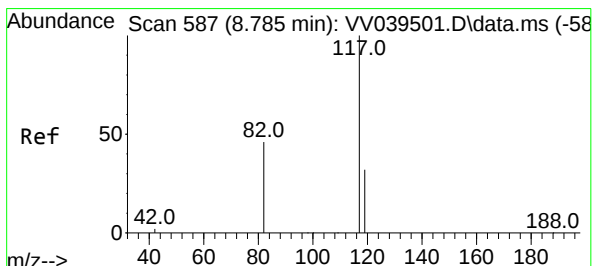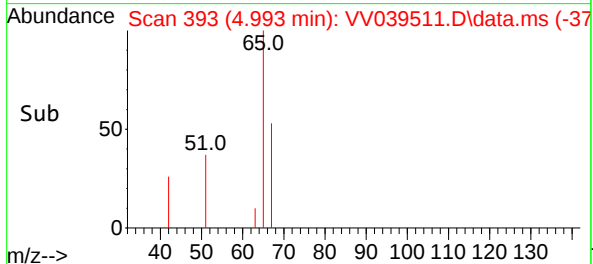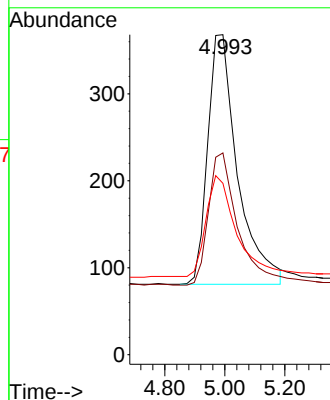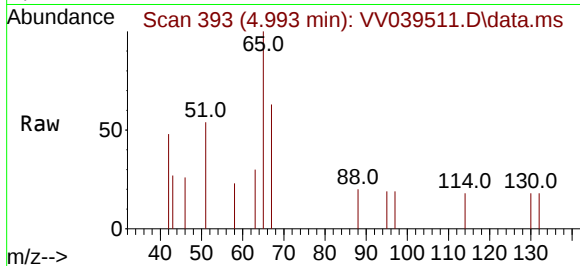

#5
Chlorobenzene-d5
Concen: 0.500 ug/L
RT: 8.785 min Scan# 587
Delta R.T. -0.000 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48

Tgt Ion: 117 Resp: 6889
Ion Ratio Lower Upper
117 100
82 48.2 39.4 59.2
119 32.4 26.2 39.2


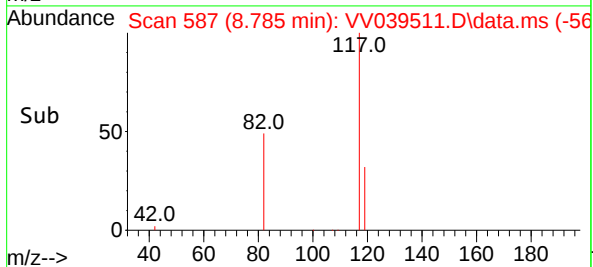
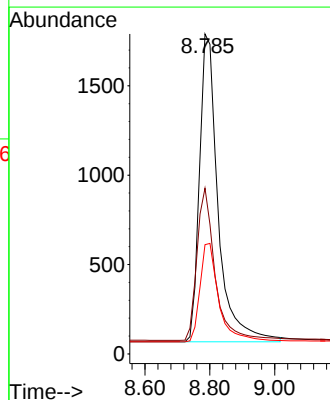
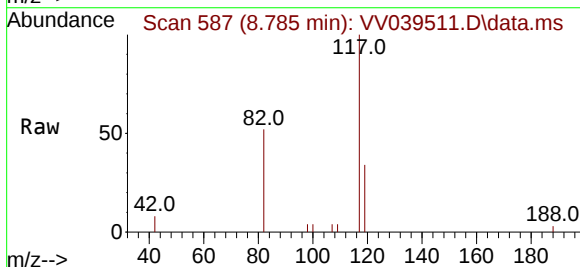


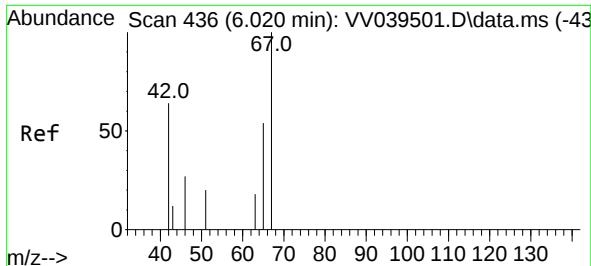

#7
1,2-Dichloropropane-d6
Concen: 0.405 ug/L
RT: 5.996 min Scan# 41
Delta R.T. -0.023 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48




Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD


Tgt Ion:	67	Resp:	2352
Ion	Ratio	Lower	Upper
67	100		
65	65.2	37.9	56.9#
46	45.1	27.4	41.0#
42	30.8	51.2	76.8#

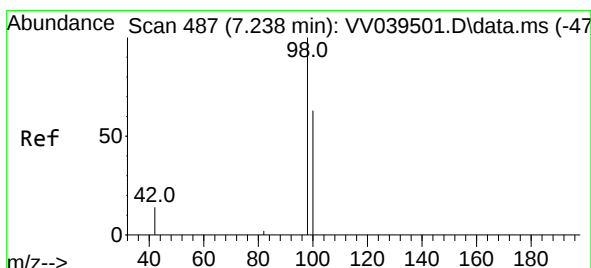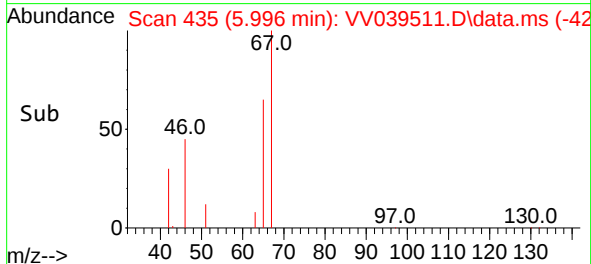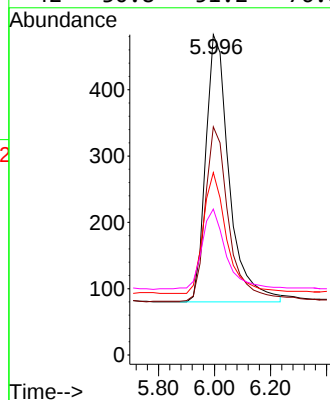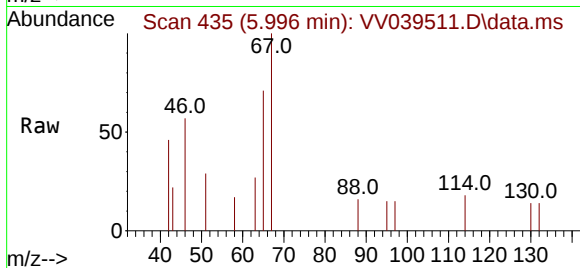

#8
Toluene-d8
Concen: 0.452 ug/L
RT: 7.254 min Scan# 488
Delta R.T. 0.016 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48

Tgt Ion:	98	Resp:	4431
Ion	Ratio	Lower	Upper
98	100		
100	61.6	44.5	82.7
42	10.7	10.1	18.7


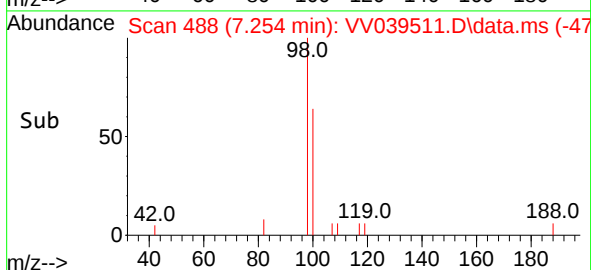
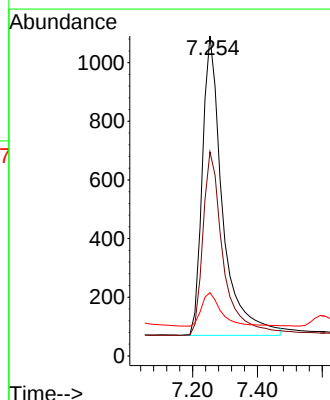
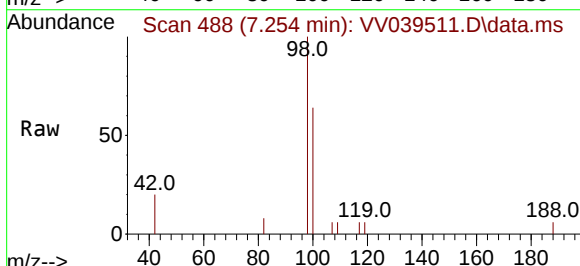


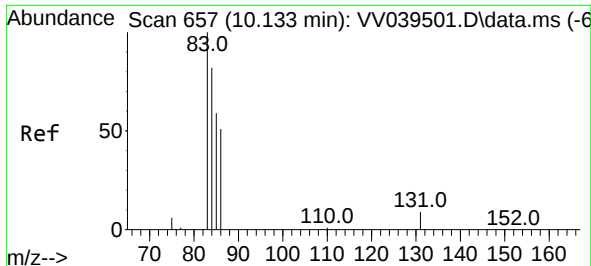

#10
1,1,2,2-Tetrachloroethane-d2
Concen: 0.494 ug/L
RT: 10.133 min Scan# 611
Delta R.T. -0.000 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48




Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-120425-SIM-FD


Tgt Ion: 84 Resp: 1617
Ion Ratio Lower Upper
84 100
86 62.9 44.4 82.5

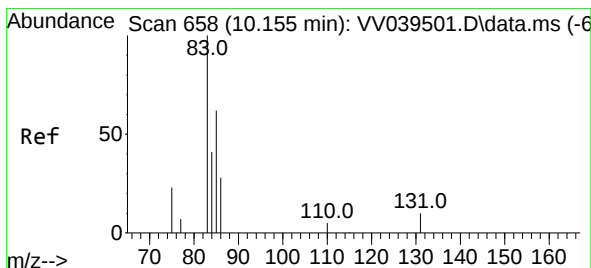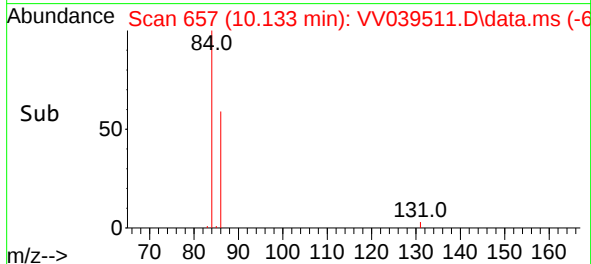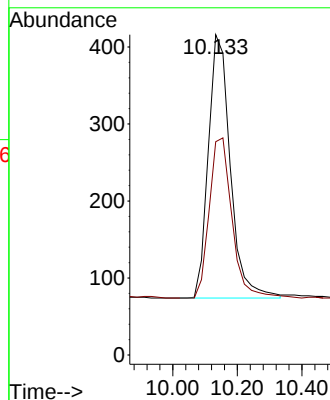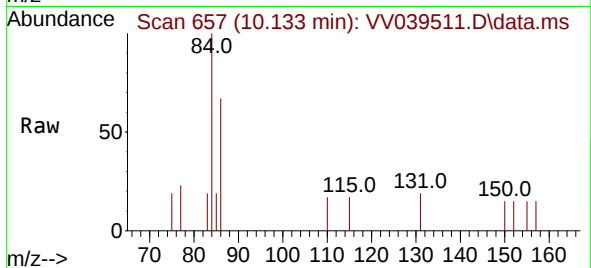

#11
1,1,2,2-Tetrachloroethane
Concen: 0.056 ug/L
RT: 9.556 min Scan# 631
Delta R.T. -0.599 min
Lab File: VV039511.D
Acq: 09 Dec 2025 17:48


Tgt Ion: 83 Resp: 384
Ion Ratio Lower Upper
83 100
85 255.7 51.0 76.6#
131 66.1 8.6 12.8#

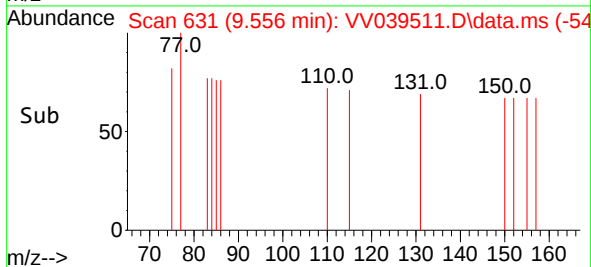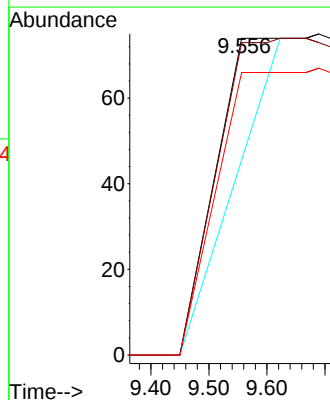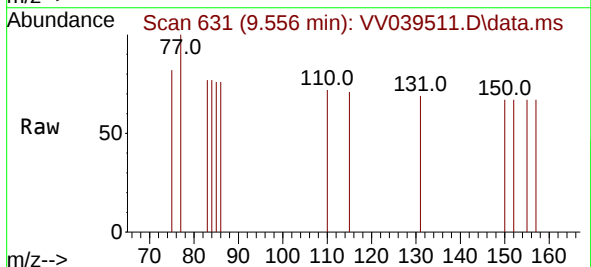

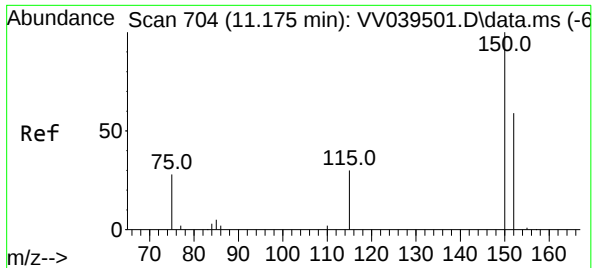

#12
 1,4-Dichlorobenzene-d4
 Concen: 0.500 ug/L
 RT: 11.197 min Scan# 70
 Delta R.T. 0.022 min
 Lab File: VV039511.D
 Acq: 09 Dec 2025 17:48

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-120425-SIM-FD

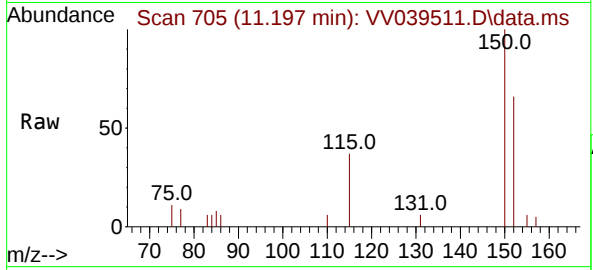

Tgt Ion:	152	Resp:	3685
Ion	Ratio	Lower	Upper
152	100		
115	53.8	0.0	101.6
150	159.5	0.0	396.2

