


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038310.D
Acq On : 11 Dec 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

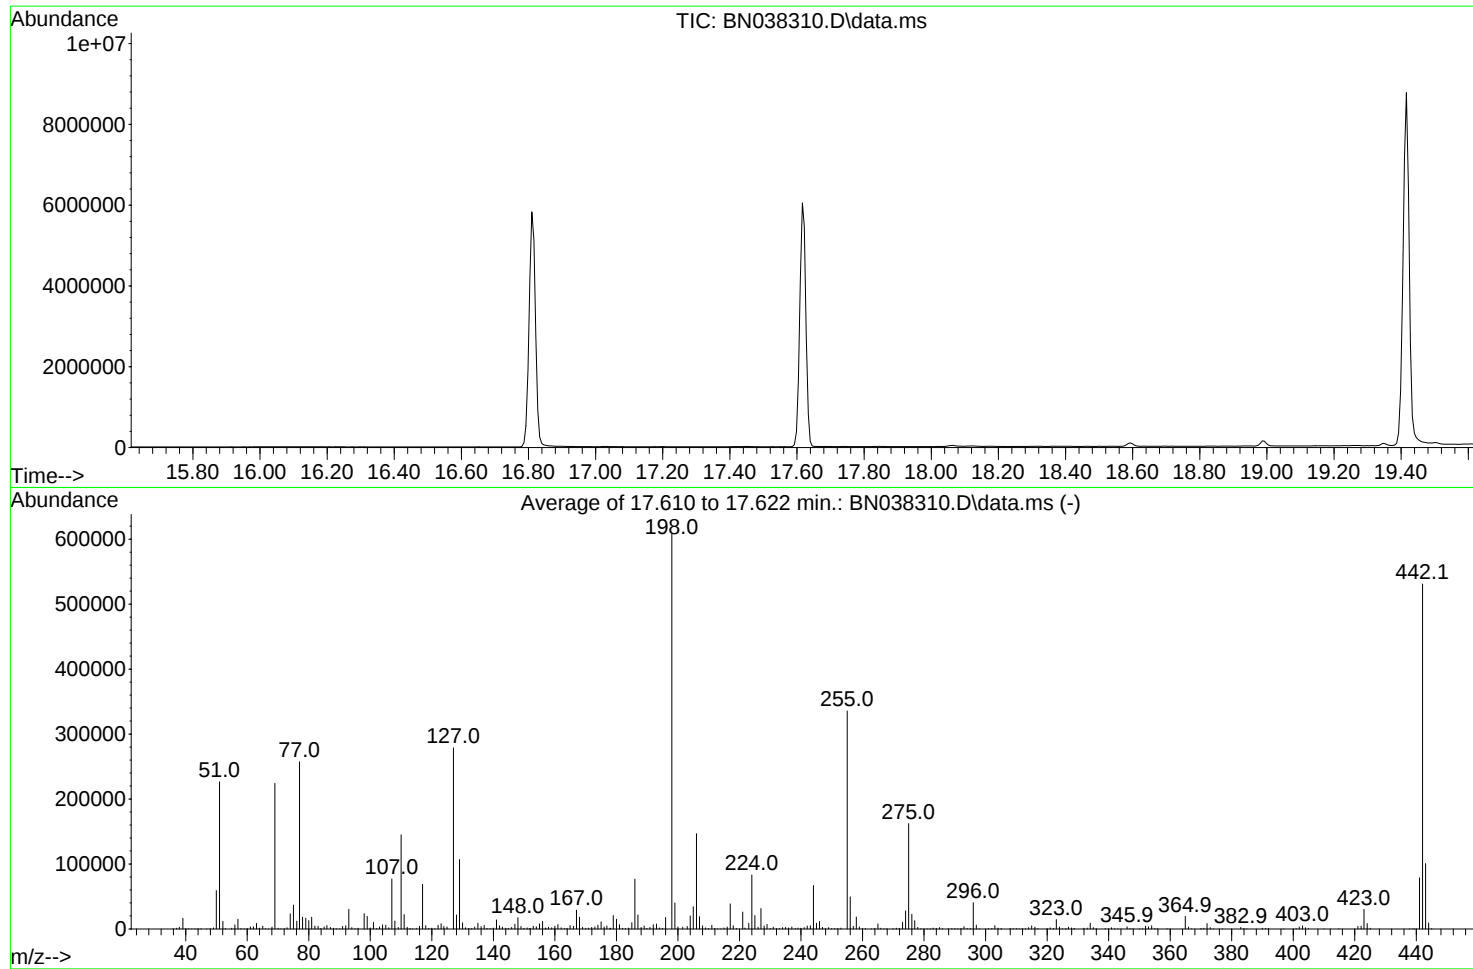




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	2793	PASS
69	69	100	100	100.0	223951	PASS
70	69	0.00	2	0.5	1194	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	607808	PASS
199	198	5	9	6.6	40149	PASS
365	198	1	100	3.2	19252	PASS
441	443	0.01	150	78.3	78795	PASS
442	442	100	100	100.0	530859	PASS
443	442	15	24	19.0	100613	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038310.D
Acq On : 11 Dec 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 11:06:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 11 11:06:13 2025
Response via : Initial Calibration

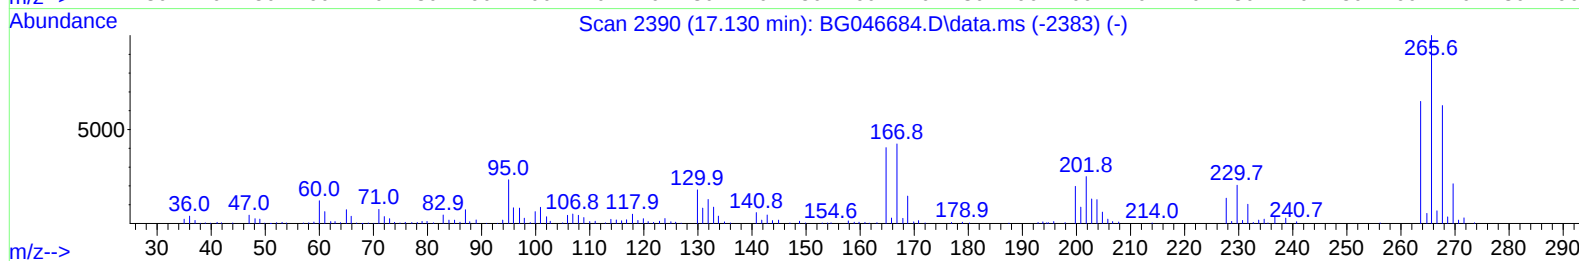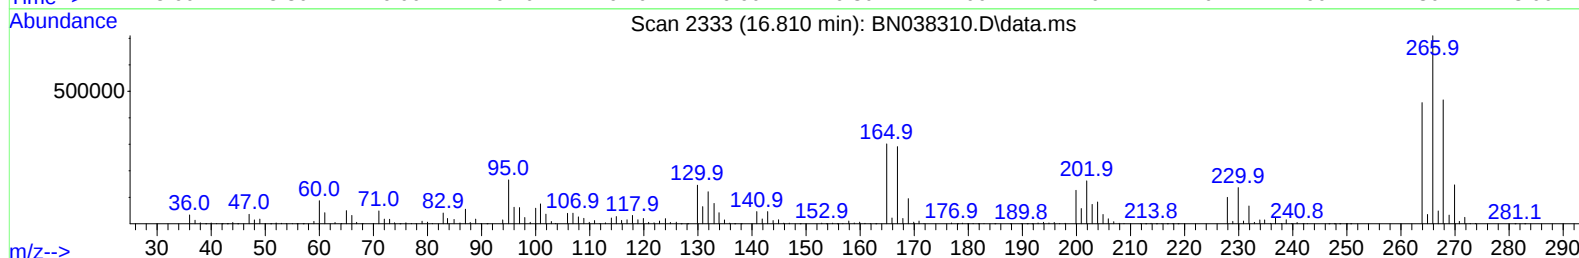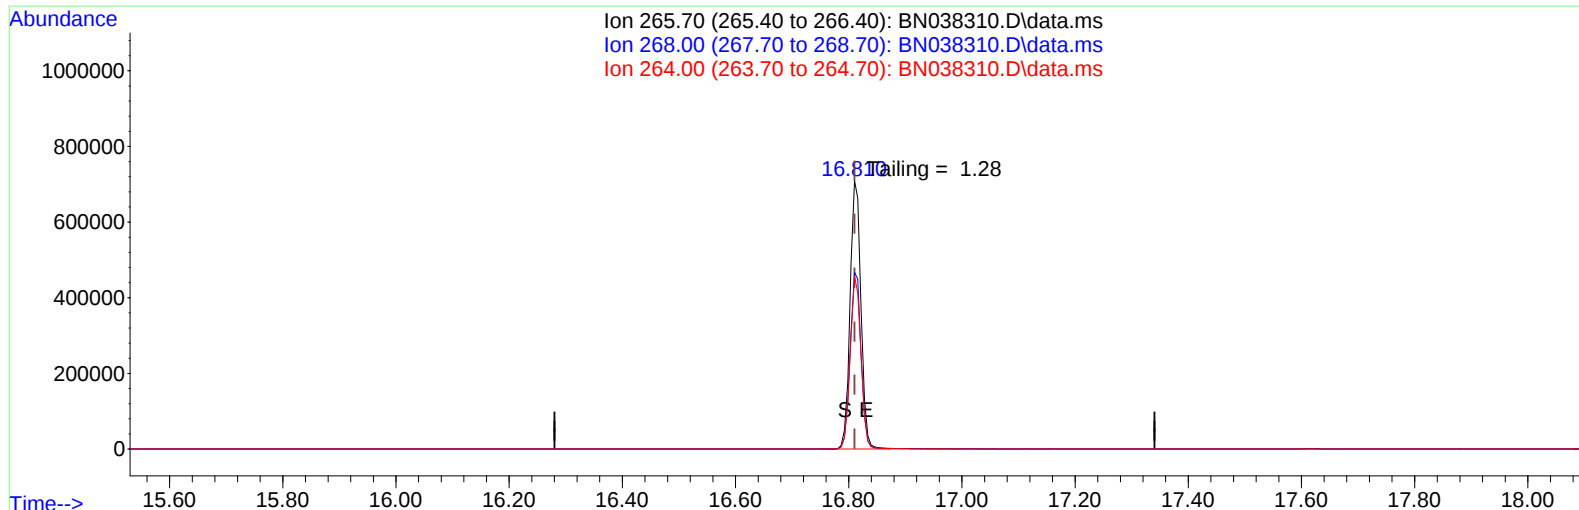

TIC: BN038310.D\data.ms

(70) Pentachlorophenol (C)

16.810min (0.000) 32618.14 ng




response 947378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.87
264.00	61.60	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038310.D
Acq On : 11 Dec 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 11:06:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 11 11:06:13 2025
Response via : Initial Calibration

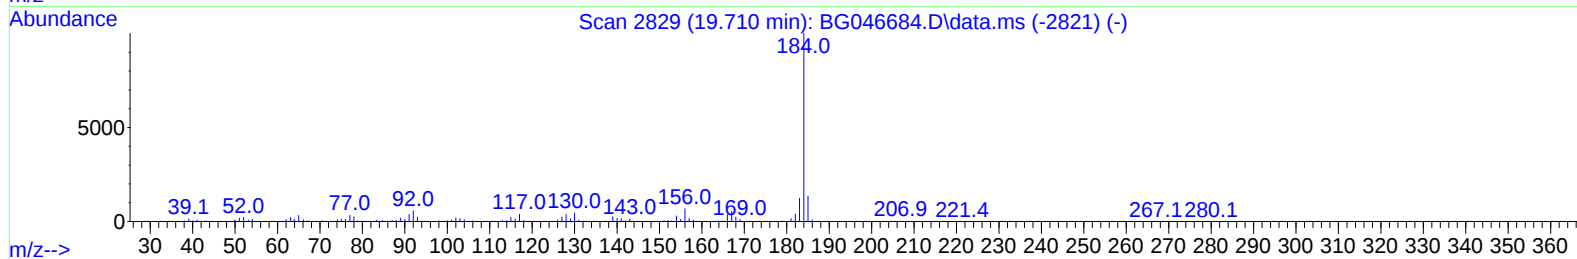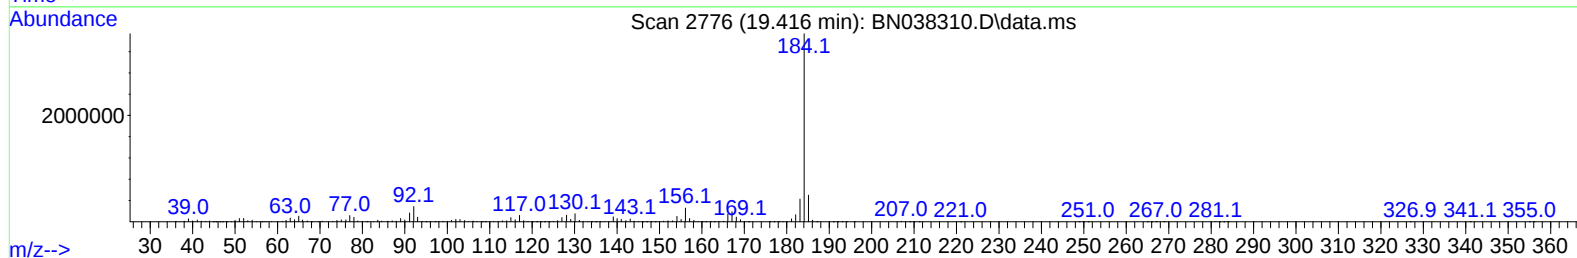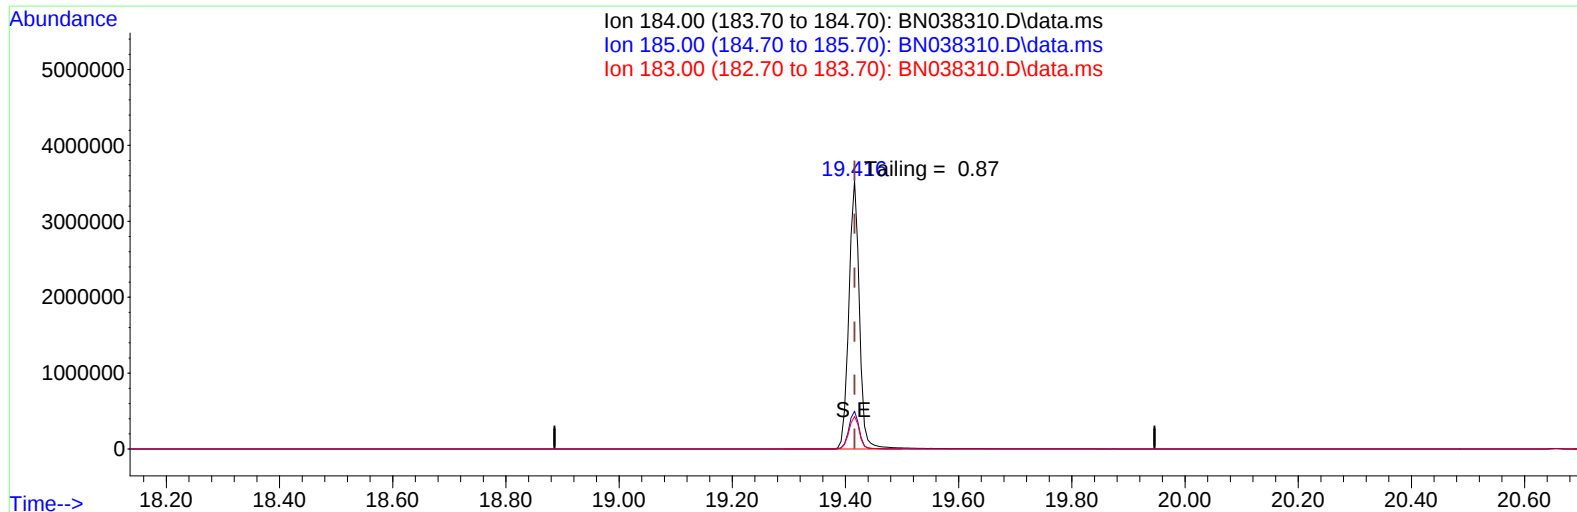

TIC: BN038310.D\data.ms

(77) Benzidine

19.416min (0.000) 0.00 ng

response 4618026

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2025	BNA_N	<u>BN038310.D</u>
Compound Name	Response	Retention Time
DDT	2326256	20.657
DDD	31356	20.216
DDE	441	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31797	2358053	1.35

Instrument :
BNA_N
ClientSampleId :
DFTPP