


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120925\
Data File : BG064901.D
Acq On : 9 Dec 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

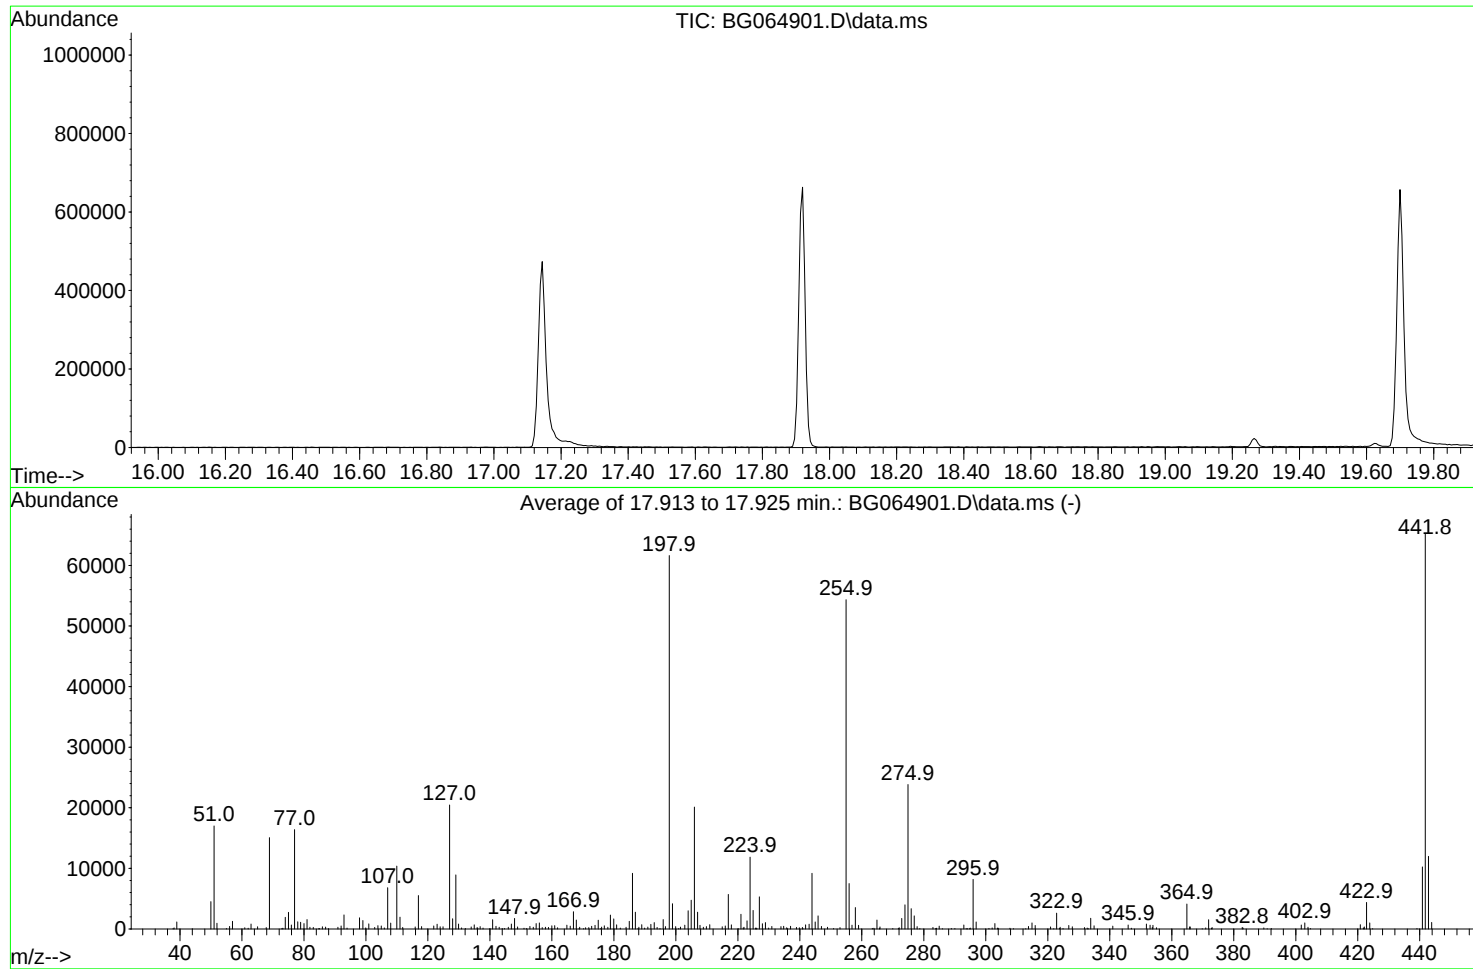




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.5	228	PASS
69	69	100	100	100.0	15069	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61624	PASS
199	198	5	9	6.8	4169	PASS
365	198	1	100	6.7	4120	PASS
441	443	0.01	150	85.5	10235	PASS
442	442	100	100	100.0	65173	PASS
443	442	15	24	18.4	11969	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120925\
Data File : BG064901.D
Acq On : 9 Dec 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 09 12:18:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

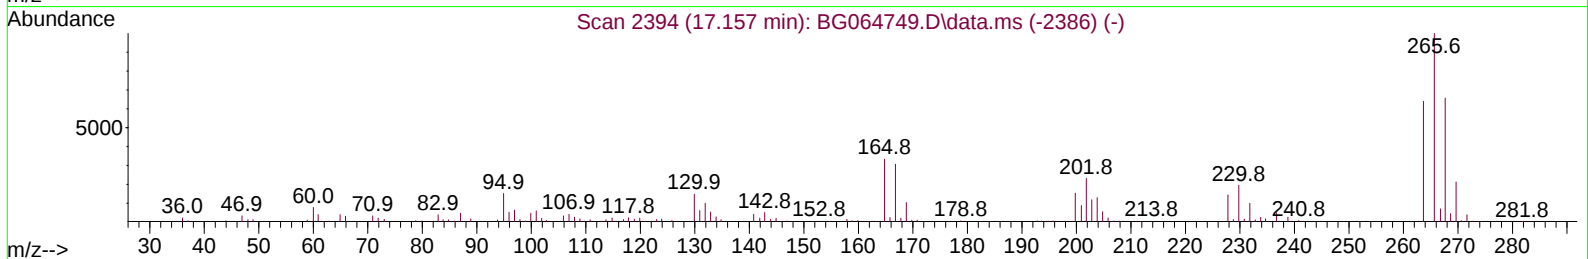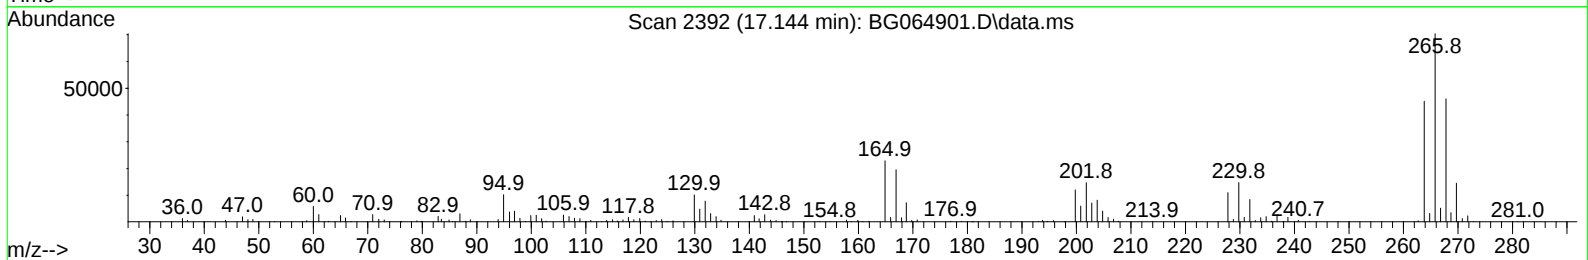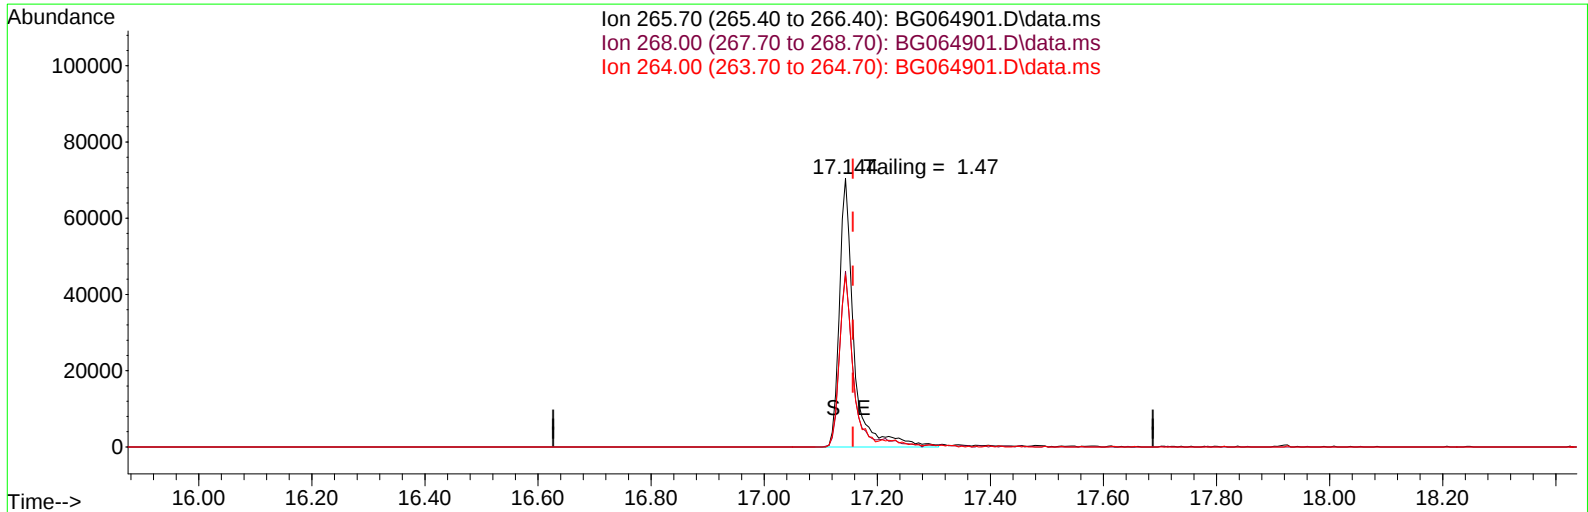

TIC: BG064901.D\data.ms

(70) Pentachlorophenol (C)

17.144min (-0.013) 25114.17 ng




response 118300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	70.42
264.00	64.00	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120925\
Data File : BG064901.D
Acq On : 9 Dec 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 09 12:18:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

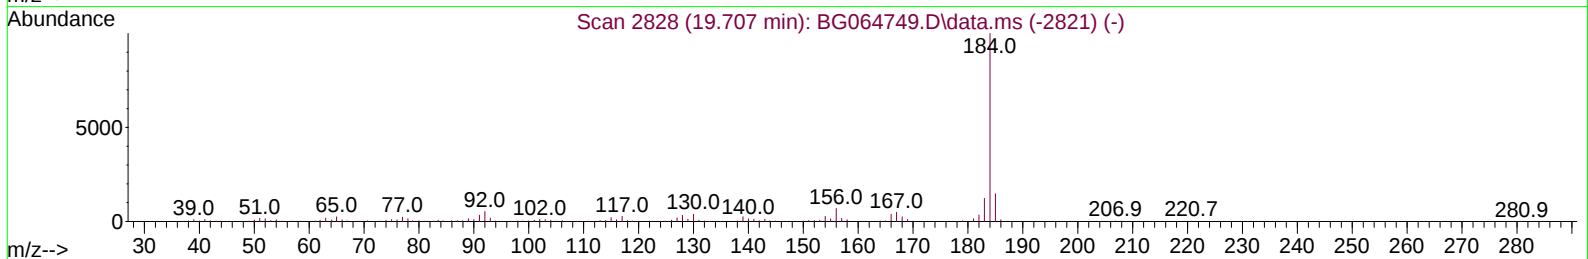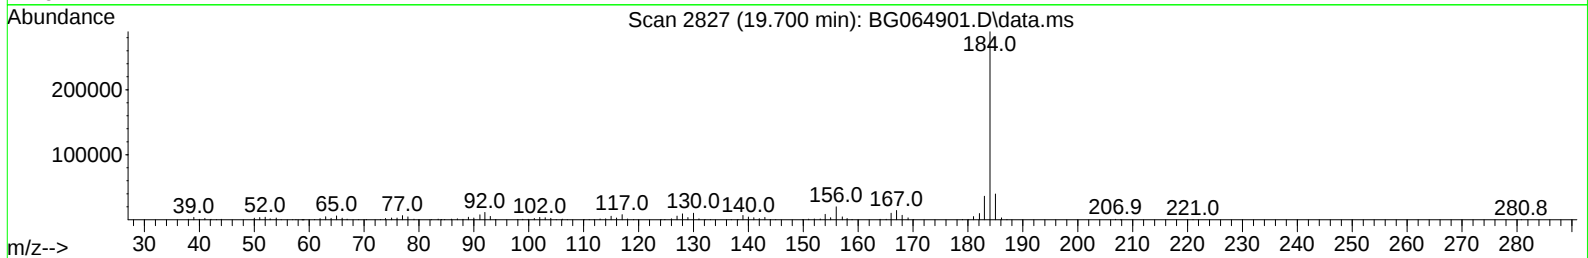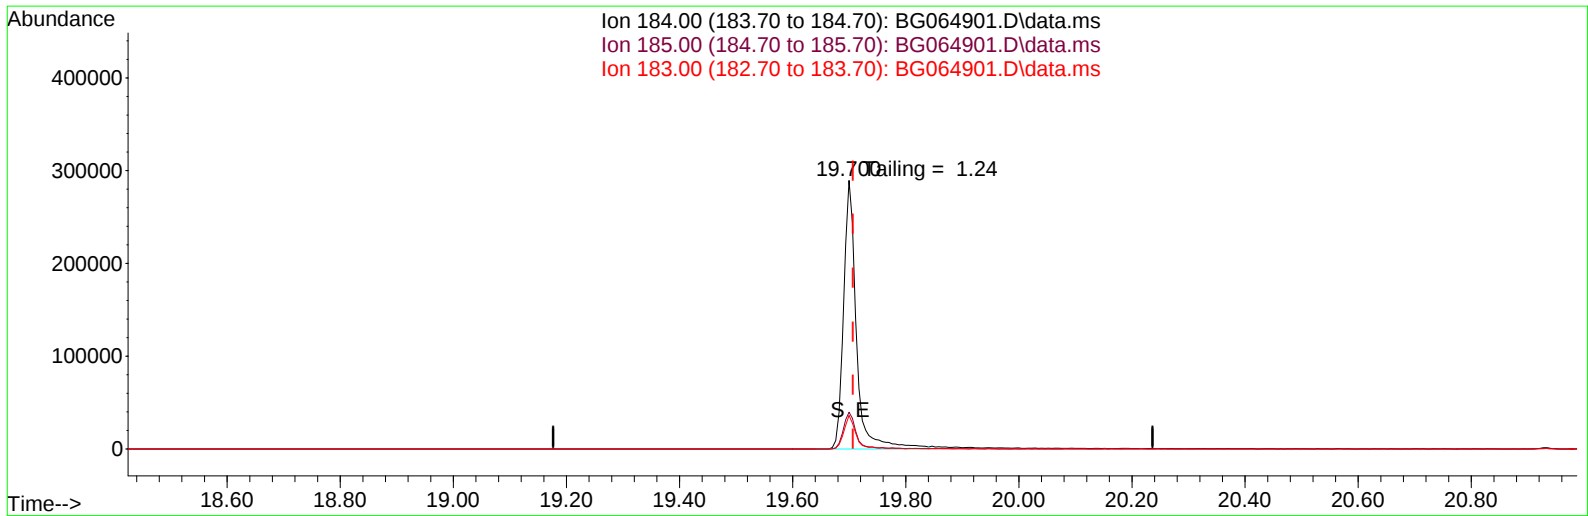

TIC: BG064901.D\data.ms

(77) Benzidine

19.700min (-0.007) 0.00 ng

response 454693

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.70
183.00	12.20	12.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/9/2025	BNA_G	<u>BG064901.D</u>
Compound Name	Response	Retention Time
DDT	313259	20.933
DDD	4298	20.487
DDE	300	19.993
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4598	317857	1.45

Instrument :
BNA_G
ClientSampleId :
DFTPP