


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120925\
Data File : BP026257.D
Acq On : 09 Dec 2025 11:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 05 14:52:44 2025

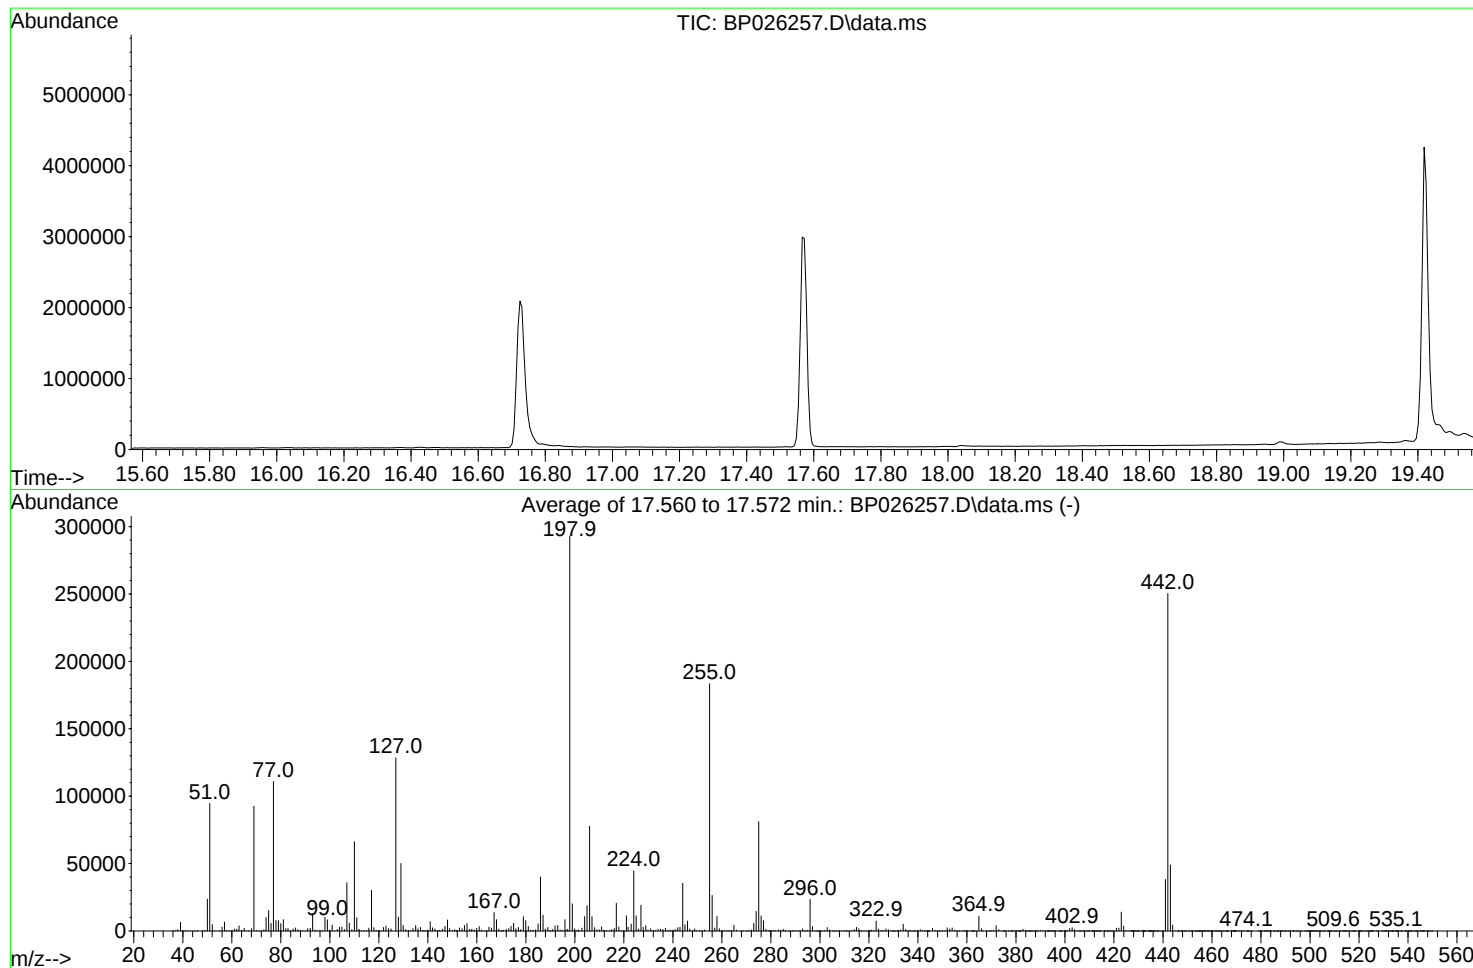


AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2473

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	1693	PASS
69	69	100	100	100.0	92594	PASS
70	69	0.00	2	0.5	456	PASS
197	198	0.00	2	0.4	1235	PASS
198	198	100	100	100.0	293025	PASS
199	198	5	9	6.9	20081	PASS
365	198	1	100	3.7	10904	PASS
441	443	0.01	150	78.1	38189	PASS
442	442	100	100	100.0	250392	PASS
443	442	15	24	19.5	48912	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120925\
Data File : BP026257.D
Acq On : 09 Dec 2025 11:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 09 11:53:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

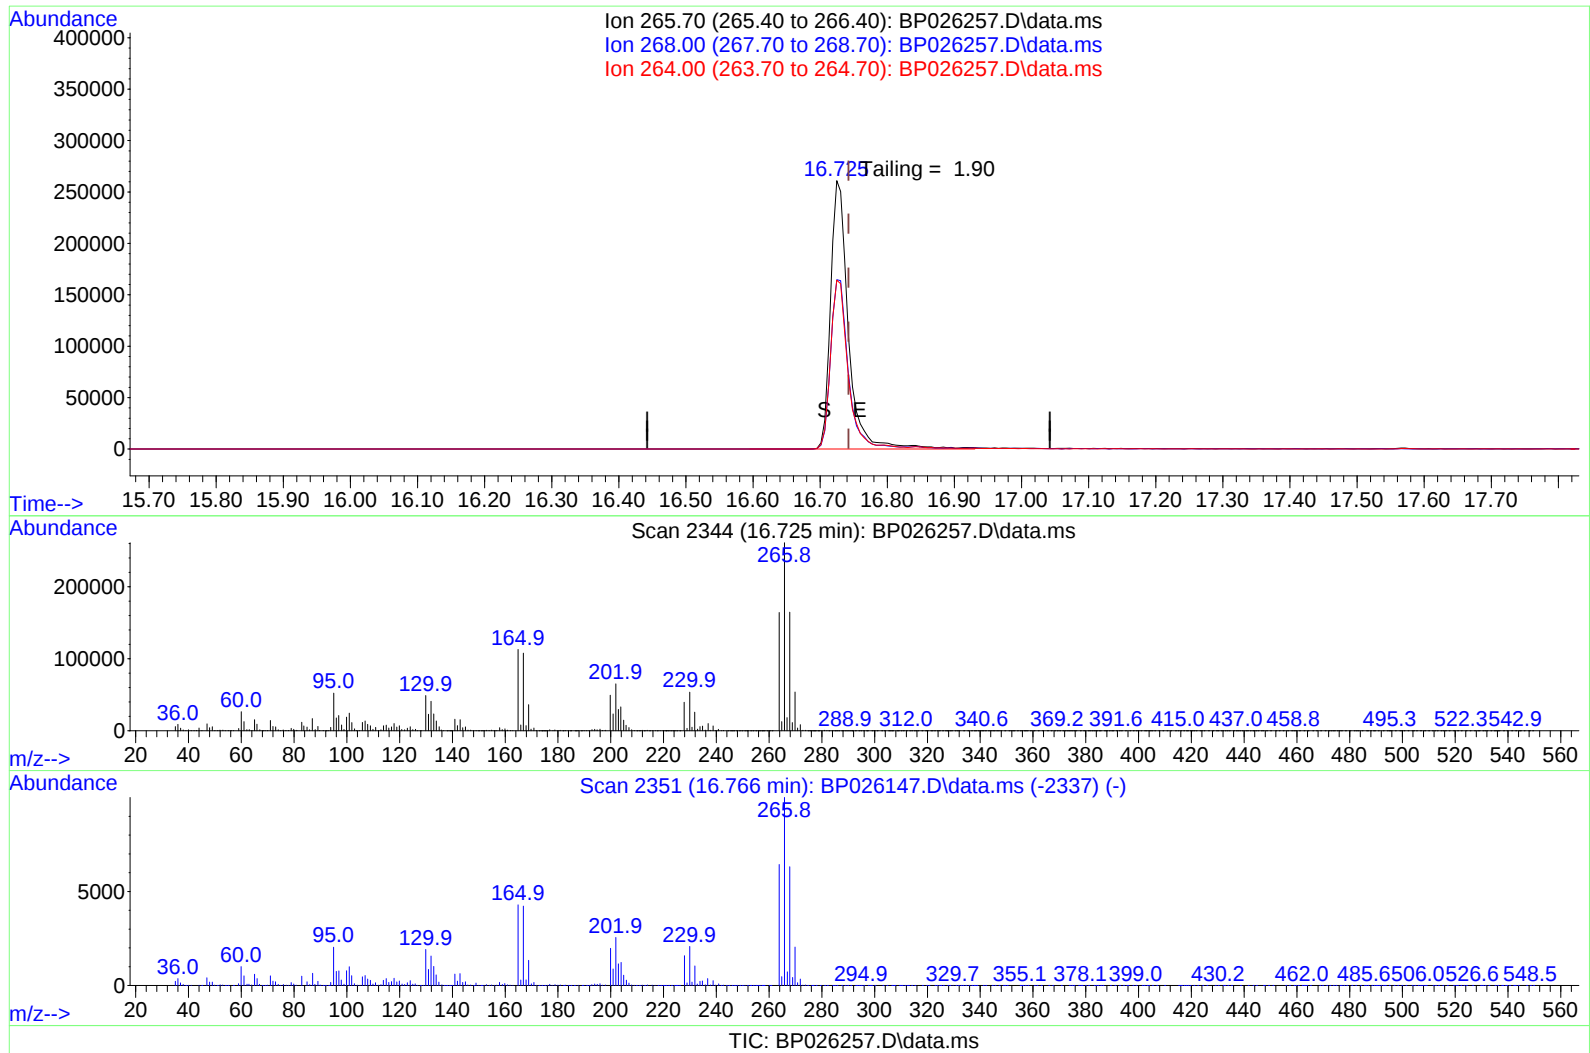

(70) Pentachlorophenol (C)

16.725min (-0.018) 2411089.14 ng




response 474123

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.10
264.00	62.70	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120925\
Data File : BP026257.D
Acq On : 09 Dec 2025 11:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 09 11:53:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

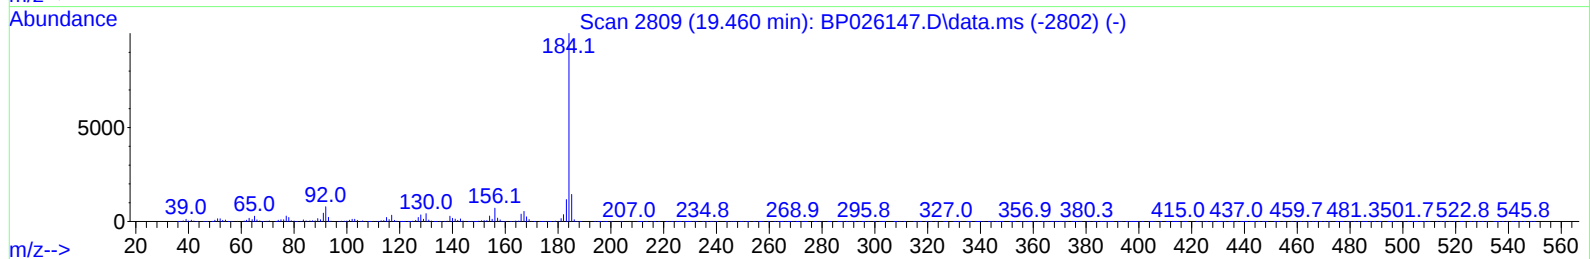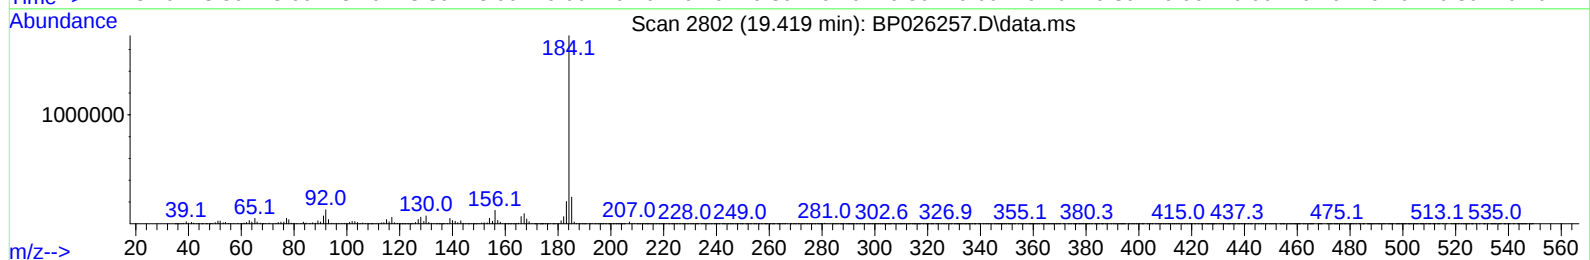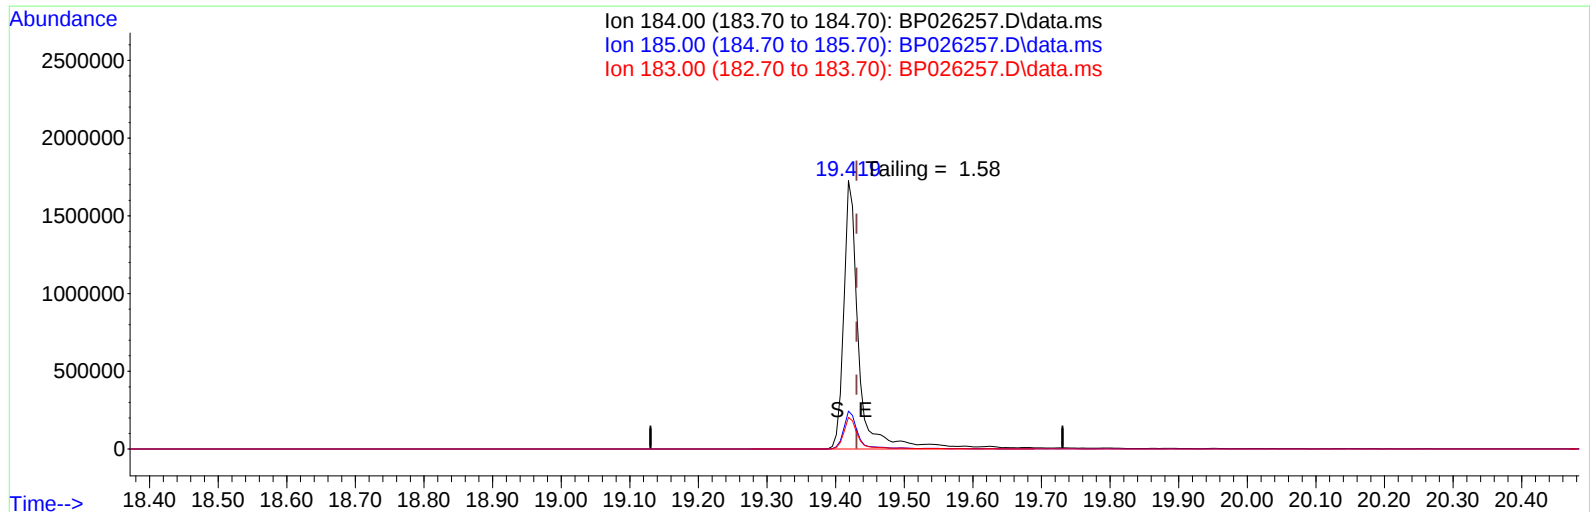

TIC: BP026257.D\data.ms

(77) Benzidine

19.419min (-0.012) 322564.15 ng

response 2420441

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.17
183.00	11.30	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/9/2025	BNA_P	<u>BP026257.D</u>
Compound Name	Response	Retention Time
DDT	1349834	20.718
DDD	21169	20.26
DDE	6807	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27976	1377810	2.03

Instrument :
BNA_P
ClientSampleId :
DFTPP