

Method Path : Z:\voasrv\HPCHEM1\MSVOA_L\methods\

Method File : VL111825AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Last Update : Wed Nov 19 01:11:25 2025

Response Via : Initial Calibration

Calibration Files

0.03=VL043209.D 0.1 =VL043208.D 0.5 =VL043203.D 1 =VL043206.D 2 =VL043205.D 10 =VL043204.D 15 =VL043210.D

Compound	0.03	0.1	0.5	1	2	10	15	Avg	%RSD

1) I Bromochloromethane	-----ISTD-----								
2) T Dichlorodifluo...			1.398	1.505	1.476	1.340	1.334	1.410	5.53
3) Chlorodifluoro...			1.545	1.404	1.437	1.317	1.231	1.387	8.60
4) Chloromethane			0.521	0.559	0.568	0.498	0.489	0.527	6.72
5) T Vinyl Chloride	0.724	0.655	0.533	0.580	0.575	0.486	0.483	0.577	15.33
6) T Bromomethane			0.300	0.302	0.286	0.253	0.258	0.280	8.30
7) Chloroethane			0.246	0.248	0.236	0.194	0.199	0.225	11.59
8) T Dichlorotetra...			1.156	1.241	1.262	1.091	1.116	1.173	6.43
9) T Propene			0.677	0.598	0.621	0.501	0.548	0.589	11.44
10) T Heptane			2.106	1.804	1.728	1.604	1.522	1.753	12.87
11) T Trichlorofluor...			1.238	1.515	1.487	1.240	1.352	1.367	9.62
12) T 1,1,2-Trichlor...			1.061	1.142	1.115	0.987	1.029	1.067	5.92
13) Ethanol			0.215	0.231	0.252	0.166	0.172	0.207	17.99
14) T Bromoethene			0.448	0.423	0.436	0.362	0.376	0.409	9.29
15) T Acetone			1.721	1.591	1.519	1.032	1.085	1.389	22.41
16) T 1,3-Butadiene			0.745	0.629	0.626	0.551	0.546	0.619	13.01
17) tert-Butyl alc...			1.784	2.014	1.880	1.705	1.735	1.824	6.87
18) T 1,1-Dichloroet...			0.555	0.530	0.515	0.441	0.443	0.497	10.52
19) T Isopropyl Alcohol			0.848	0.861	0.823	0.684	0.709	0.785	10.51
20) T Methylene Chlo...			0.906	0.710	0.585	0.398	0.403	0.600	35.87
21) T Allyl Chloride			1.139	0.895	0.936	0.849	0.855	0.935	12.75
22) T trans-1,2-Dich...			0.605	0.614	0.599	0.499	0.521	0.568	9.39
23) T Vinyl Acetate			1.885	1.632	1.682	1.622	1.565	1.677	7.36
24) T 1,1-Dichloroet...			1.050	1.173	1.194	1.018	1.044	1.096	7.42
25) T Ethyl Acetate			3.371	3.123	3.074	2.759	2.655	2.996	9.68
26) T Hexane			1.374	1.424	1.375	1.235	1.161	1.314	8.44
27) T Carbon Disulfide			1.303	1.424	1.432	1.257	1.291	1.341	6.03
28) T Methyl tert-Bu...			0.642	0.704	0.674	0.591	0.614	0.645	7.02
29) T Chloroform			1.955	1.898	1.928	1.785	1.770	1.867	4.52
30) T Cyclohexane			1.135	1.194	1.130	1.024	1.024	1.101	6.80
31) T cis-1,2-Dichlo...			1.399	1.351	1.322	1.240	1.217	1.306	5.83
32) T 1,1,1-Trichlor...	2.116	2.046	1.970	2.018	2.033	1.884	1.865	1.990	4.52


33) I 1,4-Difluorobenzene	-----ISTD-----								
34) T 2-Butanone			0.744	0.751	0.736	0.644	0.655	0.706	7.38
35) T Carbon Tetrach...	0.832	0.765	0.779	0.771	0.737	0.708	0.721	0.759	5.51
36) T Benzene			0.996	1.001	0.986	0.905	0.900	0.958	5.28
37) T 1,2-Dichloroet...			0.572	0.580	0.565	0.531	0.553	0.560	3.39
38) T Trichloroethene	0.293	0.475	0.390	0.388	0.371	0.353	0.353	0.375	14.65
39) T 1,2-Dichloropr...			0.372	0.364	0.350	0.335	0.332	0.351	4.97

Method Path : Z:\voasrv\HPCHEM1\MSVOA_L\methods\											
Method File : VL111825AIR.M											
40)	T	1,4-Dioxane			0.180	0.166	0.155	0.142	0.144	0.158	10.04
41)	T	Tetrahydrofuran			0.418	0.401	0.402	0.367	0.360	0.390	6.32
42)	T	Bromodichlorom...			0.782	0.795	0.783	0.745	0.758	0.773	2.63
43)		Methyl Methacr...			0.576	0.532	0.511	0.462	0.462	0.508	9.55
44)	T	2,2,4-Trimethy...			1.746	1.765	1.621	1.555	1.537	1.645	6.47
45)	T	t-1,3-Dichloro...			0.495	0.472	0.489	0.455	0.458	0.474	3.79
46)	T	cis-1,3-Dichlo...			0.599	0.557	0.562	0.534	0.529	0.556	5.00
47)	T	1,1,2-Trichlor...			0.424	0.372	0.378	0.344	0.342	0.372	8.91
48)	T	Dibromochlorom...			0.629	0.666	0.663	0.618	0.621	0.640	3.63
49)	T	Bromoform			0.583	0.569	0.581	0.555	0.545	0.566	2.86
50)	T	4-Methyl-2-Pen...			1.025	1.061	1.027	0.946	0.914	0.994	6.19
51)	T	2-Hexanone			0.782	0.805	0.816	0.734	0.724	0.772	5.37
52)	T	Tetrachloroethene	0.363	0.424	0.344	0.362	0.349	0.329	0.323	0.356	9.37
53)	T	Toluene			1.198	1.182	1.146	1.075	1.069	1.134	5.26
54)	T	1,2-Dibromoethane		0.528	0.587	0.569	0.549	0.525	0.526	0.547	4.79
-----ISTD-----											
55)	I	Chlorobenzene-d5									
56)		1,1,1,2-Tetrac...			0.791	0.769	0.761	0.677	0.677	0.735	7.34
57)	T	Chlorobenzene			1.035	1.088	1.089	0.969	0.953	1.027	6.24
58)	T	Ethyl Benzene			1.927	2.038	2.008	1.821	1.830	1.925	5.16
59)	T	m/p-Xylene			1.618	1.611	1.607	1.434	1.446	1.543	6.12
60)	T	o-Xylene			1.584	1.625	1.659	1.419	1.421	1.542	7.42
61)	T	Styrene			0.669	0.690	0.719	0.648	0.647	0.675	4.54
62)		Isopropylbenzene			2.807	2.946	2.945	2.556	2.536	2.758	7.31
63)	T	1,1,2,2-Tetrac...	0.999	1.034	1.016	1.012	1.028	0.891	0.884	0.981	6.58
64)		n-propylbenzene			0.722	0.758	0.757	0.657	0.649	0.709	7.47
65)		tert-Butylbenzene			2.583	2.687	2.646	2.224	2.176	2.463	9.90
66)	T	Benzyl Chloride			0.275	0.251	0.257	0.241	0.225	0.250	7.36
67)		sec-Butylbenzene			3.588	3.728	3.697	3.108	3.070	3.438	9.40
68)	S	1-Bromo-4-Fluo...	0.712	0.725	0.729	0.733	0.741	0.735	0.757	0.733	1.90
69)		p-Isopropyltol...			2.994	3.070	3.197	2.660	2.641	2.912	8.58
70)		n-Butylbenzene			2.676	3.041	3.125	2.639	2.647	2.825	8.39
71)		2-Chlorotoluene			2.198	2.257	2.210	1.960	1.975	2.120	6.65
72)	T	4-Ethyltoluene			1.934	1.948	2.009	1.749	1.747	1.877	6.46
73)	T	1,3,5-Trimethy...			1.623	1.682	1.662	1.456	1.454	1.575	7.09
74)	T	1,2,4-Trimethy...			1.796	1.844	1.871	1.548	1.537	1.719	9.51
75)	T	1,3-Dichlorobe...			1.043	1.053	1.061	0.937	0.922	1.003	6.78
76)	T	1,4-Dichlorobe...			1.056	1.033	1.060	0.940	0.930	1.003	6.34
77)	T	1,2-Dichlorobe...			0.974	1.064	1.050	0.872	0.863	0.965	9.83
78)	T	Hexachloro-1,3...			0.854	0.899	0.920	0.686	0.666	0.805	14.94
79)	T	Naphthalene		1.230	1.483	1.599	1.860	1.496	1.493	1.527	13.35
80)	T	Naphthalene,2-...			0.397	0.323	0.448	0.397	0.439	0.401	12.30
81)	T	1,2,4-Trichlor...			0.549	0.692	0.813	0.678	0.682	0.683	13.72

(#) = Out of Range

Methylene Chloride

Response Ratio

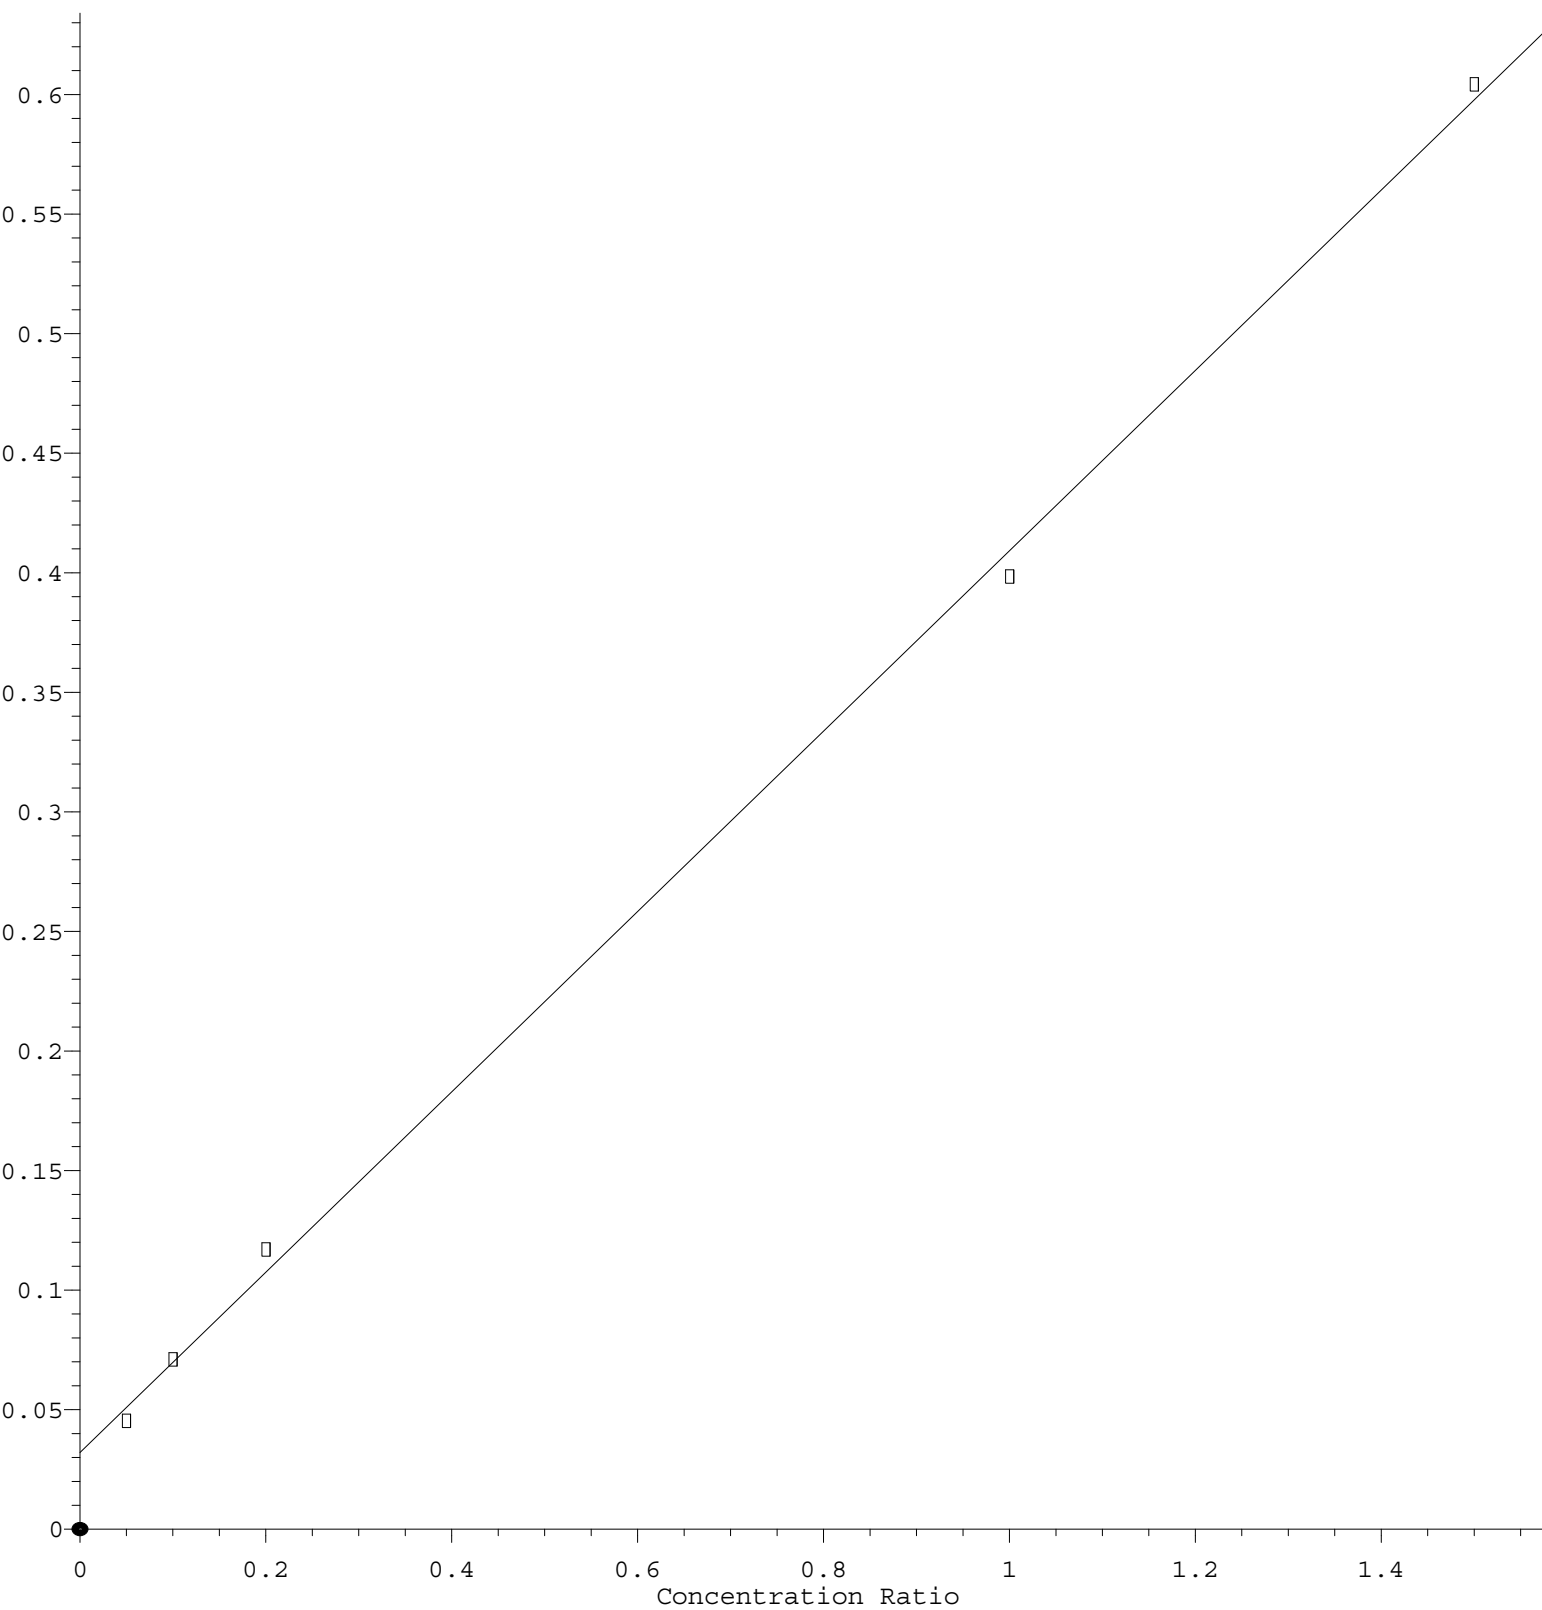

Response = 3.773e-001 * Amt + 3.213e-002
 Coef of Det (r^2) = 0.998825 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA L\methods\VL11825AIR.M
 Calibration Table Last Updated: Wed Nov 19 01:11:25 2025