

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
 Data File : BN038346.D
 Acq On : 12 Dec 2025 11:12
 Operator : RC/JU
 Sample : Q3813-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BR-04DR-451-120825

Quant Time: Dec 12 11:36:15 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 13:56:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.717	152	5531	0.400	ng	0.00
7) Naphthalene-d8	10.519	136	14873	0.400	ng	#-0.01
13) Acenaphthene-d10	14.387	164	8212	0.400	ng	-0.01
19) Phenanthrene-d10	17.148	188	16033	0.400	ng	0.00
29) Chrysene-d12	21.339	240	12704	0.400	ng	0.00
35) Perylene-d12	23.627	264	12519	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.290	112	1723	0.125	ng	0.00
5) Phenol-d6	6.886	99	1260	0.077	ng	0.00
8) Nitrobenzene-d5	8.875	82	3707	0.295	ng	0.00
11) 2-Methylnaphthalene-d10	12.121	152	5241	0.250	ng	0.00
14) 2,4,6-Tribromophenol	15.882	330	1180	0.324	ng	-0.01
15) 2-Fluorobiphenyl	13.008	172	10813	0.273	ng	0.00
27) Fluoranthene-d10	19.183	212	14269	0.360	ng	0.00
31) Terphenyl-d14	19.782	244	12001	0.423	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.189	88	12591	1.985	ng	# 96
34) Bis(2-ethylhexyl)phtha...	21.259	149	5763	0.214	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038346.D
Acq On : 12 Dec 2025 11:12
Operator : RC/JU
Sample : Q3813-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825


Quant Time: Dec 12 11:36:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 13:56:50 2025
Response via : Initial Calibration

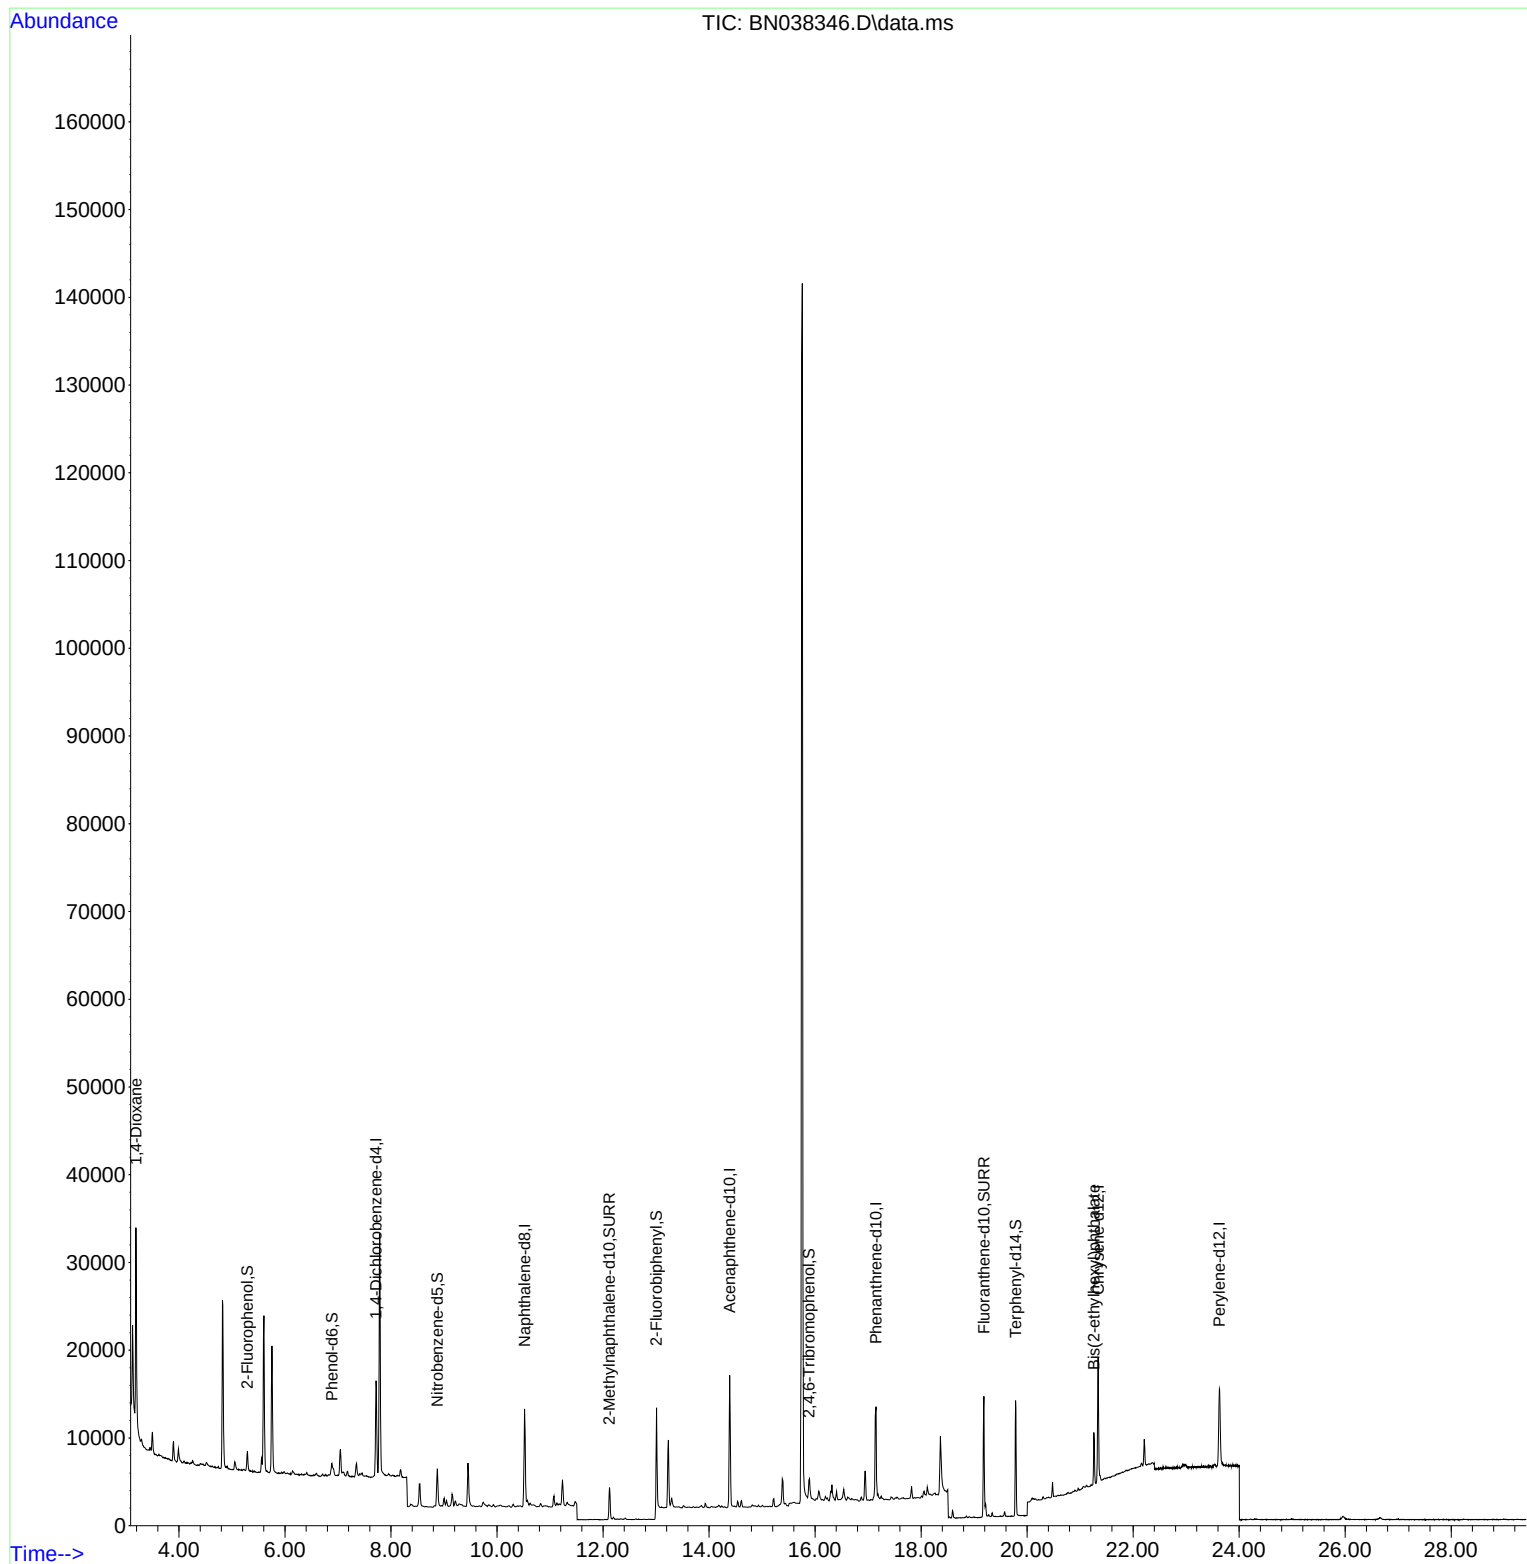



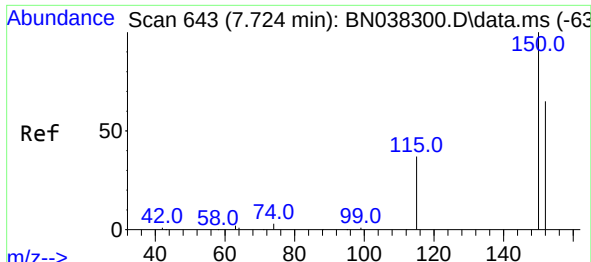


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.717 min Scan# 64
Delta R.T. -0.007 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825



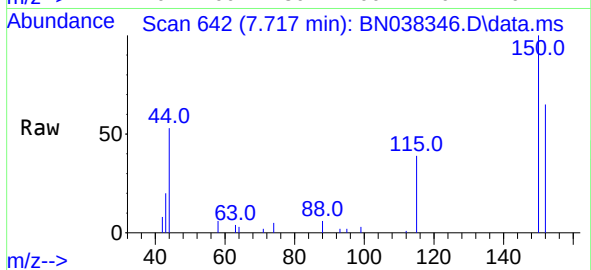



Tgt Ion:152 Resp: 5531
Ion Ratio Lower Upper
152 100
150 154.0 122.4 183.6
115 60.2 47.3 70.9

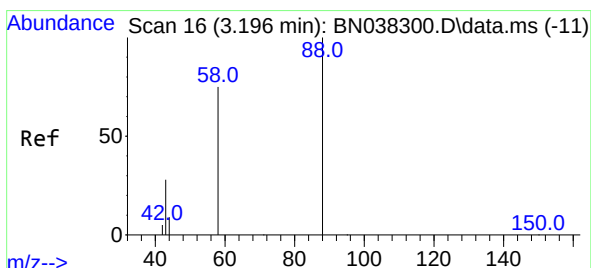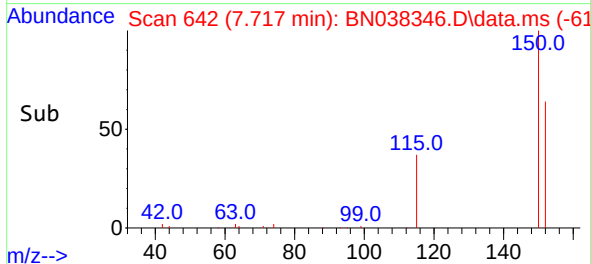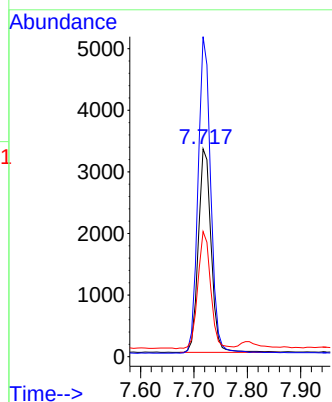

#2
1,4-Dioxane
Concen: 1.985 ng
RT: 3.189 min Scan# 15
Delta R.T. -0.007 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion: 88 Resp: 12591
Ion Ratio Lower Upper
88 100
43 38.1 24.9 37.3#
58 77.6 61.4 92.0

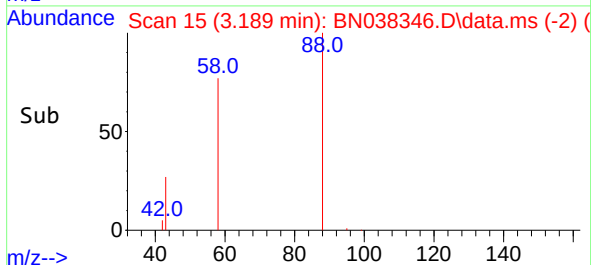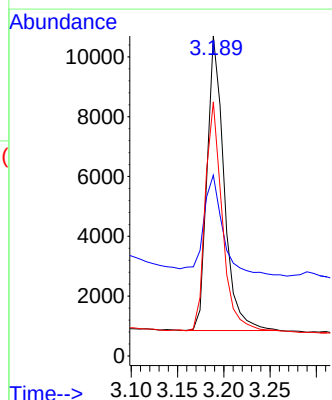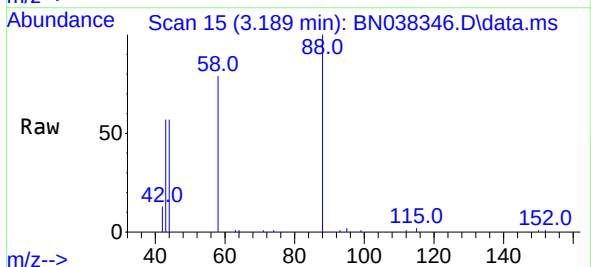




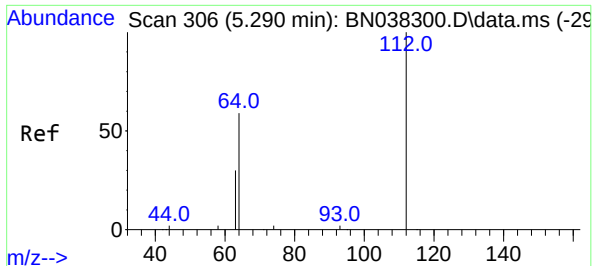


#4
2-Fluorophenol
Concen: 0.125 ng
RT: 5.290 min Scan# 306
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825

Tgt Ion:112 Resp: 1723




Ion	Ratio	Lower	Upper
112	100		
64	58.2	44.4	66.6
63	30.4	23.4	35.0

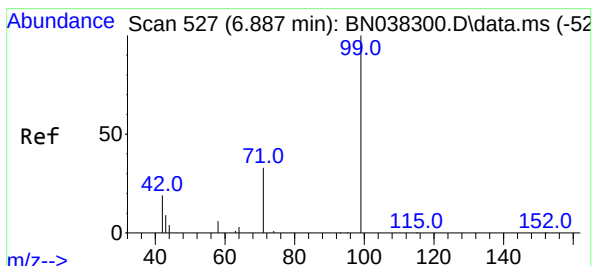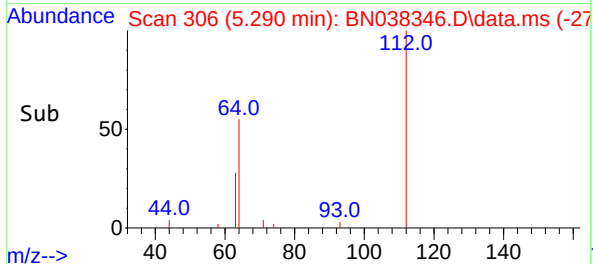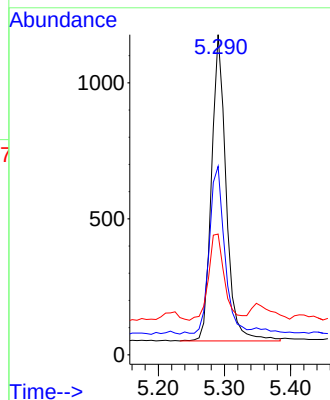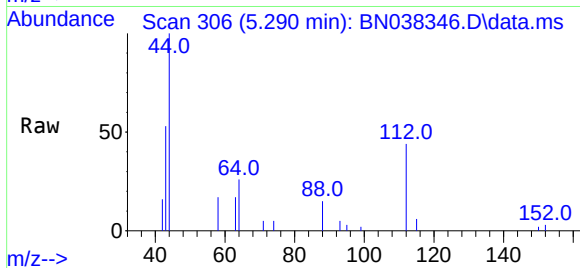


#5
Phenol-d6
Concen: 0.077 ng
RT: 6.886 min Scan# 527
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion: 99 Resp: 1260

Ion	Ratio	Lower	Upper
99	100		
42	35.4	16.5	24.7#
71	34.4	24.9	37.3


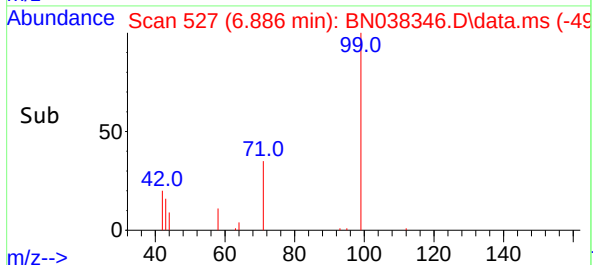
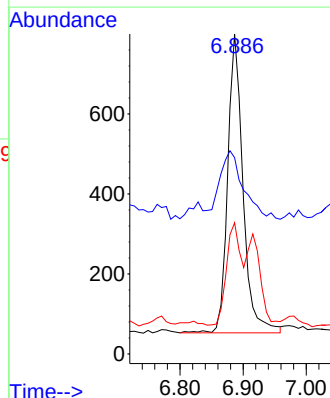
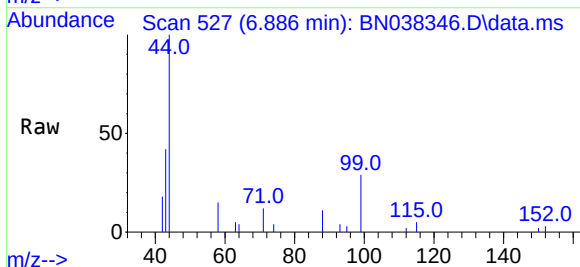


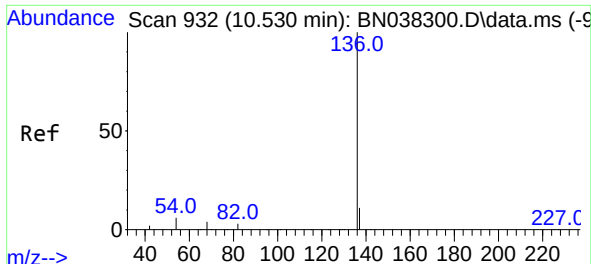

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.519 min Scan# 911
Delta R.T. -0.011 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12




Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825


Tgt Ion:	136	Resp:	14873
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.1	13.7
54	9.7	5.2	7.8#
68	7.5	4.1	6.1#

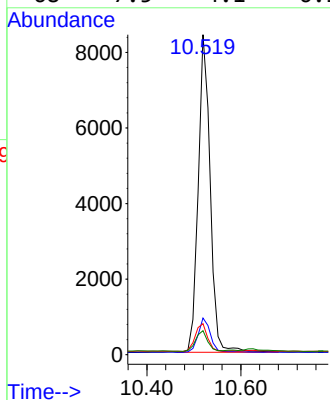

#8
Nitrobenzene-d5
Concen: 0.295 ng
RT: 8.875 min Scan# 777
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion:	82	Resp:	3707
Ion	Ratio	Lower	Upper
82	100		
128	46.2	34.0	51.0
54	54.4	44.4	66.6


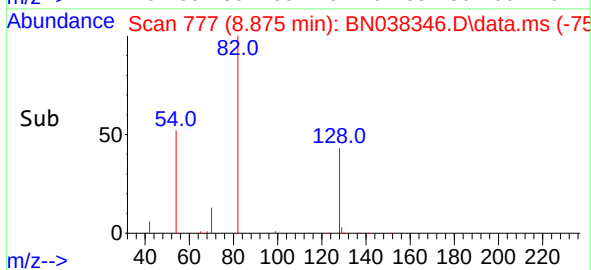
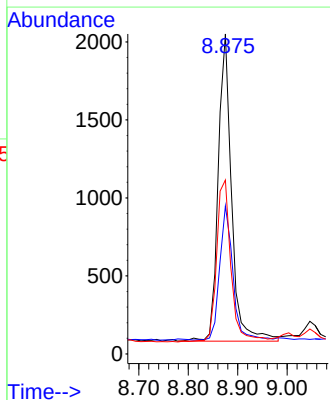
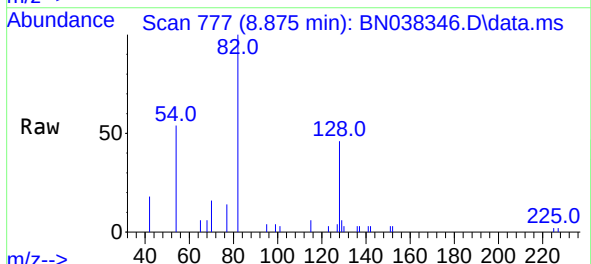


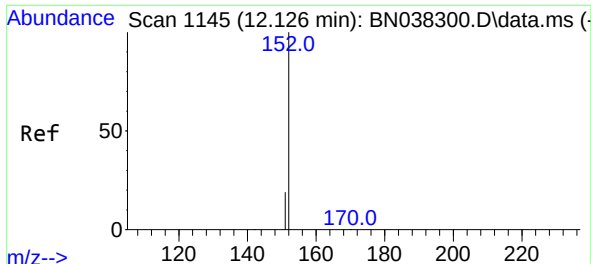

#11
2-Methylnaphthalene-d10
Concen: 0.250 ng
RT: 12.121 min Scan# 1145
Delta R.T. -0.005 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12




Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825


Tgt Ion:152 Resp: 5241
Ion Ratio Lower Upper
152 100
151 21.2 17.0 25.6

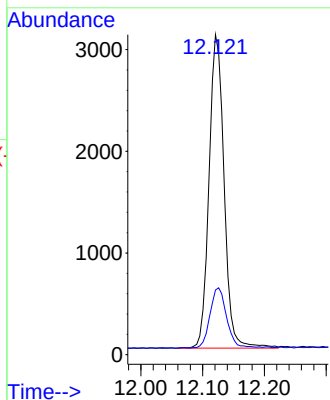

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.387 min Scan# 1448
Delta R.T. -0.011 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12


Tgt Ion:164 Resp: 8212
Ion Ratio Lower Upper
164 100
162 105.1 86.2 129.4
160 53.0 44.6 67.0

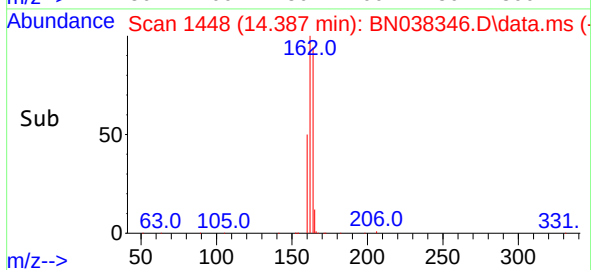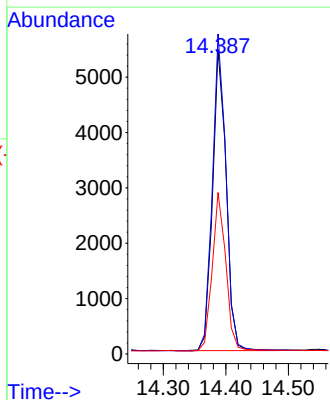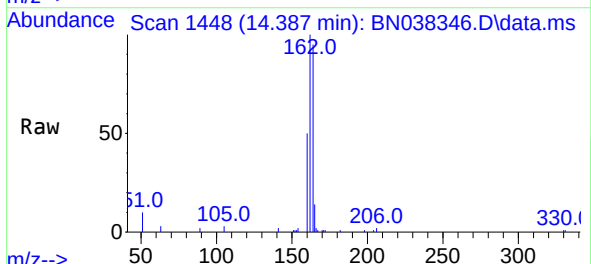






#14
2,4,6-Tribromophenol
Concen: 0.324 ng
RT: 15.882 min Scan# 1583
Delta R.T. -0.013 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825



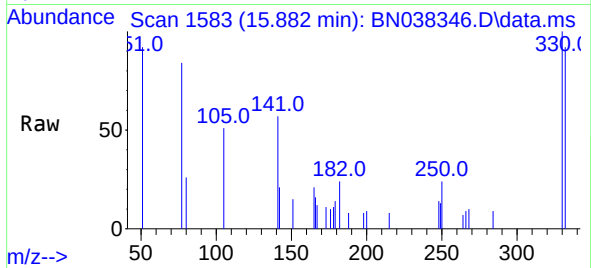



Tgt Ion:330 Resp: 1180
Ion Ratio Lower Upper
330 100
332 96.9 75.8 113.6
141 44.9 31.8 47.8

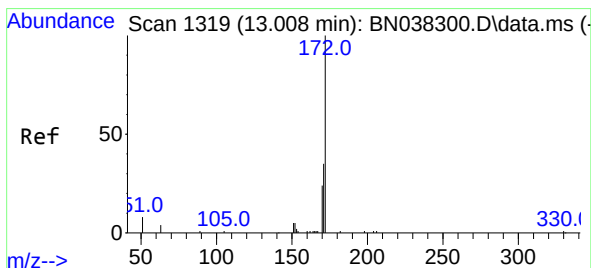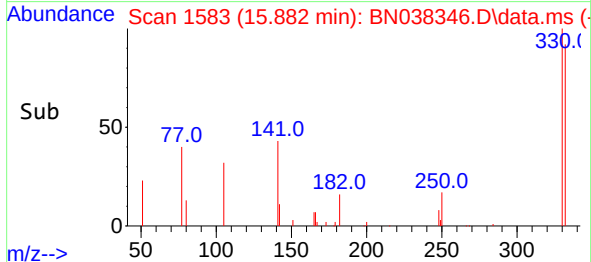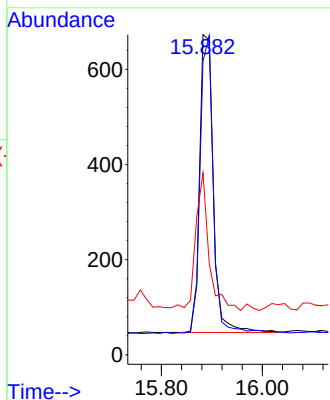

#15
2-Fluorobiphenyl
Concen: 0.273 ng
RT: 13.008 min Scan# 1319
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion:172 Resp: 10813
Ion Ratio Lower Upper
172 100
171 35.3 28.6 42.8
170 23.9 19.3 28.9


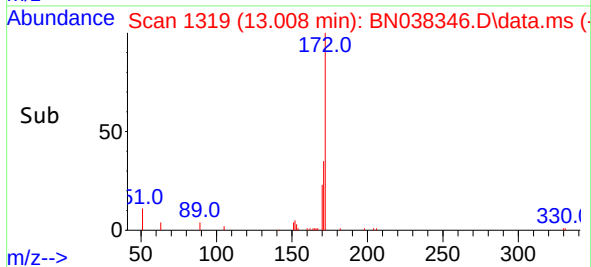
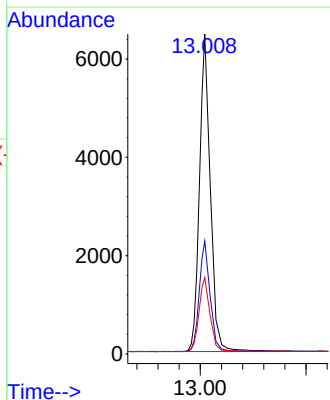
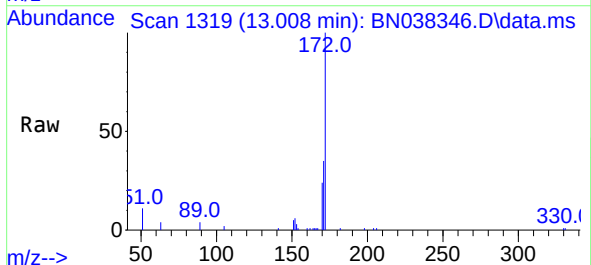




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.148 min Scan# 1685
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12




Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825


Tgt Ion:	188	Resp:	16033
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	9.0	7.4	11.0

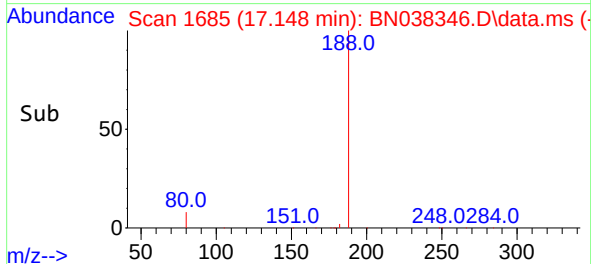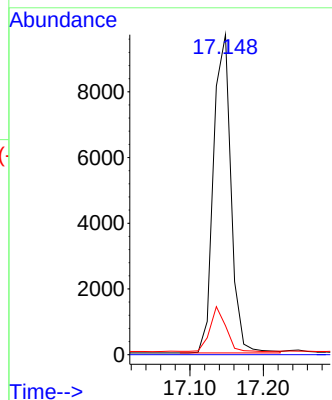

#27
Fluoranthene-d10
Concen: 0.360 ng
RT: 19.183 min Scan# 1939
Delta R.T. -0.005 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion:	212	Resp:	14269
Ion Ratio	Lower	Upper	
212	100		
106	17.9	13.7	20.5
104	9.7	7.8	11.8


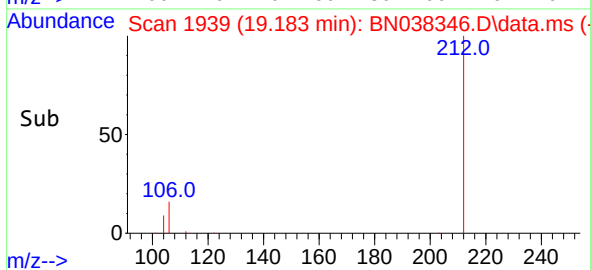
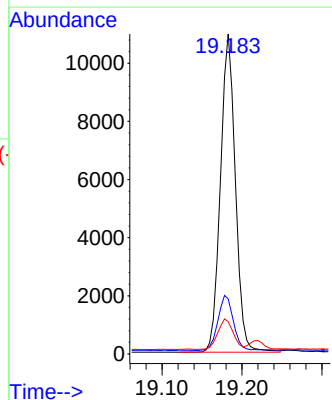
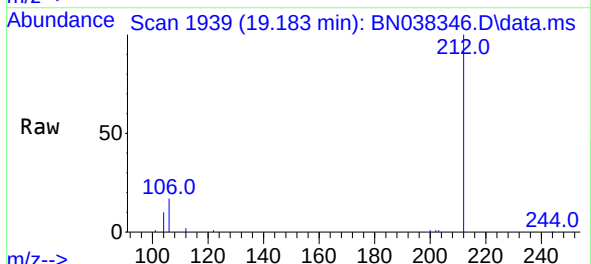




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.339 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12




Instrument :
BNA_N
ClientSampleId :
BR-04DR-451-120825


Tgt Ion:240 Resp: 12704
Ion Ratio Lower Upper
240 100
120 17.1 15.4 23.2
236 29.3 23.9 35.9

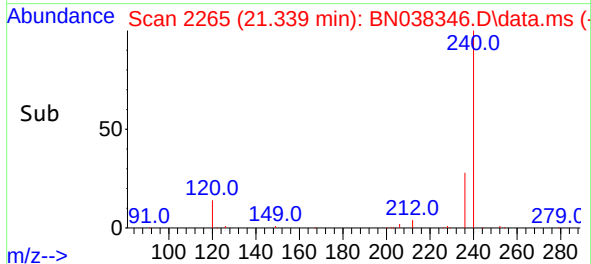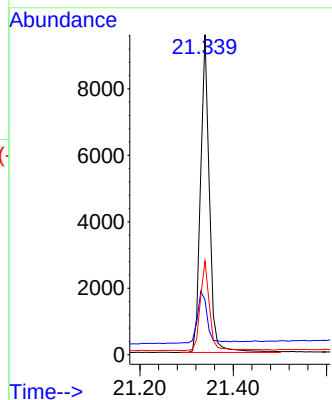

#31
Terphenyl-d14
Concen: 0.423 ng
RT: 19.782 min Scan# 2068
Delta R.T. -0.009 min
Lab File: BN038346.D
Acq: 12 Dec 2025 11:12

Tgt Ion:244 Resp: 12001
Ion Ratio Lower Upper
244 100
212 9.5 7.9 11.9
122 21.0 15.0 22.6

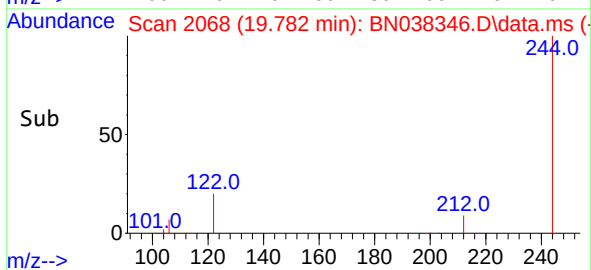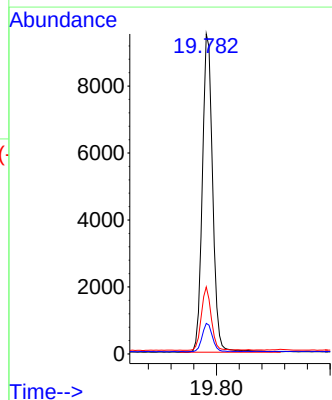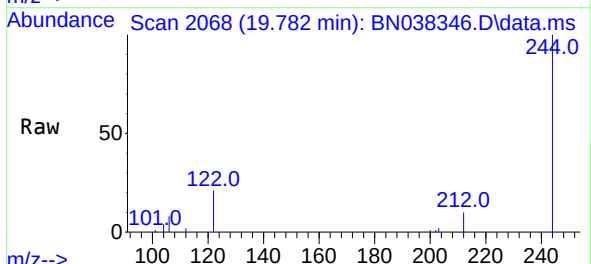




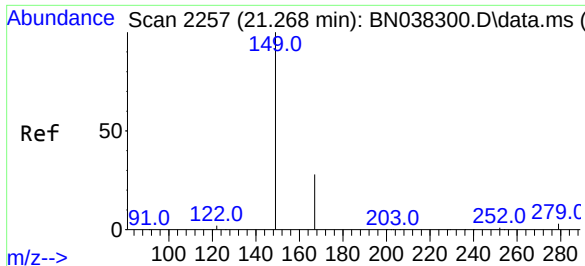


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.214 ng
 RT: 21.259 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN038346.D
 Acq: 12 Dec 2025 11:12

Instrument :
 BNA_N
 ClientSampleId :
 BR-04DR-451-120825

Tgt Ion:149 Resp: 5763

Ion	Ratio	Lower	Upper
149	100		
167	25.1	21.4	32.0
279	3.0	2.4	3.6

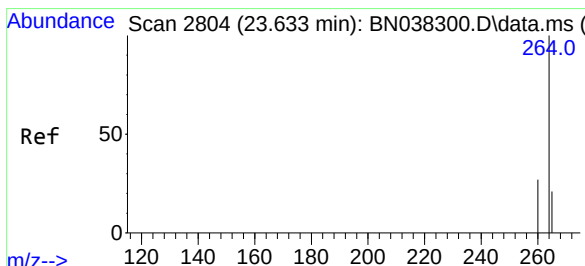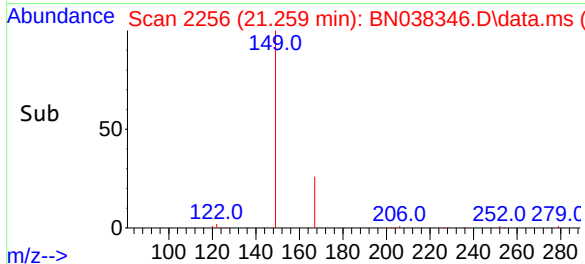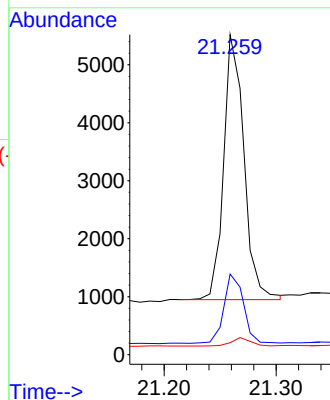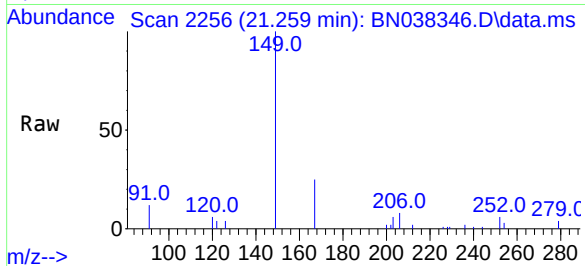

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.627 min Scan# 2802
 Delta R.T. -0.006 min
 Lab File: BN038346.D
 Acq: 12 Dec 2025 11:12

Tgt Ion:264 Resp: 12519

Ion	Ratio	Lower	Upper
264	100		
260	27.4	22.2	33.2
265	91.3	80.2	120.2

