


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN121025\
Data File : VN088486.D
Acq On : 10 Dec 2025 09:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112425W.M
Title : SW846 8260
Last Update : Tue Nov 25 01:34:52 2025

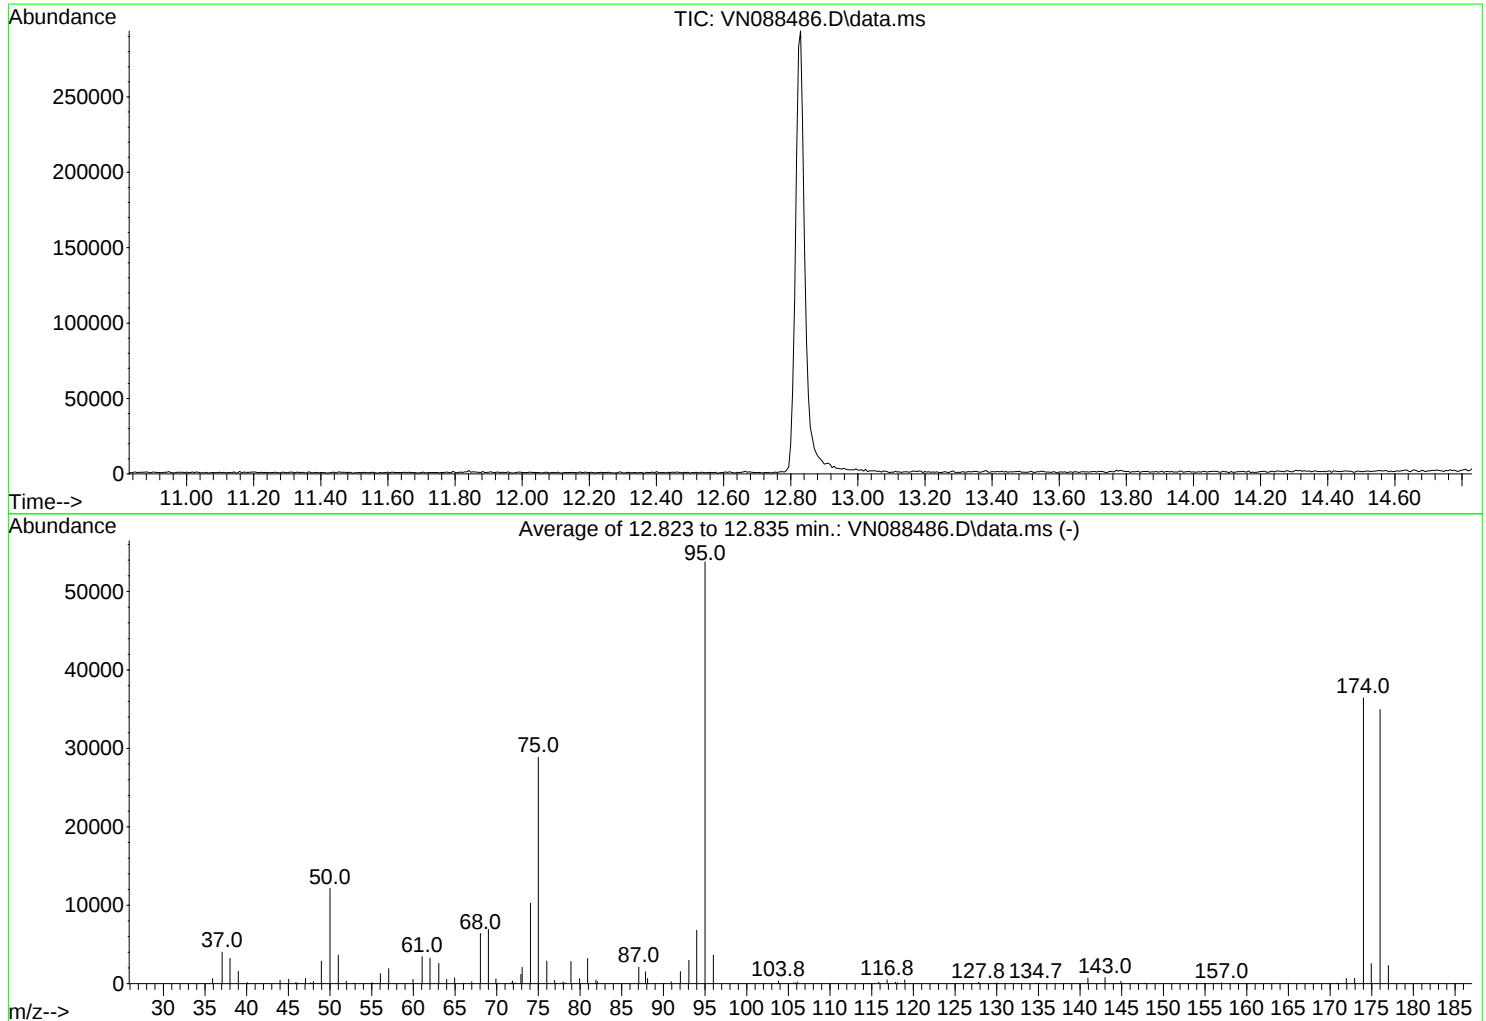

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	12138	PASS
75	95	30	60	53.7	28864	PASS
95	95	100	100	100.0	53787	PASS
96	95	5	9	6.8	3638	PASS
173	174	0.00	2	1.9	705	PASS
174	95	50	100	67.7	36437	PASS
175	174	5	9	7.0	2550	PASS
176	174	95	101	95.9	34960	PASS
177	176	5	9	6.6	2300	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	633	48.00	275	61.05	3456	71.90	321
37.05	4024	48.95	2868	62.00	3257	72.20	90
38.00	3221	50.00	12138	63.05	2595	72.90	118
39.00	1574	51.00	3627	64.00	541	73.05	207
40.10	144	51.95	300	64.95	737	74.05	10249
44.00	426	52.90	61	66.00	56	75.00	28864
45.05	569	54.90	78	67.00	248	76.00	2869
45.90	158	55.10	95	68.05	6399	76.95	415
46.10	64	56.05	1274	69.00	6922	77.20	68
47.05	671	57.05	1927	69.90	633	77.70	58
47.70	132	59.95	560	71.70	114	77.95	231

Average of 12.823 to 12.835 min.: VN088486.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.20	128	93.05	2978	118.10	124	147.80	59
78.90	2843	94.00	6804	118.95	460	155.00	52
79.95	653	95.00	53787	127.80	161	157.00	106
80.90	3200	96.00	3638	128.00	51	170.80	68
81.90	474	103.80	332	129.80	52	171.95	680
82.10	244	105.60	74	130.10	87	172.95	705
87.05	2099	105.80	113	134.70	68	174.00	36437
87.85	1506	106.05	228	135.10	55	174.95	2550
88.10	645	115.85	178	140.95	720	176.00	34960
90.95	248	116.85	491	143.00	775	177.00	2300
92.05	1527	117.85	188	144.90	312		

Instrument :

MSVOA_N

ClientSampleId :

BFB