




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
Data File : VV039540.D
Acq On : 11 Dec 2025 14:29
Operator : SY/MD
Sample : Q3828-07
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OWBR-03-138-120925-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/12/2025
Supervised By :Mahesh Dadoda 12/12/2025

Quant Time: Dec 12 00:48:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

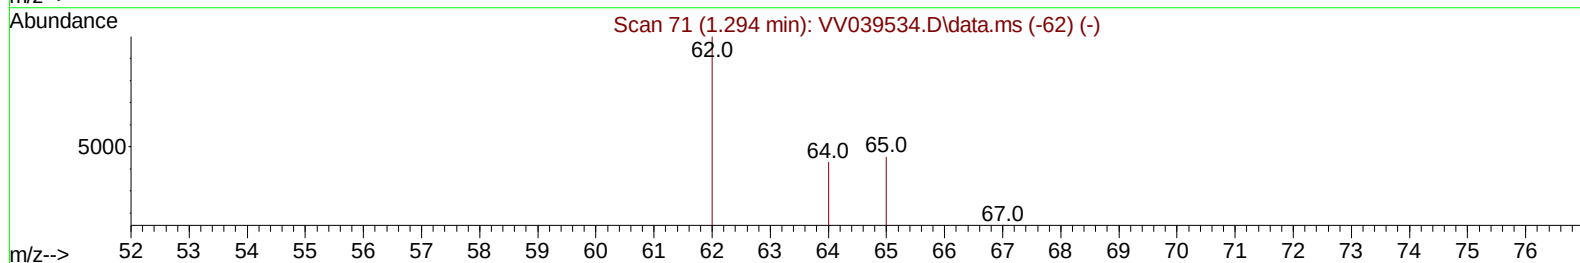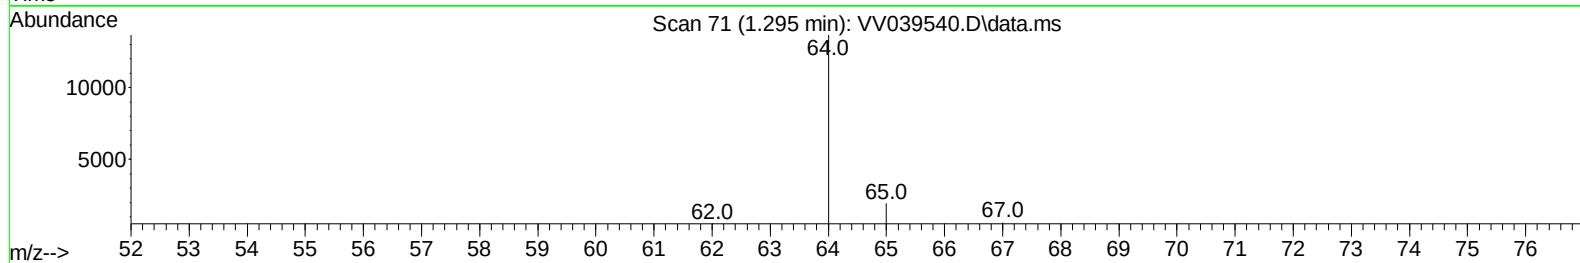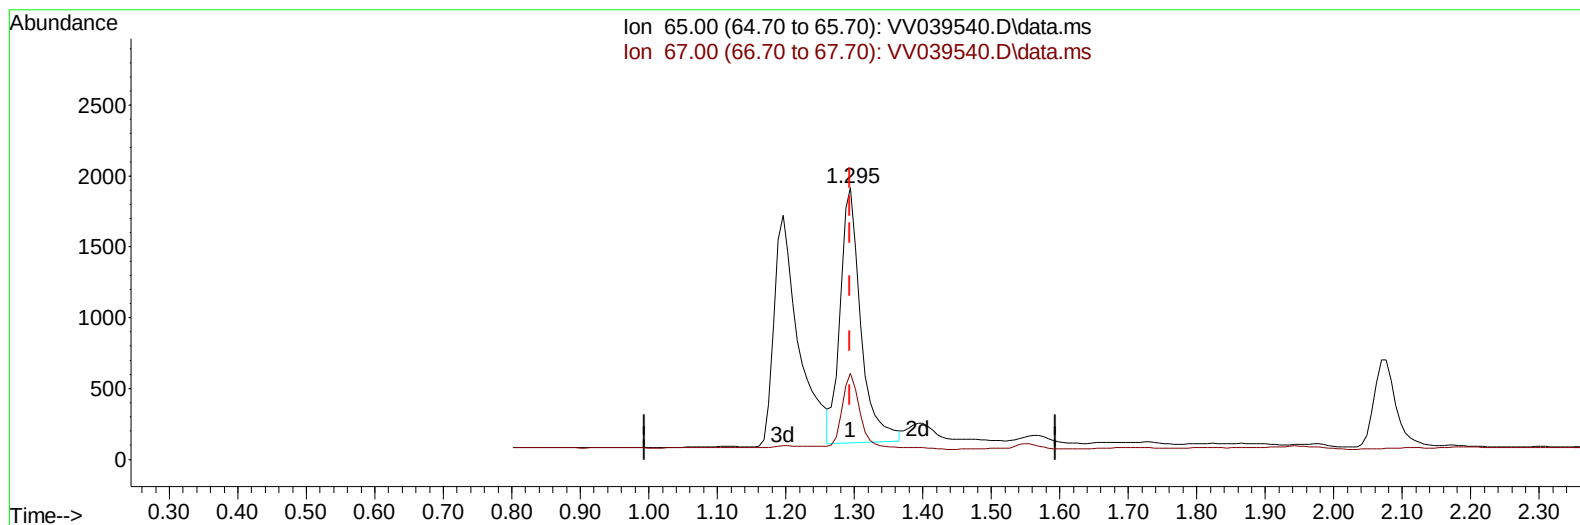

TIC: VV039540.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.66 ug/L

response 3744

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	27.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
Data File : VV039540.D
Acq On : 11 Dec 2025 14:29
Operator : SY/MD
Sample : Q3828-07
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OWBR-03-138-120925-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/12/2025
Supervised By :Mahesh Dadoda 12/12/2025

Quant Time: Dec 12 00:48:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

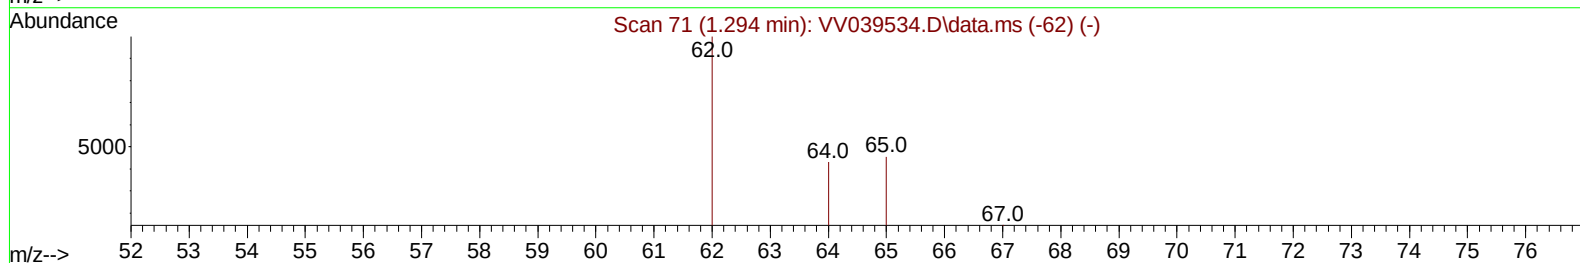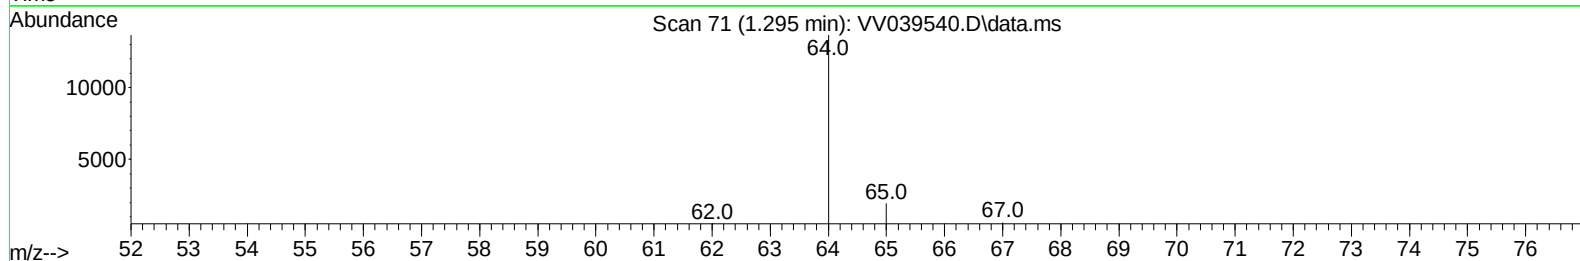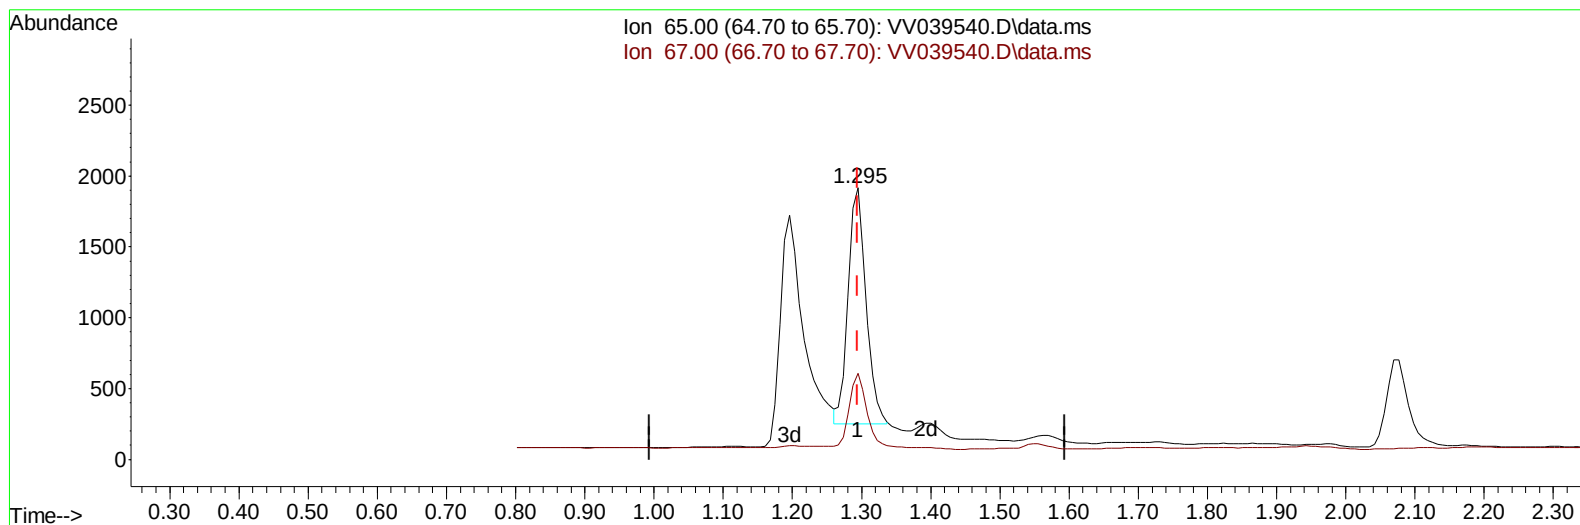

TIC: VV039540.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.52 ug/L m

response 2964

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	34.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
 Data File : VV039540.D
 Acq On : 11 Dec 2025 14:29
 Operator : SY/MD
 Sample : Q3828-07
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OWBR-03-138-120925-SIM

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 12/12/2025
 Supervised By : Mahesh Dadoda 12/12/2025

Quant Time: Dec 12 00:48:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 09 08:40:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5770	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.801	117	5766	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.175	152	3147	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.295	65	2964m	0.523	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	104.000%		
4) 1,2-Dichloroethane-d4	4.994	65	1814	0.472	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
7) 1,2-Dichloropropane-d6	5.996	67	2040	0.419	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.254	98	3750	0.457	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1514	0.552	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	110.000%		
Target Compounds						
3) Vinyl chloride	1.295	62	755	0.060	ug/L	Qvalue # 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV121125\
Data File : VV039540.D
Acq On : 11 Dec 2025 14:29
Operator : SY/MD
Sample : Q3828-07
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OWBR-03-138-120925-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/12/2025
Supervised By :Mahesh Dadoda 12/12/2025

Quant Time: Dec 12 00:48:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 09 08:40:48 2025
Response via : Initial Calibration

