

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121225\
 Data File : PD091576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2025 12:35
 Operator : AR\AJ
 Sample : Q3832-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 S-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/15/2025
 Supervised By :Yogesh Patel 12/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:48:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 04:29:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.869	77471408	1018.2E6	22.305m	25.840m
28)	SA Decachlor...	9.060	8.055	76554613	713.3E6	14.728	17.225

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121225\
Data File : PD091576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2025 12:35
Operator : AR\AJ
Sample : Q3832-03
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
S-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/15/2025
Supervised By : Yogesh Patel 12/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:48:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

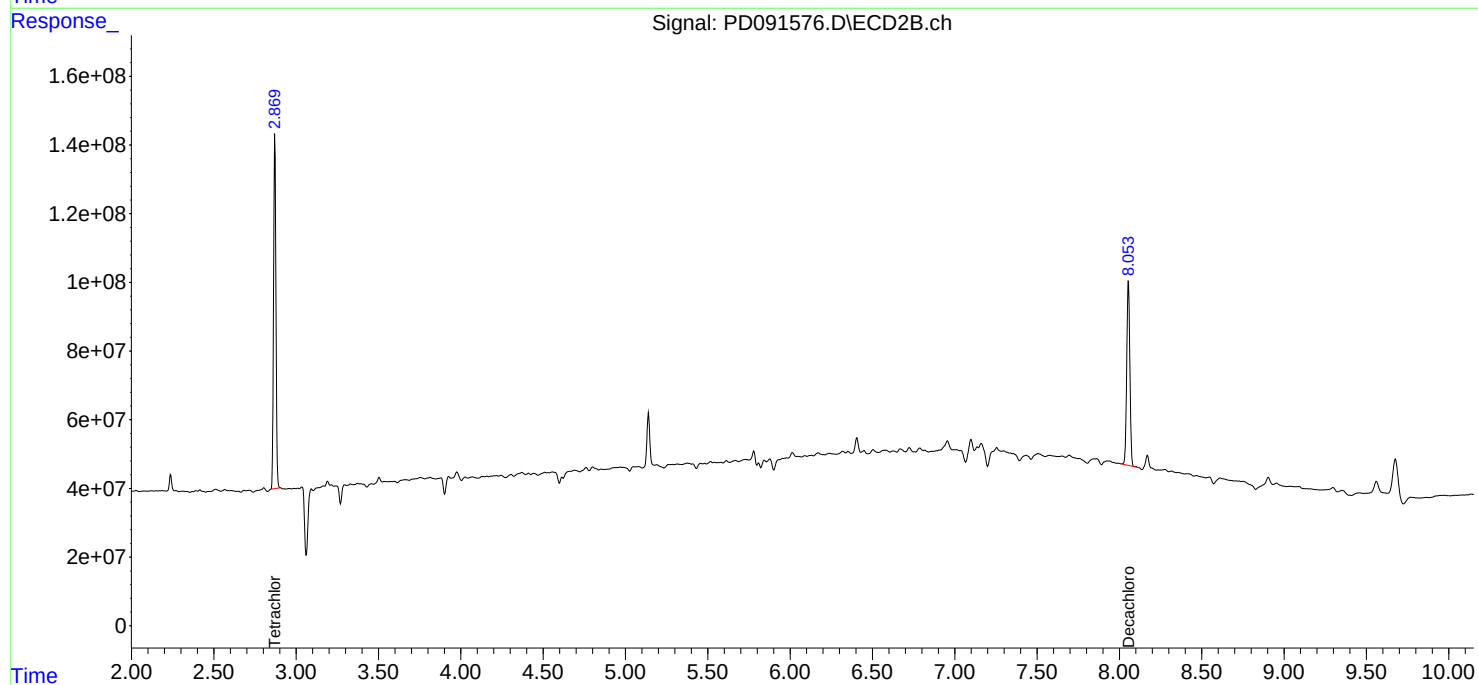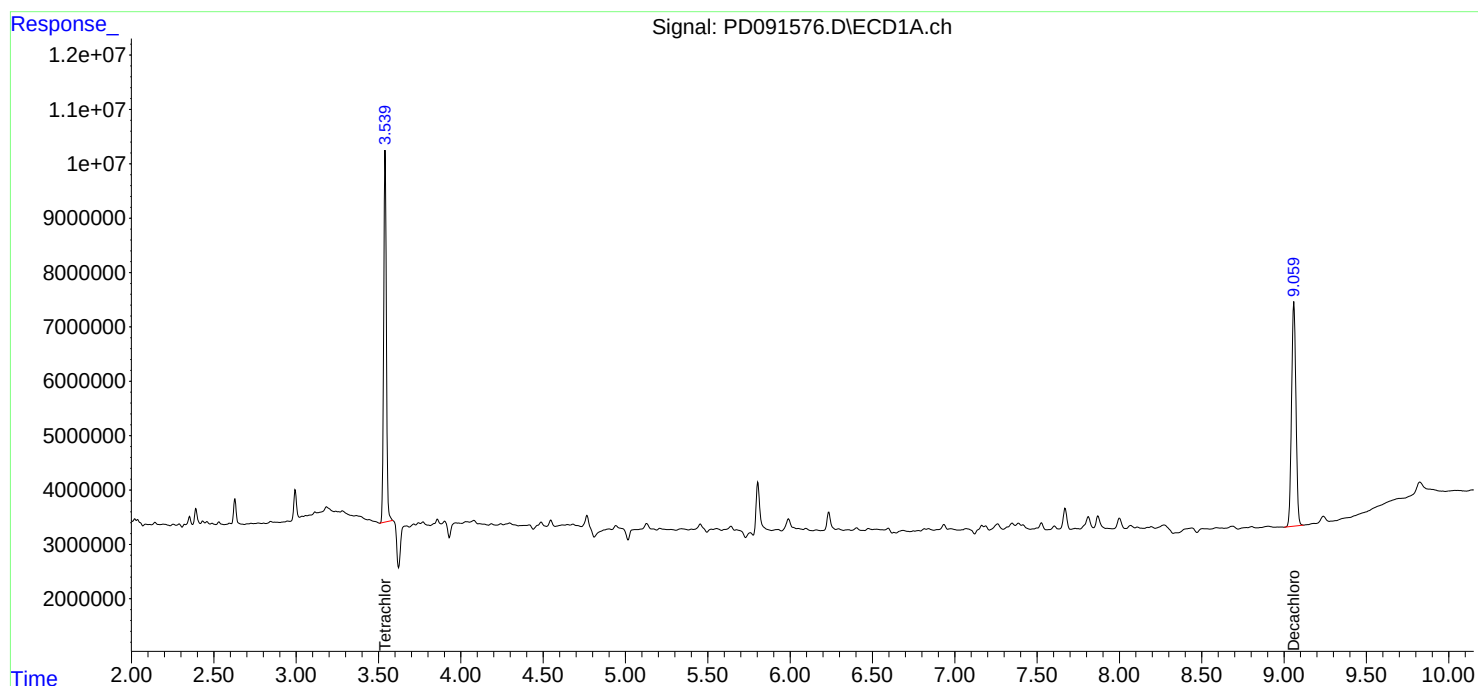

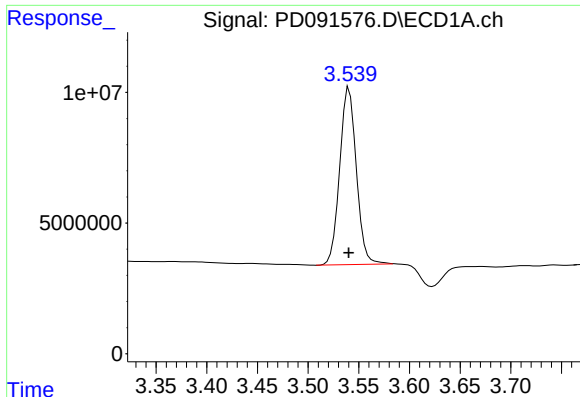


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 77471408
Conc: 22.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
S-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/15/2025
Supervised By :Yogesh Patel 12/15/2025

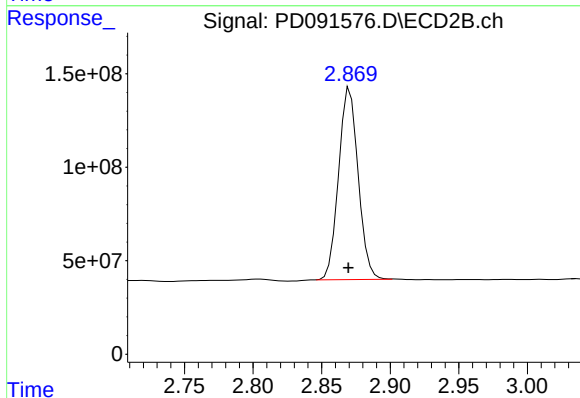


#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 1018169319
Conc: 25.84 ng/ml m

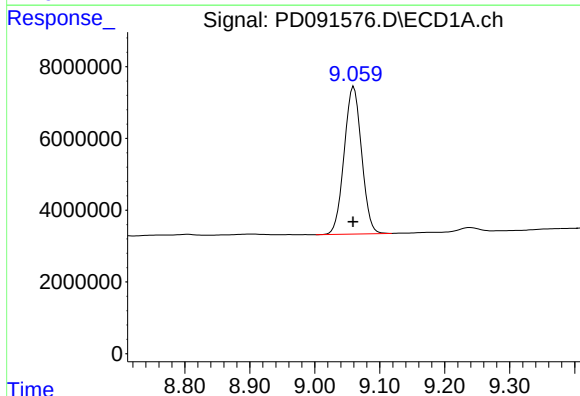

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 76554613
Conc: 14.73 ng/ml

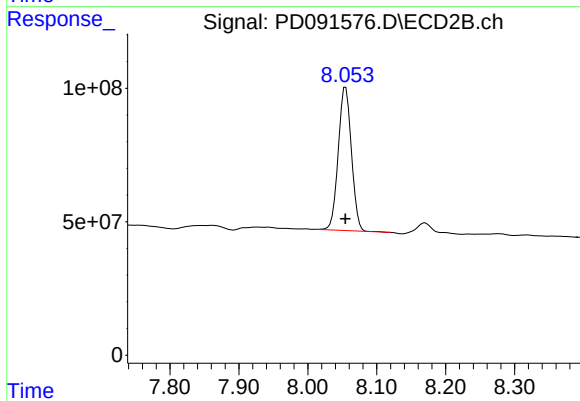

#28 Decachlorobiphenyl

R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 713319875
Conc: 17.23 ng/ml