
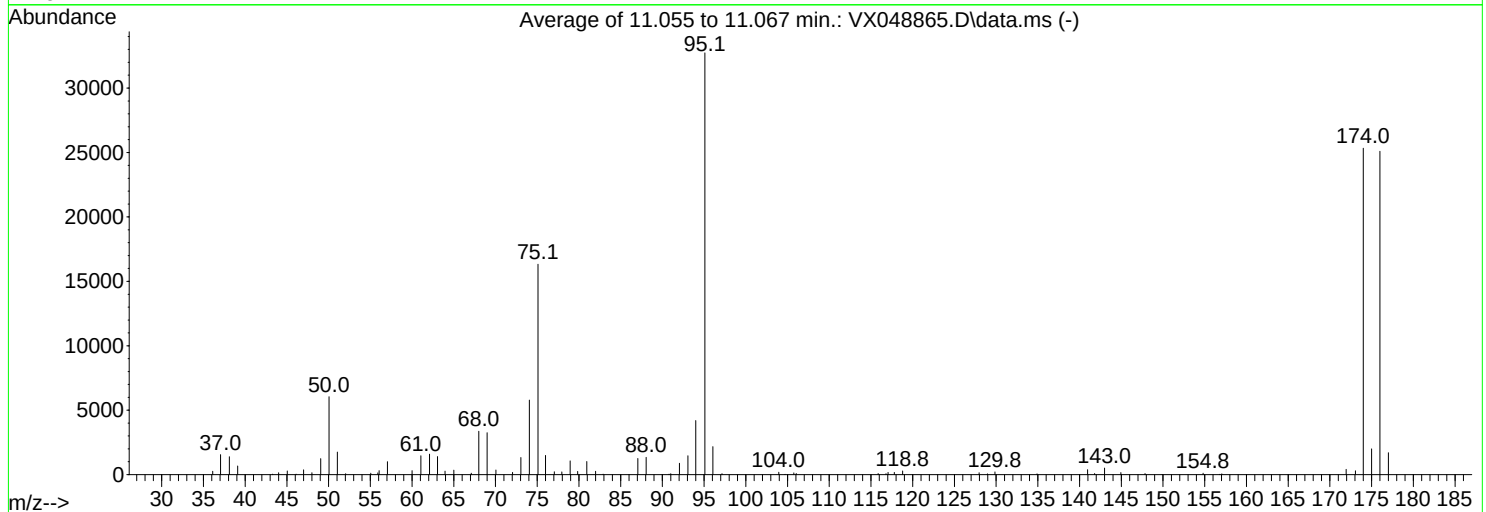


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX121525\  
Data File : VX048865.D  
Acq On : 15 Dec 2025 08:18  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120425W.M  
Title : SW846 8260  
Last Update : Tue Dec 16 14:10:57 2025

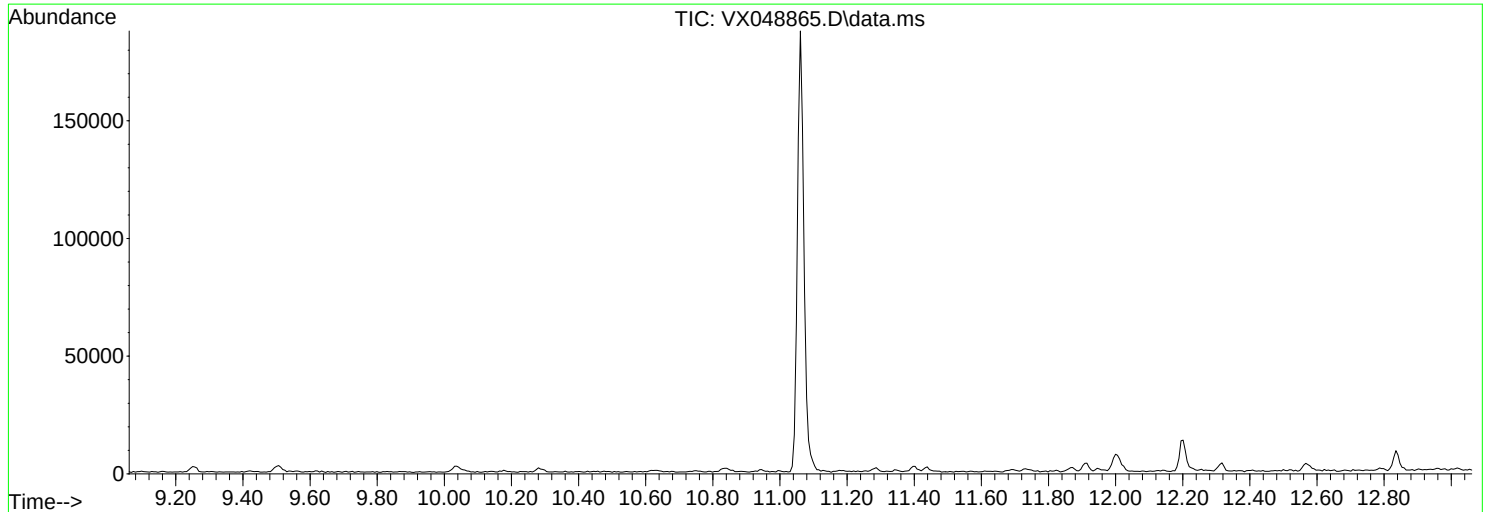

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.5  | 6044  | PASS      |
| 75     | 95      | 30     | 60     | 49.9  | 16332 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 32733 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 2177  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.2   | 299   | PASS      |
| 174    | 95      | 50     | 100    | 77.4  | 25333 | PASS      |
| 175    | 174     | 5      | 9      | 7.9   | 2005  | PASS      |
| 176    | 174     | 95     | 101    | 99.1  | 25093 | PASS      |
| 177    | 176     | 5      | 9      | 6.8   | 1702  | PASS      |