

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : LM

3/19/2015 14:26

Test: CN EPA

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.424	0.0	0.094	
ICB1	-0.294	0.0	0.005	
CCV1	240.438	0.0	0.226	
CCB1	-0.786	0.0	0.004	
PB82199BLS	-0.945	0.0	0.004	
G1565-05	-0.092	0.0	0.005	
G1565-05D	-0.244	0.0	0.005	
G1565-05S	93.945	0.0	0.091	
G1565-07	1.912	0.0	0.007	
G1565-08	-0.069	0.0	0.005	
G1565-12	0.071	0.0	0.005	
G1565-13	1.167	0.0	0.006	
G1565-14	-0.023	0.0	0.005	
G1565-06	0.764	0.0	0.006	
CCV2	251.863	0.0	0.237	
CCB2	-0.302	0.0	0.005	
N	16			
Mean	42.739			
SD	85.6931			
CV%	200.50			

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 19 13:13:44 2015

Thu Mar 19 14:21:25 2015

MM

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
S0.0	A	CN EPA	P	-0.0707	µg/l	3/19/2015 13:13:44	
S5.0	A	CN EPA	P	4.5062	µg/l	3/19/2015 13:13:45	
S10.0	A	CN EPA	P	9.0065	µg/l	3/19/2015 13:13:46	
S100.0	A	CN EPA	P	100.2342	µg/l	3/19/2015 13:13:47	
S250.0	A	CN EPA	P	252.6916	µg/l	3/19/2015 13:13:48	
S500.0	A	CN EPA	P	498.6322	µg/l	3/19/2015 13:13:49	
ICV1	S	CN EPA	P	96.4241	µg/l	3/19/2015 14:05:39	
ICB1	S	CN EPA	P	-0.2943	µg/l	3/19/2015 14:05:40	
CCV1	S	CN EPA	P	240.4377	µg/l	3/19/2015 14:05:41	
CCB1	S	CN EPA	P	-0.7864	µg/l	3/19/2015 14:05:42	
PB82199BLS	S	CN EPA	P	-0.9446	µg/l	3/19/2015 14:05:43	
G1565-05	S	CN EPA	P	-0.0924	µg/l	3/19/2015 14:05:44	
G1565-05D	S	CN EPA	P	-0.2439	µg/l	3/19/2015 14:05:45	
G1565-05S	S	CN EPA	P	93.945	µg/l	3/19/2015 14:05:46	
G1565-07	S	CN EPA	P	1.9121	µg/l	3/19/2015 14:05:48	
G1565-08	S	CN EPA	P	-0.0694	µg/l	3/19/2015 14:05:49	
G1565-12	S	CN EPA	P	0.0714	µg/l	3/19/2015 14:10:54	
G1565-13	S	CN EPA	P	1.1665	µg/l	3/19/2015 14:10:55	
G1565-14	S	CN EPA	P	-0.0229	µg/l	3/19/2015 14:10:56	
G1565-06	S	CN EPA	P	0.7644	µg/l	3/19/2015 14:19:11	
CCV2	S	CN EPA	P	251.8633	µg/l	3/19/2015 14:21:24	
CCB2	S	CN EPA	P	-0.3018	µg/l	3/19/2015 14:21:25	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : hm

3/19/2015 13:31


Test CN EPA

Accepted 3/19/2015 13:31

Factor 1085
Bias 0.005

Coeff. of det. 0.999947

Errors

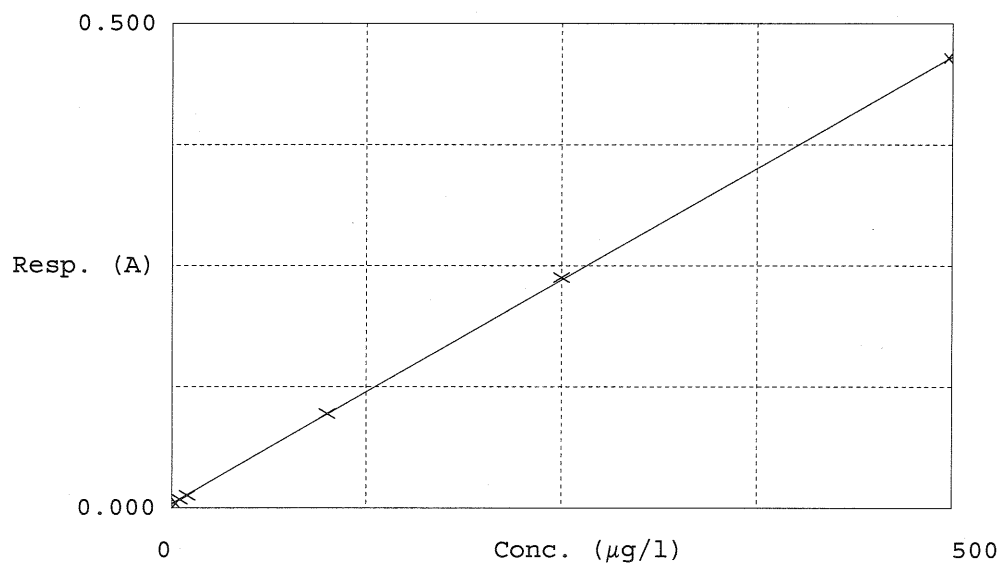

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.005	-0.0707	0.0000	
2	5.0PPBCN	0.009	4.5062	5.0000	
3	10PPBCN	0.013	9.0065	10.0000	
4	100PPBCN	0.097	100.2342	100.0000	
5	250PPBCN	0.238	252.6916	250.0000	
6	500PPBCN	0.464	498.6322	500.0000	