

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
 Data File : PD056851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:02
 Operator : AJ\MA
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 05:54:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 03 05:45:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	16994838	31088410	20.000	20.000
27)	SA Decachlor...	7.960	8.998	38876205	58192255	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.713	4.347	24592679	43534504	20.000	20.000
3)	MA gamma-BHC...	3.988	4.630	23658385	41776611	20.000	20.000
4)	MA Heptachlor	4.274	5.136	22064775	42131693	20.000	20.000
9)	A Endosulfan I	5.280	6.179	19119446	34897171	20.000	20.000
13)	MA Dieldrin	5.519	6.435	42866866	76106604	40.000	40.000
14)	MA Endrin	5.773	6.652	35822270	61686731	40.000	40.000
16)	A 4,4'-DDD	5.908	6.775	32395351	58419309	40.000	40.000
17)	MA 4,4'-DDT	6.143	7.073	29747392	56892432	40.000	40.000
20)	A Methoxychlor	6.692	7.530	80902252	158.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:02
Operator : AJ\MA
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA3001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 05:54:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 05:45:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

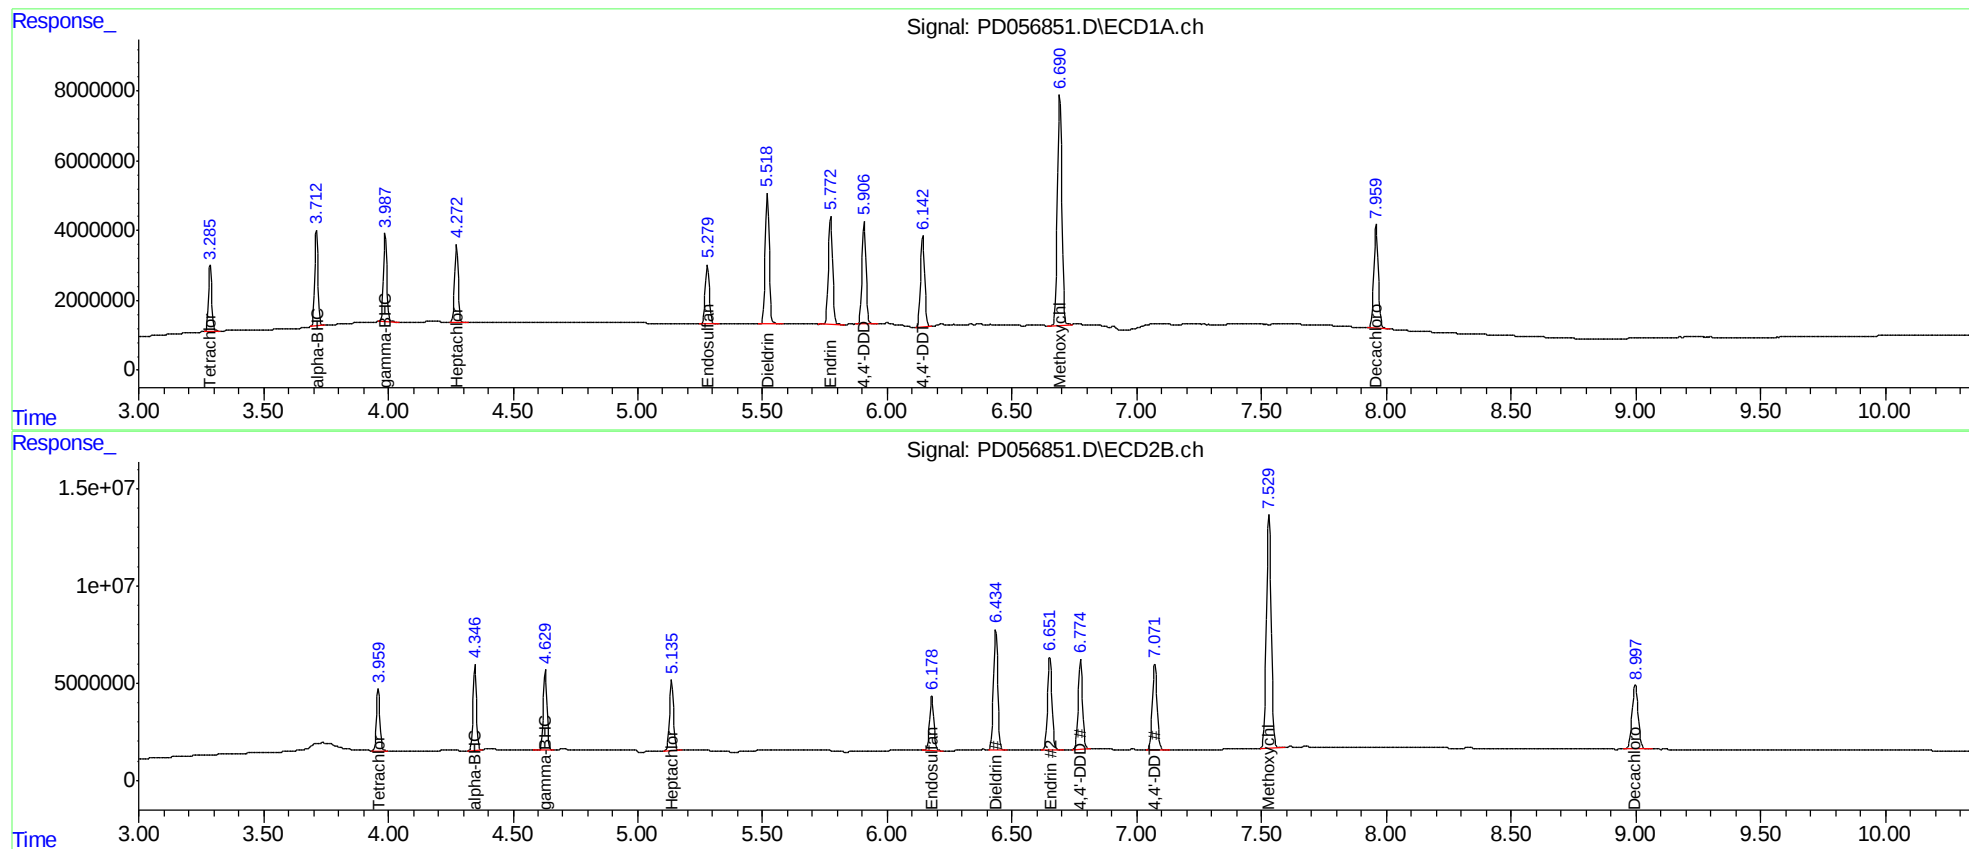


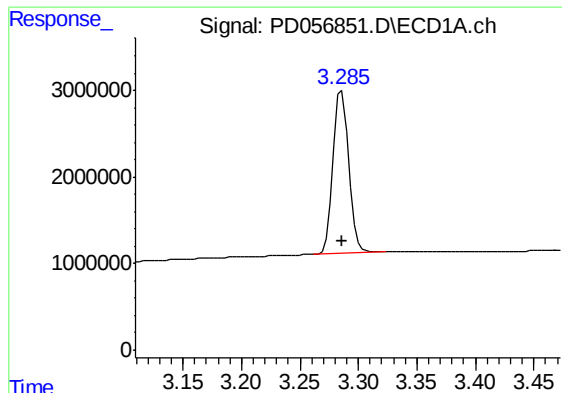

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: 0.000 min
Response: 16994838
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

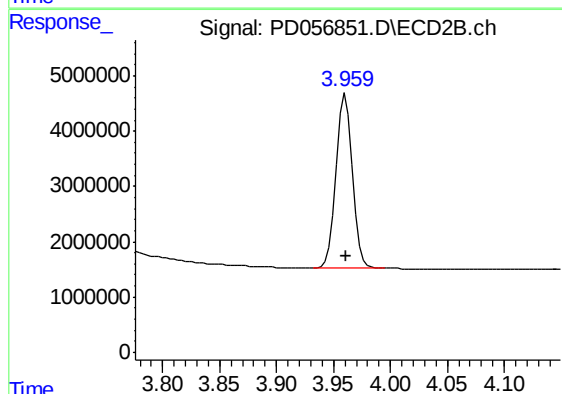


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 31088410
Conc: 20.00 ng/ml

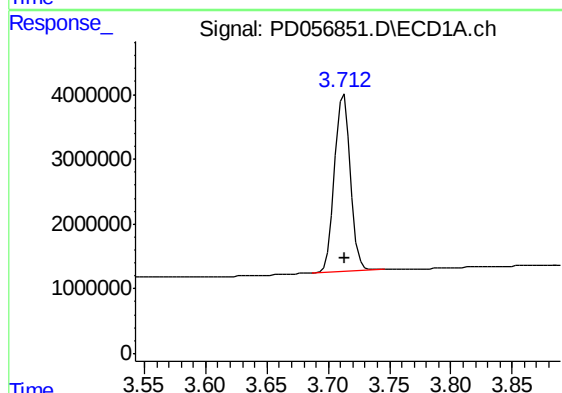


#2 alpha-BHC

R.T.: 3.713 min
Delta R.T.: 0.000 min
Response: 24592679
Conc: 20.00 ng/ml

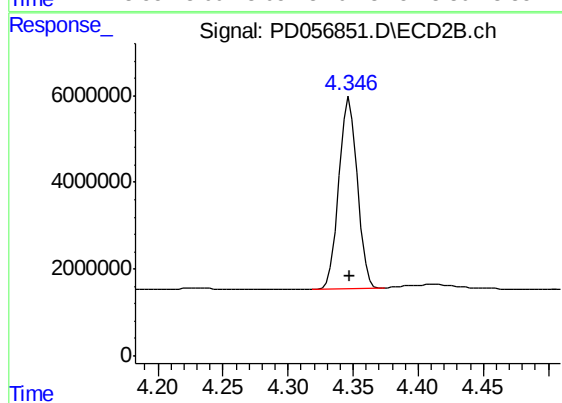

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 43534504
Conc: 20.00 ng/ml

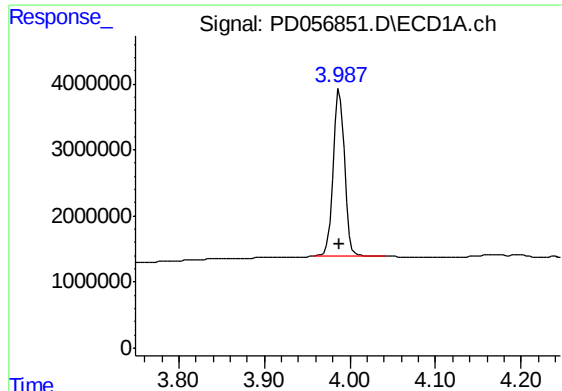

#3 gamma-BHC (Lindane)


R.T.: 3.988 min
Delta R.T.: 0.000 min
Response: 23658385
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

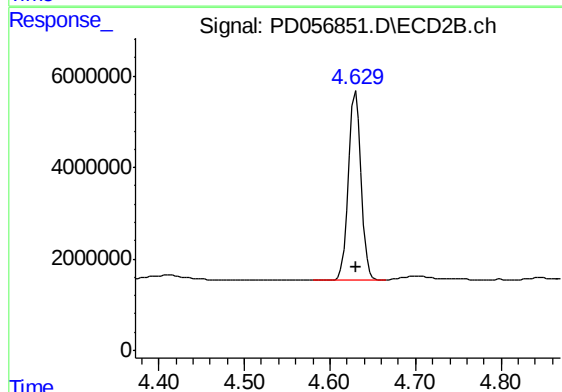


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 41776611
Conc: 20.00 ng/ml

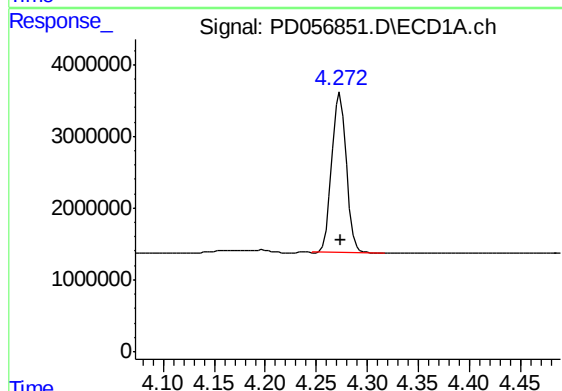


#4 Heptachlor

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 22064775
Conc: 20.00 ng/ml

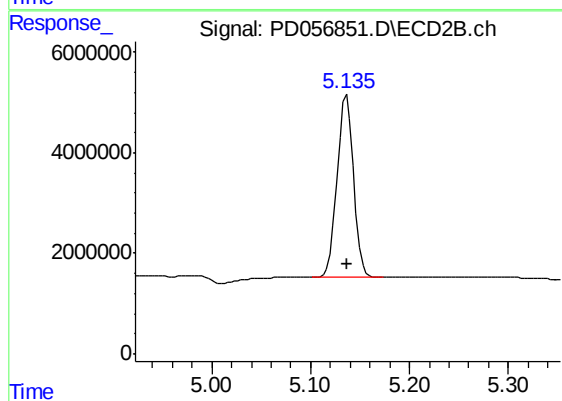

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 42131693
Conc: 20.00 ng/ml

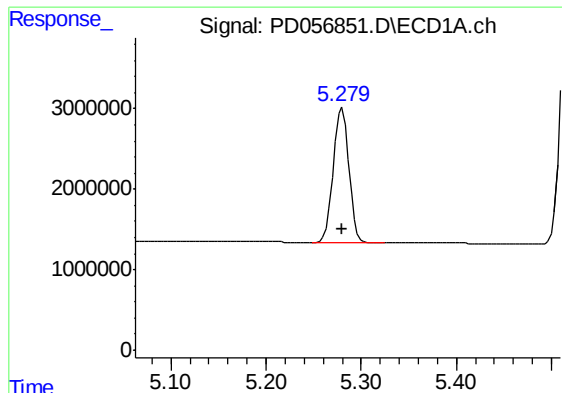

#9 Endosulfan I


R.T.: 5.280 min
Delta R.T.: 0.000 min
Response: 19119446
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

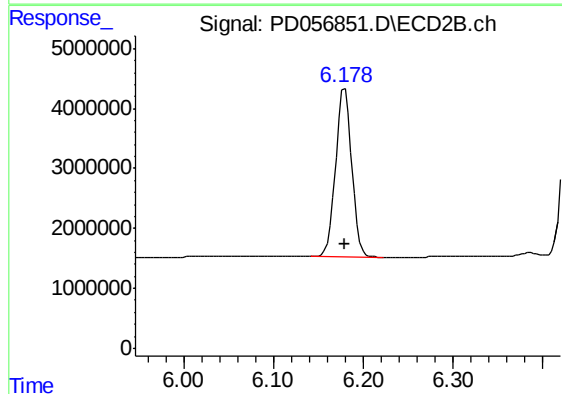


#9 Endosulfan I

R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 34897171
Conc: 20.00 ng/ml

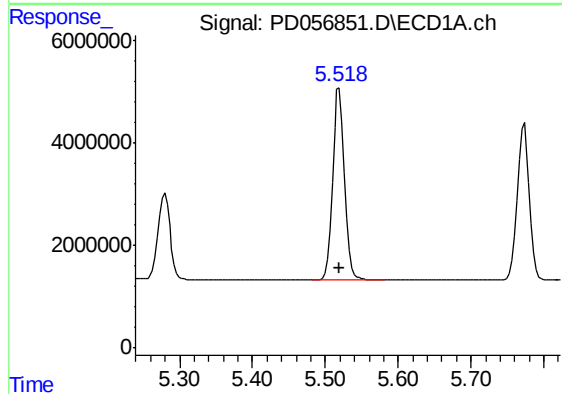


#13 Dieldrin

R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 42866866
Conc: 40.00 ng/ml

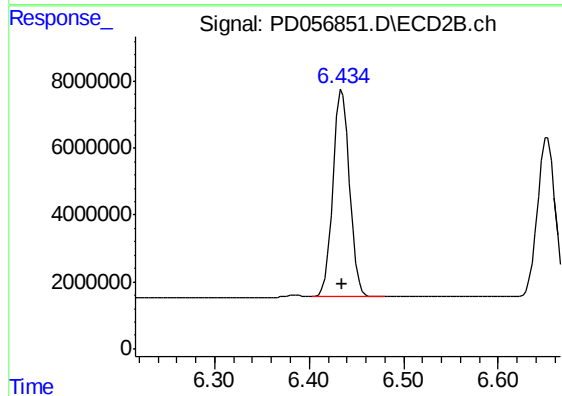

#13 Dieldrin


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 76106604
Conc: 40.00 ng/ml

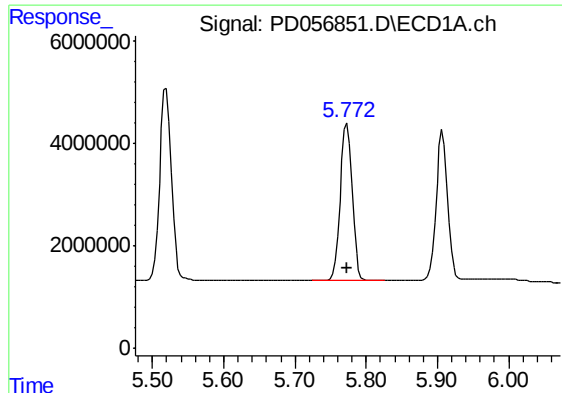

#14 Endrin


R.T.: 5.773 min
Delta R.T.: 0.000 min
Response: 35822270
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

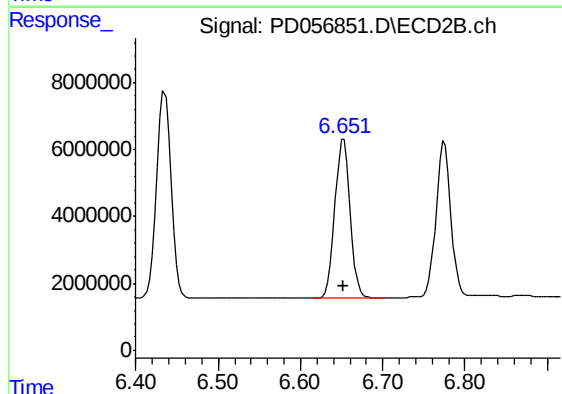


#14 Endrin

R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 61686731
Conc: 40.00 ng/ml

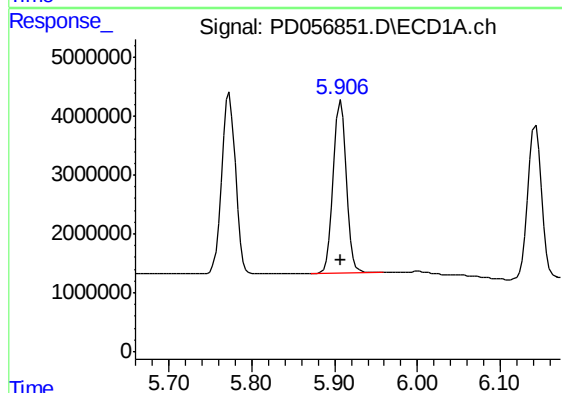


#16 4,4'-DDD

R.T.: 5.908 min
Delta R.T.: 0.000 min
Response: 32395351
Conc: 40.00 ng/ml

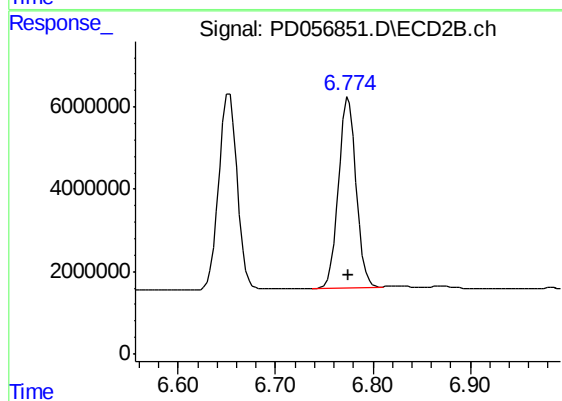

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 58419309
Conc: 40.00 ng/ml

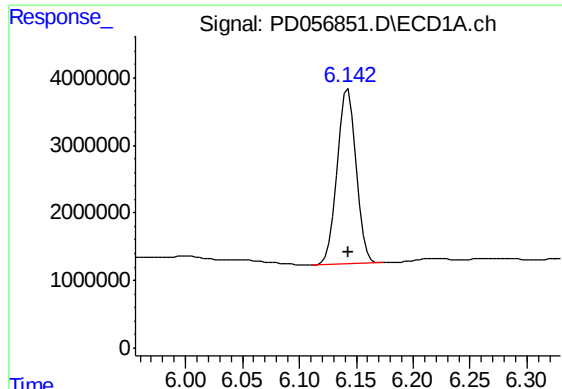

#17 4,4'-DDT


R.T.: 6.143 min
Delta R.T.: 0.000 min
Response: 29747392
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

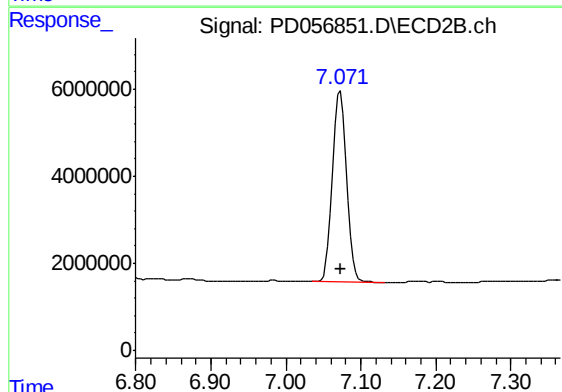


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 56892432
Conc: 40.00 ng/ml

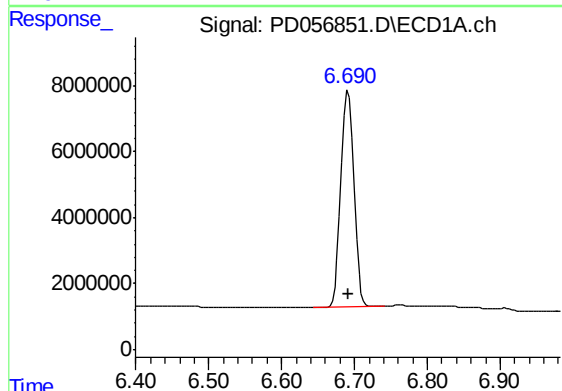


#20 Methoxychlor

R.T.: 6.692 min
Delta R.T.: 0.000 min
Response: 80902252
Conc: 200.00 ng/ml

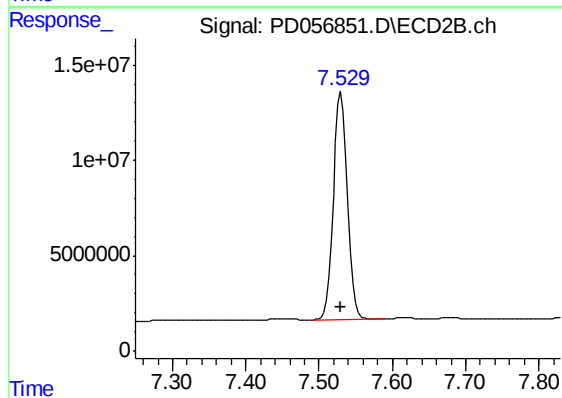

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 158738691
Conc: 200.00 ng/ml

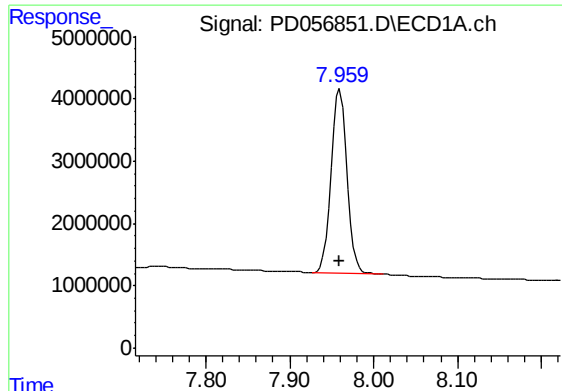

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: 0.000 min
Response: 38876205
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3001

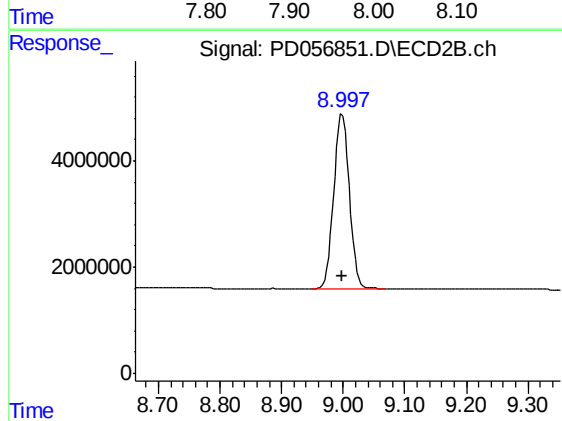

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 58192255
Conc: 40.00 ng/ml