

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
 Data File : PD056853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:30
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 05:54:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 03 05:45:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	33752920	61637480	39.721	39.653
27)	SA Decachlor...	7.959	8.998	74480831	110.8E6	76.634	76.150
Target Compounds							
2)	A alpha-BHC	3.713	4.347	50892231	91111043	41.388	41.857
3)	MA gamma-BHC...	3.987	4.630	48041190	85903273	40.612	41.125
4)	MA Heptachlor	4.273	5.136	44693088	85322234	40.511	40.503
9)	A Endosulfan I	5.279	6.179	38288745	69908414	40.052	40.065
13)	MA Dieldrin	5.520	6.435	88046560	155.7E6	82.158	81.814
14)	MA Endrin	5.772	6.652	71958455	124.4E6	80.351	80.694
16)	A 4,4'-DDD	5.907	6.775	66184151	119.6E6	81.721	81.910
17)	MA 4,4'-DDT	6.142	7.073	64795763	119.6E6	87.128	84.113
20)	A Methoxychlor	6.691	7.530	159.2E6	310.4E6	393.508	391.130


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:30
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
INDA4001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 05:54:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 05:45:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

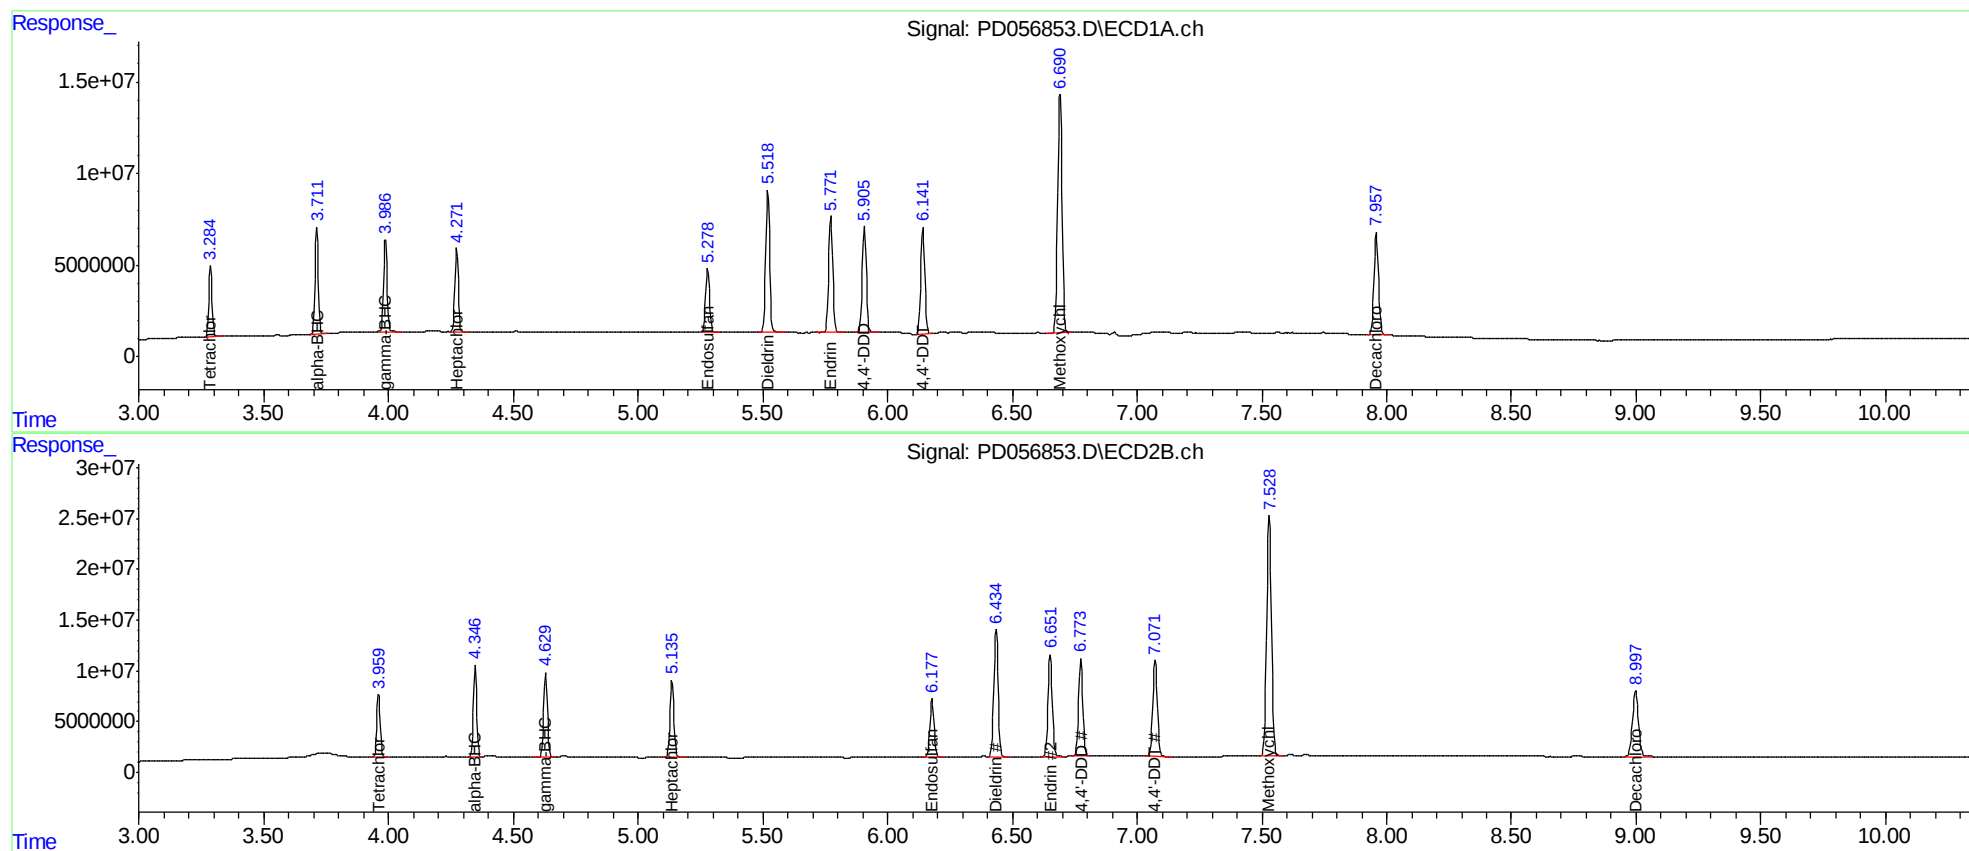


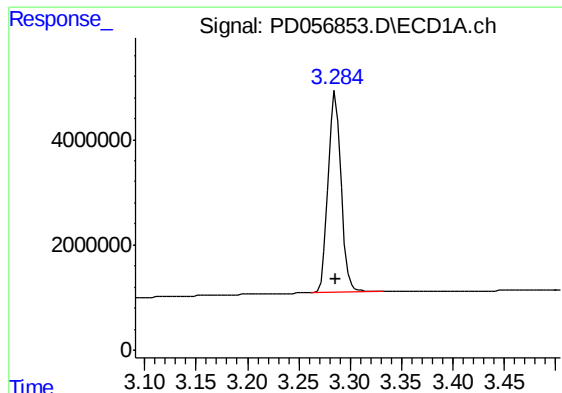

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: 0.000 min
Response: 33752920
Conc: 39.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

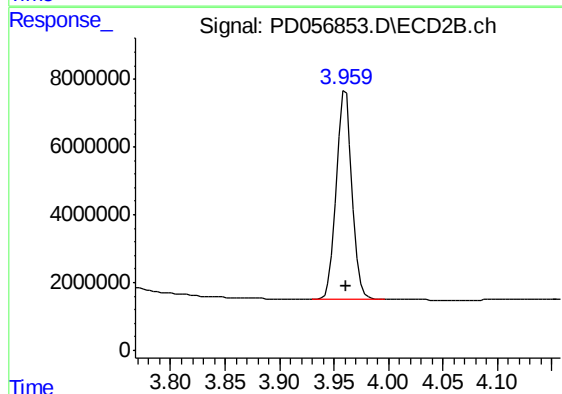


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 61637480
Conc: 39.65 ng/ml

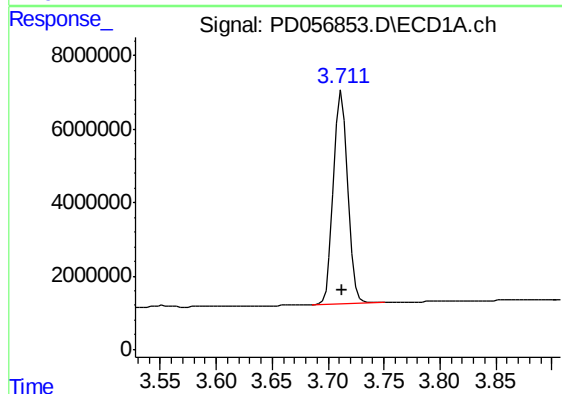


#2 alpha-BHC

R.T.: 3.713 min
Delta R.T.: 0.000 min
Response: 50892231
Conc: 41.39 ng/ml

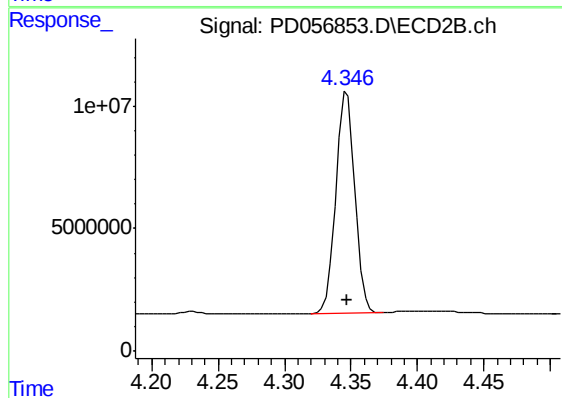

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 91111043
Conc: 41.86 ng/ml

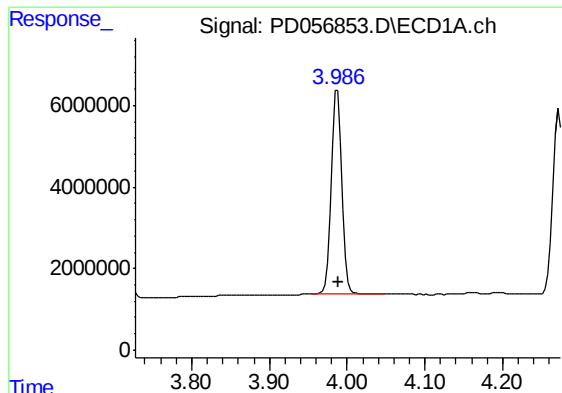

#3 gamma-BHC (Lindane)


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 48041190
Conc: 40.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

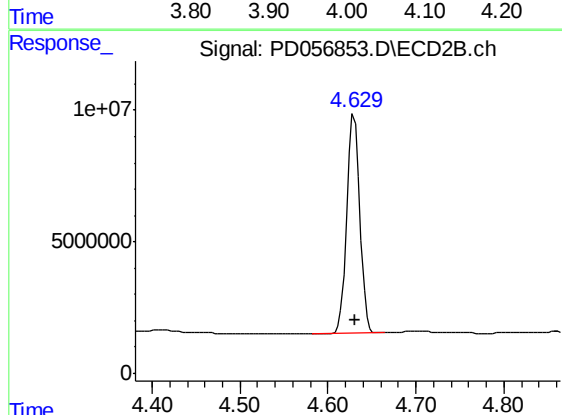


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 85903273
Conc: 41.13 ng/ml

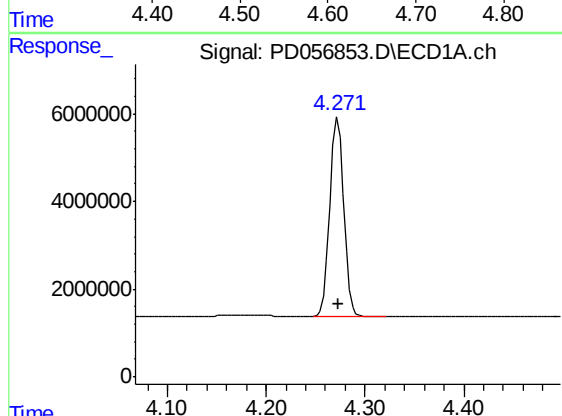


#4 Heptachlor

R.T.: 4.273 min
Delta R.T.: 0.000 min
Response: 44693088
Conc: 40.51 ng/ml

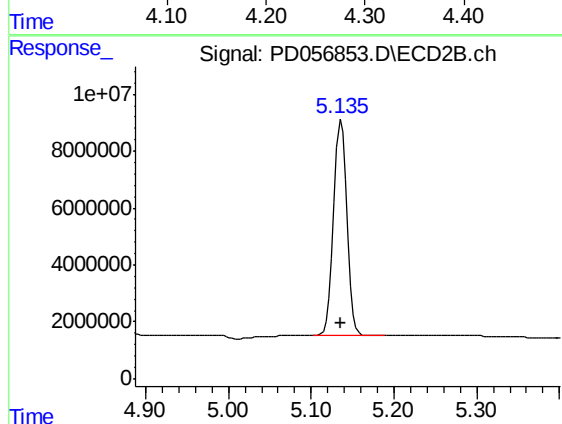

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 85322234
Conc: 40.50 ng/ml

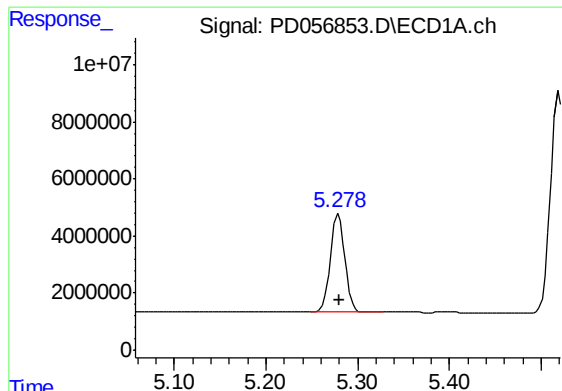

#9 Endosulfan I


R.T.: 5.279 min
Delta R.T.: 0.000 min
Response: 38288745
Conc: 40.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

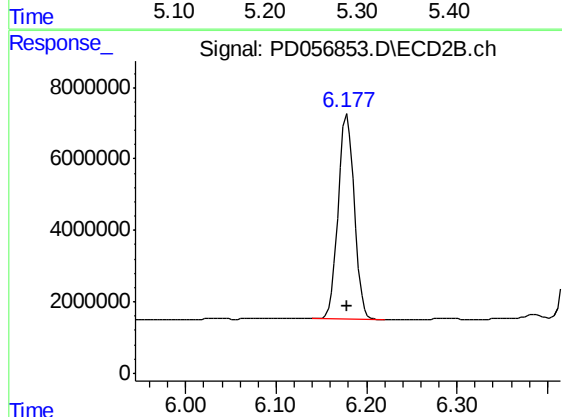


#9 Endosulfan I

R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 69908414
Conc: 40.07 ng/ml

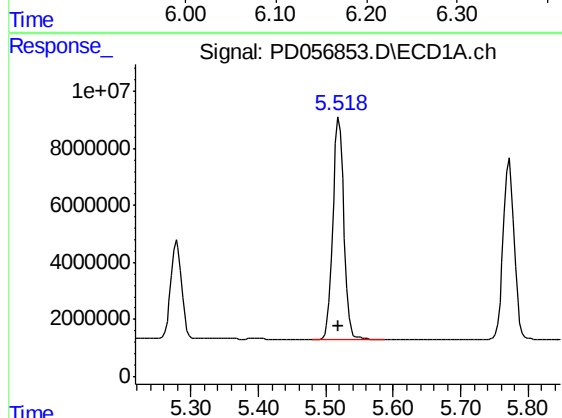


#13 Dieldrin

R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 88046560
Conc: 82.16 ng/ml

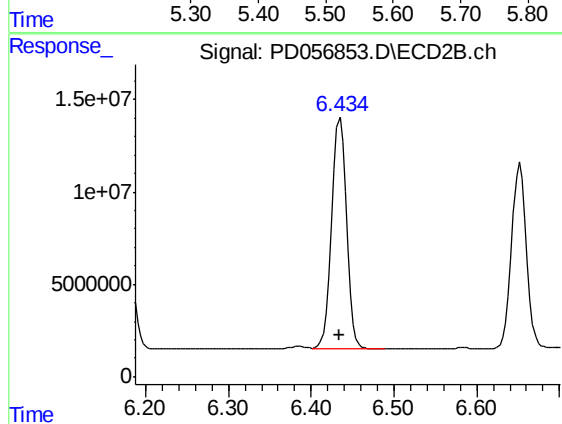

#13 Dieldrin


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 155664579
Conc: 81.81 ng/ml

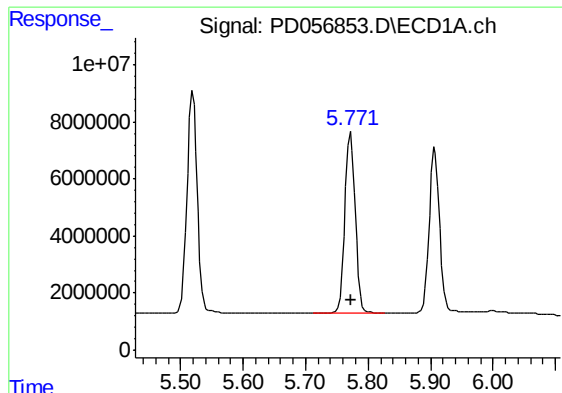

#14 Endrin


R.T.: 5.772 min
Delta R.T.: -0.001 min
Response: 71958455
Conc: 80.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

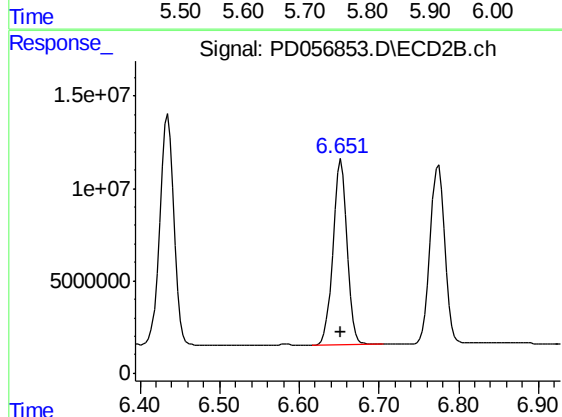


#14 Endrin

R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 124443535
Conc: 80.69 ng/ml

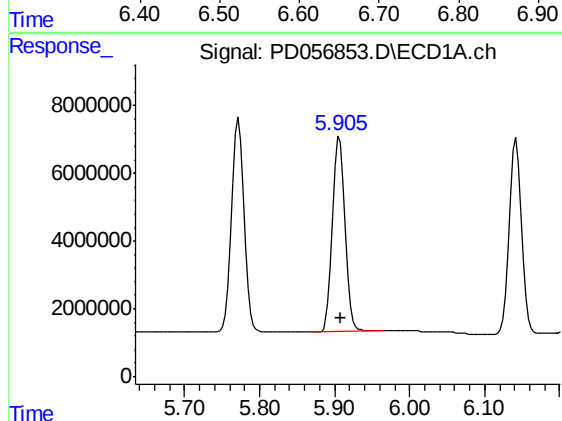


#16 4,4'-DDD

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 66184151
Conc: 81.72 ng/ml

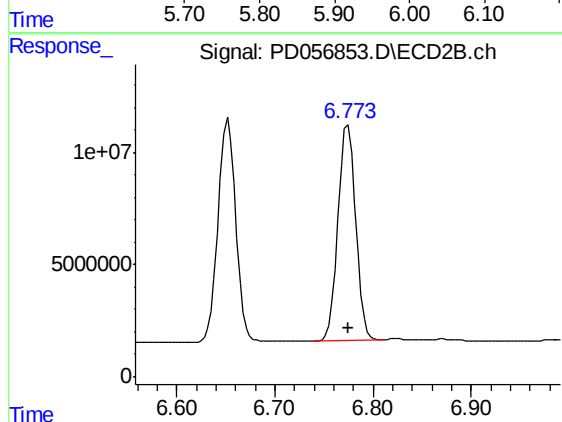

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 119628295
Conc: 81.91 ng/ml

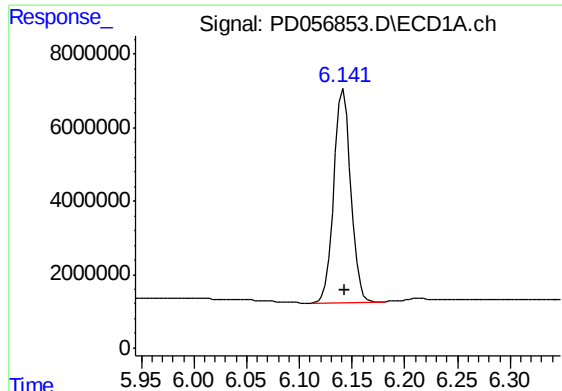

#17 4,4'-DDT


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 64795763
Conc: 87.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

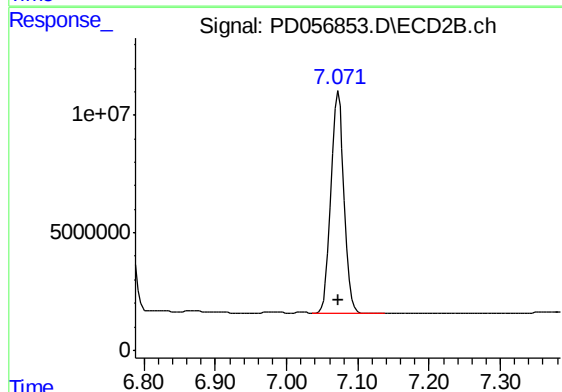


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 119634595
Conc: 84.11 ng/ml

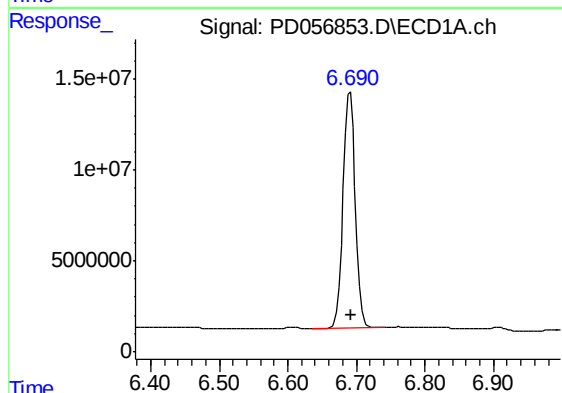


#20 Methoxychlor

R.T.: 6.691 min
Delta R.T.: 0.000 min
Response: 159178559
Conc: 393.51 ng/ml

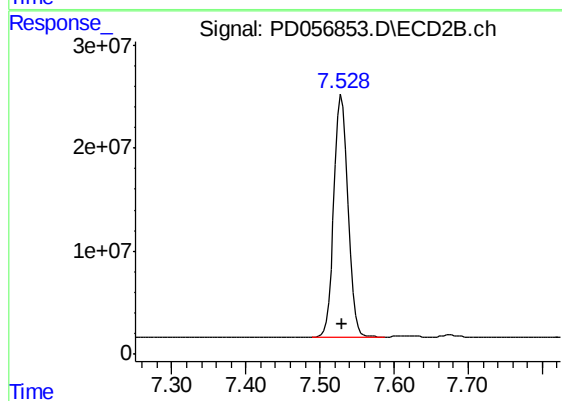

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 310437209
Conc: 391.13 ng/ml

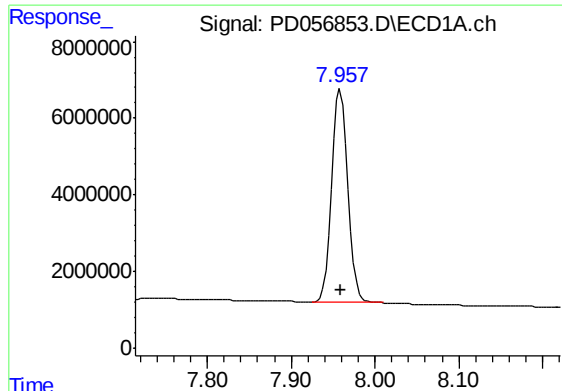

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.001 min
Response: 74480831
Conc: 76.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4001

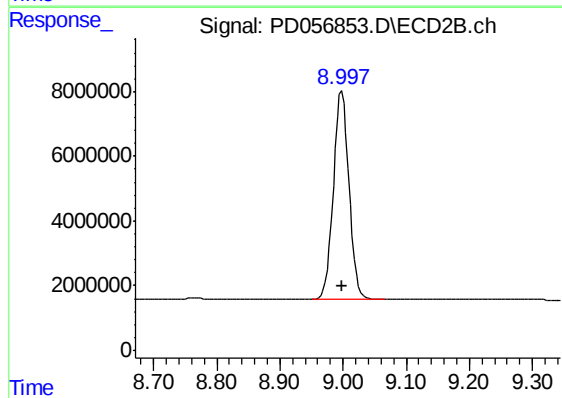

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 110783119
Conc: 76.15 ng/ml