

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
 Data File : PD056855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:58
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 06:00:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 03 05:45:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	66184934	121.4E6	77.888	78.068
27)	SA Decachlor...	7.959	8.998	144.8E6	211.4E6	148.950	145.317
Target Compounds							
2)	A alpha-BHC	3.713	4.347	104.5E6	187.0E6	84.987	85.913
3)	MA gamma-BHC...	3.988	4.630	97024977	174.9E6	82.022	83.754
4)	MA Heptachlor	4.274	5.136	90328614	171.3E6	81.876	81.328
9)	A Endosulfan I	5.280	6.180	76847572	139.2E6	80.387	79.783
13)	MA Dieldrin	5.520	6.436	178.9E6	313.7E6	166.895	164.859
14)	MA Endrin	5.773	6.653	144.0E6	250.4E6	160.781	162.345
16)	A 4,4'-DDD	5.907	6.775	134.7E6	241.0E6	166.363	165.027
17)	MA 4,4'-DDT	6.142	7.073	137.8E6	247.3E6	185.327	173.862
20)	A Methoxychlor	6.691	7.530	307.4E6	595.2E6	760.017	749.964


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:58
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA5001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 06:00:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 05:45:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

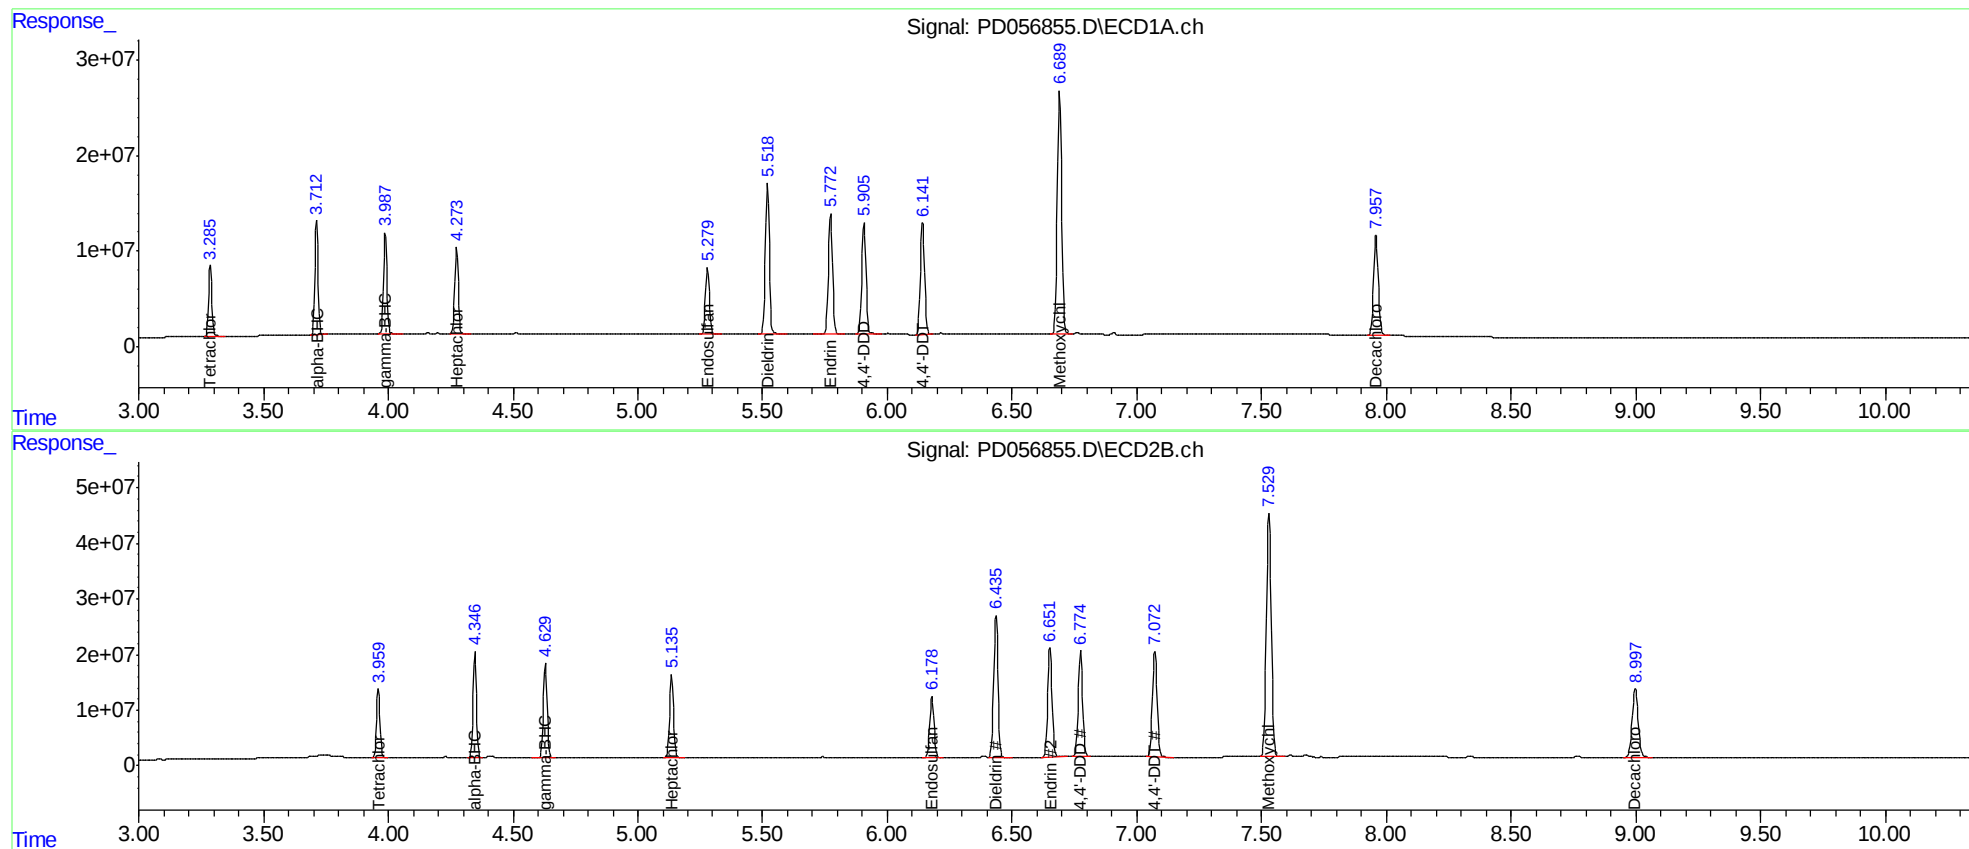


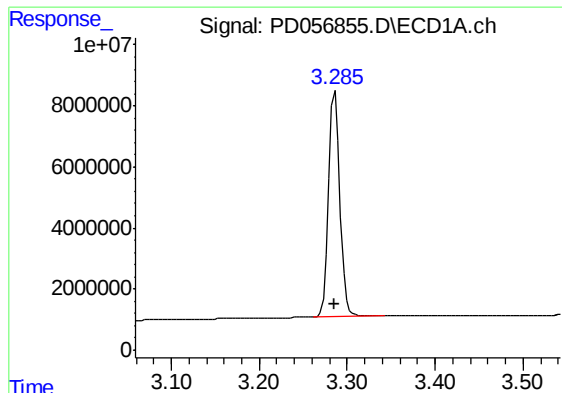

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: 0.000 min
Response: 66184934
Conc: 77.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

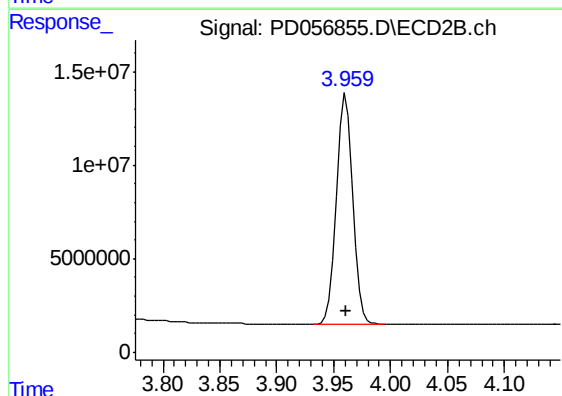


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 121350295
Conc: 78.07 ng/ml

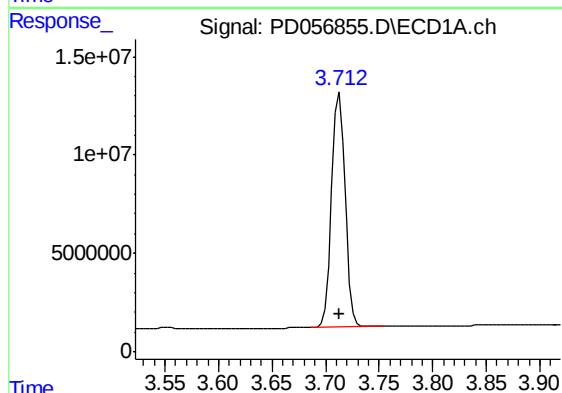


#2 alpha-BHC

R.T.: 3.713 min
Delta R.T.: 0.000 min
Response: 104502412
Conc: 84.99 ng/ml

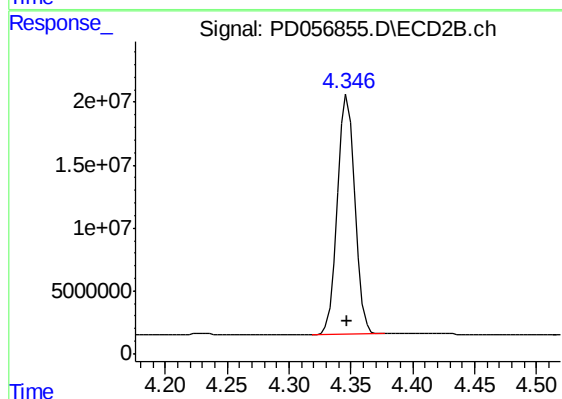

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 187009954
Conc: 85.91 ng/ml

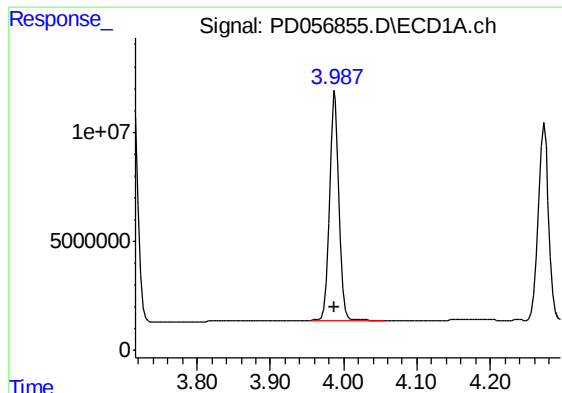

#3 gamma-BHC (Lindane)


R.T.: 3.988 min
Delta R.T.: 0.000 min
Response: 97024977
Conc: 82.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

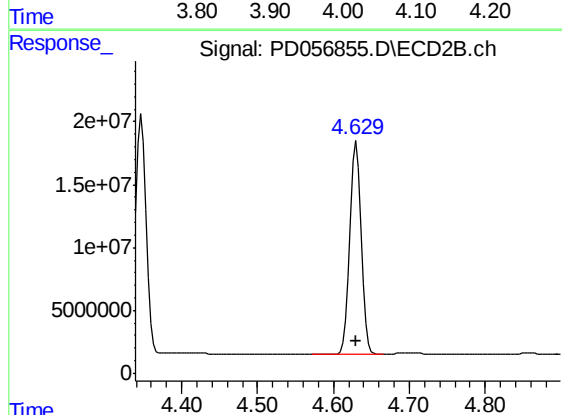


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 174948284
Conc: 83.75 ng/ml

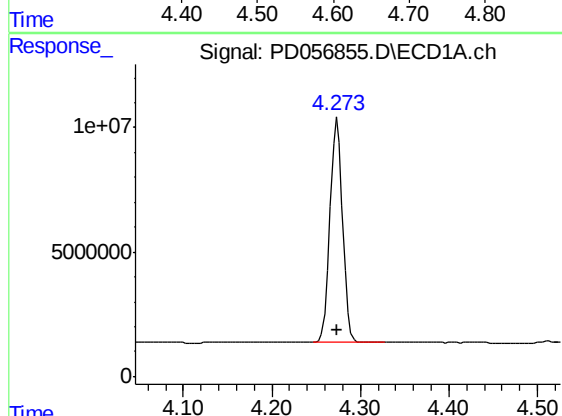


#4 Heptachlor

R.T.: 4.274 min
Delta R.T.: 0.000 min
Response: 90328614
Conc: 81.88 ng/ml

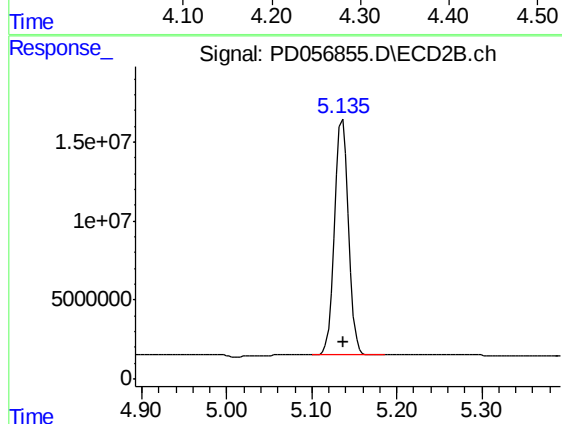

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 171323433
Conc: 81.33 ng/ml

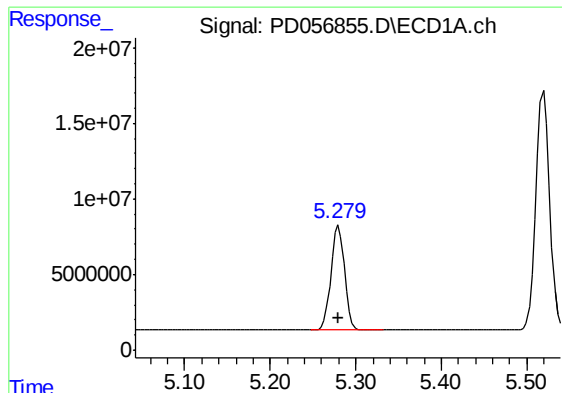

#9 Endosulfan I


R.T.: 5.280 min
Delta R.T.: 0.000 min
Response: 76847572
Conc: 80.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

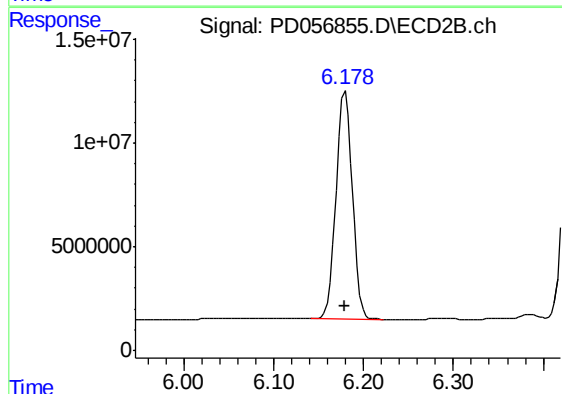


#9 Endosulfan I

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 139209280
Conc: 79.78 ng/ml

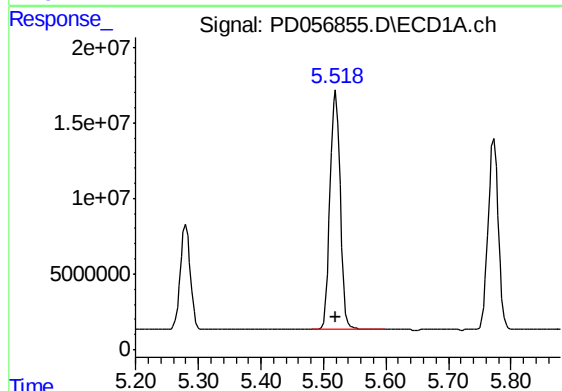


#13 Dieldrin

R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 178856804
Conc: 166.90 ng/ml

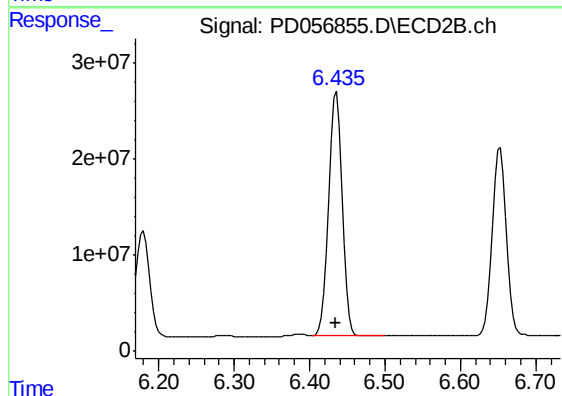

#13 Dieldrin


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 313671611
Conc: 164.86 ng/ml

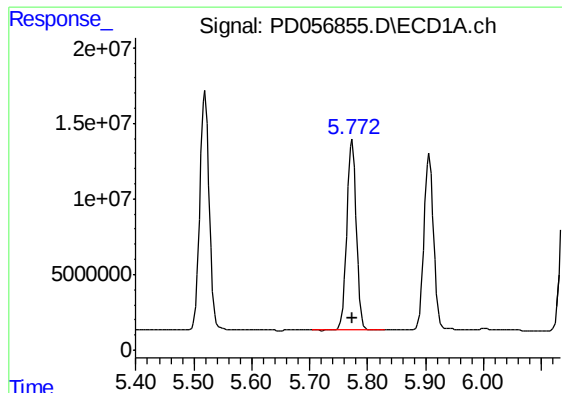

#14 Endrin


R.T.: 5.773 min
Delta R.T.: 0.000 min
Response: 143988197
Conc: 160.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

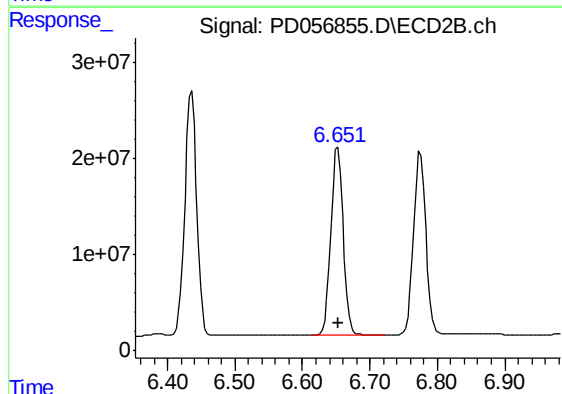


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 250362898
Conc: 162.34 ng/ml

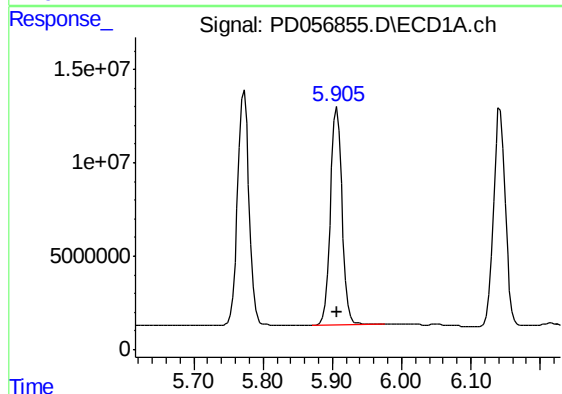


#16 4,4'-DDD

R.T.: 5.907 min
Delta R.T.: 0.000 min
Response: 134734584
Conc: 166.36 ng/ml

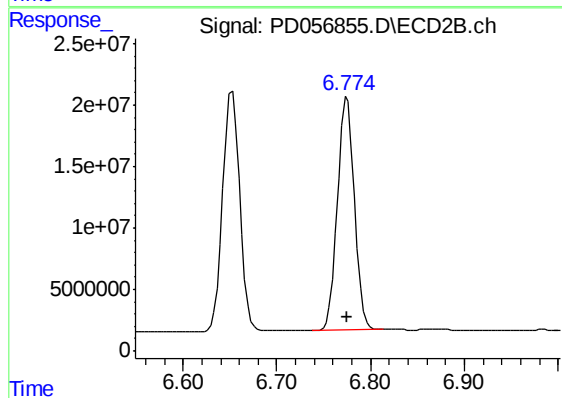

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 241019600
Conc: 165.03 ng/ml

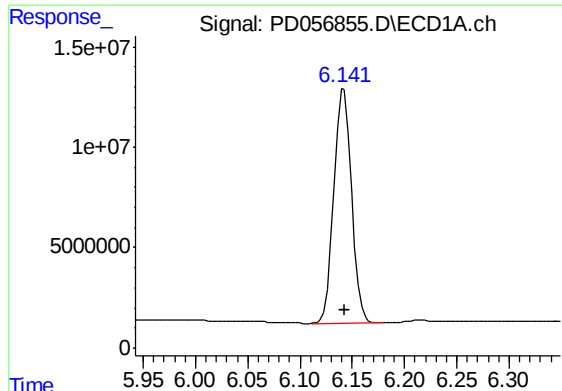

#17 4,4'-DDT


R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 137824796
Conc: 185.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

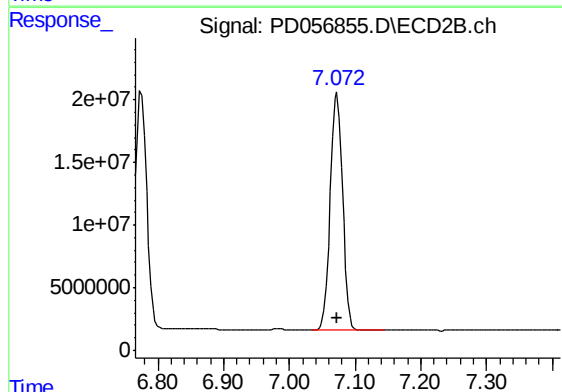


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 247285134
Conc: 173.86 ng/ml

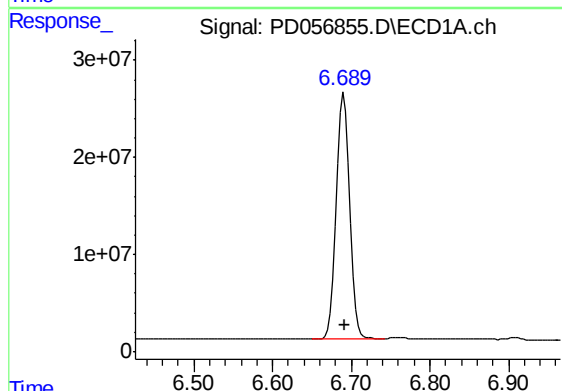


#20 Methoxychlor

R.T.: 6.691 min
Delta R.T.: -0.001 min
Response: 307435610
Conc: 760.02 ng/ml

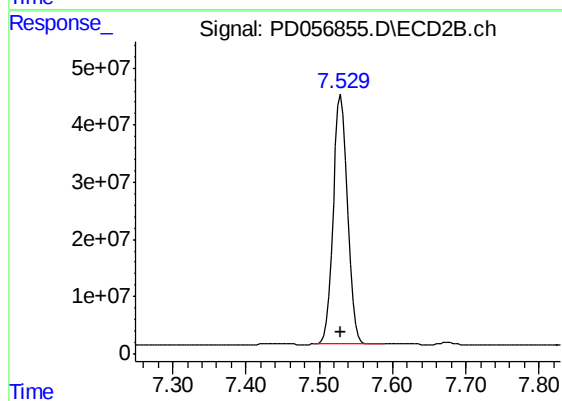

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 595241585
Conc: 749.96 ng/ml

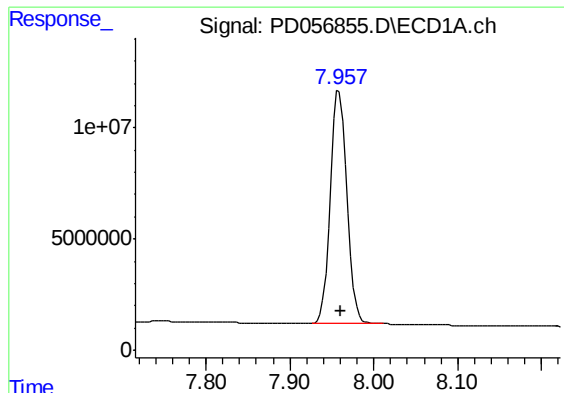

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.001 min
Response: 144765537
Conc: 148.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5001

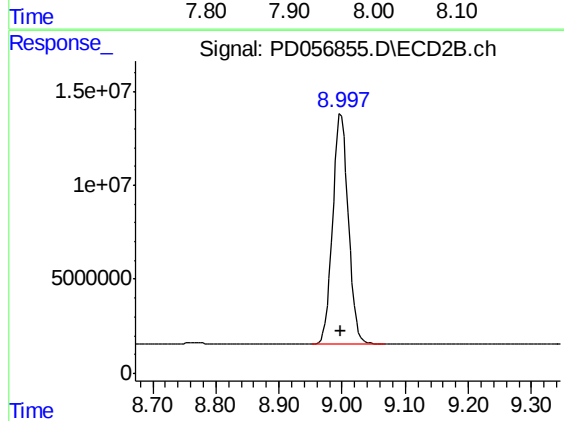

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 211407731
Conc: 145.32 ng/ml